
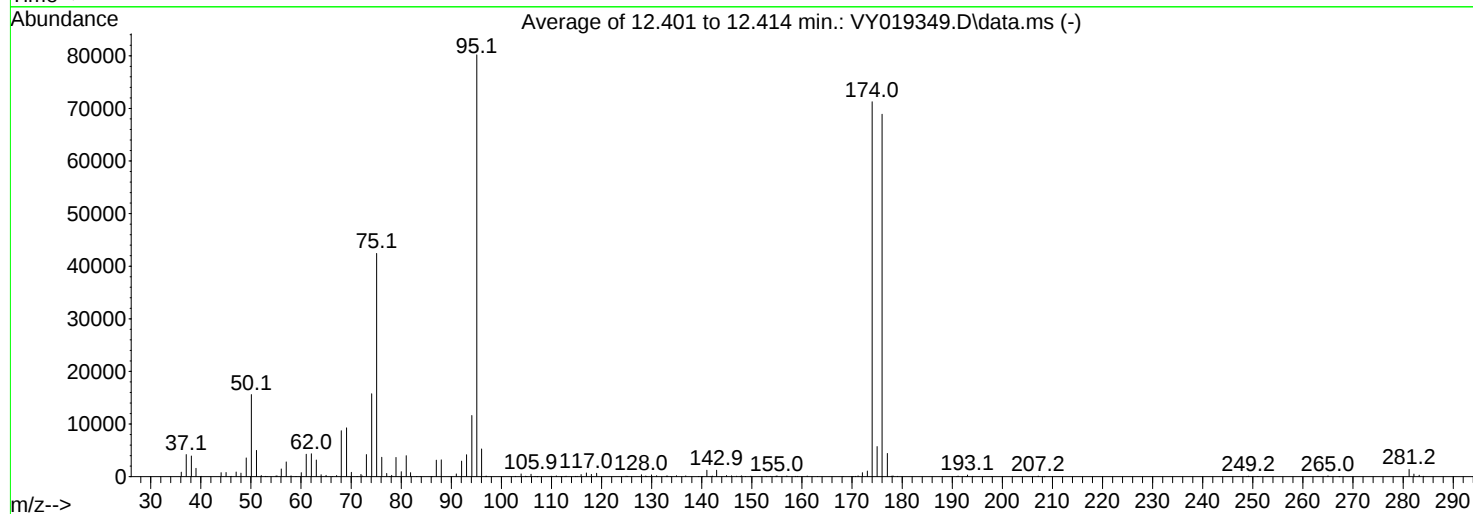


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082824\
Data File : VY019349.D
Acq On : 28 Aug 2024 23:29
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
Title : SW846 8260
Last Update : Fri Aug 16 05:10:30 2024

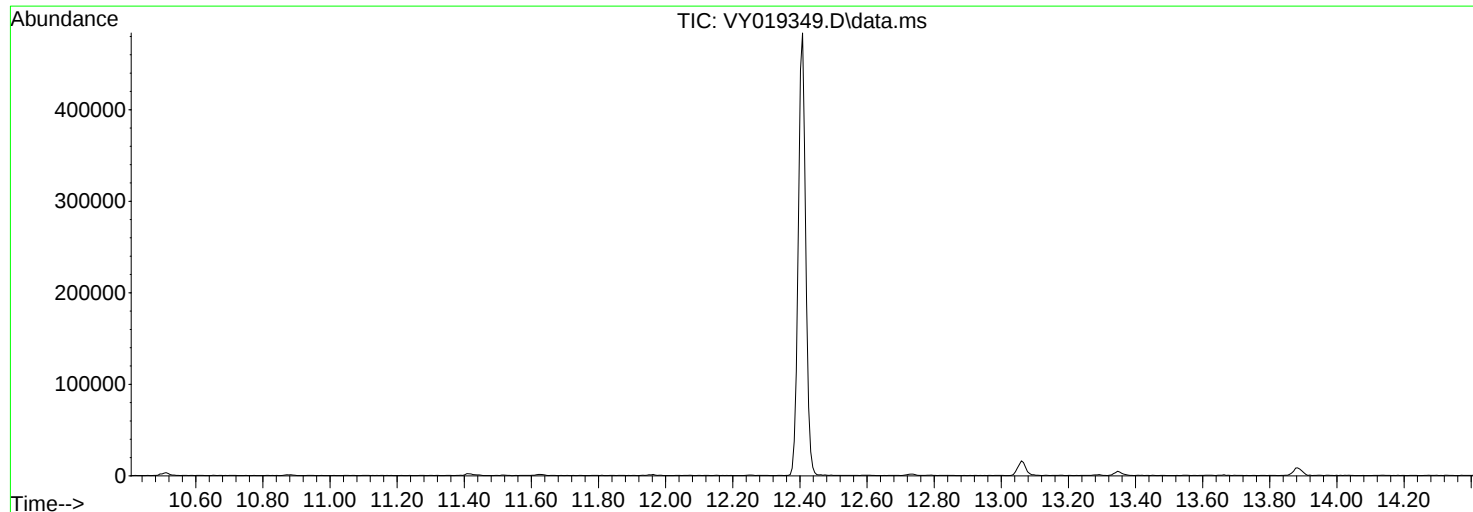

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	15617	PASS
75	95	30	60	52.9	42445	PASS
95	95	100	100	100.0	80184	PASS
96	95	5	9	6.6	5271	PASS
173	174	0.00	2	1.5	1059	PASS
174	95	50	100	88.9	71277	PASS
175	174	5	9	8.0	5718	PASS
176	174	95	101	96.7	68904	PASS
177	176	5	9	6.4	4417	PASS