

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082825\
 Data File : VY023228.D
 Acq On : 28 Aug 2025 15:51
 Operator : SY/MD
 Sample : Q2969-01
 Misc : 5.05g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TR-05-08272025

Quant Time: Aug 29 02:12:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	425323	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	799580	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	729108	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	295626	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	240329	59.288	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	118.580%
35) Dibromofluoromethane	7.634	113	265535	55.500	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	111.000%
50) Toluene-d8	10.109	98	955913	51.144	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	102.280%
62) 4-Bromofluorobenzene	12.402	95	279689	46.530	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	93.060%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082825\
Data File : VY023228.D
Acq On : 28 Aug 2025 15:51
Operator : SY/MD
Sample : Q2969-01
Misc : 5.05g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TR-05-08272025

Quant Time: Aug 29 02:12:07 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration




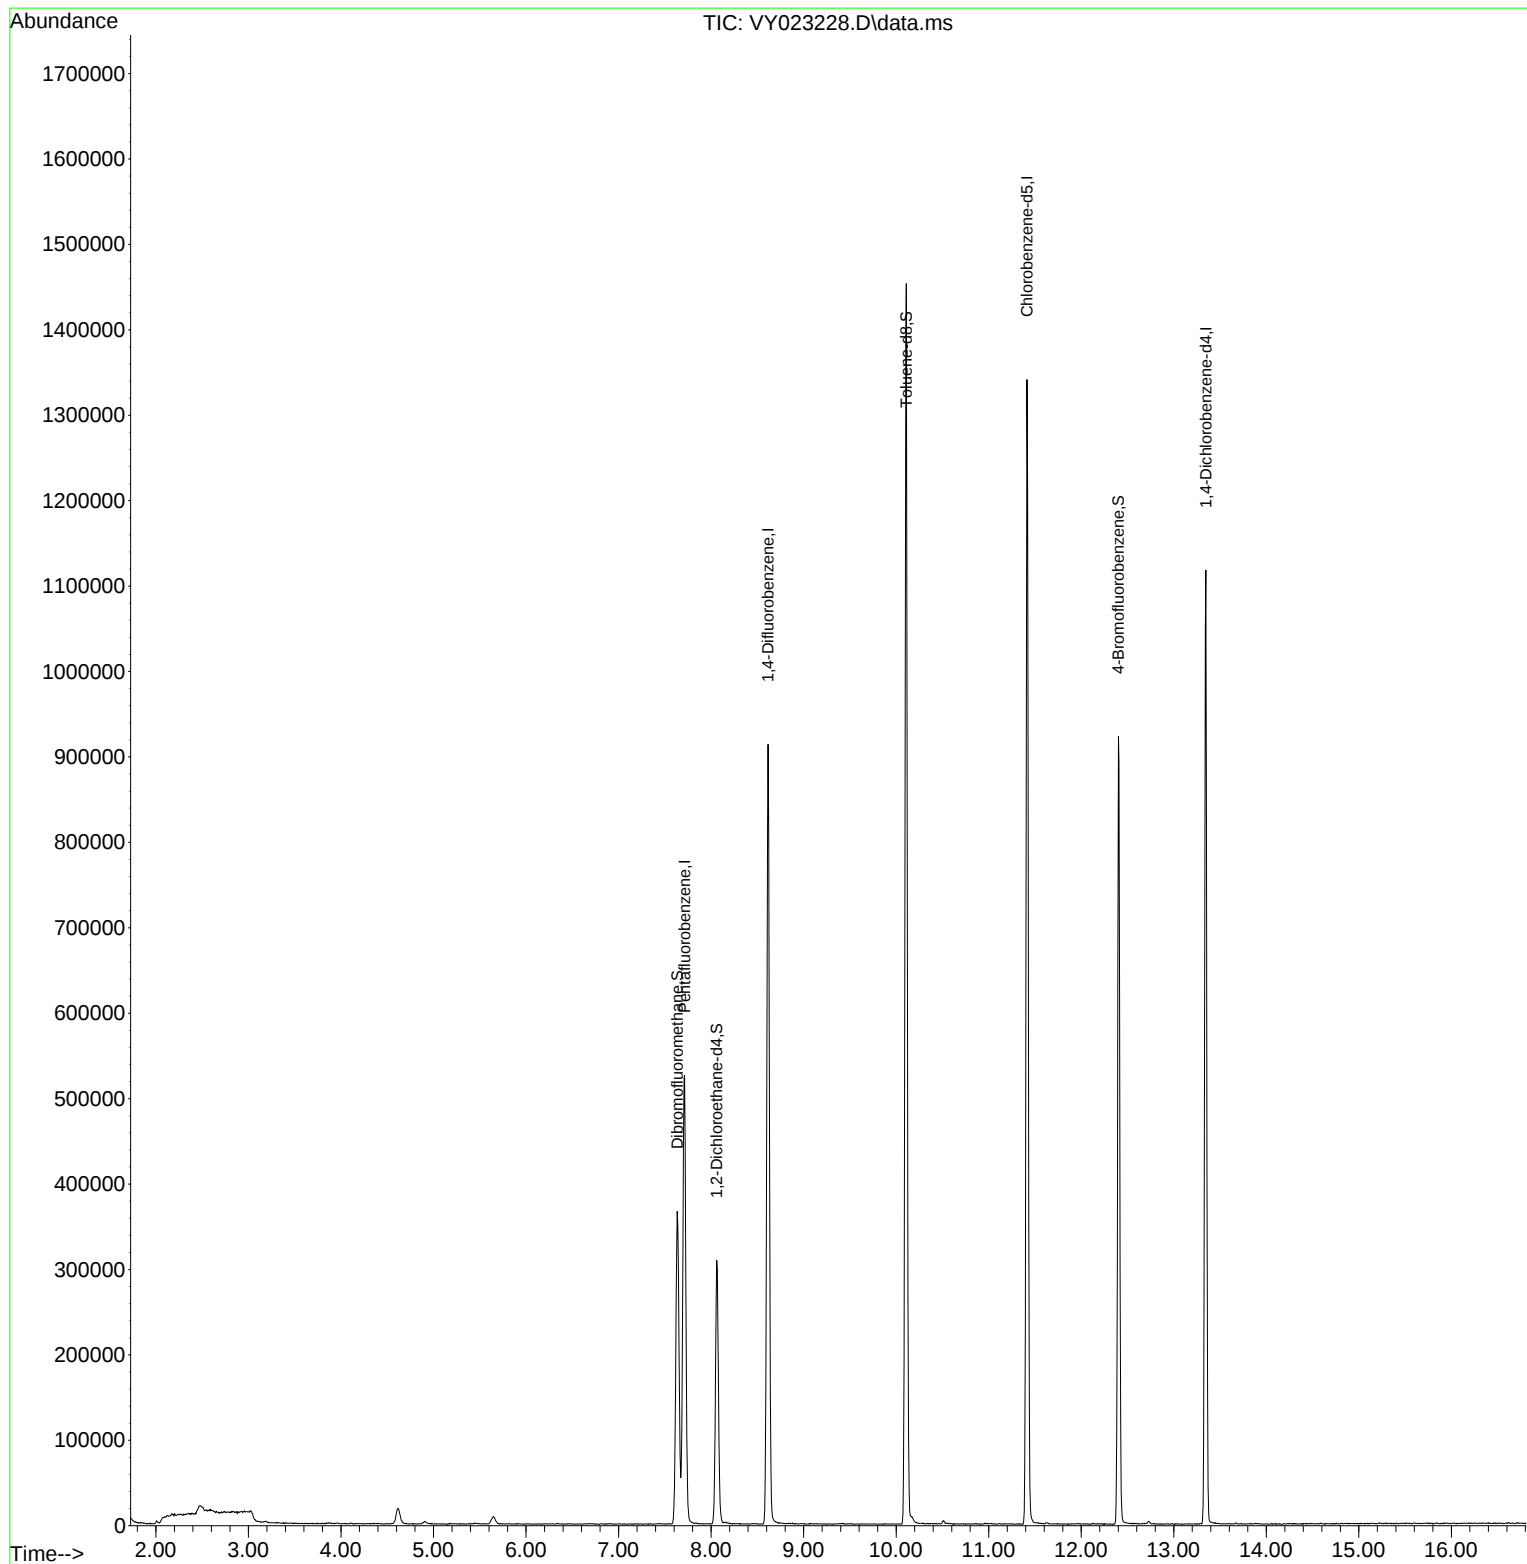




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY023228.D
Acq: 28 Aug 2025 15:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-05-08272025


Tgt Ion:168 Resp: 425323
Ion Ratio Lower Upper
168 100
99 53.2 42.8 64.2

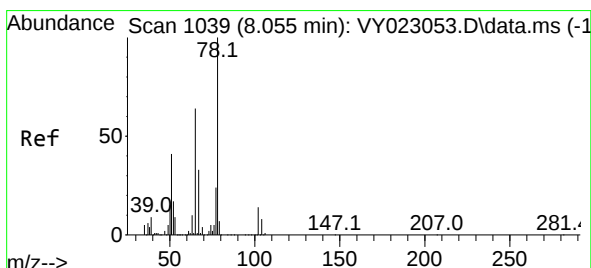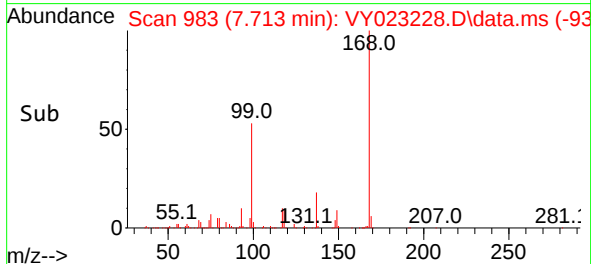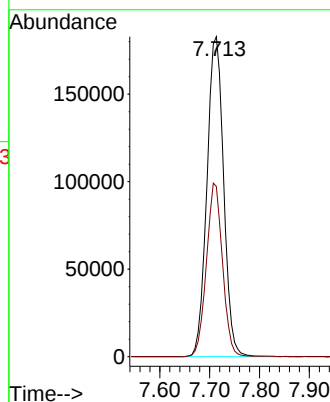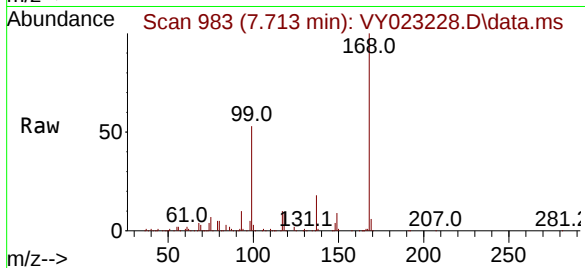

#33
1,2-Dichloroethane-d4
Concen: 59.288 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VY023228.D
Acq: 28 Aug 2025 15:51

Tgt Ion: 65 Resp: 240329
Ion Ratio Lower Upper
65 100
67 53.3 0.0 106.8

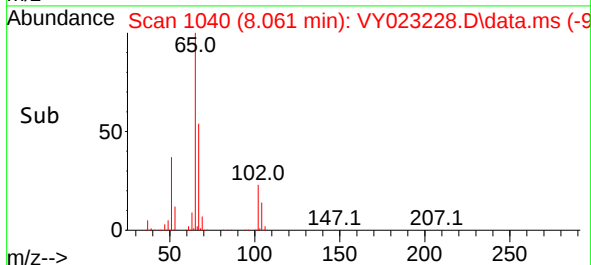
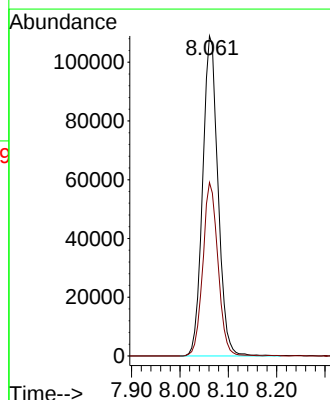
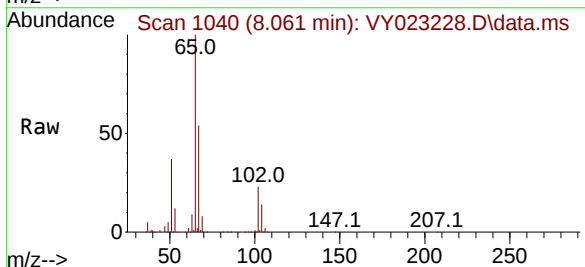


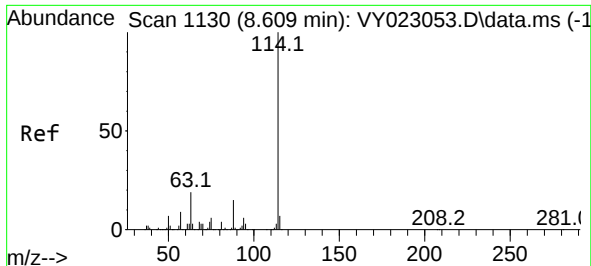

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.006 min
Lab File: VY023228.D
Acq: 28 Aug 2025 15:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-05-08272025

Tgt Ion:114 Resp: 799580
Ion Ratio Lower Upper
114 100
63 18.5 0.0 38.4
88 14.8 0.0 30.0

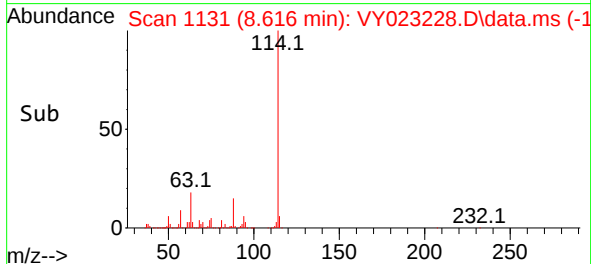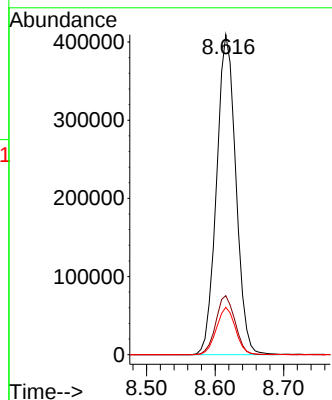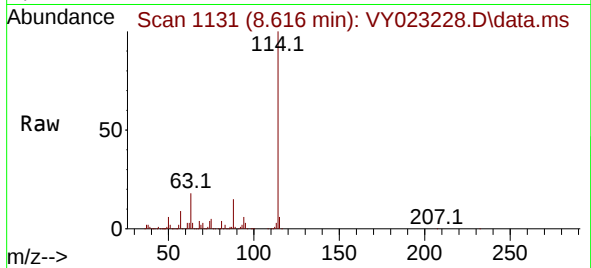

#35
Dibromofluoromethane
Concen: 55.500 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.006 min
Lab File: VY023228.D
Acq: 28 Aug 2025 15:51

Tgt Ion:113 Resp: 265535
Ion Ratio Lower Upper
113 100
111 102.8 81.1 121.7
192 20.0 16.2 24.4


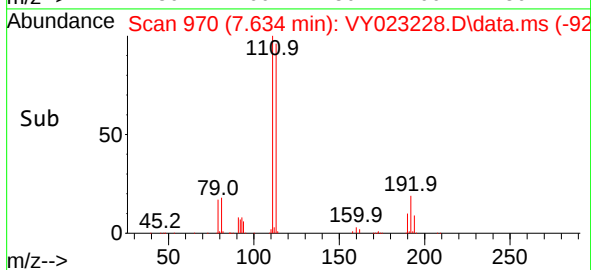
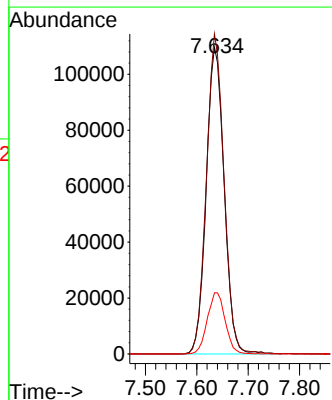
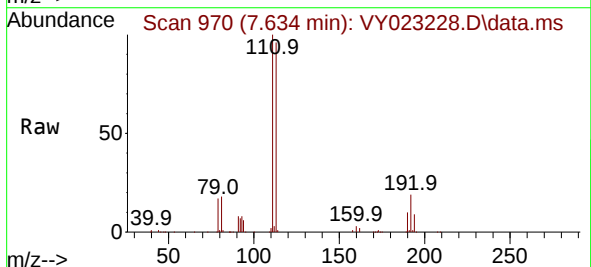




#50
Toluene-d8
Concen: 51.144 ug/l
RT: 10.109 min Scan# 1375
Delta R.T. 0.006 min
Lab File: VY023228.D
Acq: 28 Aug 2025 15:51




Instrument :
MSVOA_Y
ClientSampleId :
TR-05-08272025


Tgt Ion: 98 Resp: 955913
Ion Ratio Lower Upper
98 100
100 65.3 52.3 78.5

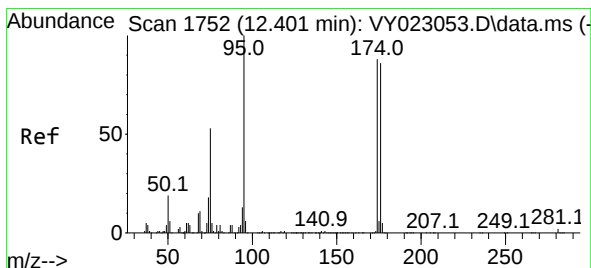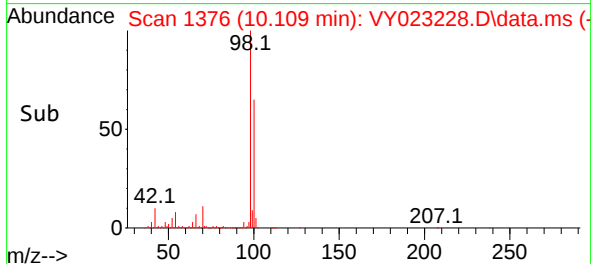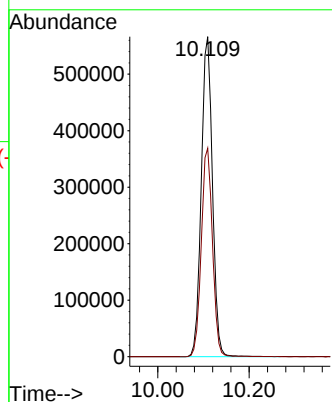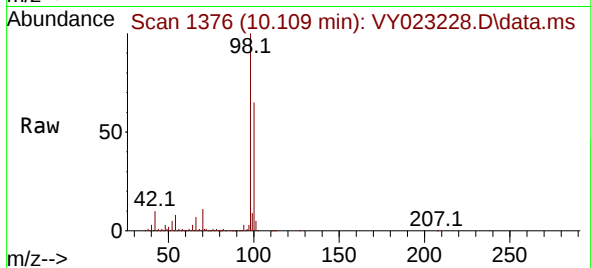

#62
4-Bromofluorobenzene
Concen: 46.530 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. 0.000 min
Lab File: VY023228.D
Acq: 28 Aug 2025 15:51

Tgt Ion: 95 Resp: 279689
Ion Ratio Lower Upper
95 100
174 90.9 0.0 171.6
176 85.9 0.0 167.6

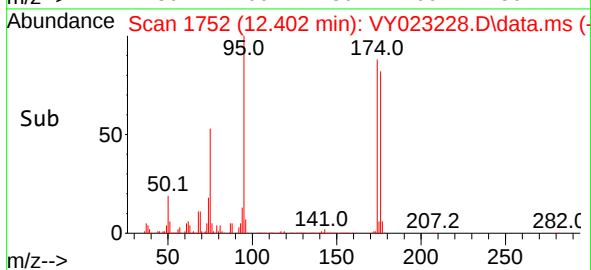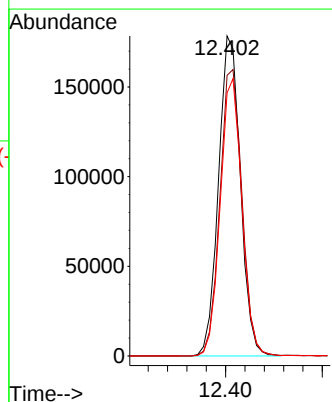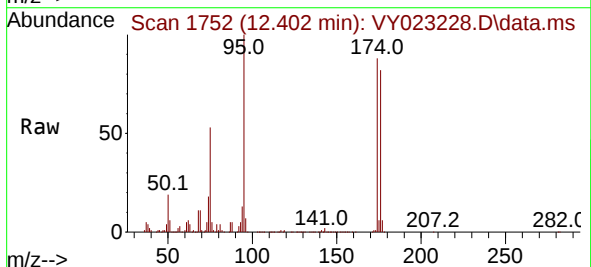

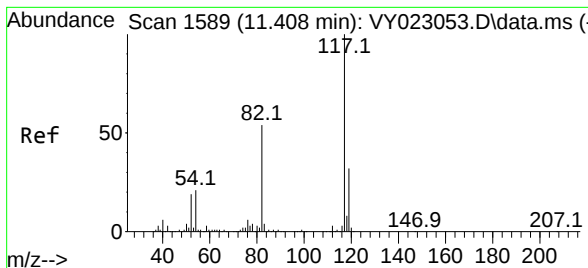

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY023228.D

Acq: 28 Aug 2025 15:51

Instrument :

MSVOA_Y

ClientSampleId :

TR-05-08272025





Tgt Ion:117 Resp: 729108

Ion Ratio Lower Upper

117 100

82 53.2 43.4 65.0

119 31.6 25.6 38.4

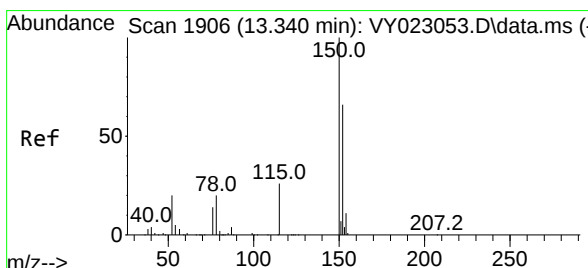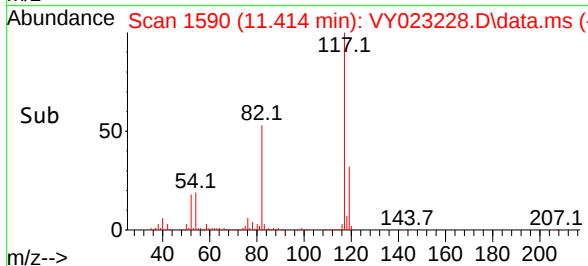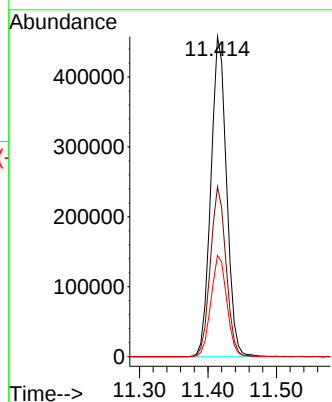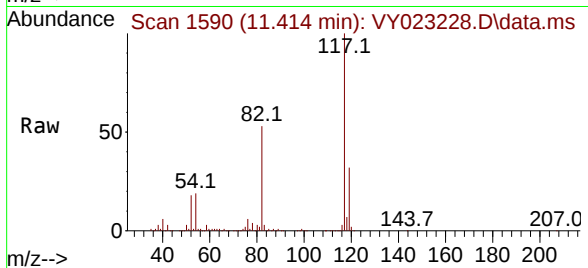

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. 0.006 min

Lab File: VY023228.D

Acq: 28 Aug 2025 15:51

Tgt Ion:152 Resp: 295626

Ion Ratio Lower Upper

152 100

115 55.4 28.2 84.6

150 156.2 0.0 348.0

