
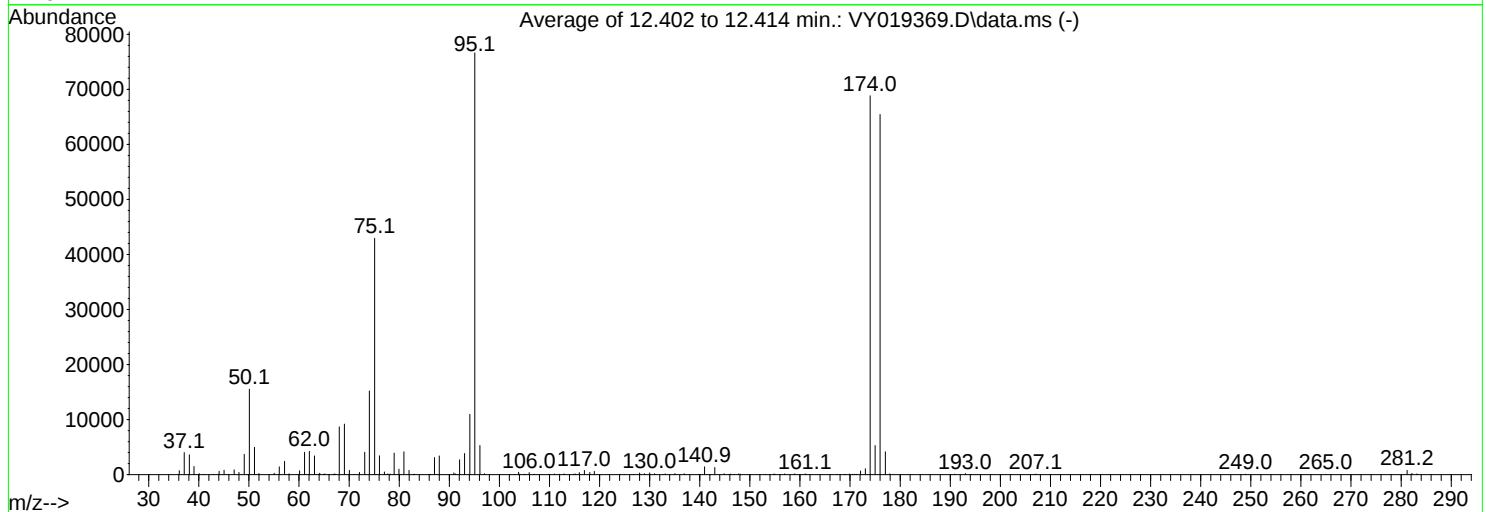


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082924\
Data File : VY019369.D
Acq On : 29 Aug 2024 10:03
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082924S.M
Title : SW846 8260
Last Update : Fri Aug 30 02:45:30 2024

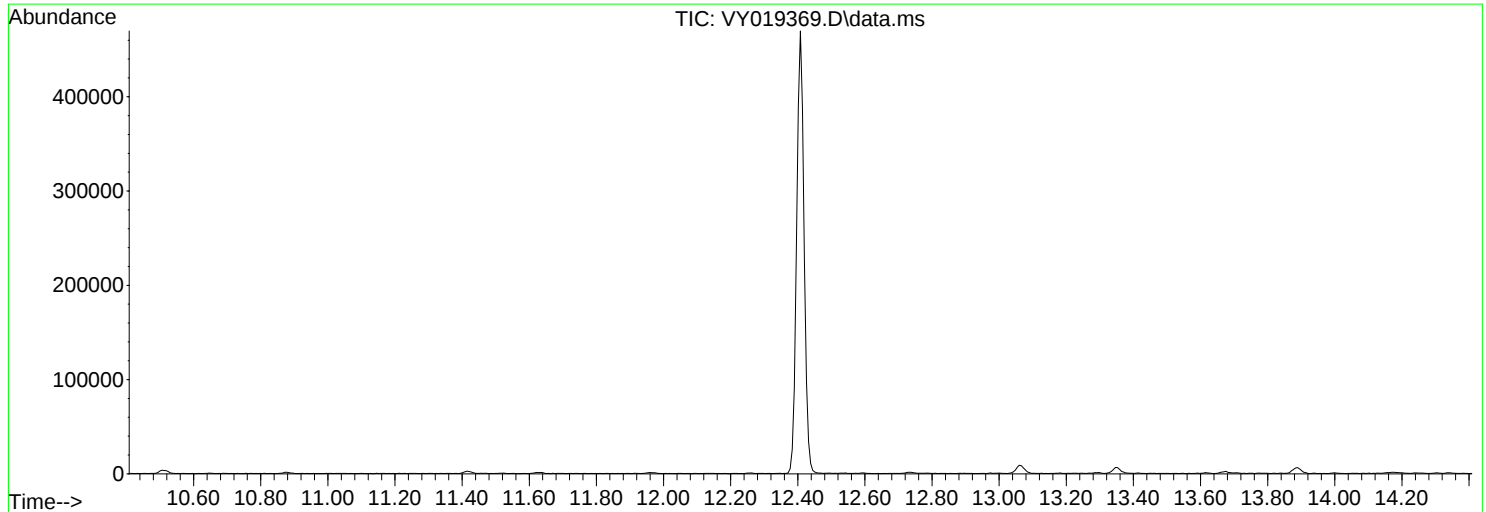

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	15531	PASS
75	95	30	60	56.0	42947	PASS
95	95	100	100	100.0	76632	PASS
96	95	5	9	6.9	5306	PASS
173	174	0.00	2	1.6	1078	PASS
174	95	50	100	89.8	68837	PASS
175	174	5	9	7.7	5288	PASS
176	174	95	101	95.1	65437	PASS
177	176	5	9	6.4	4162	PASS