

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082925\
 Data File : VY023244.D
 Acq On : 29 Aug 2025 13:55
 Operator : SY/MD
 Sample : Q2986-03
 Misc : 5.02g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 NORTH-TP-2


Quant Time: Aug 30 01:21:46 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	2537	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.622	114	3785	50.000	ug/l	0.01
63) Chlorobenzene-d5	11.420	117	1830	50.000	ug/l	# 0.01
72) 1,4-Dichlorobenzene-d4	13.352	152	527	50.000	ug/l	0.01
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	1539	63.649	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 127.300%	
35) Dibromofluoromethane	7.640	113	1531	67.599	ug/l	0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	= 135.200%	
50) Toluene-d8	10.109	98	2559	28.923	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 57.840%#	
62) 4-Bromofluorobenzene	12.395	95	565	19.857	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 39.720%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.074	50	80	2.385	ug/l #	47
5) Bromomethane	2.616	94	368	11.885	ug/l #	18
10) Methyl Iodide	4.006	142	155	5.775	ug/l #	78
12) 1,1-Dichloroethene	3.854	96	78	3.191	ug/l #	1
14) Allyl chloride	4.324	41	46	1.279	ug/l #	20
16) Acetone	3.689	43	23	4.391	ug/l #	41
18) Methyl Acetate	4.378	43	82	5.260	ug/l #	48
19) Methyl tert-butyl Ether	5.128	73	94	1.484	ug/l #	55
20) Methylene Chloride	4.586	84	19	Below Cal	#	8
21) trans-1,2-Dichloroethene	5.122	96	76	2.766	ug/l #	1
25) 2-Butanone	6.707	43	27	3.790	ug/l #	45
27) cis-1,2-Dichloroethene	6.902	96	49	1.543	ug/l #	1
29) Tetrahydrofuran	7.232	42	28	6.340	ug/l #	29
31) Cyclohexane	7.677	56	51	1.132	ug/l #	12
36) 1,1-Dichloropropene	7.719	75	58	1.723	ug/l #	41
37) Ethyl Acetate	7.073	43	23	1.627	ug/l #	67
38) Carbon Tetrachloride	7.707	117	302	8.261	ug/l #	13
41) Methacrylonitrile	7.286	41	20	2.451	ug/l #	21
43) Isopropyl Acetate	8.183	43	58	2.030	ug/l #	59
48) Methyl methacrylate	9.219	41	76	5.558	ug/l #	11
51) 4-Methyl-2-Pentanone	10.012	43	23	1.560	ug/l #	34
53) t-1,3-Dichloropropene	10.316	75	52	1.629	ug/l #	43
54) cis-1,3-Dichloropropene	9.896	75	41	1.086	ug/l #	36
59) 2-Hexanone	10.804	43	63	6.276	ug/l #	21
65) Chlorobenzene	11.578	112	43	1.089	ug/l #	41
74) N-amyl acetate	12.060	43	21	2.662	ug/l #	40
75) 1,1,2,2-Tetrachloroethane	12.218	83	29	4.566	ug/l #	26
76) 1,2,3-Trichloropropane	12.407	75	288	56.625	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.407	75	288	137.071	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	14.413	75	46	46.520	ug/l #	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Aug 30 01:21:46 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration




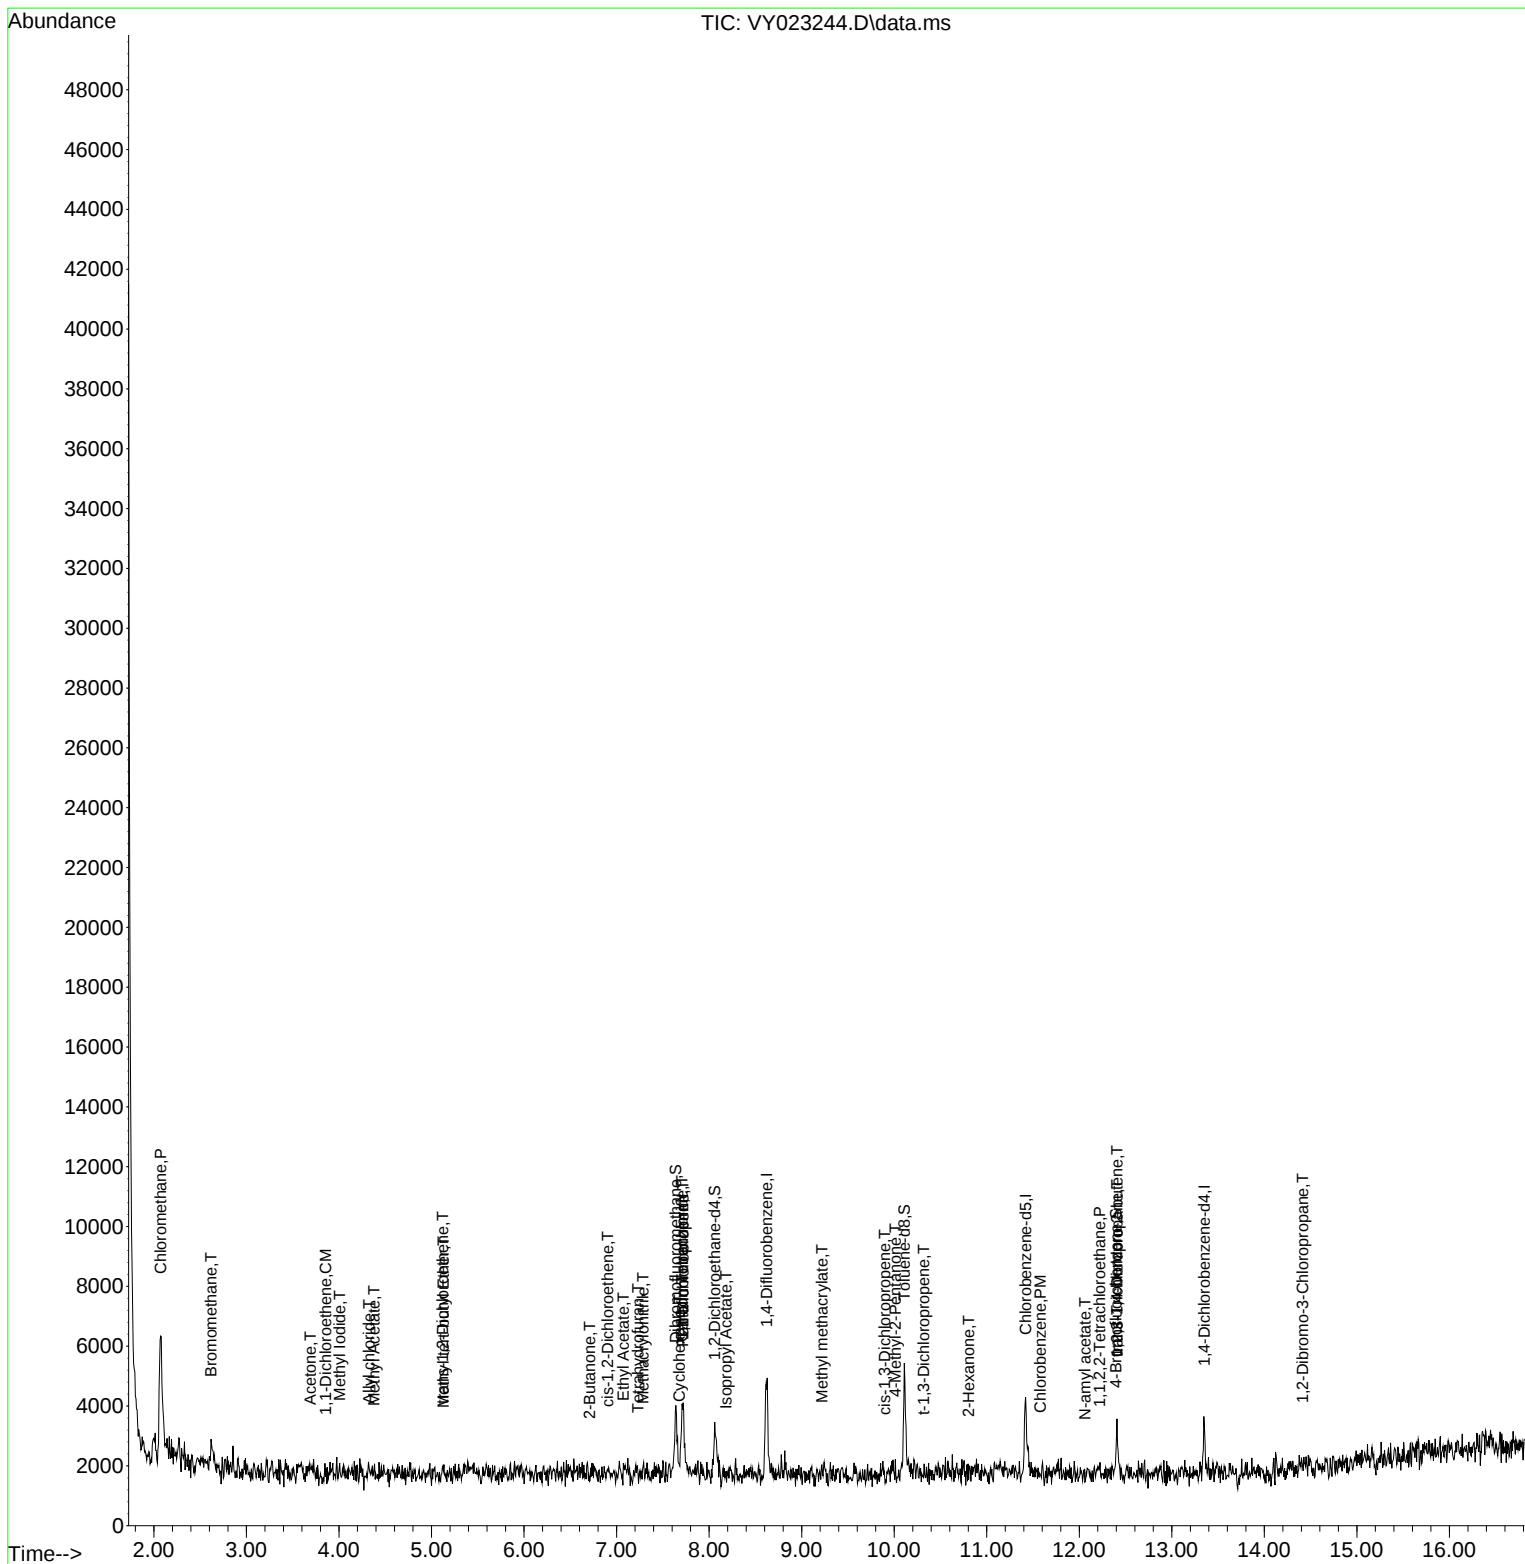




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55




Instrument :
MSVOA_Y
ClientSampleId :
NORTH-TP-2


Tgt Ion:168 Resp: 2537
Ion Ratio Lower Upper
168 100
99 53.6 42.8 64.2

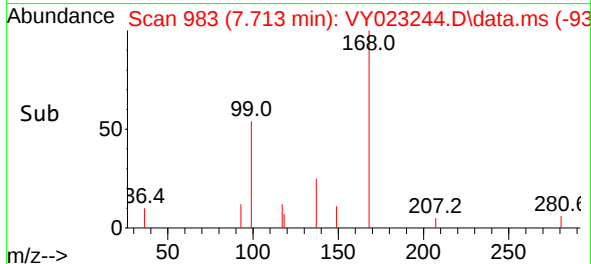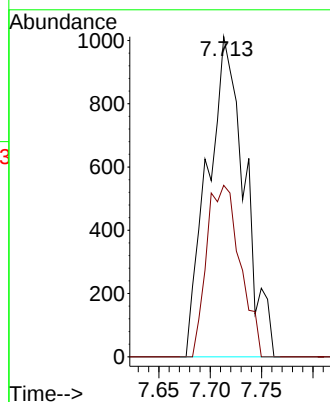

#3
Chloromethane
Concen: 2.385 ug/l
RT: 2.074 min Scan# 58
Delta R.T. 0.006 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55

Tgt Ion: 50 Resp: 80
Ion Ratio Lower Upper
50 100
52 63.4 26.7 40.1#


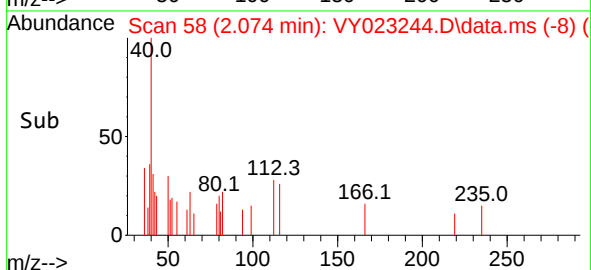
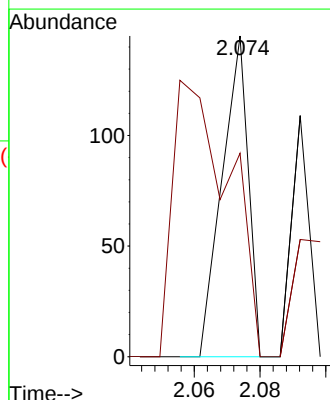



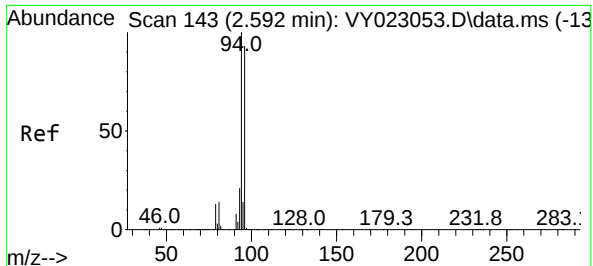

#5
Bromomethane
Concen: 11.885 ug/l
RT: 2.616 min Scan# 143
Delta R.T. 0.024 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55




Instrument :
MSVOA_Y
ClientSampleId :
NORTH-TP-2


Tgt Ion: 94 Resp: 368
Ion Ratio Lower Upper
94 100
96 171.7 74.6 112.0#

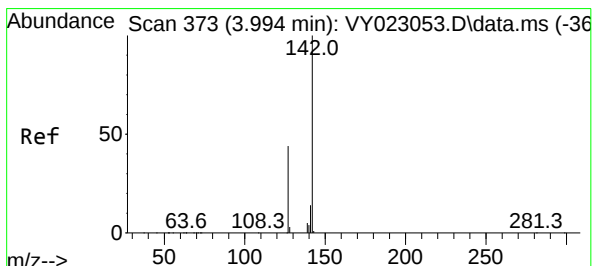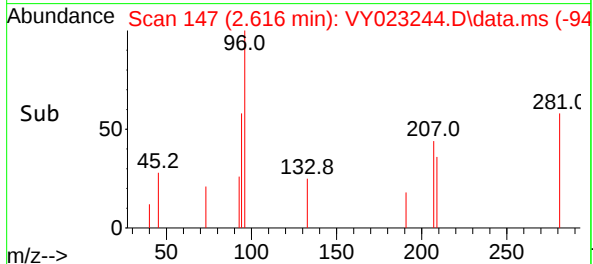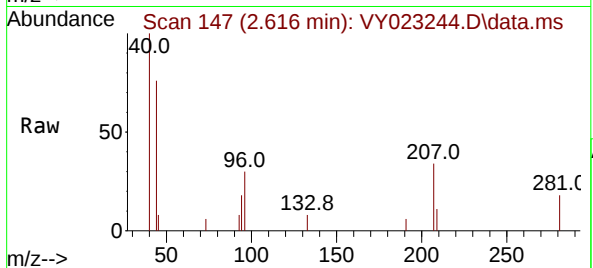

#10
Methyl Iodide
Concen: 5.775 ug/l
RT: 4.006 min Scan# 375
Delta R.T. 0.012 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55

Tgt Ion: 142 Resp: 155
Ion Ratio Lower Upper
142 100
127 54.8 34.9 52.3#
141 0.0 11.3 16.9#

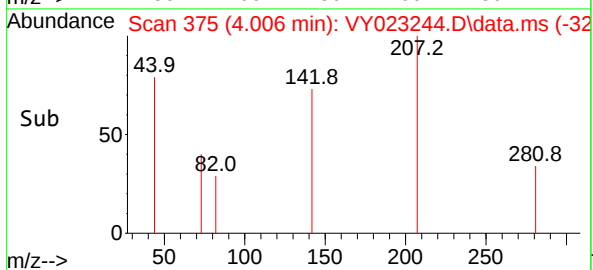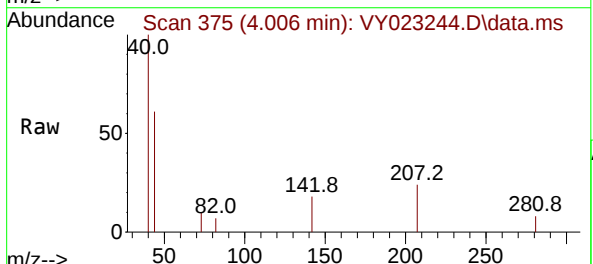



#12

1,1-Dichloroethene

Concen: 3.191 ug/l

RT: 3.854 min Scan# 31

Delta R.T. 0.073 min

Lab File: VY023244.D

Acq: 29 Aug 2025 13:55

Instrument :

MSVOA_Y

ClientSampleId :

NORTH-TP-2





Tgt Ion: 96 Resp: 78

Ion Ratio Lower Upper

96 100

61 0.0 129.4 194.2#

98 0.0 52.8 79.2#

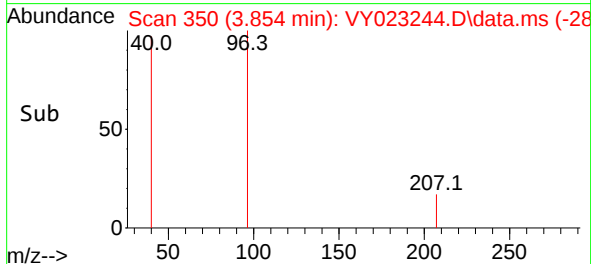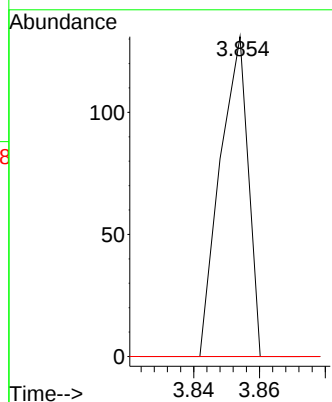

#14

Allyl chloride

Concen: 1.279 ug/l

RT: 4.324 min Scan# 427

Delta R.T. -0.055 min

Lab File: VY023244.D

Acq: 29 Aug 2025 13:55




Tgt Ion: 41 Resp: 46


Ion Ratio Lower Upper

41 100

39 0.0 59.8 89.6#

76 0.0 33.7 50.5#


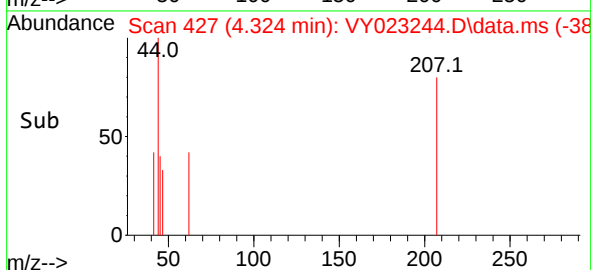






#16
Acetone
Concen: 4.391 ug/l
RT: 3.689 min Scan# 31
Delta R.T. -0.171 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55




Instrument :
MSVOA_Y
ClientSampleId :
NORTH-TP-2


Tgt Ion: 43 Resp: 23
Ion Ratio Lower Upper
43 100
58 0.0 27.1 40.7#

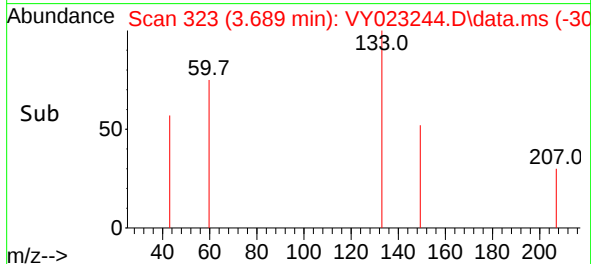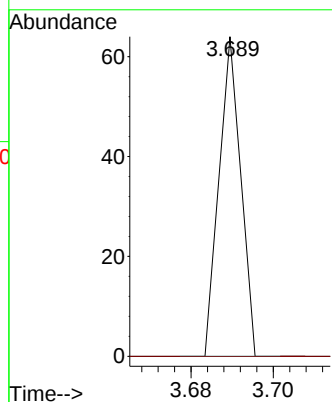

#18
Methyl Acetate
Concen: 5.260 ug/l
RT: 4.378 min Scan# 436
Delta R.T. -0.000 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55

Tgt Ion: 43 Resp: 82
Ion Ratio Lower Upper
43 100
74 0.0 21.2 31.8#

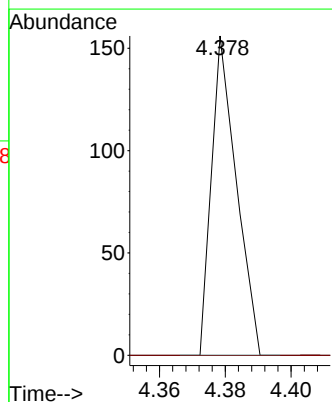



#19

Methyl tert-butyl Ether

Concen: 1.484 ug/l

RT: 5.128 min Scan# 51

Delta R.T. 0.018 min

Lab File: VY023244.D

Acq: 29 Aug 2025 13:55

Instrument :

MSVOA_Y

ClientSampleId :





NORTH-TP-2

Tgt Ion: 73 Resp: 94

Ion Ratio Lower Upper

73 100

57 0.0 17.1 25.7#

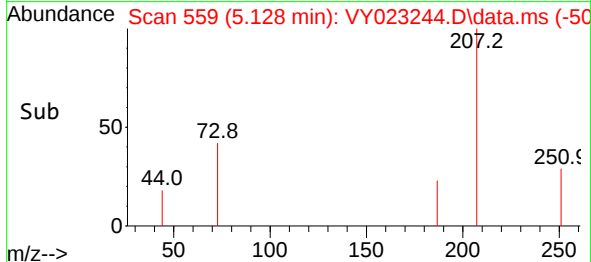

#20

Methylene Chloride

Concen: Below Cal

RT: 4.586 min Scan# 470

Delta R.T. -0.018 min

Lab File: VY023244.D

Acq: 29 Aug 2025 13:55

Tgt Ion: 84 Resp: 19




Ion Ratio Lower Upper


84 100

49 0.0 93.0 139.6#

51 0.0 29.0 43.4#

86 0.0 50.2 75.4#


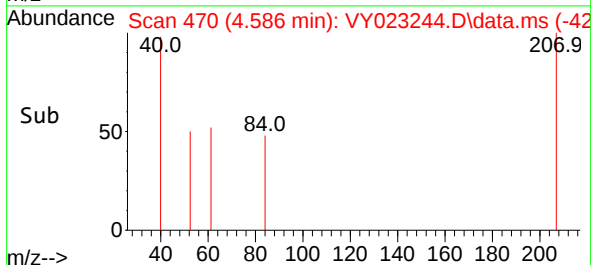
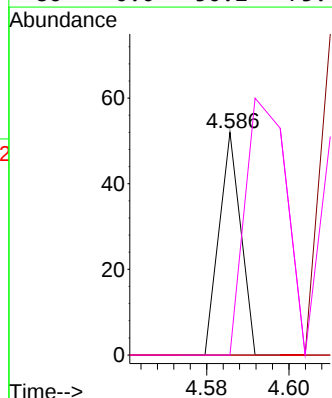
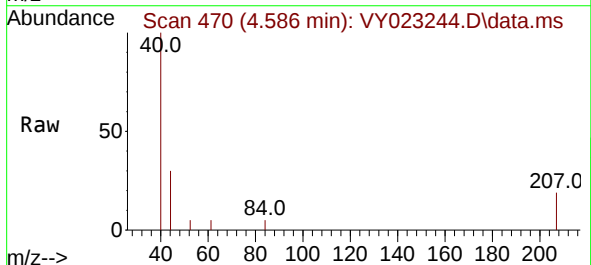




#21
trans-1,2-Dichloroethene
Concen: 2.766 ug/l
RT: 5.122 min Scan# 51
Delta R.T. 0.018 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55




Instrument :
MSVOA_Y
ClientSampleId :
NORTH-TP-2


Tgt Ion: 96 Resp: 76
Ion Ratio Lower Upper
96 100
61 0.0 104.8 157.2#
98 0.0 50.1 75.1#

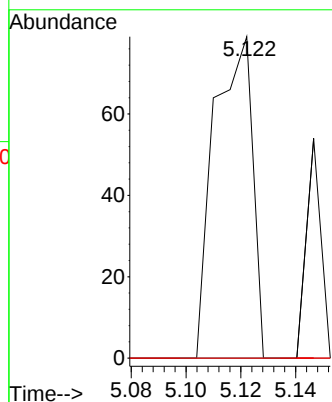

#25
2-Butanone
Concen: 3.790 ug/l
RT: 6.707 min Scan# 818
Delta R.T. -0.177 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55

Tgt Ion: 43 Resp: 27
Ion Ratio Lower Upper
43 100
72 0.0 23.5 35.3#

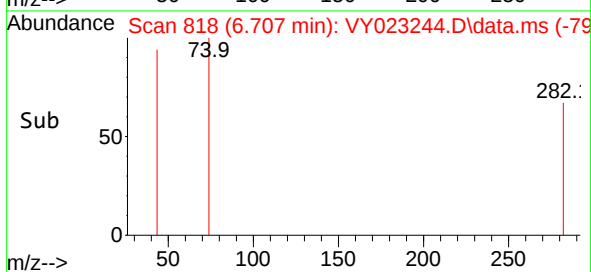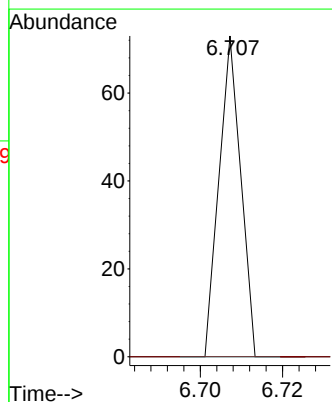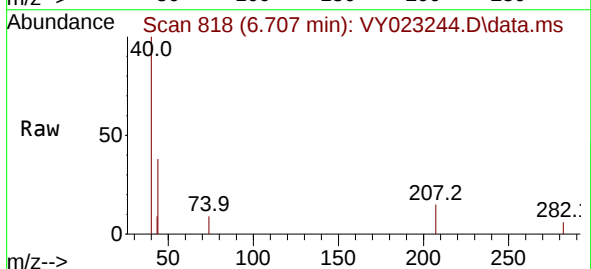



#27

cis-1,2-Dichloroethene

Concen: 1.543 ug/l

RT: 6.902 min Scan# 847

Delta R.T. 0.018 min

Lab File: VY023244.D

Acq: 29 Aug 2025 13:55

Instrument :

MSVOA_Y

ClientSampleId :

NORTH-TP-2





Tgt Ion: 96 Resp: 49

Ion Ratio Lower Upper

96 100

61 0.0 0.0 278.6

98 0.0 0.0 130.4

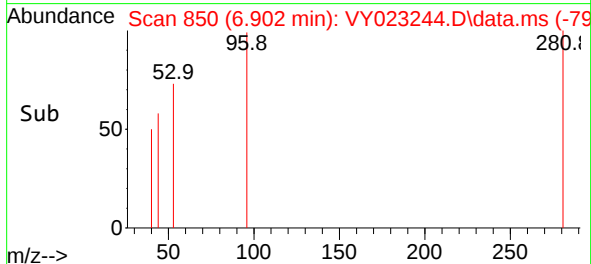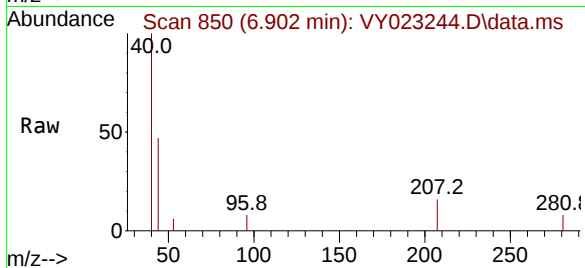

#29

Tetrahydrofuran

Concen: 6.340 ug/l

RT: 7.232 min Scan# 904

Delta R.T. -0.024 min

Lab File: VY023244.D

Acq: 29 Aug 2025 13:55




Tgt Ion: 42 Resp: 28


Ion Ratio Lower Upper

42 100

72 0.0 39.4 59.2#

71 0.0 36.5 54.7#


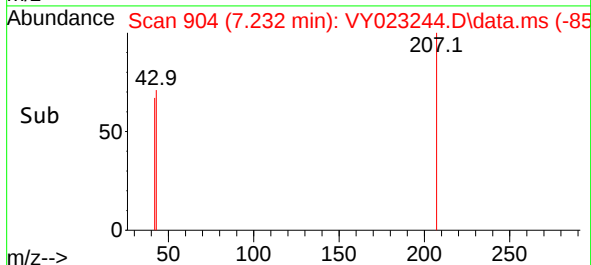
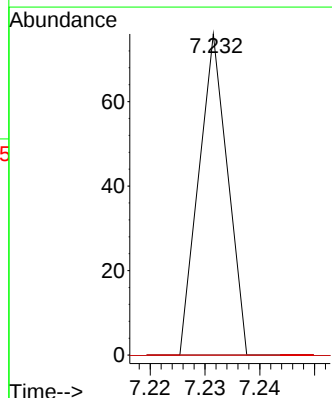
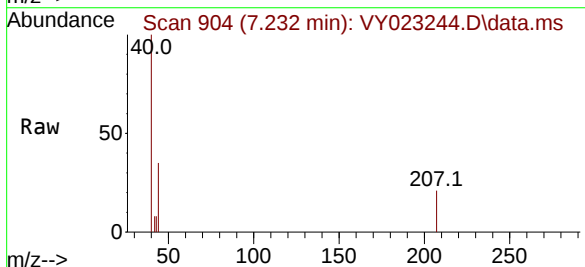




#31
Cyclohexane
Concen: 1.132 ug/l
RT: 7.677 min Scan# 91
Delta R.T. -0.018 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55




Instrument :
MSVOA_Y
ClientSampleId :
NORTH-TP-2


Tgt Ion: 56 Resp: 51
Ion Ratio Lower Upper
56 100
69 0.0 28.2 42.2#
84 0.0 76.6 114.8#

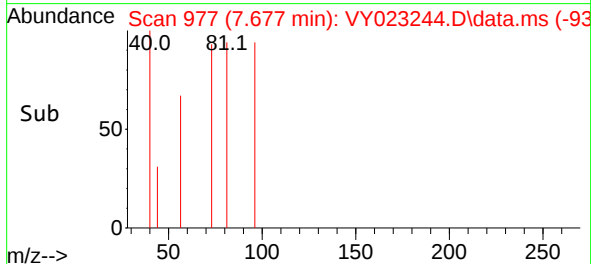

#33
1,2-Dichloroethane-d4
Concen: 63.649 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55

Tgt Ion: 65 Resp: 1539
Ion Ratio Lower Upper
65 100
67 50.9 0.0 106.8


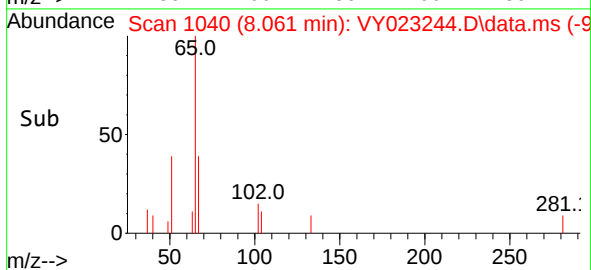






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.622 min Scan# 1132
Delta R.T. 0.012 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55




Instrument :
MSVOA_Y
ClientSampleId :
NORTH-TP-2


Tgt Ion:114	Resp:	3785
Ion Ratio	Lower	Upper
114	100	
63	12.7	0.0 38.4
88	16.0	0.0 30.0

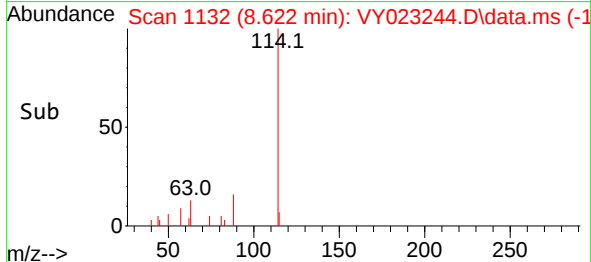

#35
Dibromofluoromethane
Concen: 67.599 ug/l
RT: 7.640 min Scan# 971
Delta R.T. 0.012 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55

Tgt Ion:113	Resp:	1531
Ion Ratio	Lower	Upper
113	100	
111	101.2	81.1 121.7
192	21.0	16.2 24.4

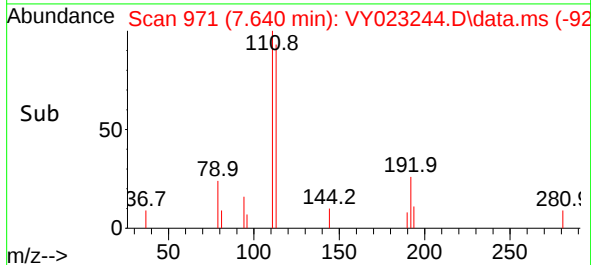

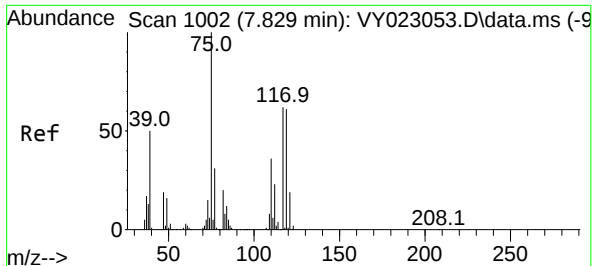

#36

1,1-Dichloropropene

Concen: 1.723 ug/l

RT: 7.719 min Scan# 91

Delta R.T. -0.110 min

Lab File: VY023244.D

Acq: 29 Aug 2025 13:55

Instrument :

MSVOA_Y

ClientSampleId :

NORTH-TP-2





Tgt Ion: 75 Resp: 58

Ion Ratio Lower Upper

75 100

110 0.0 18.1 54.4#

77 0.0 24.6 37.0#

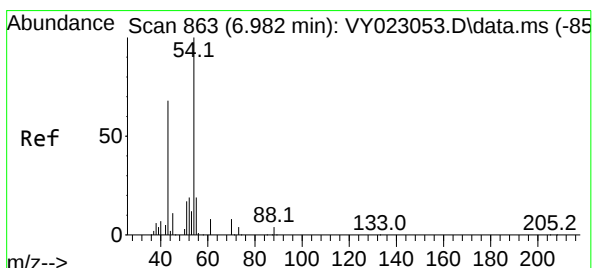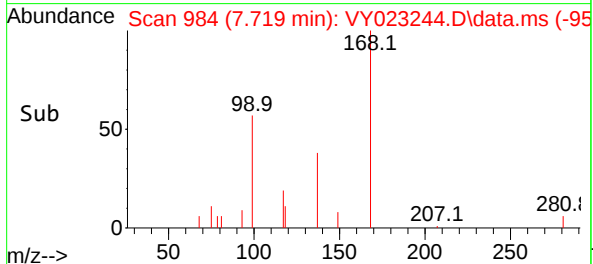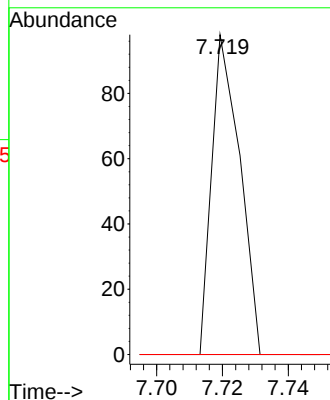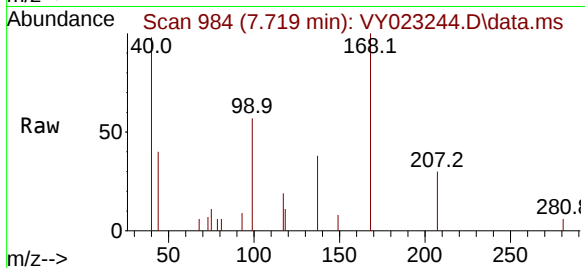

#37

Ethyl Acetate

Concen: 1.627 ug/l

RT: 7.073 min Scan# 878

Delta R.T. 0.091 min

Lab File: VY023244.D

Acq: 29 Aug 2025 13:55




Tgt Ion: 43 Resp: 23


Ion Ratio Lower Upper

43 100

61 0.0 11.9 17.9#

70 0.0 8.8 13.2#


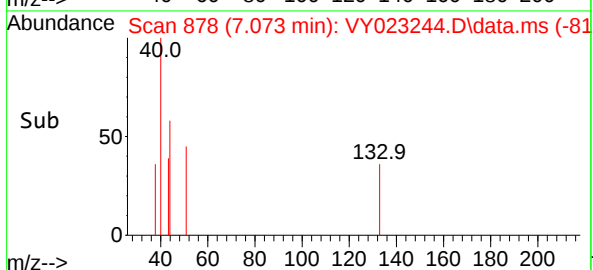
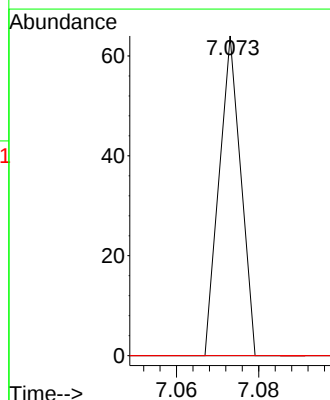
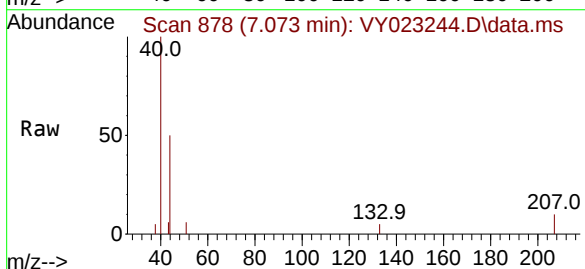


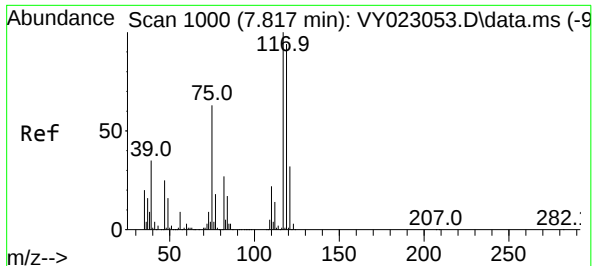

#38
Carbon Tetrachloride
Concen: 8.261 ug/l
RT: 7.707 min Scan# 913
Delta R.T. -0.110 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55




Instrument :
MSVOA_Y
ClientSampleId :
NORTH-TP-2


Tgt Ion: 117 Resp: 302
Ion Ratio Lower Upper
117 100
119 0.0 75.6 113.4#
121 0.0 25.8 38.8#

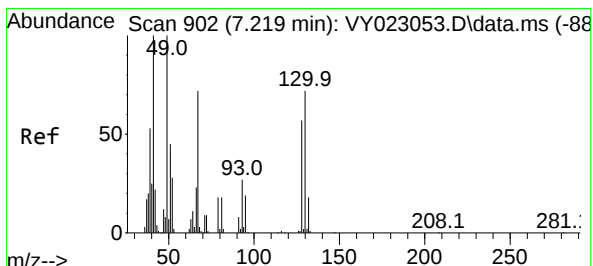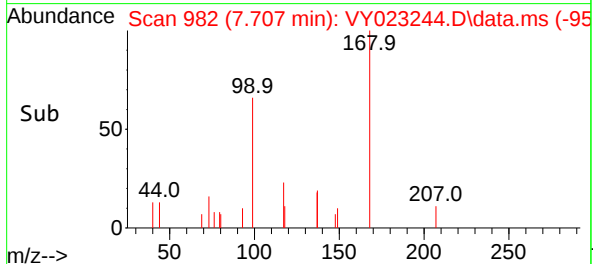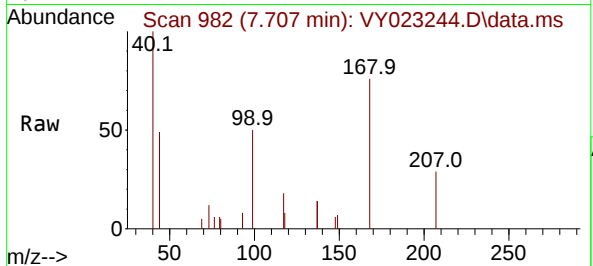

#41
Methacrylonitrile
Concen: 2.451 ug/l
RT: 7.286 min Scan# 913
Delta R.T. 0.067 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55

Tgt Ion: 41 Resp: 20
Ion Ratio Lower Upper
41 100
39 0.0 43.4 65.2#
67 0.0 63.6 95.4#
52 0.0 25.4 38.2#

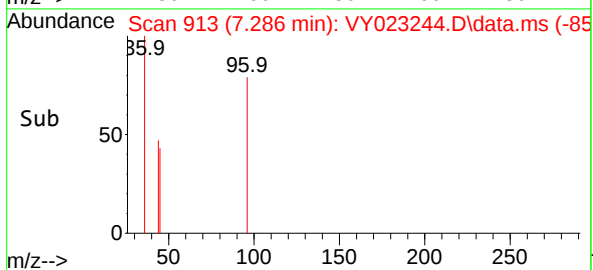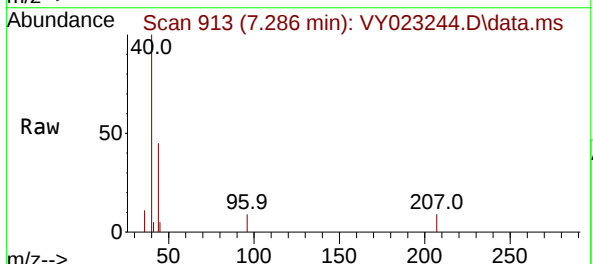

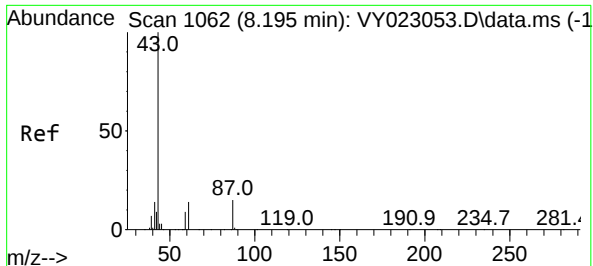

#43

Isopropyl Acetate

Concen: 2.030 ug/l

RT: 8.183 min Scan# 1

Delta R.T. -0.012 min

Lab File: VY023244.D

Acq: 29 Aug 2025 13:55

Instrument :

MSVOA_Y

ClientSampleId :

NORTH-TP-2





Tgt Ion: 43 Resp: 58

Ion Ratio Lower Upper

43 100

61 0.0 16.4 24.6#

87 0.0 11.8 17.6#

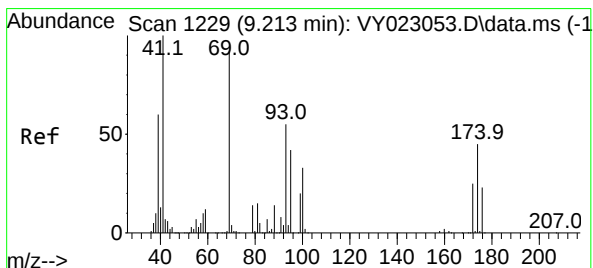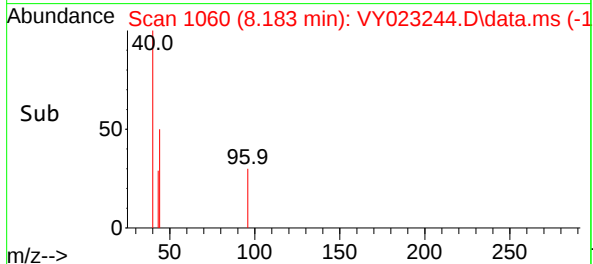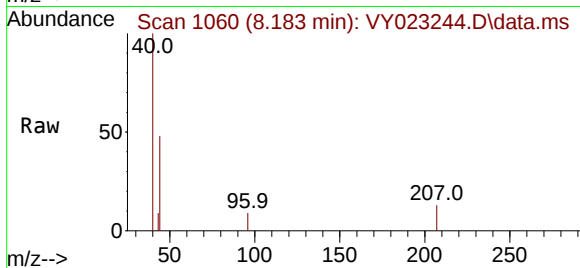

#48

Methyl methacrylate

Concen: 5.558 ug/l

RT: 9.219 min Scan# 1230

Delta R.T. 0.006 min

Lab File: VY023244.D

Acq: 29 Aug 2025 13:55




Tgt Ion: 41 Resp: 76


Ion Ratio Lower Upper

41 100

69 0.0 73.2 109.8#

39 0.0 47.0 70.4#


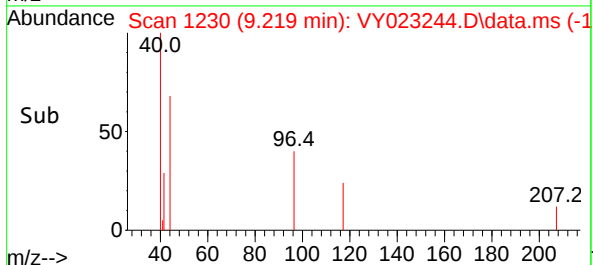
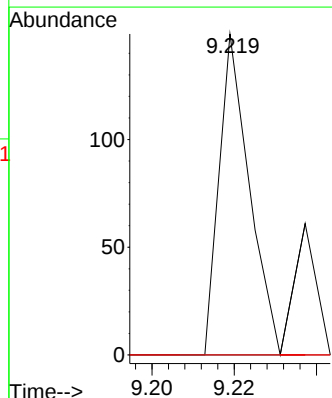
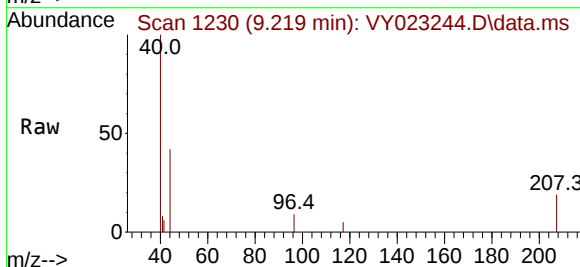




#50
Toluene-d8
Concen: 28.923 ug/l
RT: 10.109 min Scan# 1375
Delta R.T. 0.006 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55




Instrument :
MSVOA_Y
ClientSampleId :
NORTH-TP-2


Tgt Ion: 98 Resp: 2559
Ion Ratio Lower Upper
98 100
100 70.8 52.3 78.5

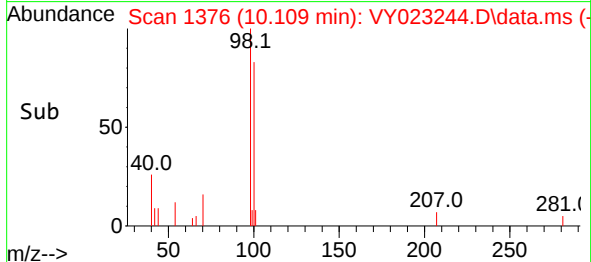

#51
4-Methyl-2-Pentanone
Concen: 1.560 ug/l
RT: 10.012 min Scan# 1360
Delta R.T. 0.018 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55

Tgt Ion: 43 Resp: 23
Ion Ratio Lower Upper
43 100
58 0.0 33.5 50.3#


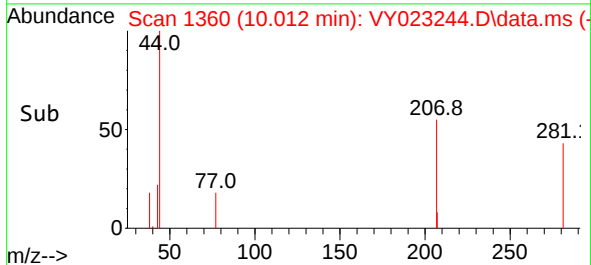






#53
 t-1,3-Dichloropropene
 Concen: 1.629 ug/l
 RT: 10.316 min Scan# 1410
 Delta R.T. -0.073 min
 Lab File: VY023244.D
 Acq: 29 Aug 2025 13:55




Instrument :
 MSVOA_Y
 ClientSampleId :
 NORTH-TP-2


Tgt Ion: 75 Resp: 52
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.7 38.5#

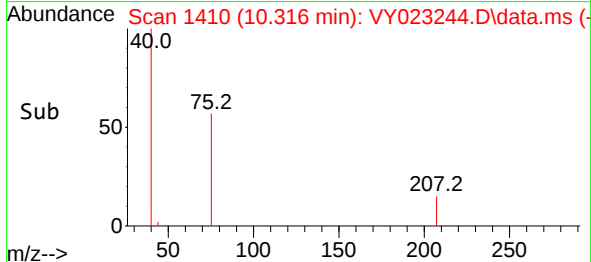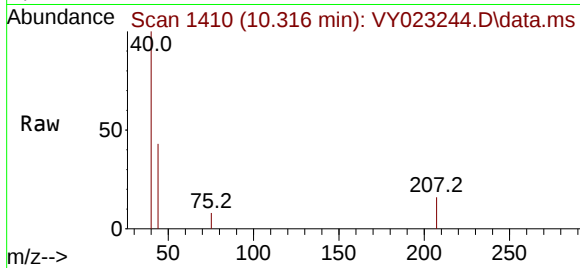

#54
 cis-1,3-Dichloropropene
 Concen: 1.086 ug/l
 RT: 9.896 min Scan# 1341
 Delta R.T. 0.043 min
 Lab File: VY023244.D
 Acq: 29 Aug 2025 13:55

Tgt Ion: 75 Resp: 41
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.4 38.0#
 39 0.0 35.6 53.4#




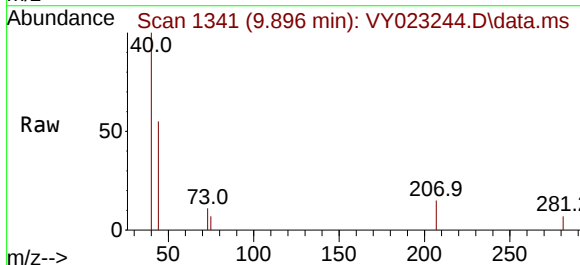




#59
2-Hexanone
Concen: 6.276 ug/l
RT: 10.804 min Scan# 1482
Delta R.T. 0.049 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55




Instrument :
MSVOA_Y
ClientSampleId :
NORTH-TP-2


Tgt Ion: 43 Resp: 63
Ion Ratio Lower Upper
43 100
58 0.0 29.5 88.5#

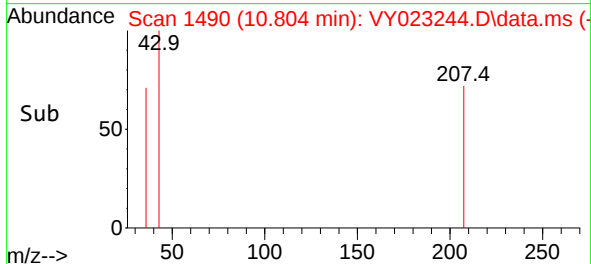

#62
4-Bromofluorobenzene
Concen: 19.857 ug/l
RT: 12.395 min Scan# 1751
Delta R.T. -0.006 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55

Tgt Ion: 95 Resp: 565
Ion Ratio Lower Upper
95 100
174 104.1 0.0 171.6
176 101.1 0.0 167.6

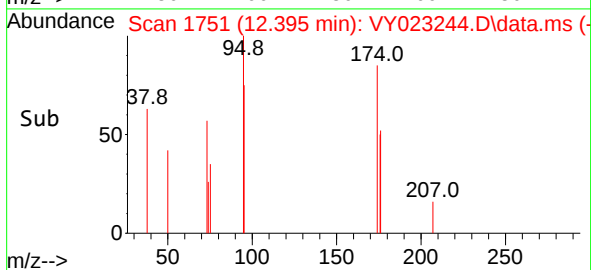



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.420 min Scan# 11

Delta R.T. 0.012 min

Lab File: VY023244.D

Acq: 29 Aug 2025 13:55

Instrument :

MSVOA_Y

ClientSampleId :

NORTH-TP-2





Tgt Ion:117 Resp: 1830

Ion Ratio Lower Upper

117 100

82 43.9 43.4 65.0

119 45.7 25.6 38.4#

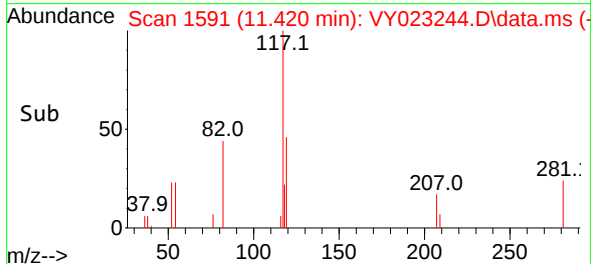

#65

Chlorobenzene

Concen: 1.089 ug/l

RT: 11.578 min Scan# 1617

Delta R.T. 0.140 min

Lab File: VY023244.D




Acq: 29 Aug 2025 13:55


Tgt Ion:112 Resp: 43

Ion Ratio Lower Upper

112 100

114 0.0 27.0 40.4#


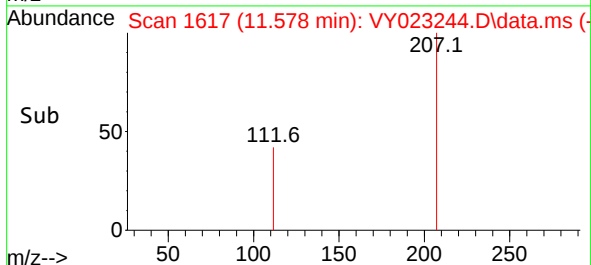






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.352 min Scan# 1908
Delta R.T. 0.012 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55




Instrument :
MSVOA_Y
ClientSampleId :
NORTH-TP-2


Tgt Ion:152 Resp: 527
Ion Ratio Lower Upper
152 100
115 54.1 28.2 84.6
150 164.9 0.0 348.0

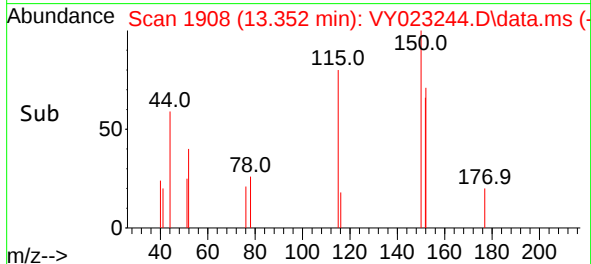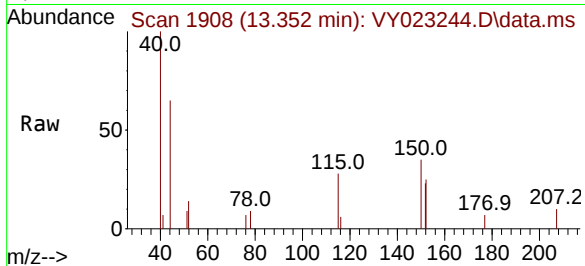

#74
N-ethyl acetate
Concen: 2.662 ug/l
RT: 12.060 min Scan# 1696
Delta R.T. -0.006 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55

Tgt Ion: 43 Resp: 21
Ion Ratio Lower Upper
43 100
70 0.0 37.5 56.3#
55 0.0 20.7 31.1#
61 0.0 20.7 31.1#




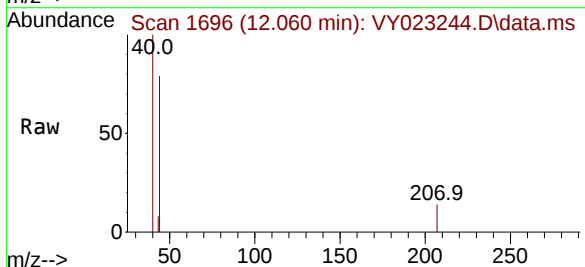




#75
1,1,2,2-Tetrachloroethane
Concen: 4.566 ug/l
RT: 12.218 min Scan# 1753
Delta R.T. -0.281 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55




Instrument :
MSVOA_Y
ClientSampleId :
NORTH-TP-2


Tgt Ion: 83 Resp: 29
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.3#
85 0.0 31.8 95.3#

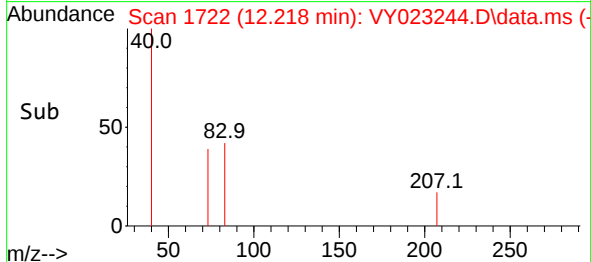

#76
1,2,3-Trichloropropane
Concen: 56.625 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. -0.140 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55

Tgt Ion: 75 Resp: 288
Ion Ratio Lower Upper
75 100
77 0.0 0.0 0.0


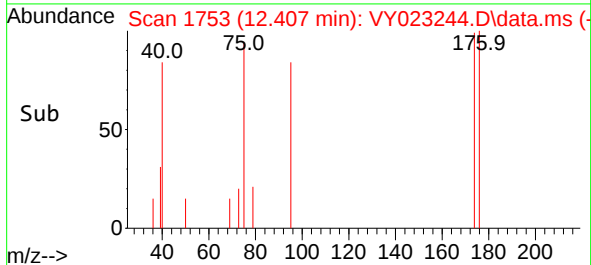






#81
trans-1,4-Dichloro-2-butene
Concen: 137.071 ug/l
RT: 12.407 min Scan# 11
Delta R.T. 0.110 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55

Instrument :
MSVOA_Y
ClientSampleId :
NORTH-TP-2

Tgt Ion: 75 Resp: 288
Ion Ratio Lower Upper
75 100
53 0.0 70.8 106.2#
89 0.0 38.1 57.1#

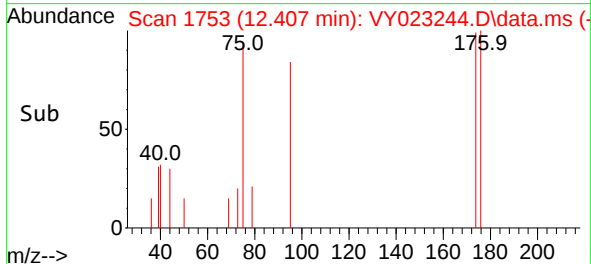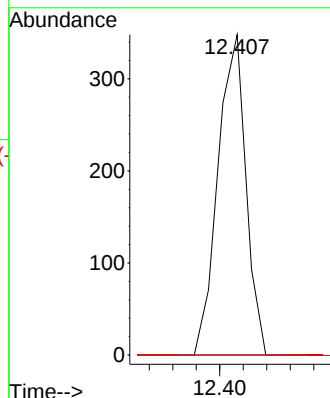

#92
1,2-Dibromo-3-Chloropropane
Concen: 46.520 ug/l
RT: 14.413 min Scan# 2082
Delta R.T. 0.146 min
Lab File: VY023244.D
Acq: 29 Aug 2025 13:55

Tgt Ion: 75 Resp: 46
Ion Ratio Lower Upper
75 100
155 0.0 43.9 131.6#
157 0.0 57.2 171.6#

