

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082925\
 Data File : VY023234.D
 Acq On : 29 Aug 2025 09:35
 Operator : SY/MD
 Sample : VY0829SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0829SBL01

Quant Time: Aug 30 01:17:36 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	604207	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	1141963	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	1030161	50.000	ug/l	0.01
72) 1,4-Dichlorobenzene-d4	13.346	152	410618	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	320945	55.734	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	111.460%
35) Dibromofluoromethane	7.634	113	367076	53.720	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	107.440%
50) Toluene-d8	10.109	98	1356696	50.824	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	101.640%
62) 4-Bromofluorobenzene	12.408	95	400273	46.626	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	93.260%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082925\
Data File : VY023234.D
Acq On : 29 Aug 2025 09:35
Operator : SY/MD
Sample : VY0829SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0829SBL01

Quant Time: Aug 30 01:17:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration




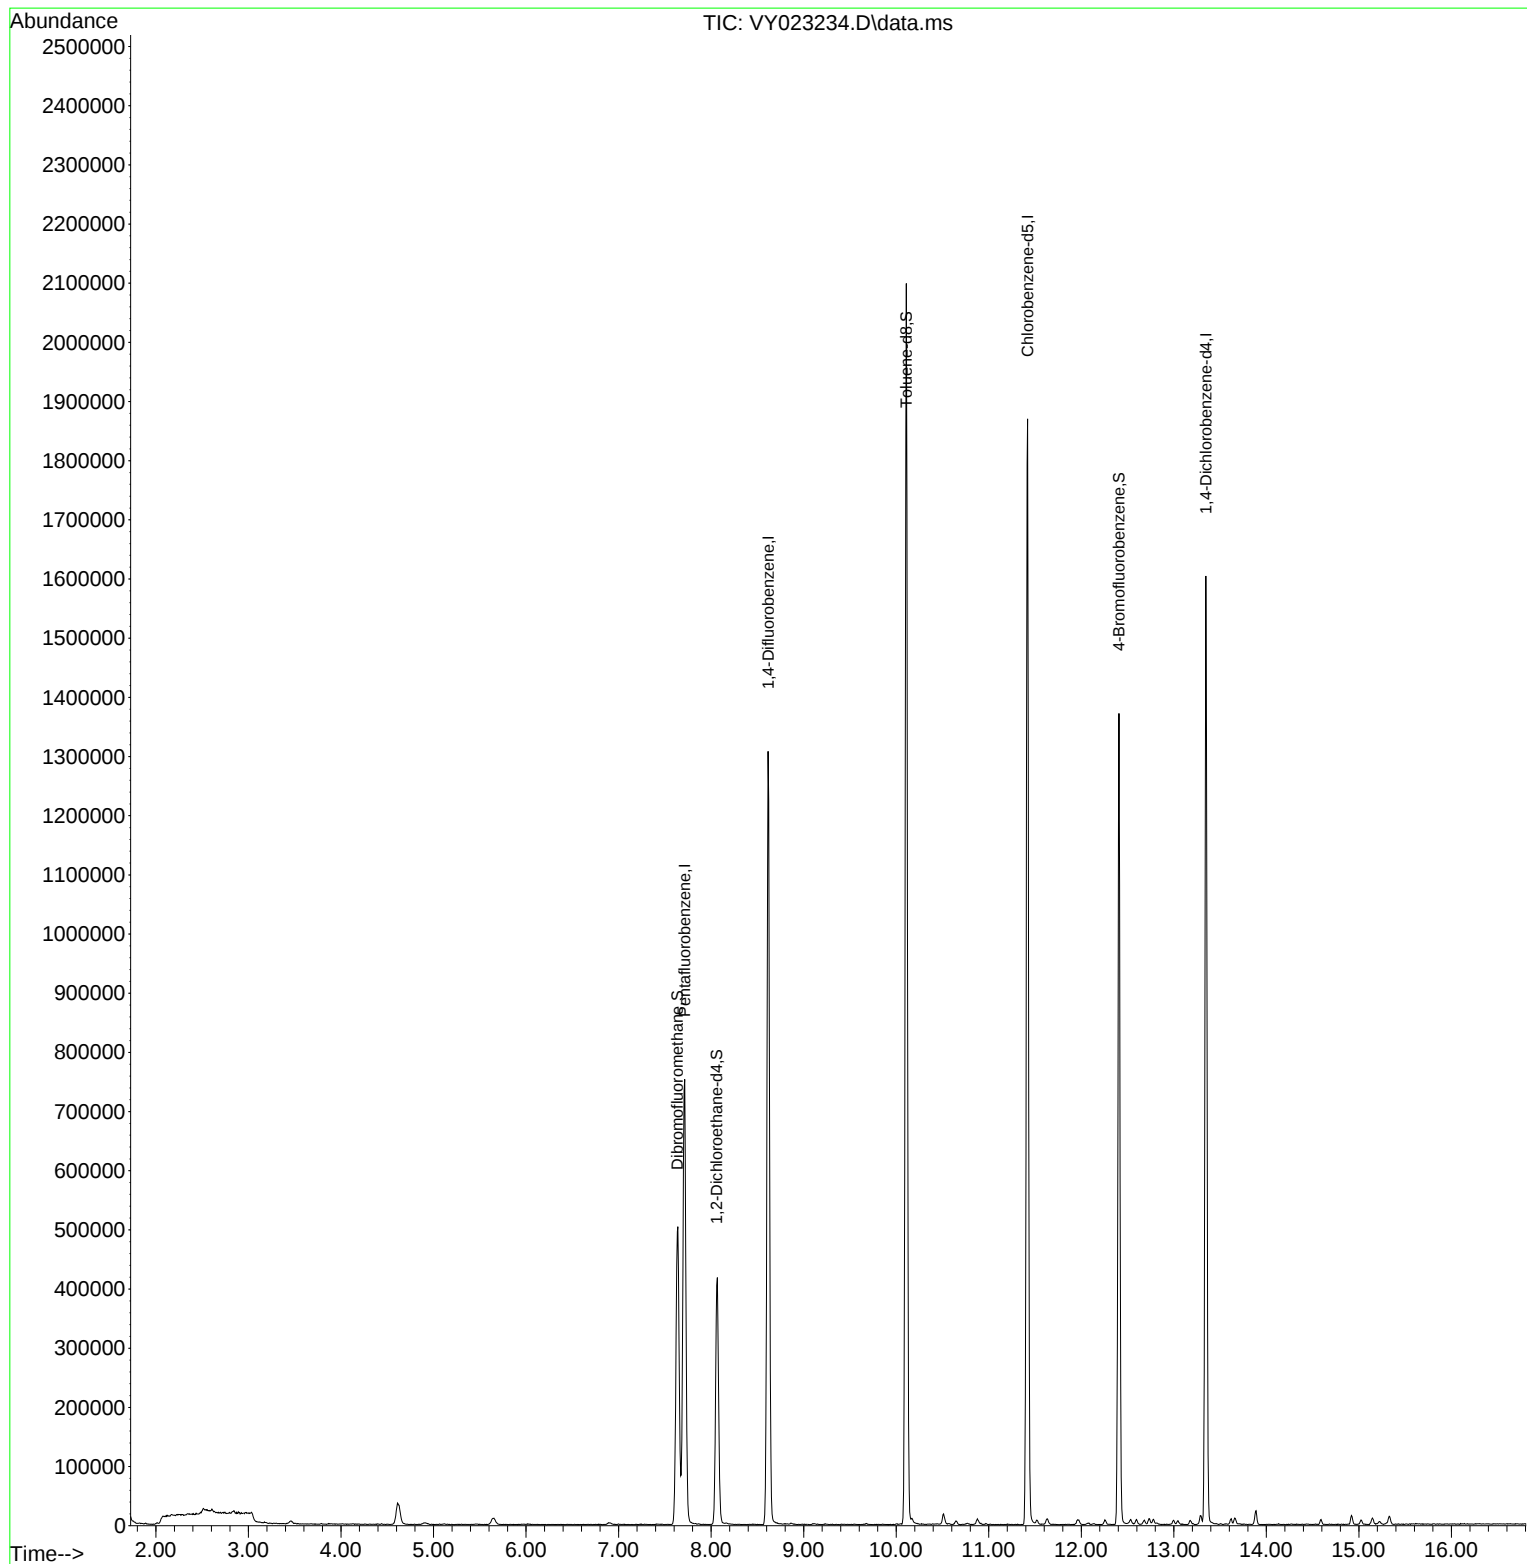


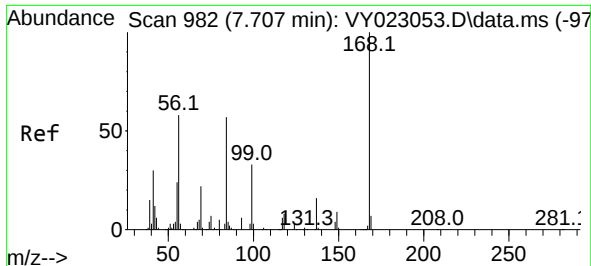

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY023234.D
Acq: 29 Aug 2025 09:35




Instrument :
MSVOA_Y
ClientSampleId :
VY0829SBL01


Tgt Ion:168 Resp: 604207
Ion Ratio Lower Upper
168 100
99 51.4 42.8 64.2

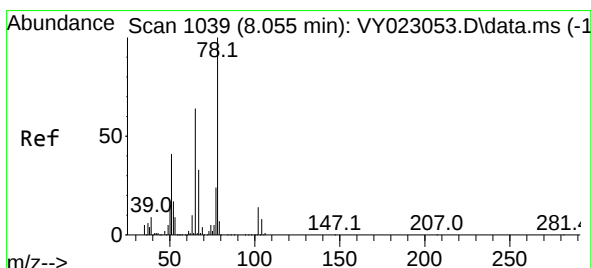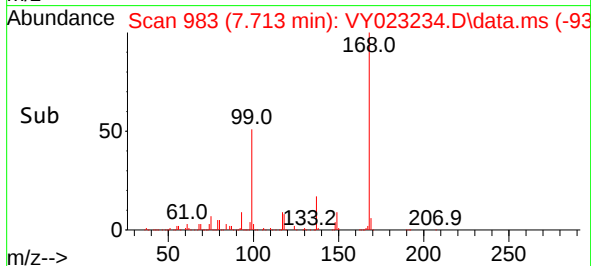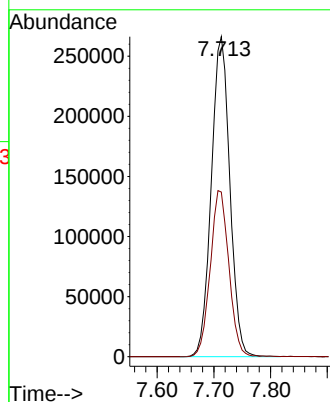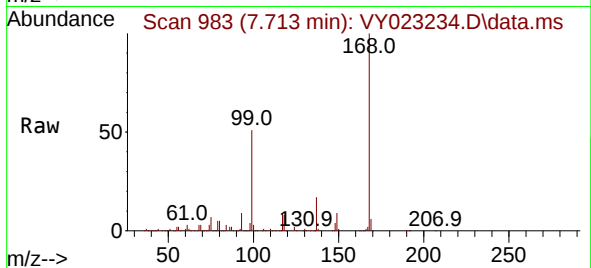

#33
1,2-Dichloroethane-d4
Concen: 55.734 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VY023234.D
Acq: 29 Aug 2025 09:35

Tgt Ion: 65 Resp: 320945
Ion Ratio Lower Upper
65 100
67 53.3 0.0 106.8


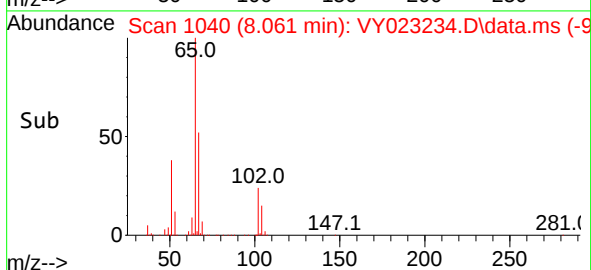
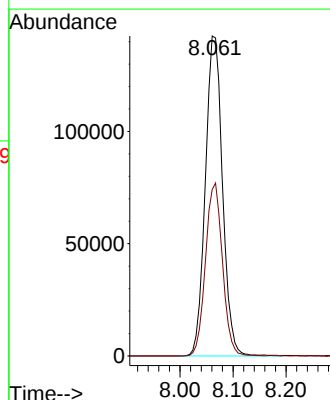
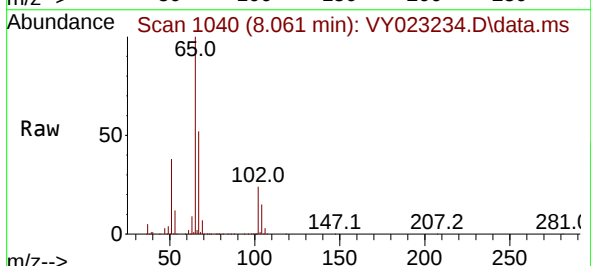


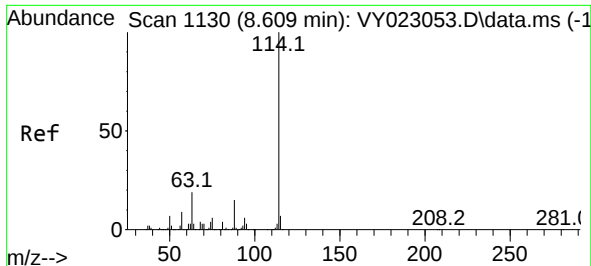

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.006 min
Lab File: VY023234.D
Acq: 29 Aug 2025 09:35




Instrument :
MSVOA_Y
ClientSampleId :
VY0829SBL01


Tgt Ion:114 Resp: 1141963
Ion Ratio Lower Upper
114 100
63 17.9 0.0 38.4
88 14.4 0.0 30.0

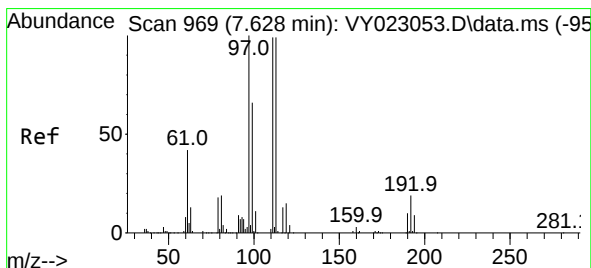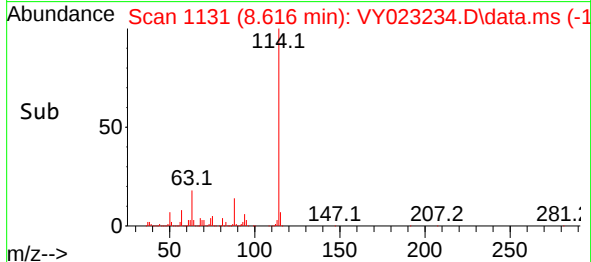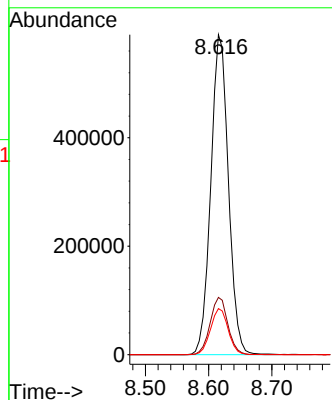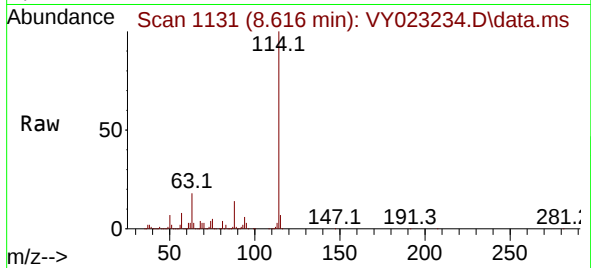

#35
Dibromofluoromethane
Concen: 53.720 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.006 min
Lab File: VY023234.D
Acq: 29 Aug 2025 09:35

Tgt Ion:113 Resp: 367076
Ion Ratio Lower Upper
113 100
111 102.8 81.1 121.7
192 20.6 16.2 24.4


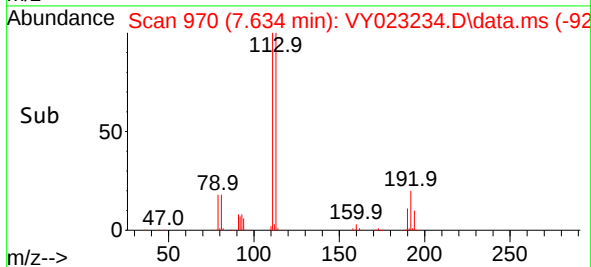
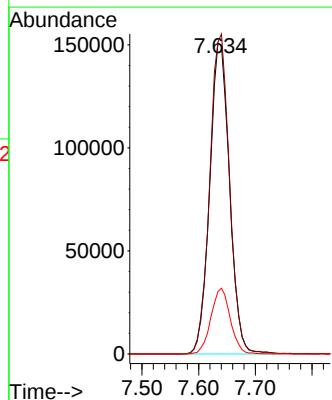
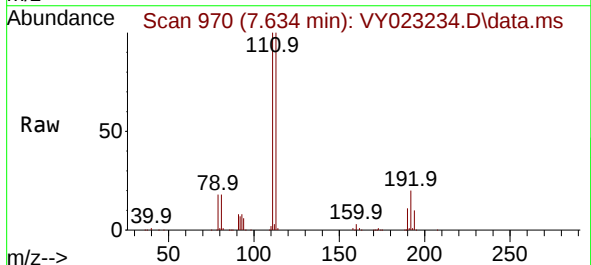


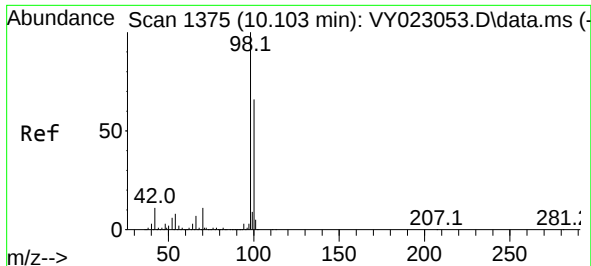

#50
Toluene-d8
Concen: 50.824 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY023234.D
Acq: 29 Aug 2025 09:35




Instrument :
MSVOA_Y
ClientSampleId :
VY0829SBL01


Tgt Ion: 98 Resp: 1356696
Ion Ratio Lower Upper
98 100
100 65.7 52.3 78.5

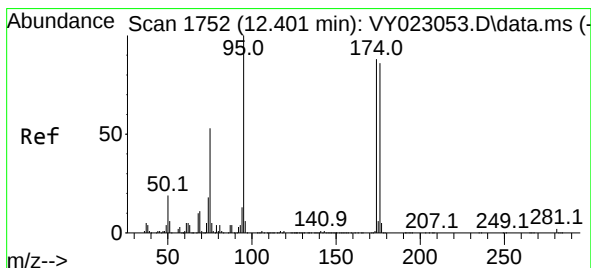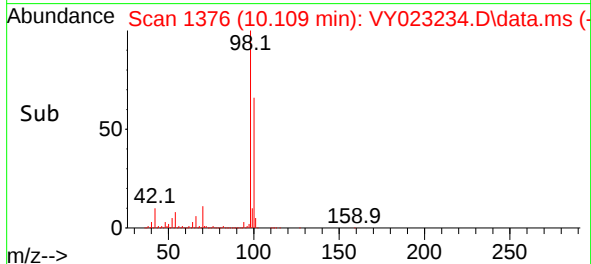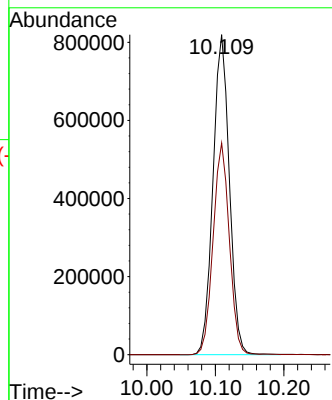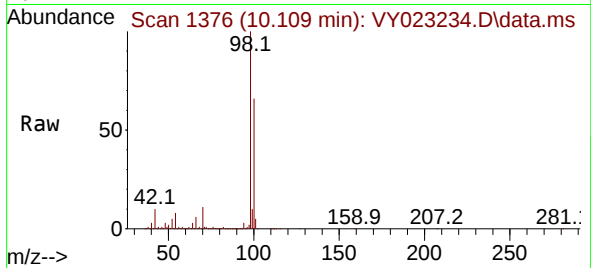

#62
4-Bromofluorobenzene
Concen: 46.626 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY023234.D
Acq: 29 Aug 2025 09:35

Tgt Ion: 95 Resp: 400273
Ion Ratio Lower Upper
95 100
174 90.7 0.0 171.6
176 86.2 0.0 167.6


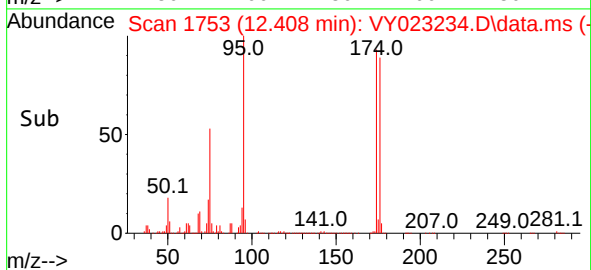
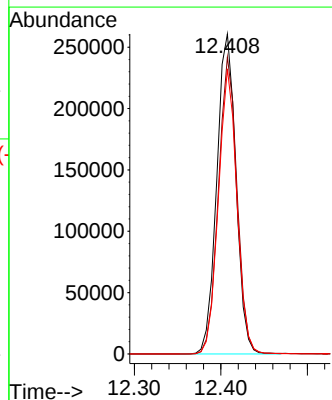
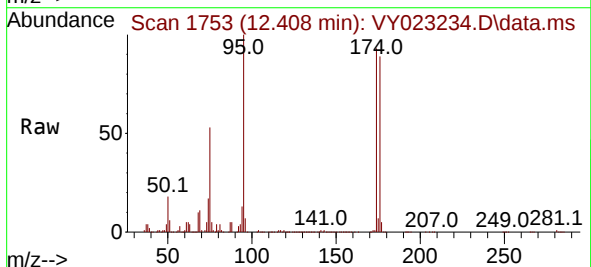


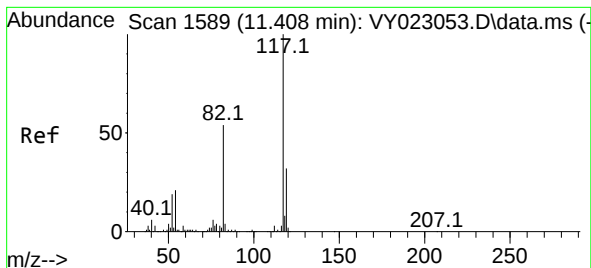

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.420 min Scan# 11
Delta R.T. 0.012 min
Lab File: VY023234.D
Acq: 29 Aug 2025 09:35

Instrument :
MSVOA_Y
ClientSampleId :
VY0829SBL01

Tgt Ion:117 Resp: 1030161
Ion Ratio Lower Upper
117 100
82 52.3 43.4 65.0
119 32.8 25.6 38.4

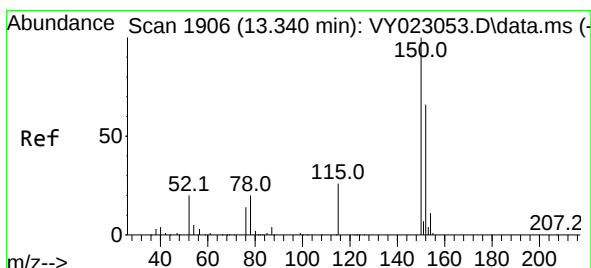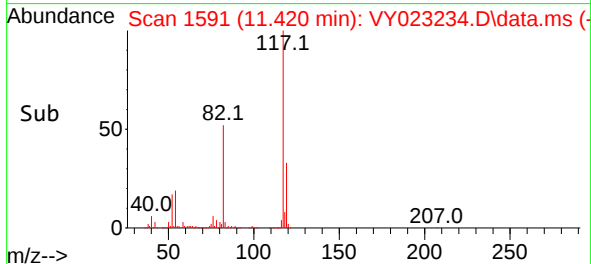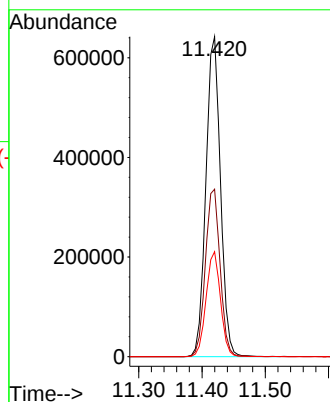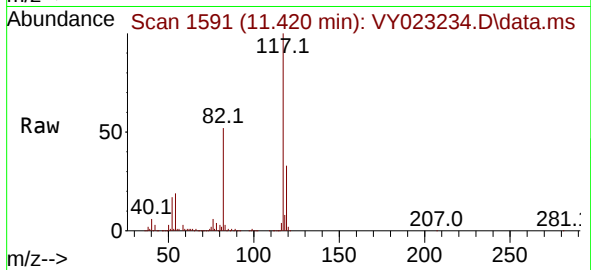

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. 0.006 min
Lab File: VY023234.D
Acq: 29 Aug 2025 09:35

Tgt Ion:152 Resp: 410618
Ion Ratio Lower Upper
152 100
115 55.6 28.2 84.6
150 156.8 0.0 348.0

