

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY082925\  
 Data File : VY023239.D  
 Acq On : 29 Aug 2025 11:57  
 Operator : SY/MD  
 Sample : Q2973-01RE  
 Misc : 5.33g/5.0mL/MSVOA\_Y/SOIL/B  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 OK-01-082825RE

Quant Time: Aug 30 01:19:51 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y081225S.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Aug 13 02:10:11 2025  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.713  | 168  | 59734    | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.616  | 114  | 81355    | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.420 | 117  | 58605    | 50.000 | ug/l  | 0.01     |
| 72) 1,4-Dichlorobenzene-d4 | 13.347 | 152  | 14897    | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.067  | 65    | 22965    | 40.339   | ug/l | 0.01     |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 80.680%  |
| 35) Dibromofluoromethane    | 7.634  | 113   | 26241    | 53.905   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 107.800% |
| 50) Toluene-d8              | 10.109 | 98    | 88355    | 46.460   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 58 - 134 | Recovery | =    | 92.920%  |
| 62) 4-Bromofluorobenzene    | 12.408 | 95    | 18284    | 29.896   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 30 - 143 | Recovery | =    | 59.800%  |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY082925\  
Data File : VY023239.D  
Acq On : 29 Aug 2025 11:57  
Operator : SY/MD  
Sample : Q2973-01RE  
Misc : 5.33g/5.0mL/MSVOA\_Y/SOIL/B  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
OK-01-082825RE

Quant Time: Aug 30 01:19:51 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y081225S.M  
Quant Title : SW846 8260  
QLast Update : Wed Aug 13 02:10:11 2025  
Response via : Initial Calibration




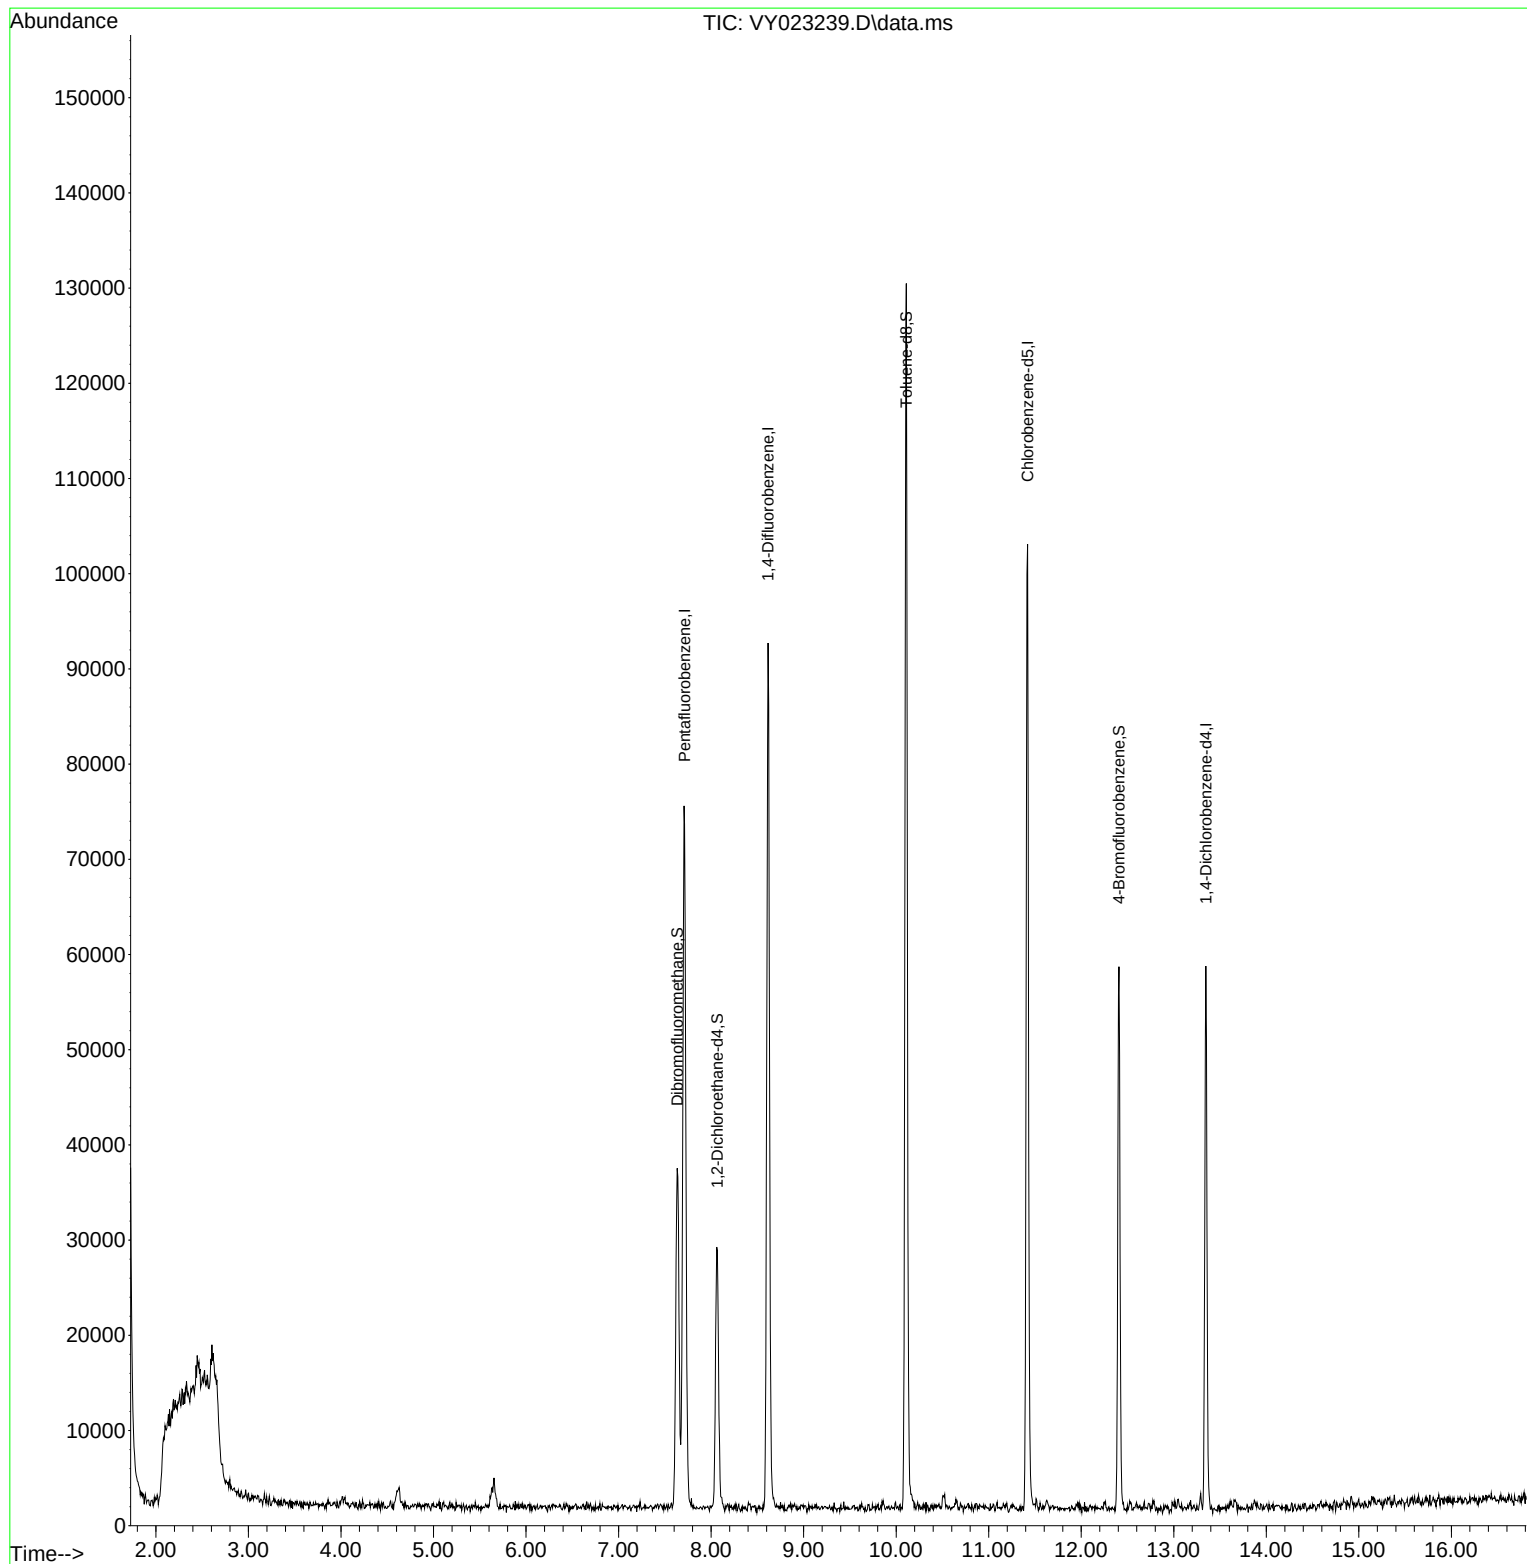


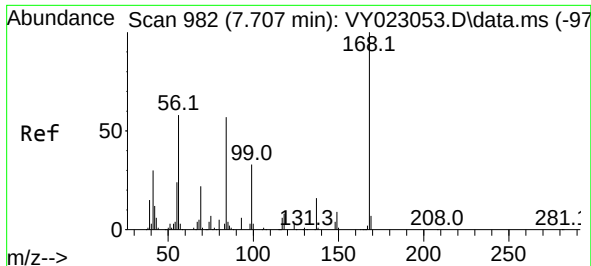

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.713 min Scan# 91  
Delta R.T. 0.006 min  
Lab File: VY023239.D  
Acq: 29 Aug 2025 11:57




Instrument :  
MSVOA\_Y  
ClientSampleId :  
OK-01-082825RE


Tgt Ion:168 Resp: 59734  
Ion Ratio Lower Upper  
168 100  
99 50.3 42.8 64.2

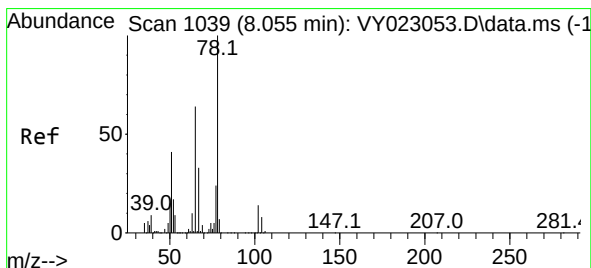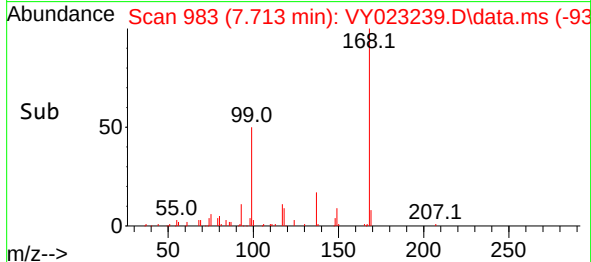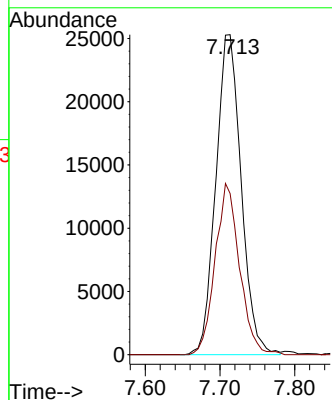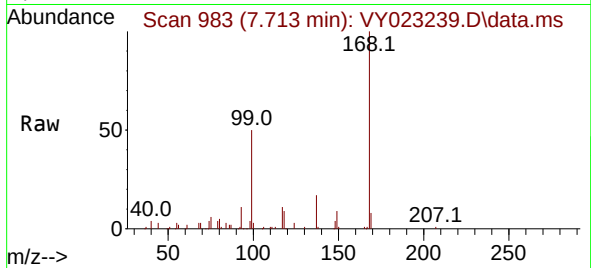

#33  
1,2-Dichloroethane-d4  
Concen: 40.339 ug/l  
RT: 8.067 min Scan# 1041  
Delta R.T. 0.012 min  
Lab File: VY023239.D  
Acq: 29 Aug 2025 11:57

Tgt Ion: 65 Resp: 22965  
Ion Ratio Lower Upper  
65 100  
67 52.8 0.0 106.8


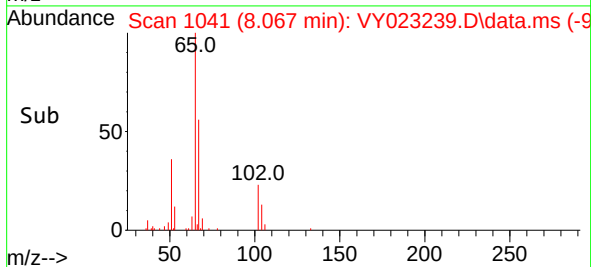
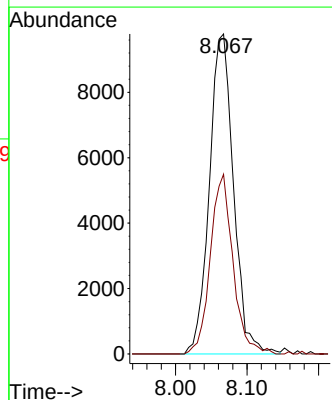
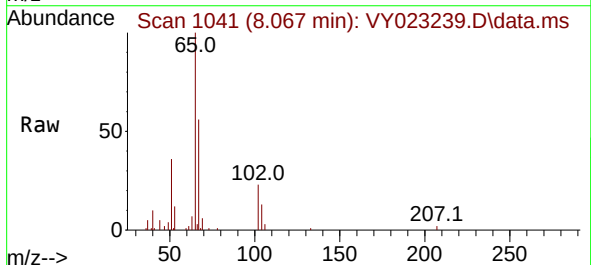


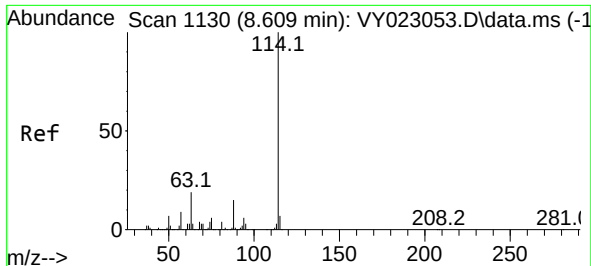

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 8.616 min Scan# 1130  
Delta R.T. 0.006 min  
Lab File: VY023239.D  
Acq: 29 Aug 2025 11:57




Instrument :  
MSVOA\_Y  
ClientSampleId :  
OK-01-082825RE


Tgt Ion:114 Resp: 81355  
Ion Ratio Lower Upper  
114 100  
63 18.5 0.0 38.4  
88 13.7 0.0 30.0

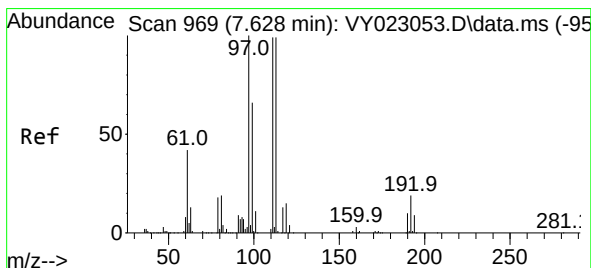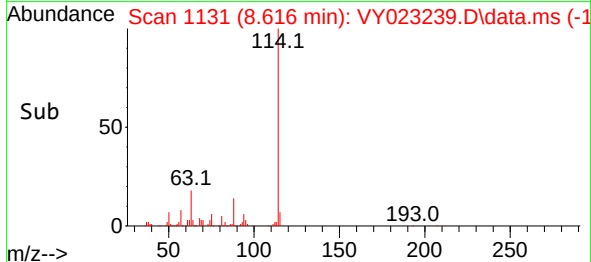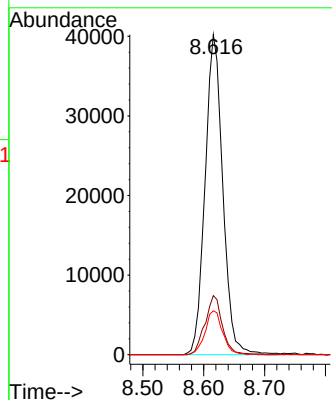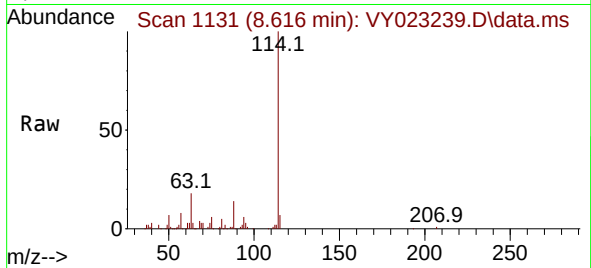

#35  
Dibromofluoromethane  
Concen: 53.905 ug/l  
RT: 7.634 min Scan# 970  
Delta R.T. 0.006 min  
Lab File: VY023239.D  
Acq: 29 Aug 2025 11:57

Tgt Ion:113 Resp: 26241  
Ion Ratio Lower Upper  
113 100  
111 105.7 81.1 121.7  
192 22.2 16.2 24.4


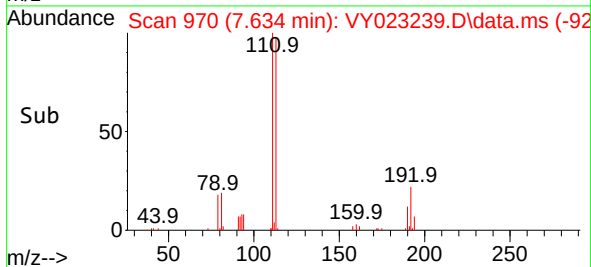
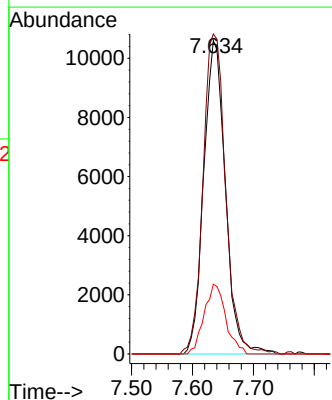
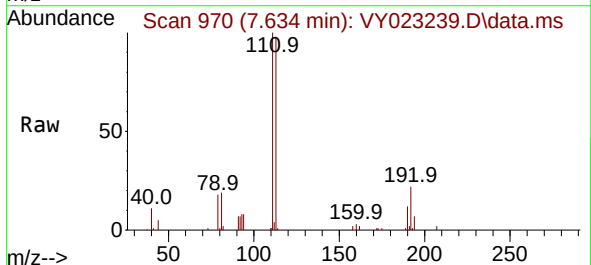


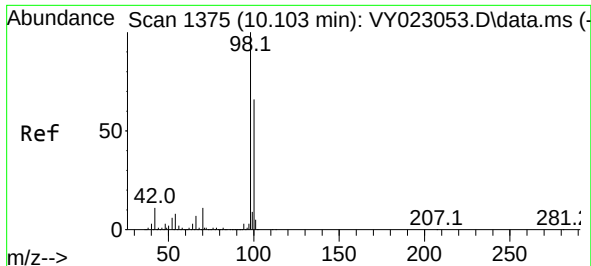

#50  
Toluene-d8  
Concen: 46.460 ug/l  
RT: 10.109 min Scan# 11  
Delta R.T. 0.006 min  
Lab File: VY023239.D  
Acq: 29 Aug 2025 11:57




Instrument :  
MSVOA\_Y  
ClientSampleId :  
OK-01-082825RE


Tgt Ion: 98 Resp: 88355  
Ion Ratio Lower Upper  
98 100  
100 64.7 52.3 78.5

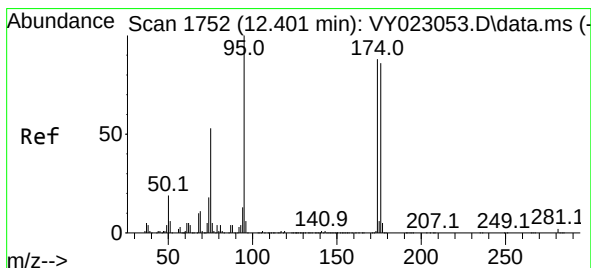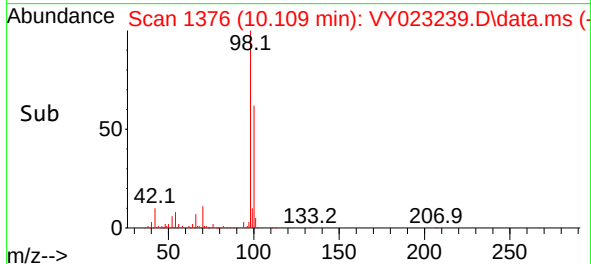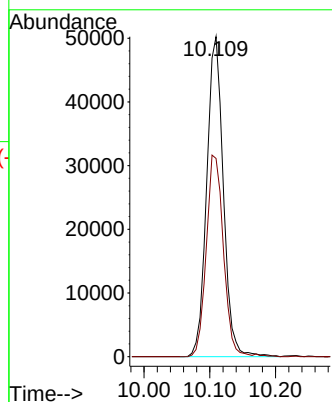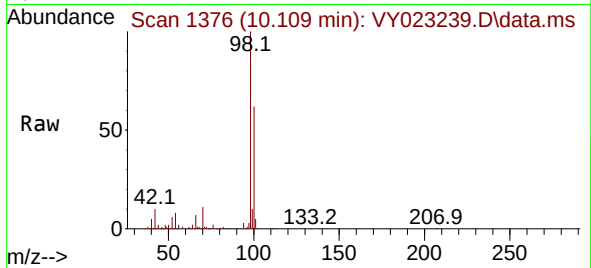

#62  
4-Bromofluorobenzene  
Concen: 29.896 ug/l  
RT: 12.408 min Scan# 1753  
Delta R.T. 0.006 min  
Lab File: VY023239.D  
Acq: 29 Aug 2025 11:57

Tgt Ion: 95 Resp: 18284  
Ion Ratio Lower Upper  
95 100  
174 92.1 0.0 171.6  
176 86.0 0.0 167.6

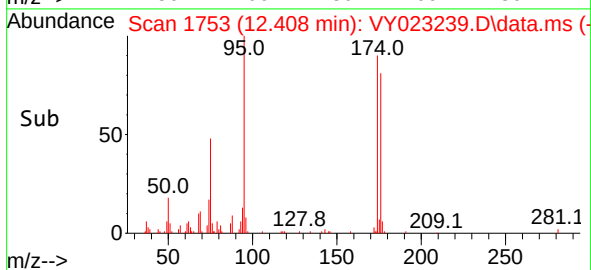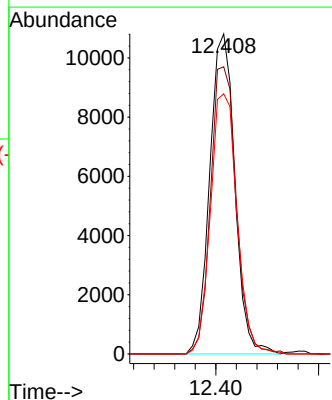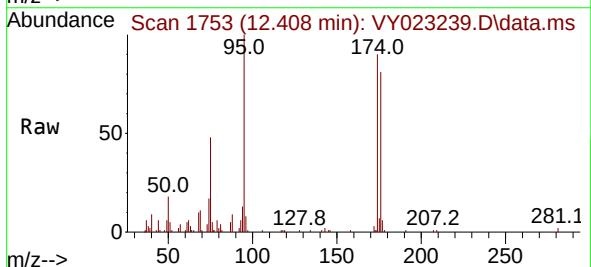

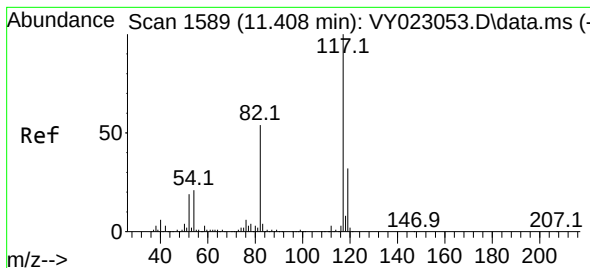

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.420 min Scan# 11

Delta R.T. 0.012 min

Lab File: VY023239.D

Acq: 29 Aug 2025 11:57

Instrument :

MSVOA\_Y

ClientSampleId :

OK-01-082825RE





Tgt Ion:117 Resp: 58605

Ion Ratio Lower Upper

117 100

82 51.5 43.4 65.0

119 31.1 25.6 38.4

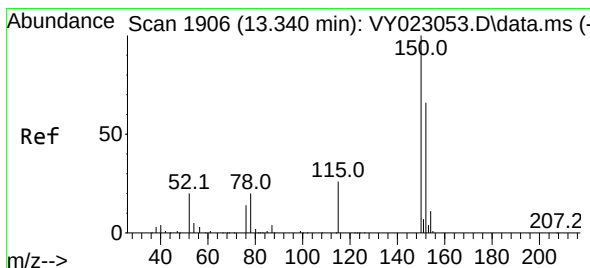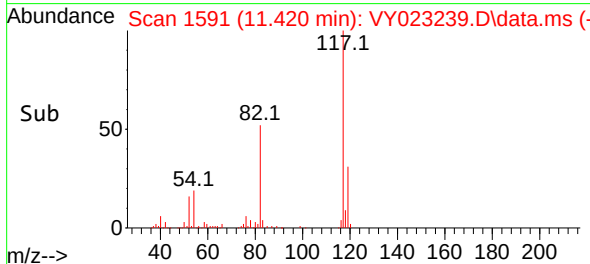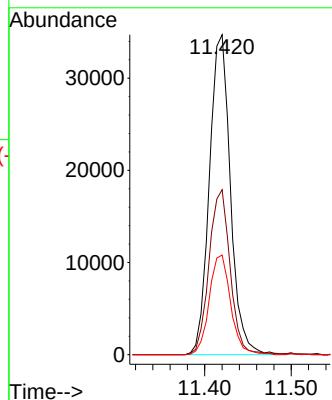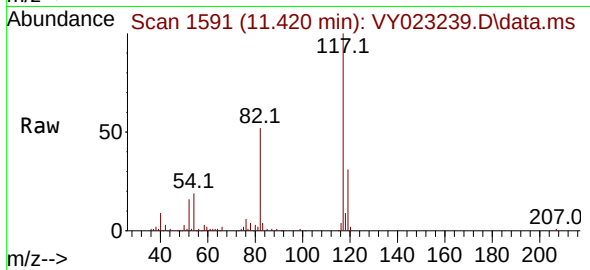

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.006 min

Lab File: VY023239.D

Acq: 29 Aug 2025 11:57

Tgt Ion:152 Resp: 14897

Ion Ratio Lower Upper

152 100

115 59.8 28.2 84.6

150 162.0 0.0 348.0

