
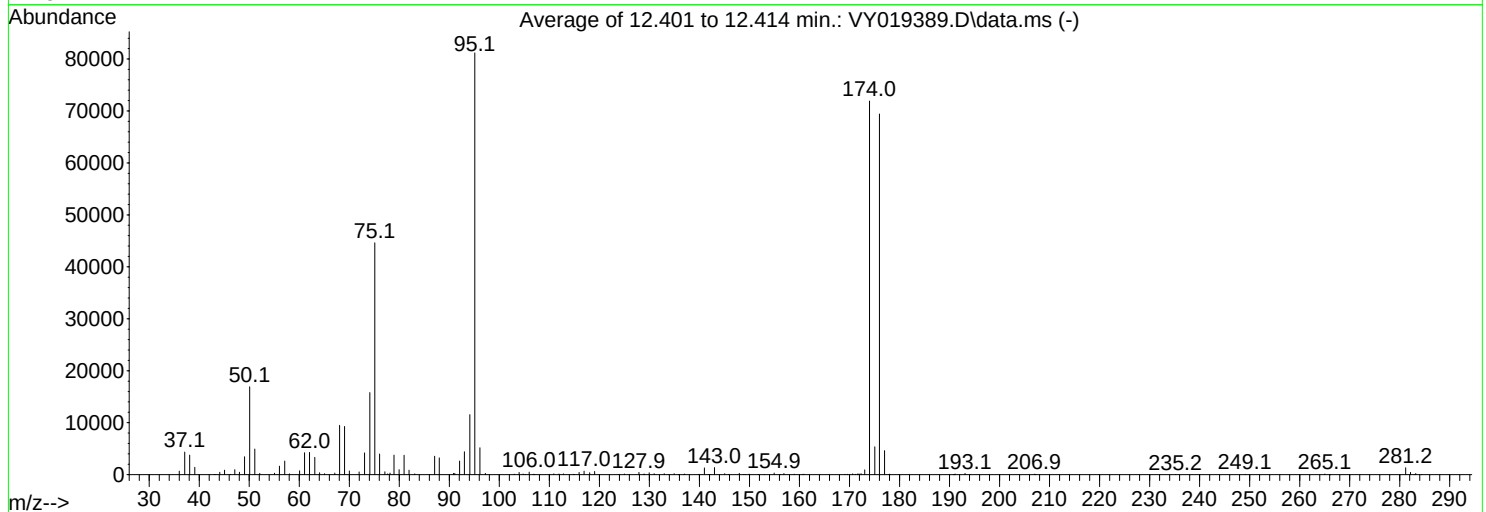


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY083024\
Data File : VY019389.D
Acq On : 30 Aug 2024 12:15
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082924S.M
Title : SW846 8260
Last Update : Fri Aug 30 02:45:30 2024

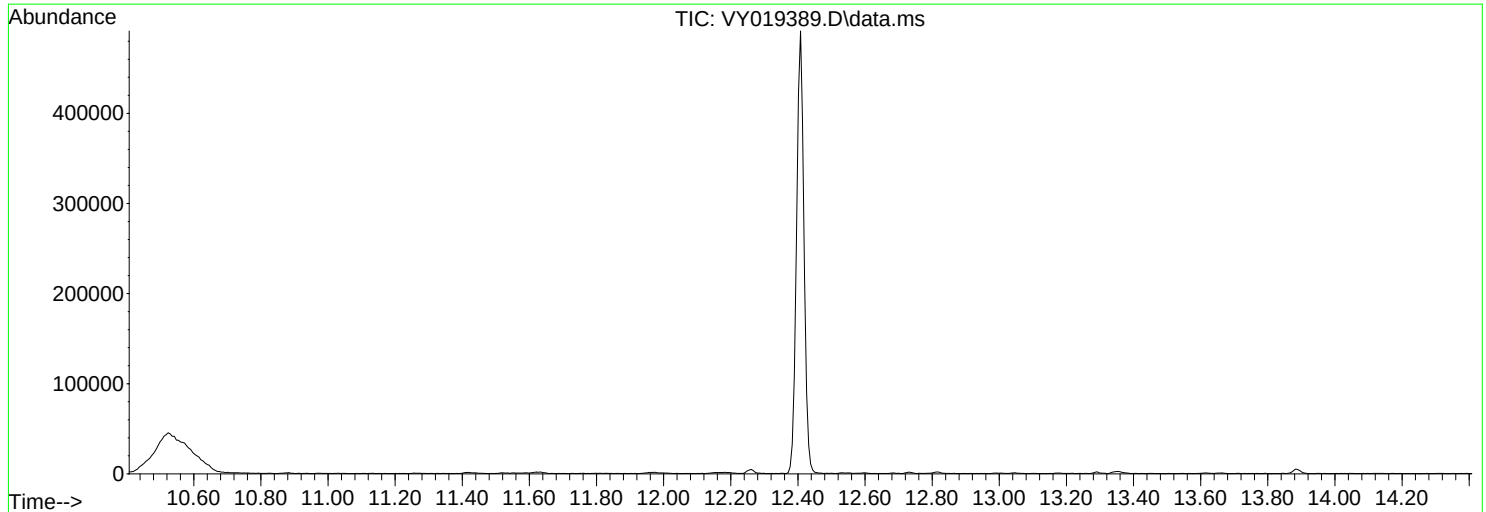

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	16896	PASS
75	95	30	60	55.0	44629	PASS
95	95	100	100	100.0	81189	PASS
96	95	5	9	6.4	5187	PASS
173	174	0.00	2	1.3	943	PASS
174	95	50	100	88.6	71917	PASS
175	174	5	9	7.5	5360	PASS
176	174	95	101	96.5	69435	PASS
177	176	5	9	6.6	4616	PASS