
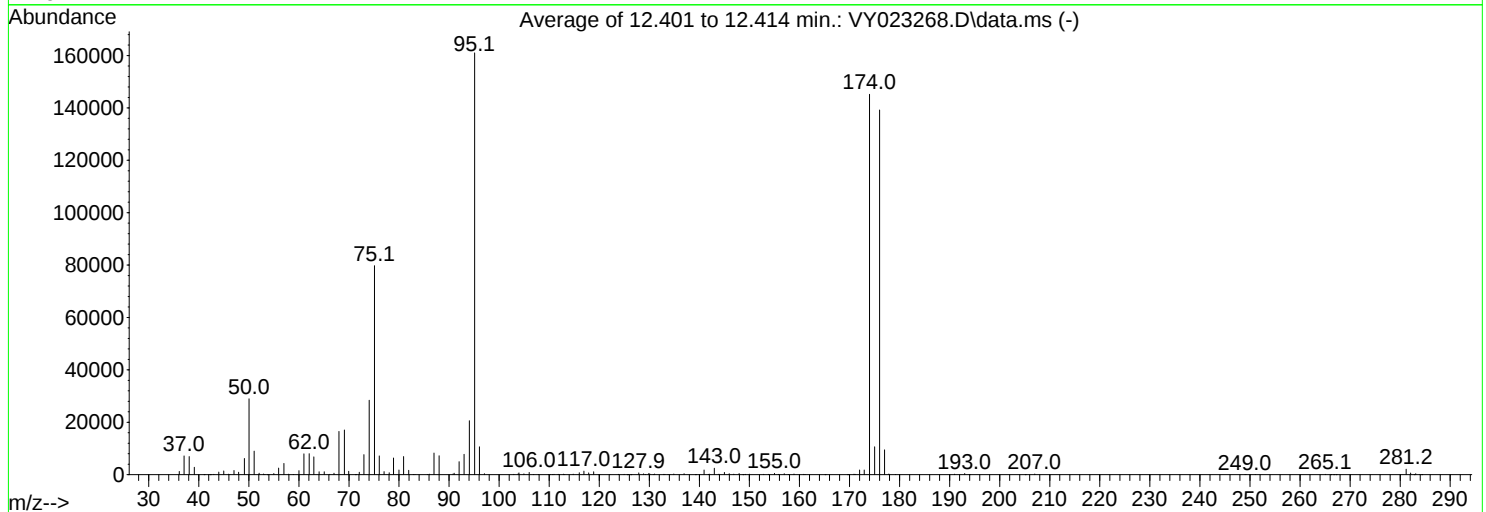


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090325\
Data File : VY023268.D
Acq On : 03 Sep 2025 08:30
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Title : SW846 8260
Last Update : Wed Aug 13 02:10:11 2025

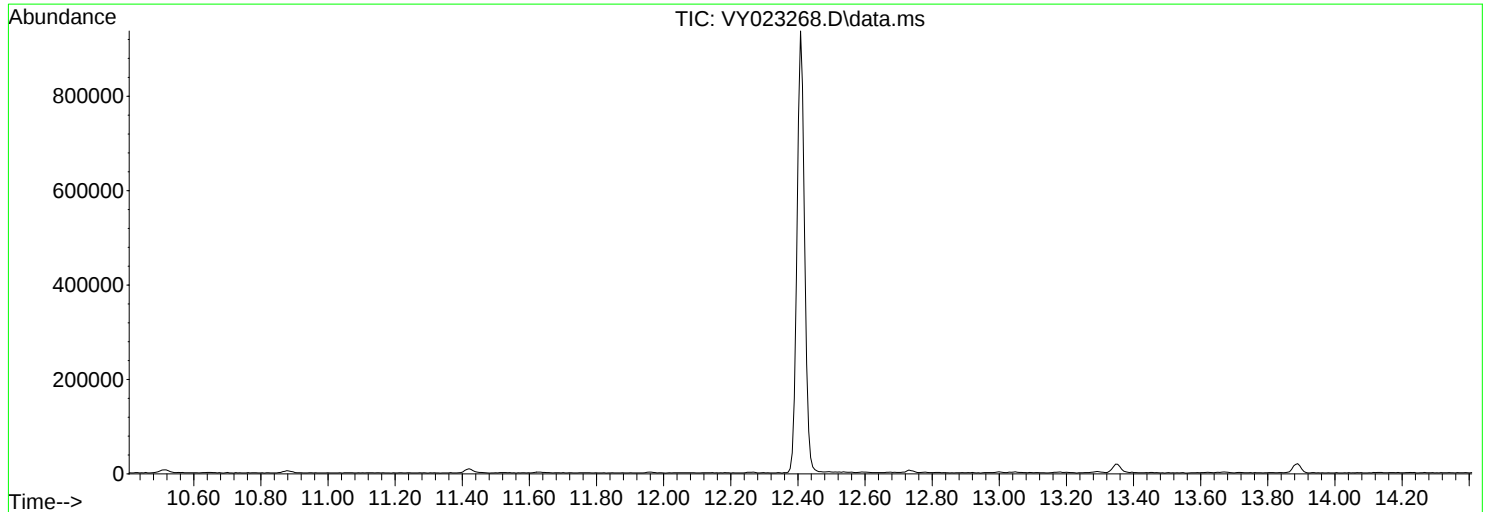

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	28931	PASS
75	95	30	60	49.6	79792	PASS
95	95	100	100	100.0	161024	PASS
96	95	5	9	6.6	10627	PASS
173	174	0.00	2	1.2	1752	PASS
174	95	50	100	90.2	145221	PASS
175	174	5	9	7.3	10618	PASS
176	174	95	101	95.8	139176	PASS
177	176	5	9	6.8	9488	PASS