
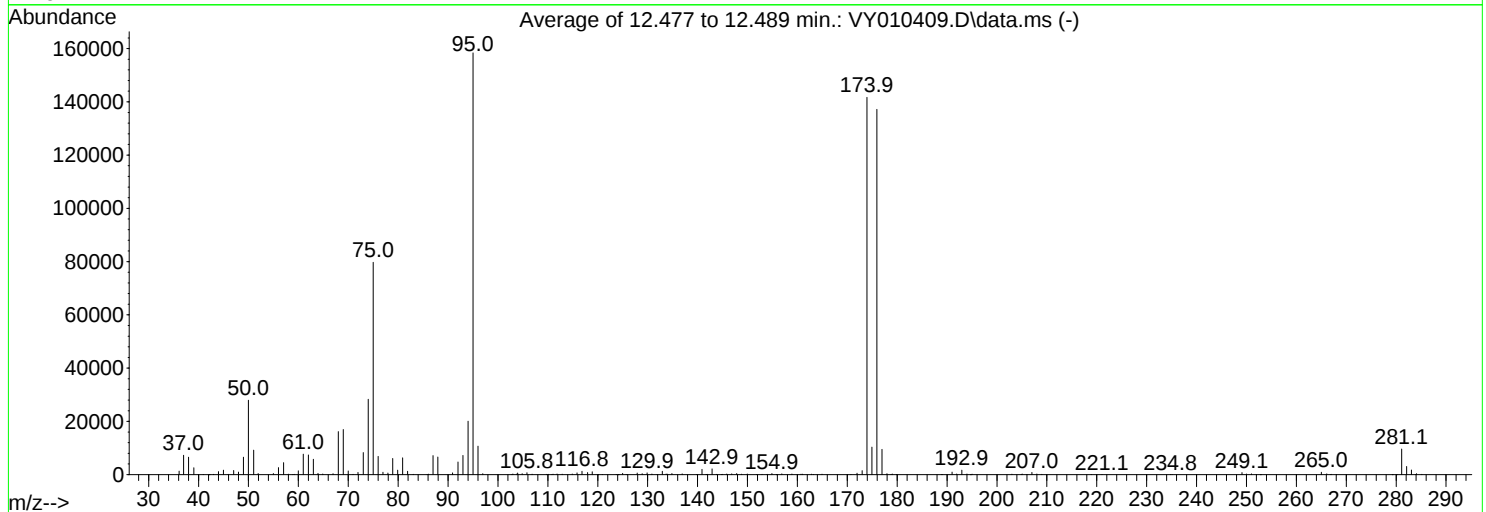


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090922\
Data File : VY010409.D
Acq On : 09 Sep 2022 09:25
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090922S.M
Title : SW846 8260
Last Update : Fri Sep 09 17:08:30 2022

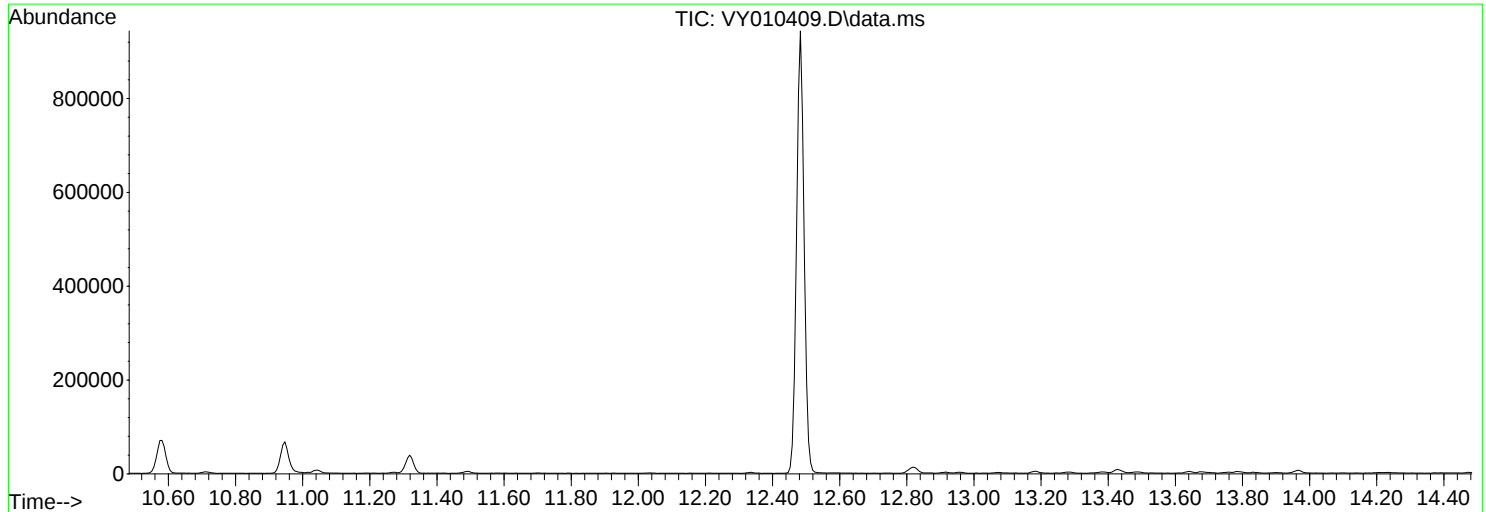

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	27920	PASS
75	95	30	60	50.3	79739	PASS
95	95	100	100	100.0	158400	PASS
96	95	5	9	6.8	10725	PASS
173	174	0.00	2	1.1	1506	PASS
174	95	50	100	89.5	141707	PASS
175	174	5	9	7.3	10318	PASS
176	174	95	101	96.8	137157	PASS
177	176	5	9	6.9	9506	PASS