
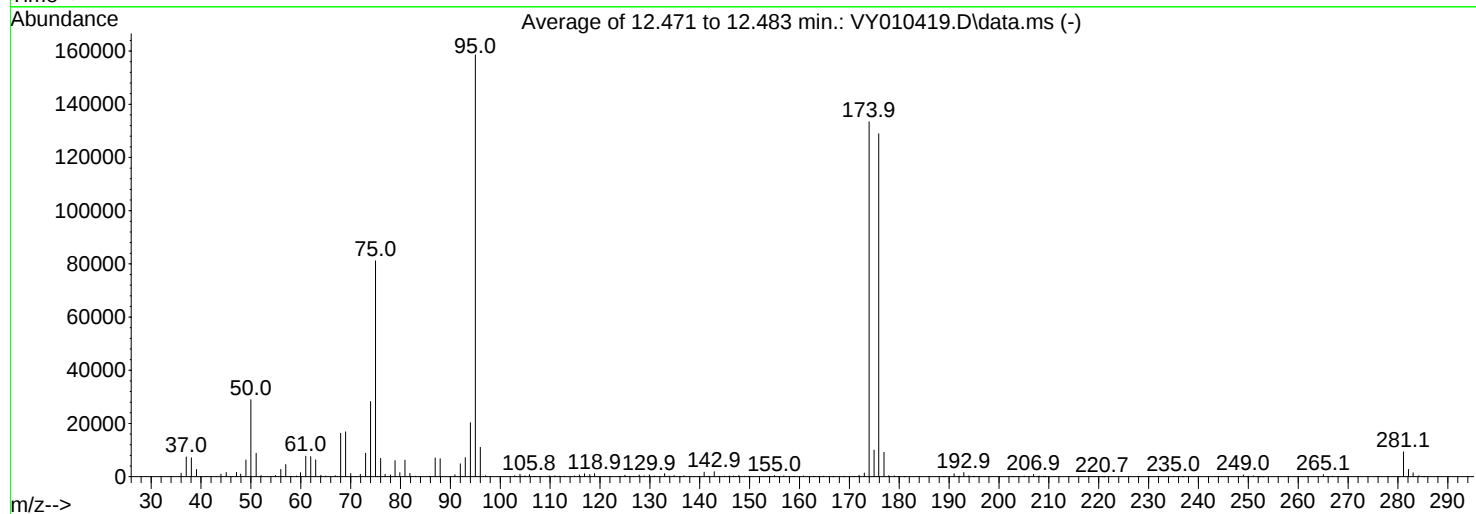


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090922\
Data File : VY010419.D
Acq On : 09 Sep 2022 15:17
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090922S.M
Title : SW846 8260
Last Update : Fri Sep 09 17:08:30 2022

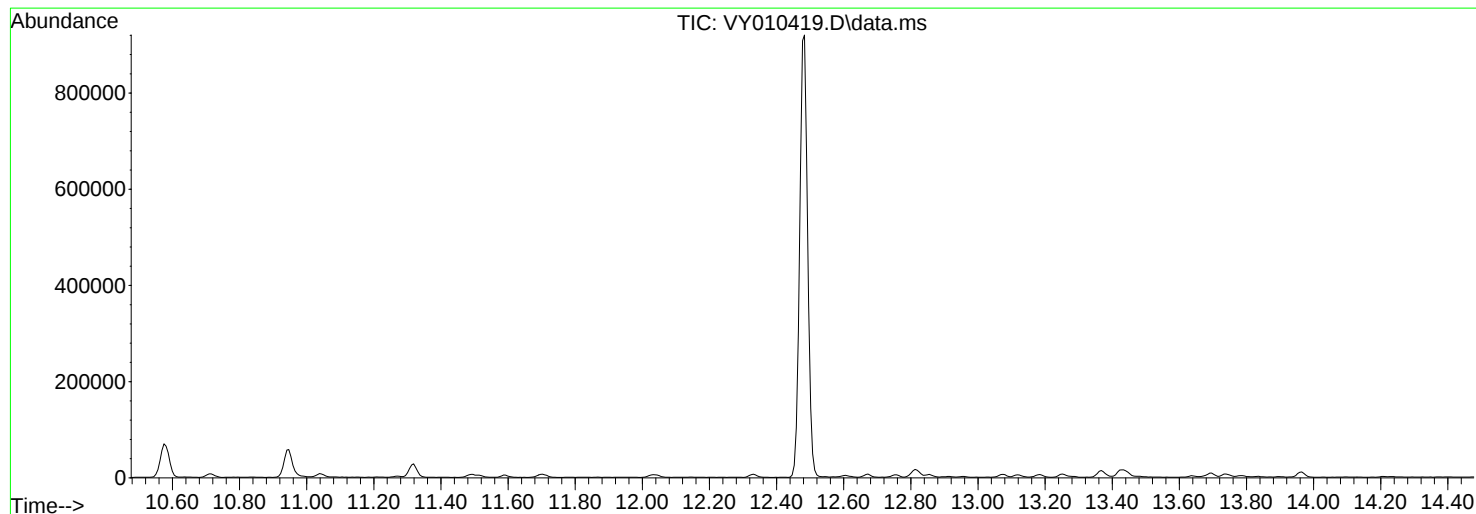

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	28960	PASS
75	95	30	60	51.2	81120	PASS
95	95	100	100	100.0	158568	PASS
96	95	5	9	6.9	10985	PASS
173	174	0.00	2	1.0	1364	PASS
174	95	50	100	84.2	133440	PASS
175	174	5	9	7.5	10017	PASS
176	174	95	101	96.6	128933	PASS
177	176	5	9	7.1	9121	PASS