
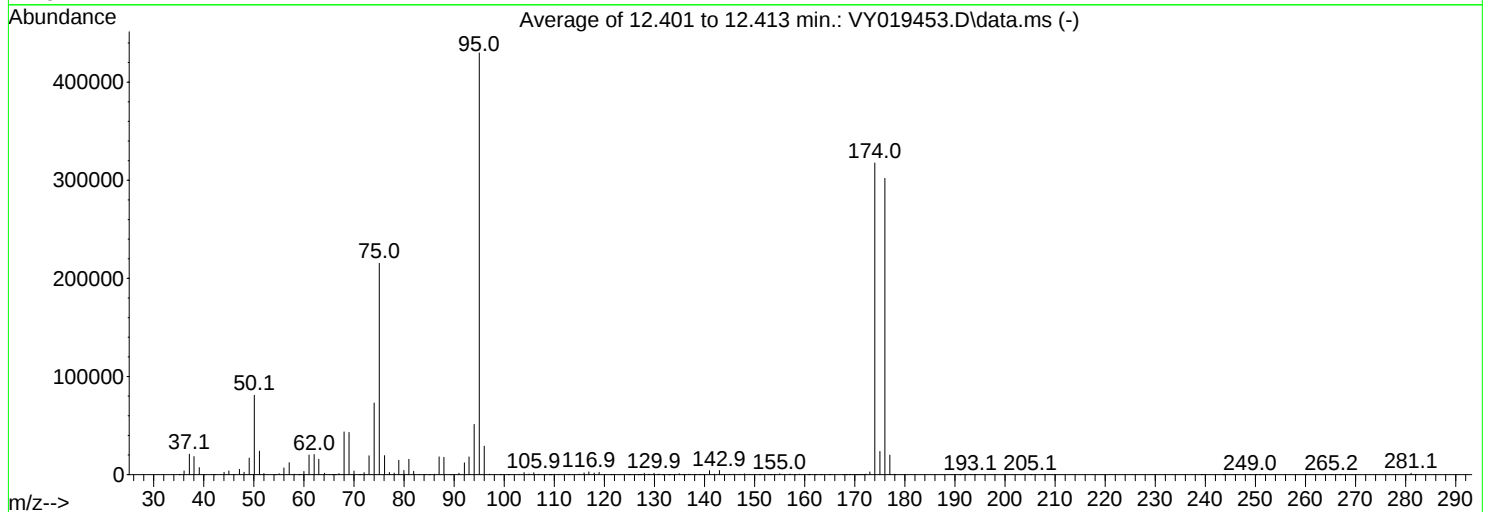


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090924\
Data File : VY019453.D
Acq On : 09 Sep 2024 09:20
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090924S.M
Title : SW846 8260
Last Update : Mon Sep 09 16:00:30 2024

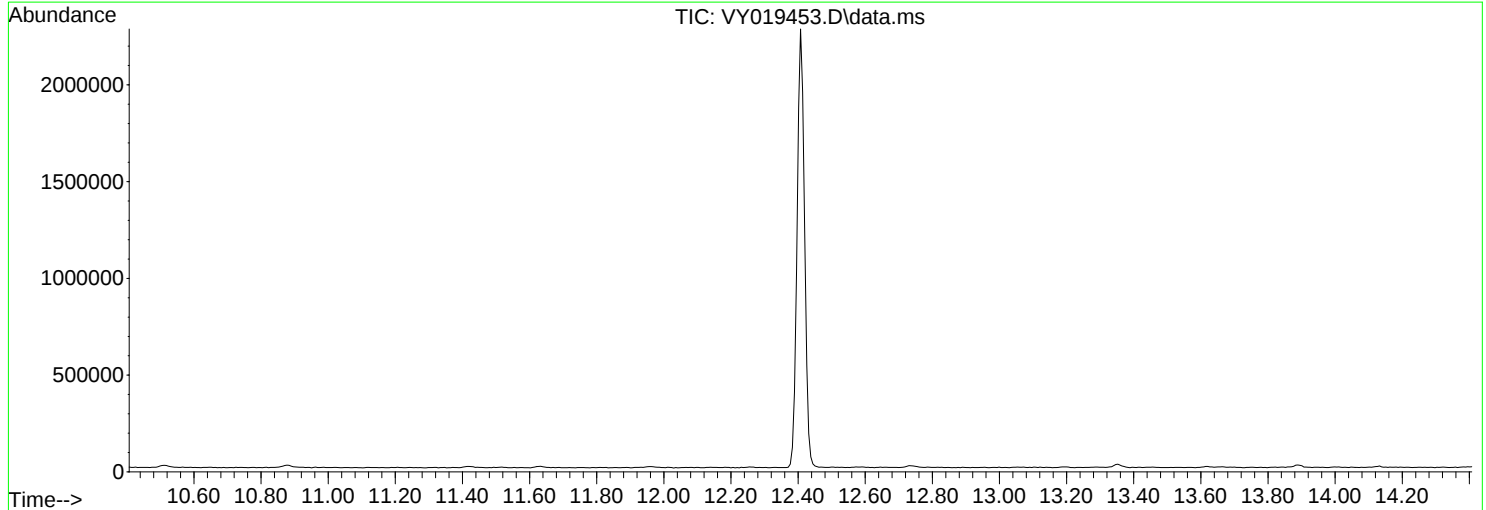

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	80903	PASS
75	95	30	60	50.1	215445	PASS
95	95	100	100	100.0	429859	PASS
96	95	5	9	6.7	28981	PASS
173	174	0.00	2	0.9	2825	PASS
174	95	50	100	73.9	317696	PASS
175	174	5	9	7.5	23725	PASS
176	174	95	101	95.1	302037	PASS
177	176	5	9	6.6	19861	PASS