


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091125\
Data File : VY023335.D
Acq On : 11 Sep 2025 08:36
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090825S.M
Title : SW846 8260
Last Update : Wed Sep 10 01:44:33 2025

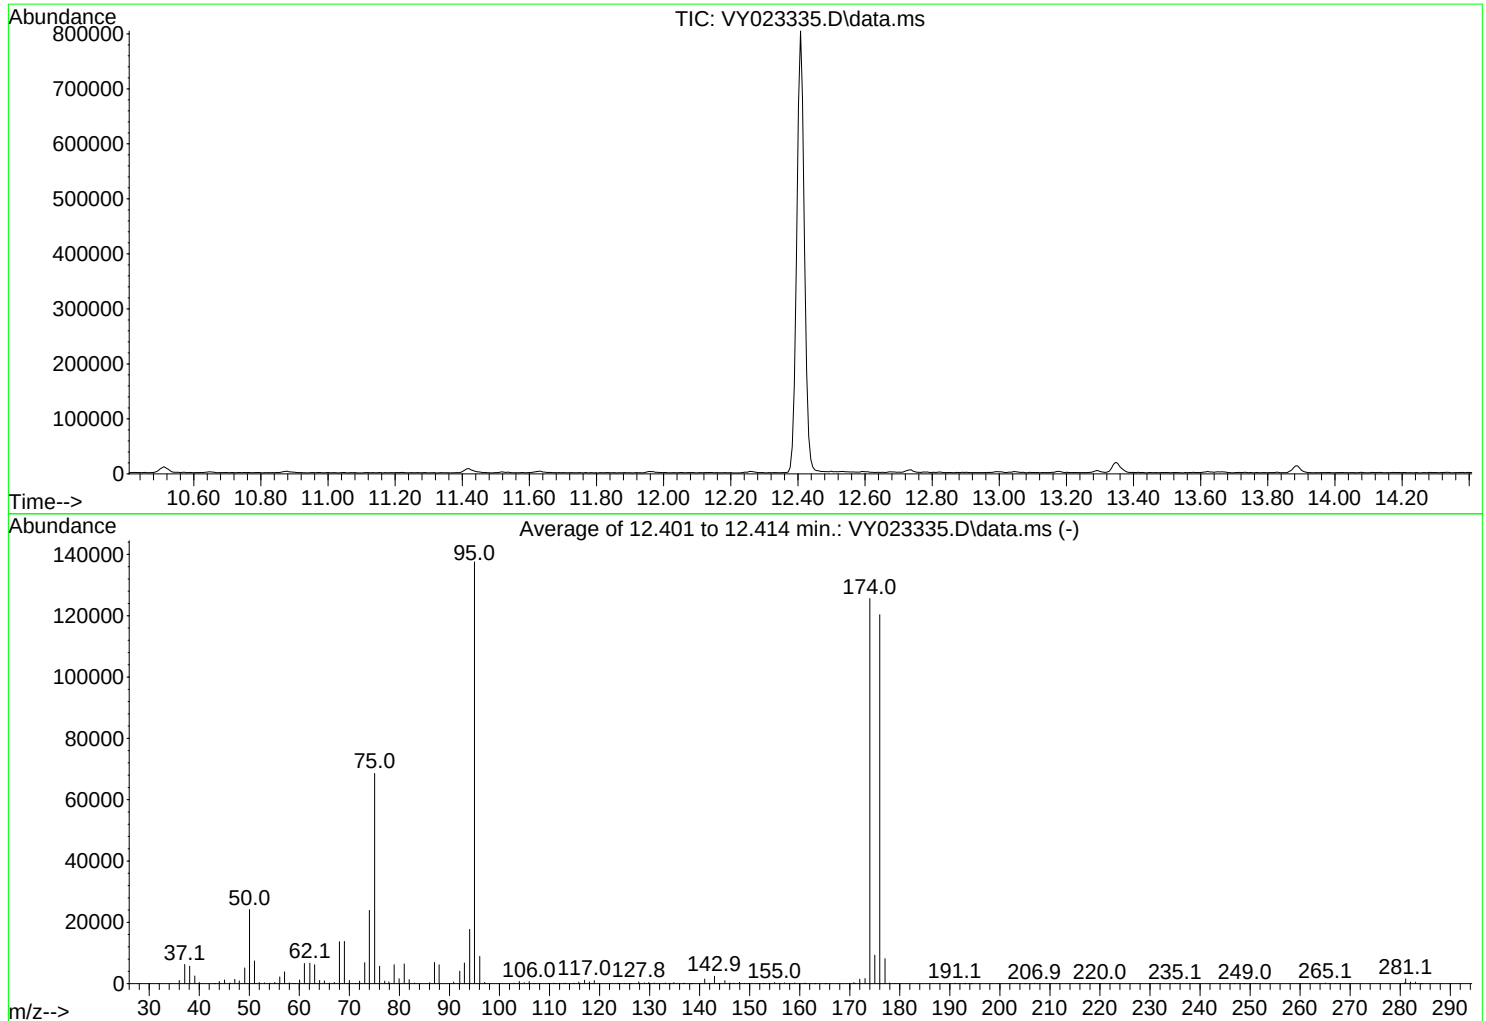

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	24160	PASS
75	95	30	60	49.9	68592	PASS
95	95	100	100	100.0	137584	PASS
96	95	5	9	6.4	8865	PASS
173	174	0.00	2	1.3	1668	PASS
174	95	50	100	91.3	125621	PASS
175	174	5	9	7.4	9274	PASS
176	174	95	101	95.8	120365	PASS
177	176	5	9	6.8	8134	PASS