
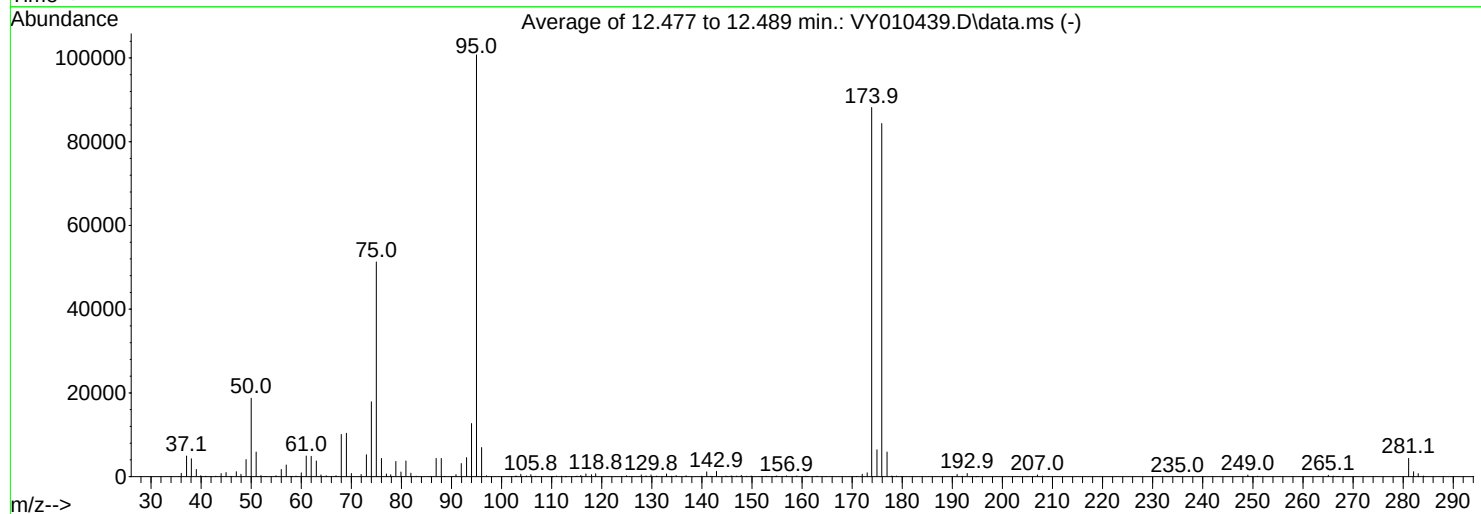


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091222\
Data File : VY010439.D
Acq On : 12 Sep 2022 09:44
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090922S.M
Title : SW846 8260
Last Update : Fri Sep 09 17:08:30 2022

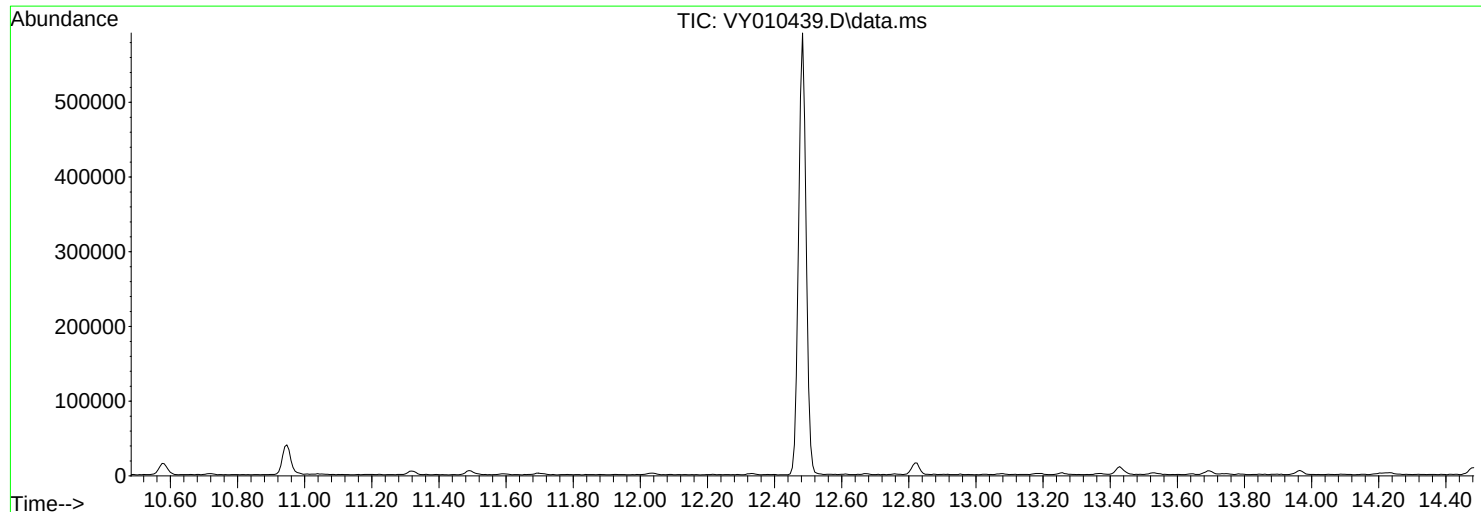

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	18735	PASS
75	95	30	60	50.9	51283	PASS
95	95	100	100	100.0	100747	PASS
96	95	5	9	6.9	6943	PASS
173	174	0.00	2	1.0	923	PASS
174	95	50	100	87.5	88165	PASS
175	174	5	9	7.3	6427	PASS
176	174	95	101	95.7	84347	PASS
177	176	5	9	7.0	5883	PASS