

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091225\
 Data File : VY023356.D
 Acq On : 12 Sep 2025 09:26
 Operator : SY/MD
 Sample : VY0912SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0912SBL01

Quant Time: Sep 12 23:57:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090825S.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 10 01:44:33 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	604675	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	1122529	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	1055856	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	437474	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	301299	56.706	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	113.420%
35) Dibromofluoromethane	7.634	113	361991	52.756	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	105.520%
50) Toluene-d8	10.109	98	1335176	51.532	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	103.060%
62) 4-Bromofluorobenzene	12.408	95	408358	50.082	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	100.160%
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	4.811	59	1259	4.101	ug/l #	71
20) Methylene Chloride	4.616	84	13054	2.016	ug/l #	86
25) 2-Butanone	6.890	43	2954	1.983	ug/l #	73
31) Cyclohexane	7.707	56	10540	1.134	ug/l #	1
36) 1,1-Dichloropropene	7.707	75	40742	4.169	ug/l #	49
38) Carbon Tetrachloride	7.713	117	56625	5.035	ug/l #	16
76) 1,2,3-Trichloropropane	12.402	75	202914	45.802	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.402	75	202914	124.906	ug/l #	14


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091225\
Data File : VY023356.D
Acq On : 12 Sep 2025 09:26
Operator : SY/MD
Sample : VY0912SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0912SBL01

Quant Time: Sep 12 23:57:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090825S.M
Quant Title : SW846 8260
QLast Update : Wed Sep 10 01:44:33 2025
Response via : Initial Calibration




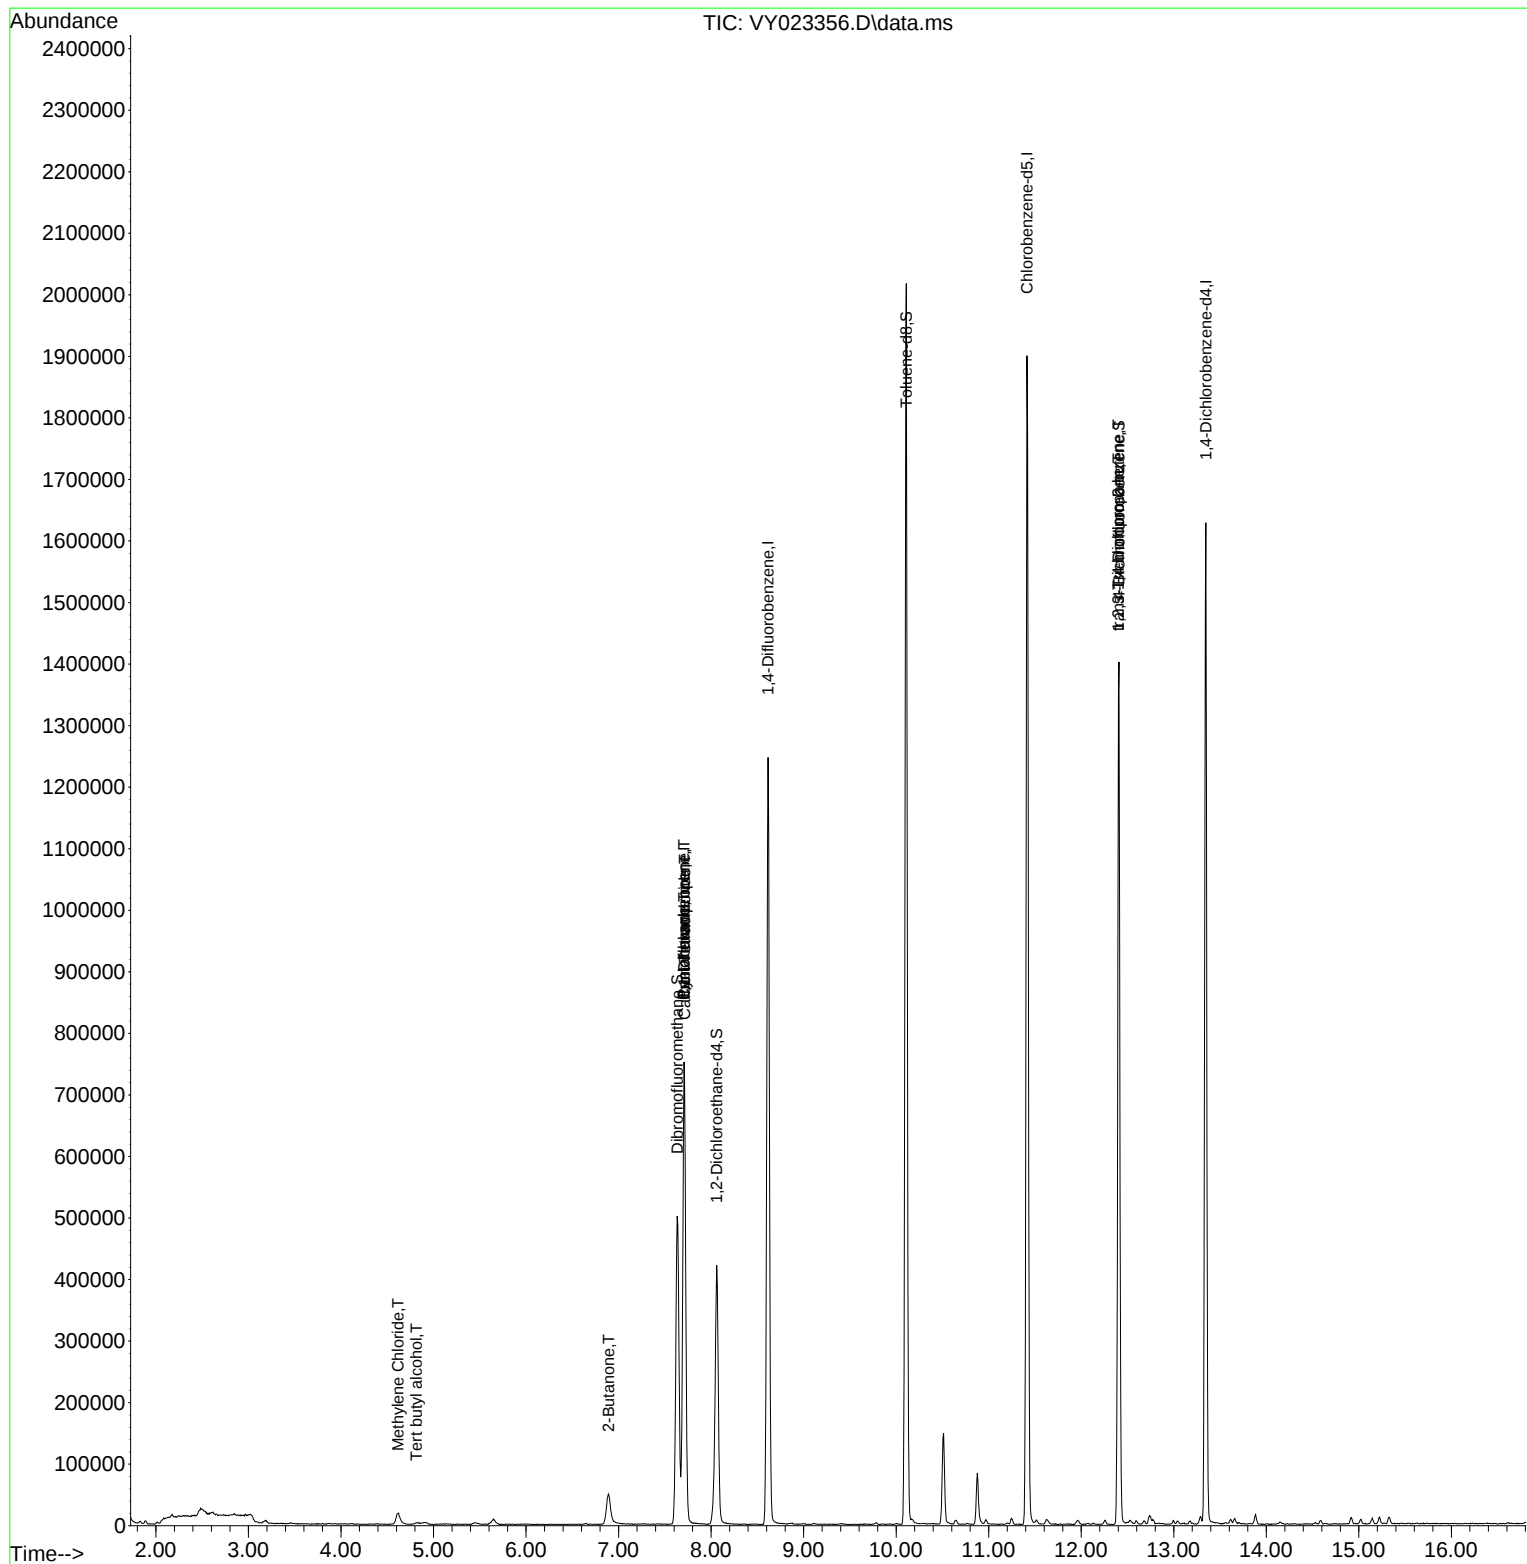


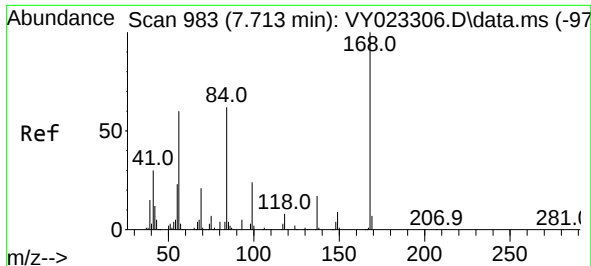

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY023356.D
Acq: 12 Sep 2025 09:26




Instrument :
MSVOA_Y
ClientSampleId :
VY0912SBL01


Tgt Ion:168 Resp: 604675
Ion Ratio Lower Upper
168 100
99 51.7 42.8 64.2

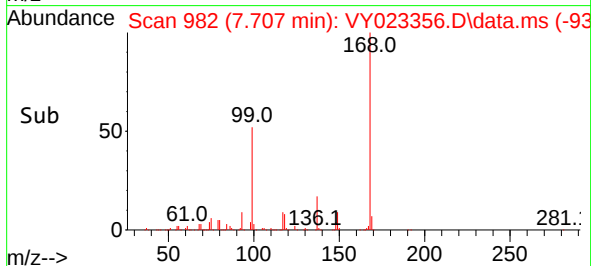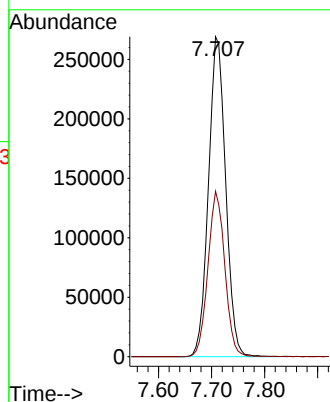

#11
Tert butyl alcohol
Concen: 4.101 ug/l
RT: 4.811 min Scan# 507
Delta R.T. -0.049 min
Lab File: VY023356.D
Acq: 12 Sep 2025 09:26

Tgt Ion: 59 Resp: 1259
Ion Ratio Lower Upper
59 100
57 0.0 8.6 13.0#


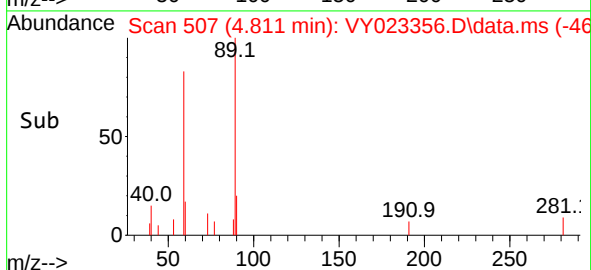
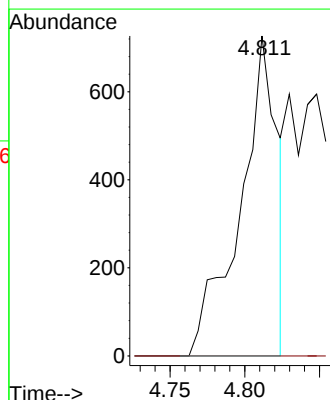
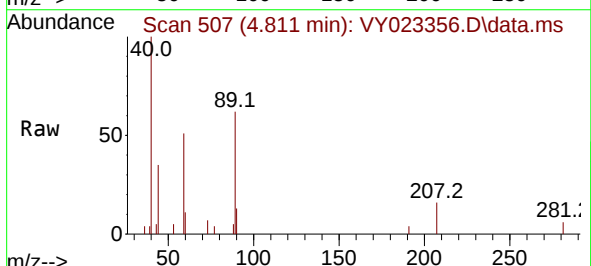


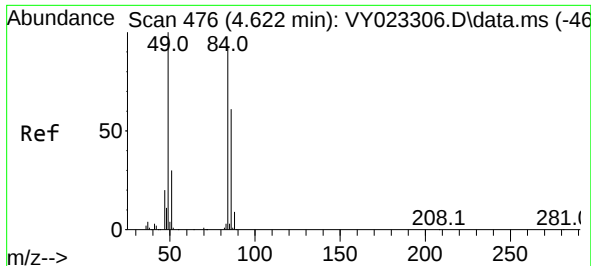

#20
Methylene Chloride
Concen: 2.016 ug/l
RT: 4.616 min Scan# 41
Delta R.T. 0.012 min
Lab File: VY023356.D
Acq: 12 Sep 2025 09:26




Instrument :
MSVOA_Y
ClientSampleId :
VY0912SBL01


Tgt Ion: 84	Resp: 13054
Ion Ratio	Lower Upper
84 100	
49 95.0	93.0 139.6
51 25.5	29.0 43.4#
86 61.4	50.2 75.4

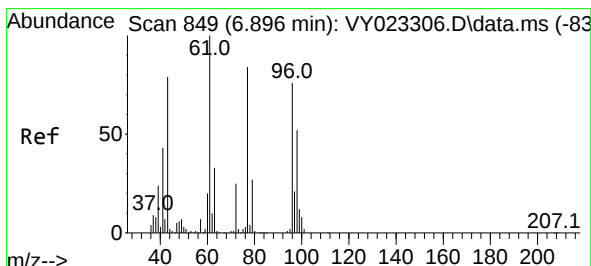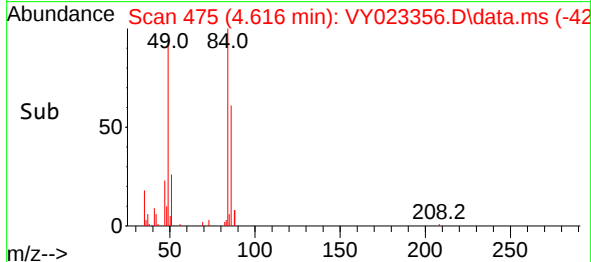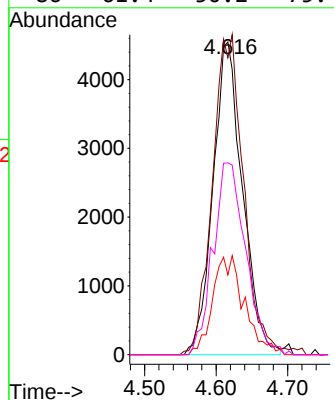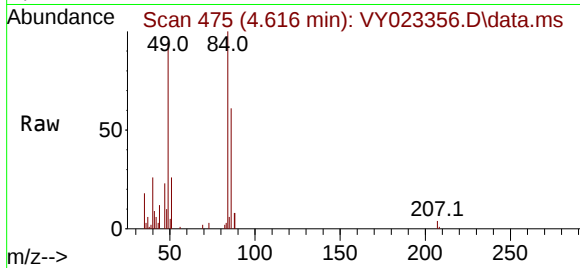

#25
2-Butanone
Concen: 1.983 ug/l
RT: 6.890 min Scan# 848
Delta R.T. 0.006 min
Lab File: VY023356.D
Acq: 12 Sep 2025 09:26

Tgt Ion: 43	Resp: 2954
Ion Ratio	Lower Upper
43 100	
72 14.7	23.5 35.3#


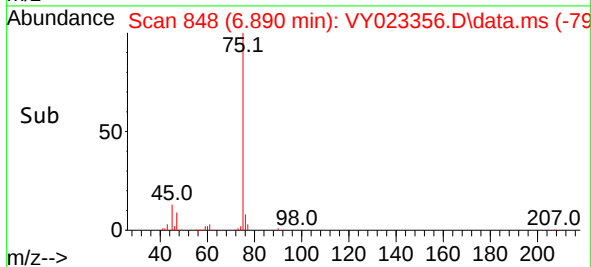
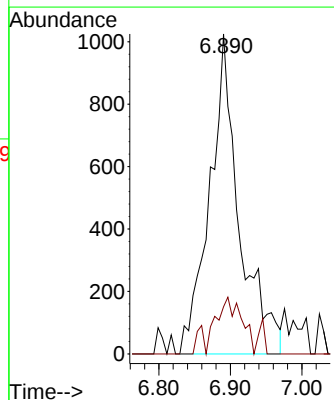
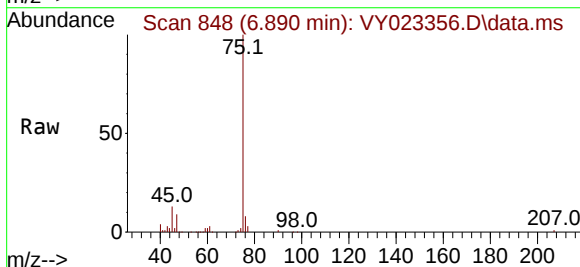


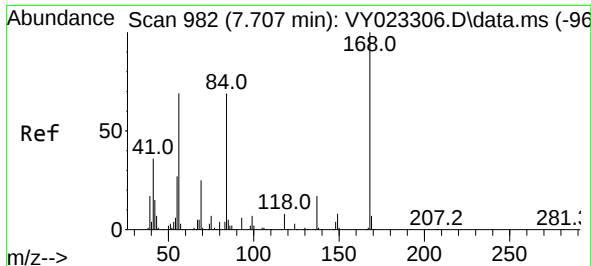

#31
Cyclohexane
Concen: 1.134 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.012 min
Lab File: VY023356.D
Acq: 12 Sep 2025 09:26




Instrument :
MSVOA_Y
ClientSampleId :
VY0912SBL01


Tgt Ion: 56 Resp: 10540
Ion Ratio Lower Upper
56 100
69 174.8 28.2 42.2#
84 168.2 76.6 114.8#

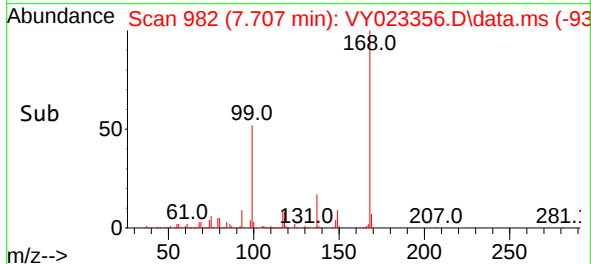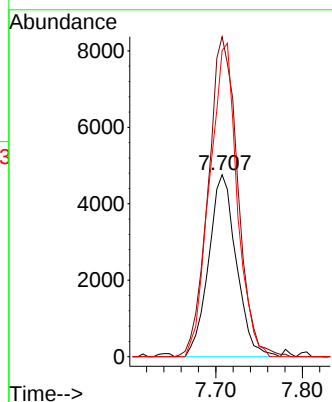

#33
1,2-Dichloroethane-d4
Concen: 56.706 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VY023356.D
Acq: 12 Sep 2025 09:26

Tgt Ion: 65 Resp: 301299
Ion Ratio Lower Upper
65 100
67 53.4 0.0 106.8


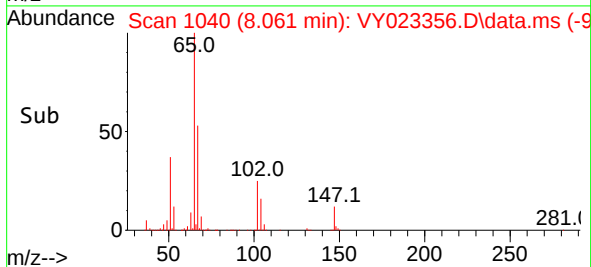
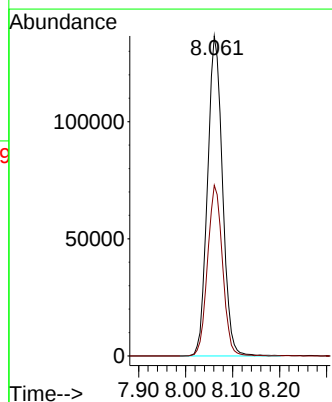
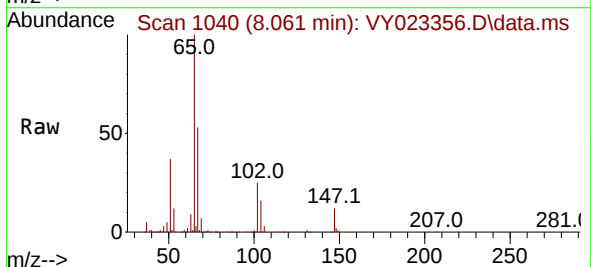


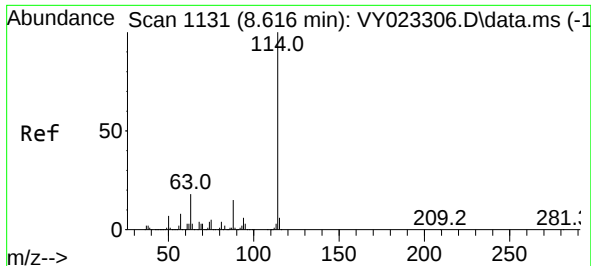

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.006 min
Lab File: VY023356.D
Acq: 12 Sep 2025 09:26




Instrument :
MSVOA_Y
ClientSampleId :
VY0912SBL01


Tgt Ion:114 Resp: 1122529
Ion Ratio Lower Upper
114 100
63 17.3 0.0 38.4
88 14.3 0.0 30.0

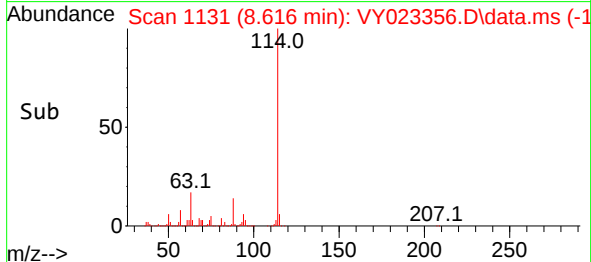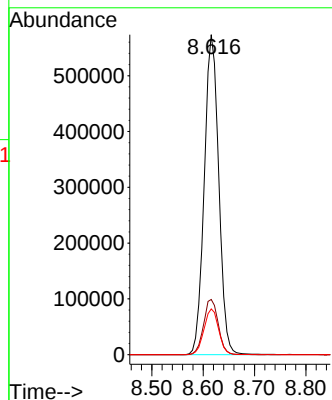

#35
Dibromofluoromethane
Concen: 52.756 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.006 min
Lab File: VY023356.D
Acq: 12 Sep 2025 09:26

Tgt Ion:113 Resp: 361991
Ion Ratio Lower Upper
113 100
111 102.8 81.1 121.7
192 21.2 16.2 24.4

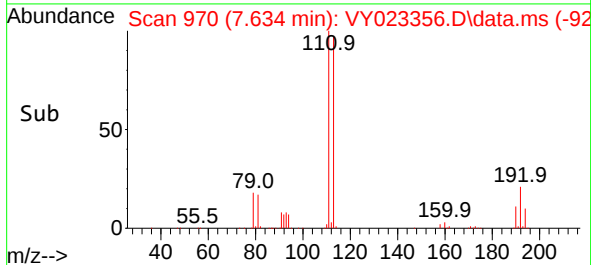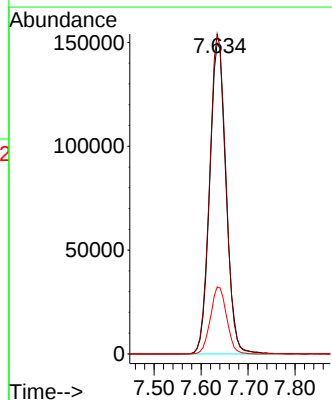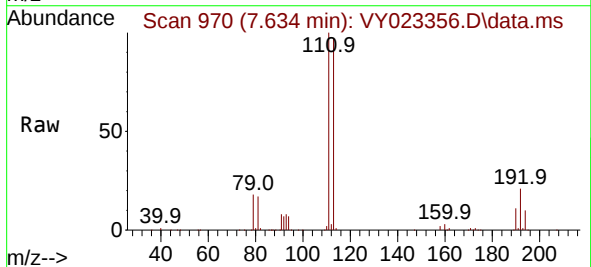

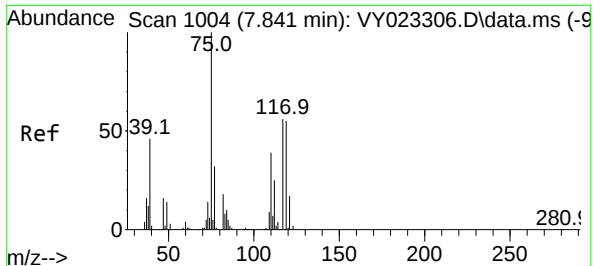

#36

1,1-Dichloropropene

Concen: 4.169 ug/l

RT: 7.707 min Scan# 91

Delta R.T. -0.122 min

Lab File: VY023356.D

Acq: 12 Sep 2025 09:26

Instrument :

MSVOA_Y

ClientSampleId :

VY0912SBL01





Tgt Ion: 75 Resp: 40742

Ion Ratio Lower Upper

75 100

110 9.1 18.1 54.4#

77 0.1 24.6 37.0#

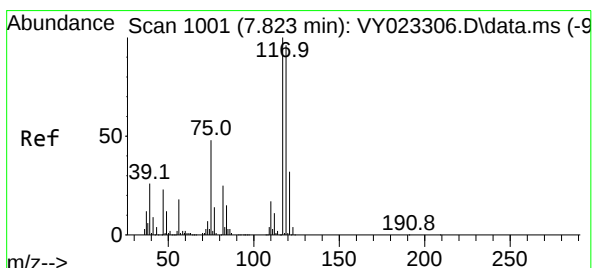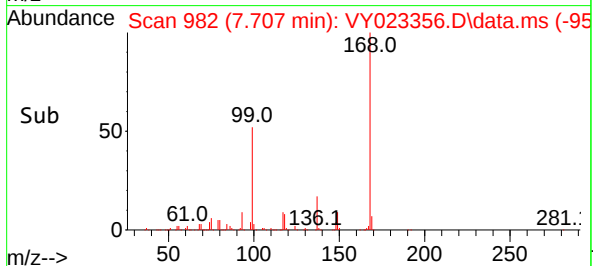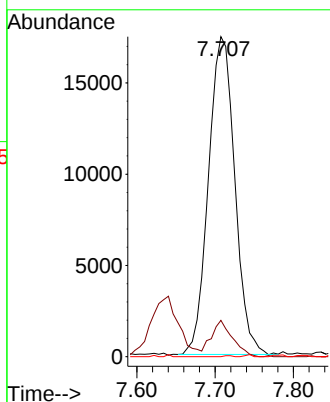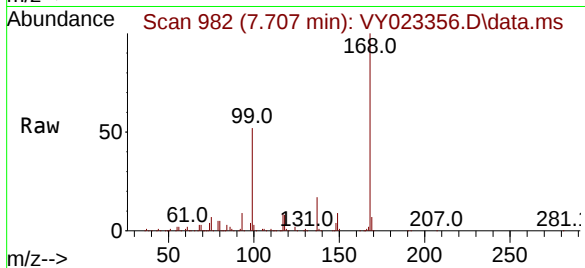

#38

Carbon Tetrachloride

Concen: 5.035 ug/l

RT: 7.713 min Scan# 983

Delta R.T. -0.103 min

Lab File: VY023356.D

Acq: 12 Sep 2025 09:26




Tgt Ion: 117 Resp: 56625


Ion Ratio Lower Upper

117 100

119 4.8 75.6 113.4#

121 0.0 25.8 38.8#

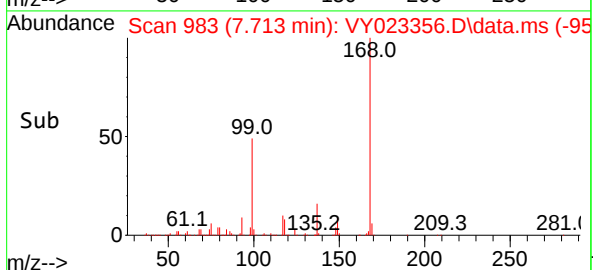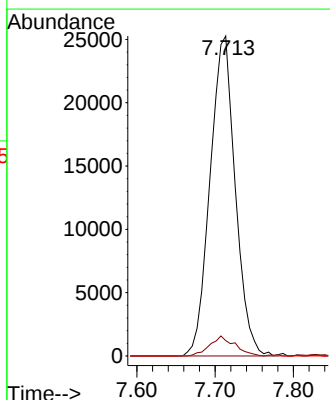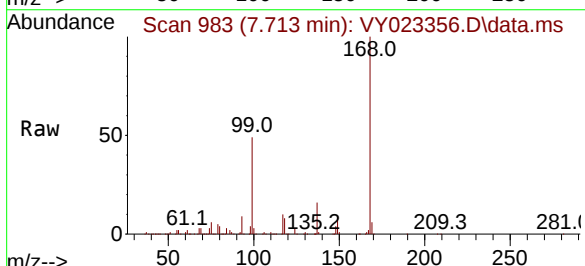



#50

Toluene-d8

Concen: 51.532 ug/l

RT: 10.109 min Scan# 1376

Delta R.T. 0.006 min

Lab File: VY023356.D

Acq: 12 Sep 2025 09:26

Instrument :

MSVOA_Y

ClientSampleId :





VY0912SBL01

Tgt Ion: 98 Resp: 1335176

Ion Ratio Lower Upper

98 100

100 65.1 52.3 78.5

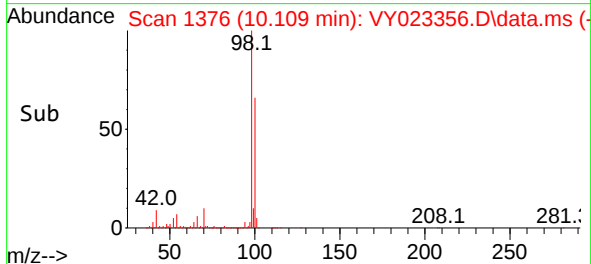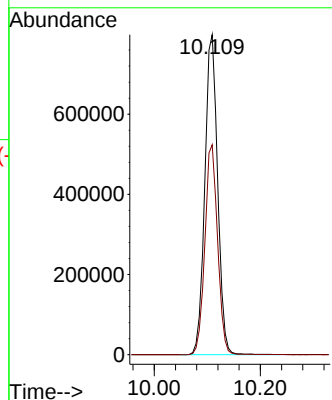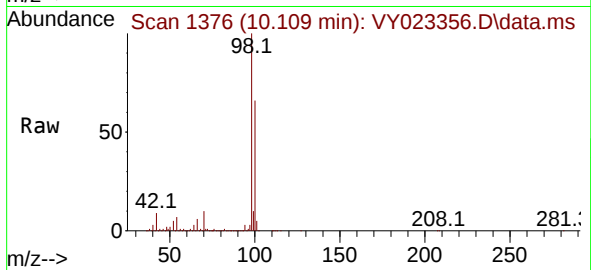

#62

4-Bromofluorobenzene

Concen: 50.082 ug/l

RT: 12.408 min Scan# 1753

Delta R.T. 0.006 min

Lab File: VY023356.D

Acq: 12 Sep 2025 09:26




Tgt Ion: 95 Resp: 408358


Ion Ratio Lower Upper

95 100

174 94.3 0.0 171.6

176 90.4 0.0 167.6

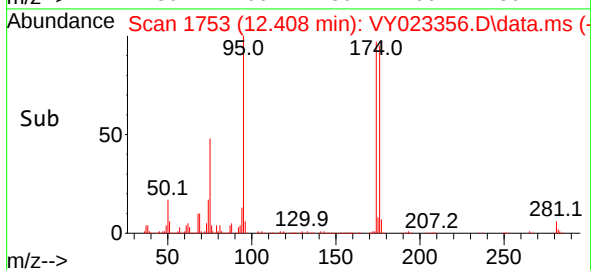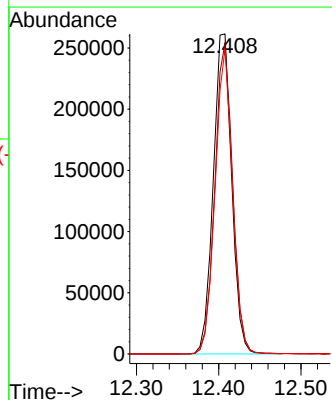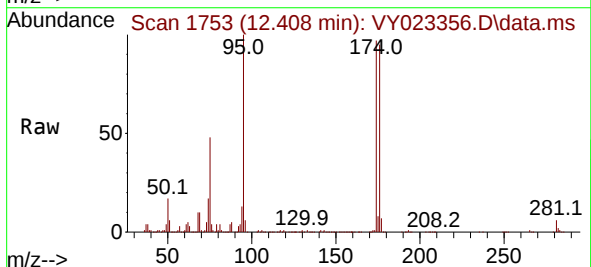



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY023356.D

Acq: 12 Sep 2025 09:26

Instrument :

MSVOA_Y

ClientSampleId :

VY0912SBL01





Tgt Ion:117 Resp: 1055856

Ion Ratio Lower Upper

117 100

82 50.4 43.4 65.0

119 31.6 25.6 38.4

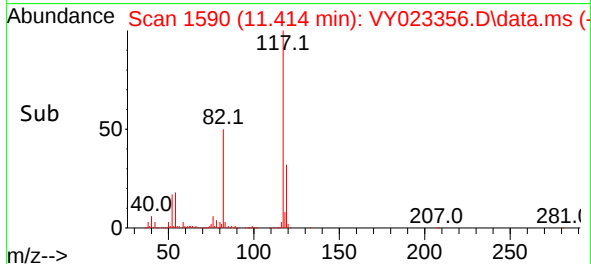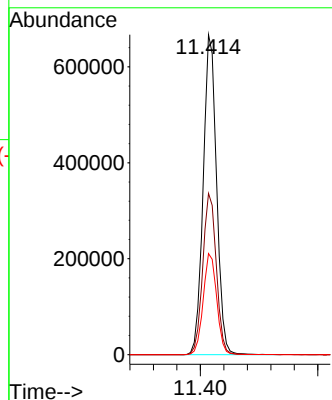

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.006 min

Lab File: VY023356.D

Acq: 12 Sep 2025 09:26




Tgt Ion:152 Resp: 437474


Ion Ratio Lower Upper

152 100

115 54.5 28.2 84.6

150 155.3 0.0 348.0


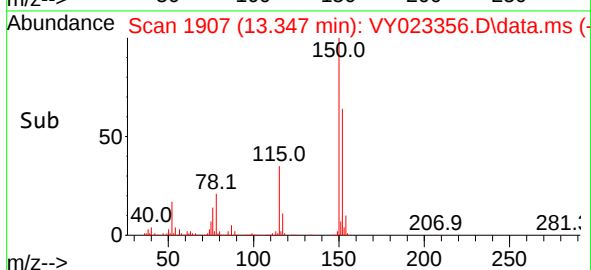
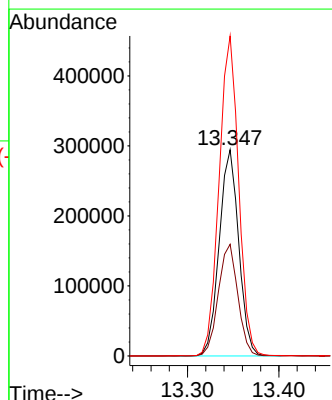
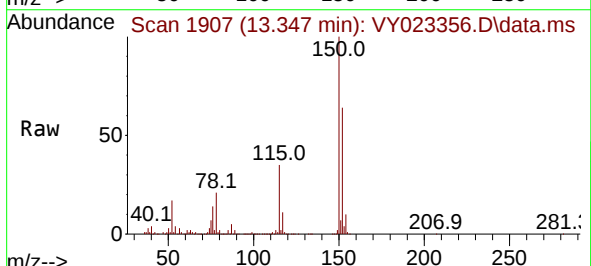


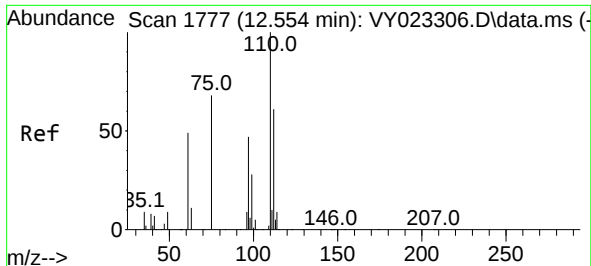

#76
1,2,3-Trichloropropane
Concen: 45.802 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. -0.146 min
Lab File: VY023356.D
Acq: 12 Sep 2025 09:26

Instrument :
MSVOA_Y
ClientSampleId :
VY0912SBL01

Tgt Ion: 75 Resp: 202914
Ion Ratio Lower Upper
75 100
77 1.3 0.0 0.0#

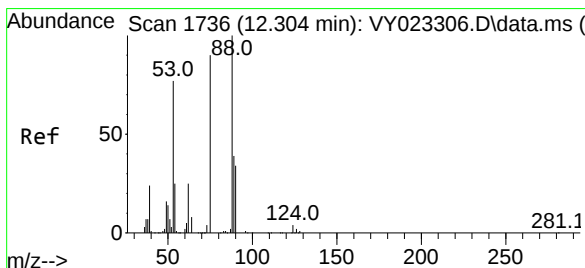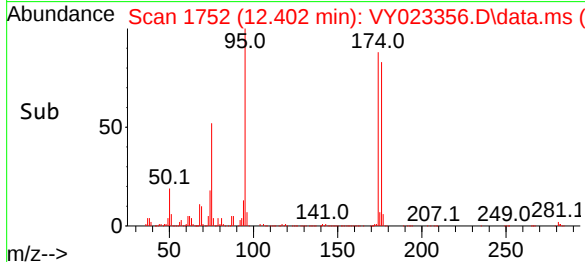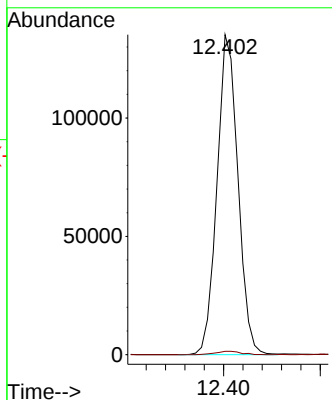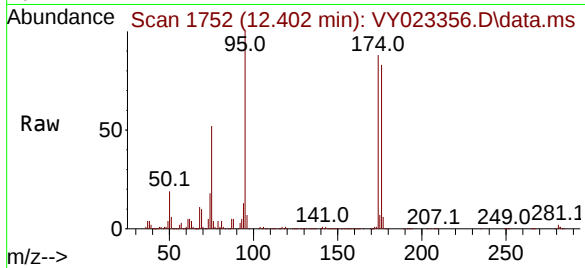

#81
trans-1,4-Dichloro-2-butene
Concen: 124.906 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. 0.104 min
Lab File: VY023356.D
Acq: 12 Sep 2025 09:26

Tgt Ion: 75 Resp: 202914
Ion Ratio Lower Upper
75 100
53 0.1 70.8 106.2#
89 0.0 38.1 57.1#

