


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091225\
Data File : VY023354.D
Acq On : 12 Sep 2025 08:26
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090825S.M
Title : SW846 8260
Last Update : Wed Sep 10 01:44:33 2025

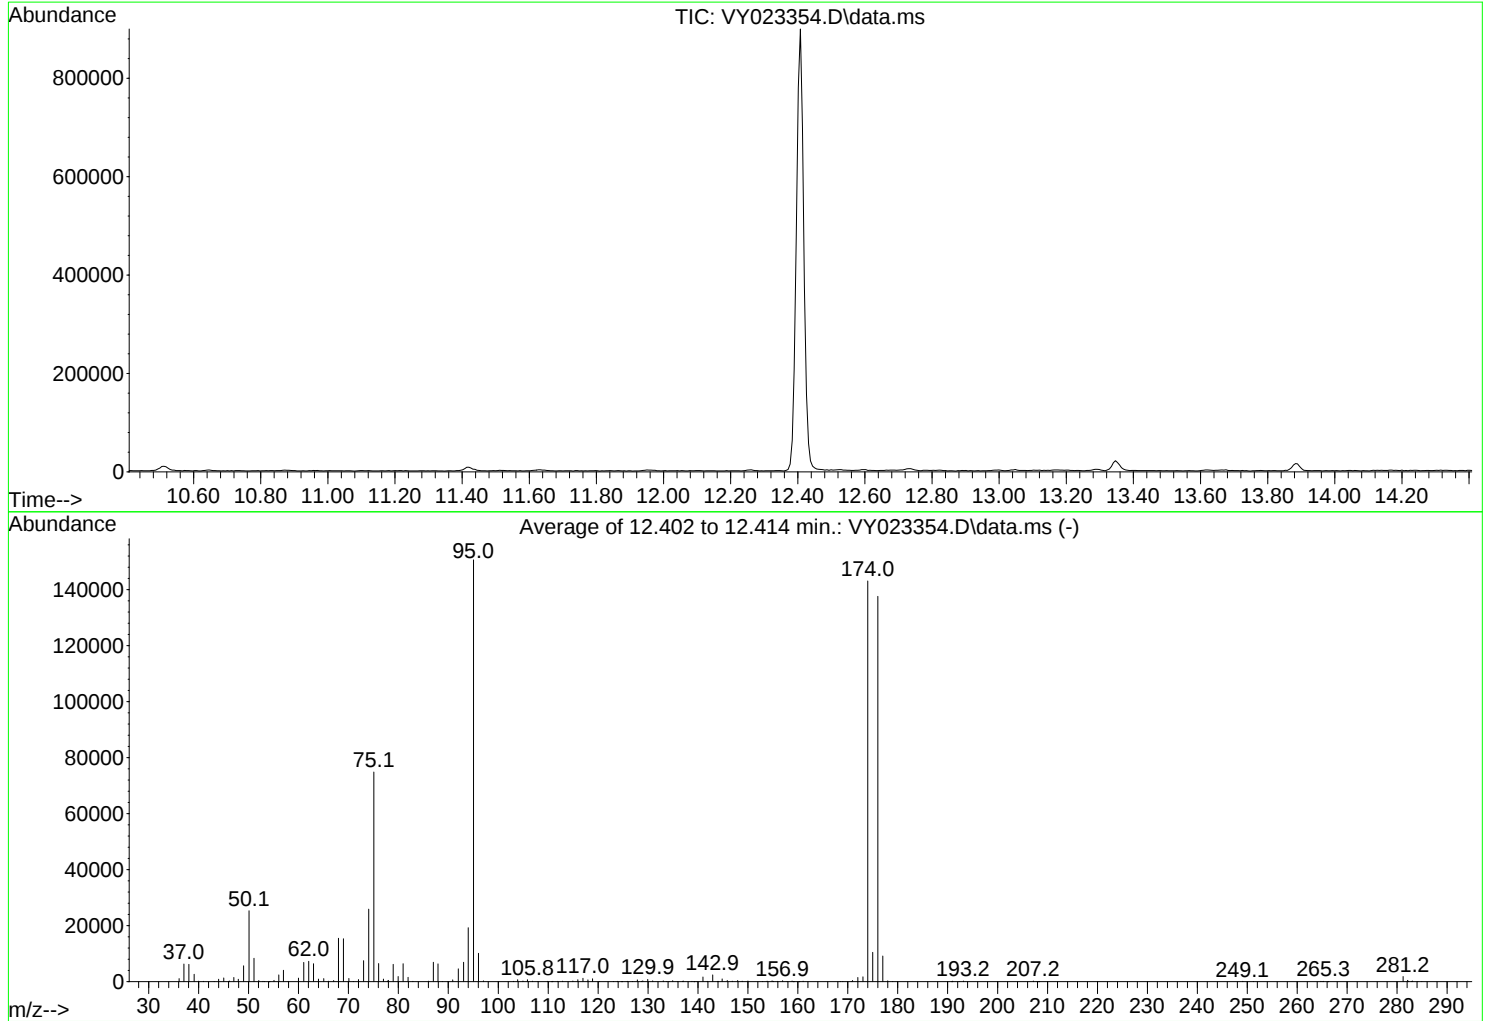

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	25331	PASS
75	95	30	60	49.7	74861	PASS
95	95	100	100	100.0	150659	PASS
96	95	5	9	6.7	10106	PASS
173	174	0.00	2	1.2	1717	PASS
174	95	50	100	95.0	143083	PASS
175	174	5	9	7.3	10432	PASS
176	174	95	101	96.2	137640	PASS
177	176	5	9	6.6	9125	PASS