

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091521\
 Data File : VY006029.D
 Acq On : 15 Sep 2021 17:13
 Operator : SY/MD
 Sample : M3733-07
 Misc : 7.21G/5ML/MSVOA_Y/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 NAPL-AREA-02-(5-8)

Quant Time: Sep 16 01:23:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091421S.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 15 05:01:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	0.000	168	0	0.000	ug/l	-7.79
34) 1,4-Difluorobenzene	0.000	114	0	0.000	ug/l	-8.70
63) Chlorobenzene-d5	0.000	117	0	0.000	ug/l	-11.50
72) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ug/l	-13.43
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.000	65	0	0.000	ug/l	
Spiked Amount	50.000	Range	50 - 163	Recovery	=	0.000%#
35) Dibromofluoromethane	0.000	113	0	0.000	ug/l	
Spiked Amount	50.000	Range	54 - 147	Recovery	=	0.000%#
50) Toluene-d8	0.000	98	0	0.000	ug/l	
Spiked Amount	50.000	Range	49 - 140	Recovery	=	0.000%#
62) 4-Bromofluorobenzene	0.000	95	0	0.000	ug/l	
Spiked Amount	50.000	Range	25 - 144	Recovery	=	0.000%#


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091521\
Data File : VY006029.D
Acq On : 15 Sep 2021 17:13
Operator : SY/MD
Sample : M3733-07
Misc : 7.21G/5ML/MSVOA_Y/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-02-(5-8)

Quant Time: Sep 16 01:23:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091421S.M
Quant Title : SW846 8260
QLast Update : Wed Sep 15 05:01:47 2021
Response via : Initial Calibration

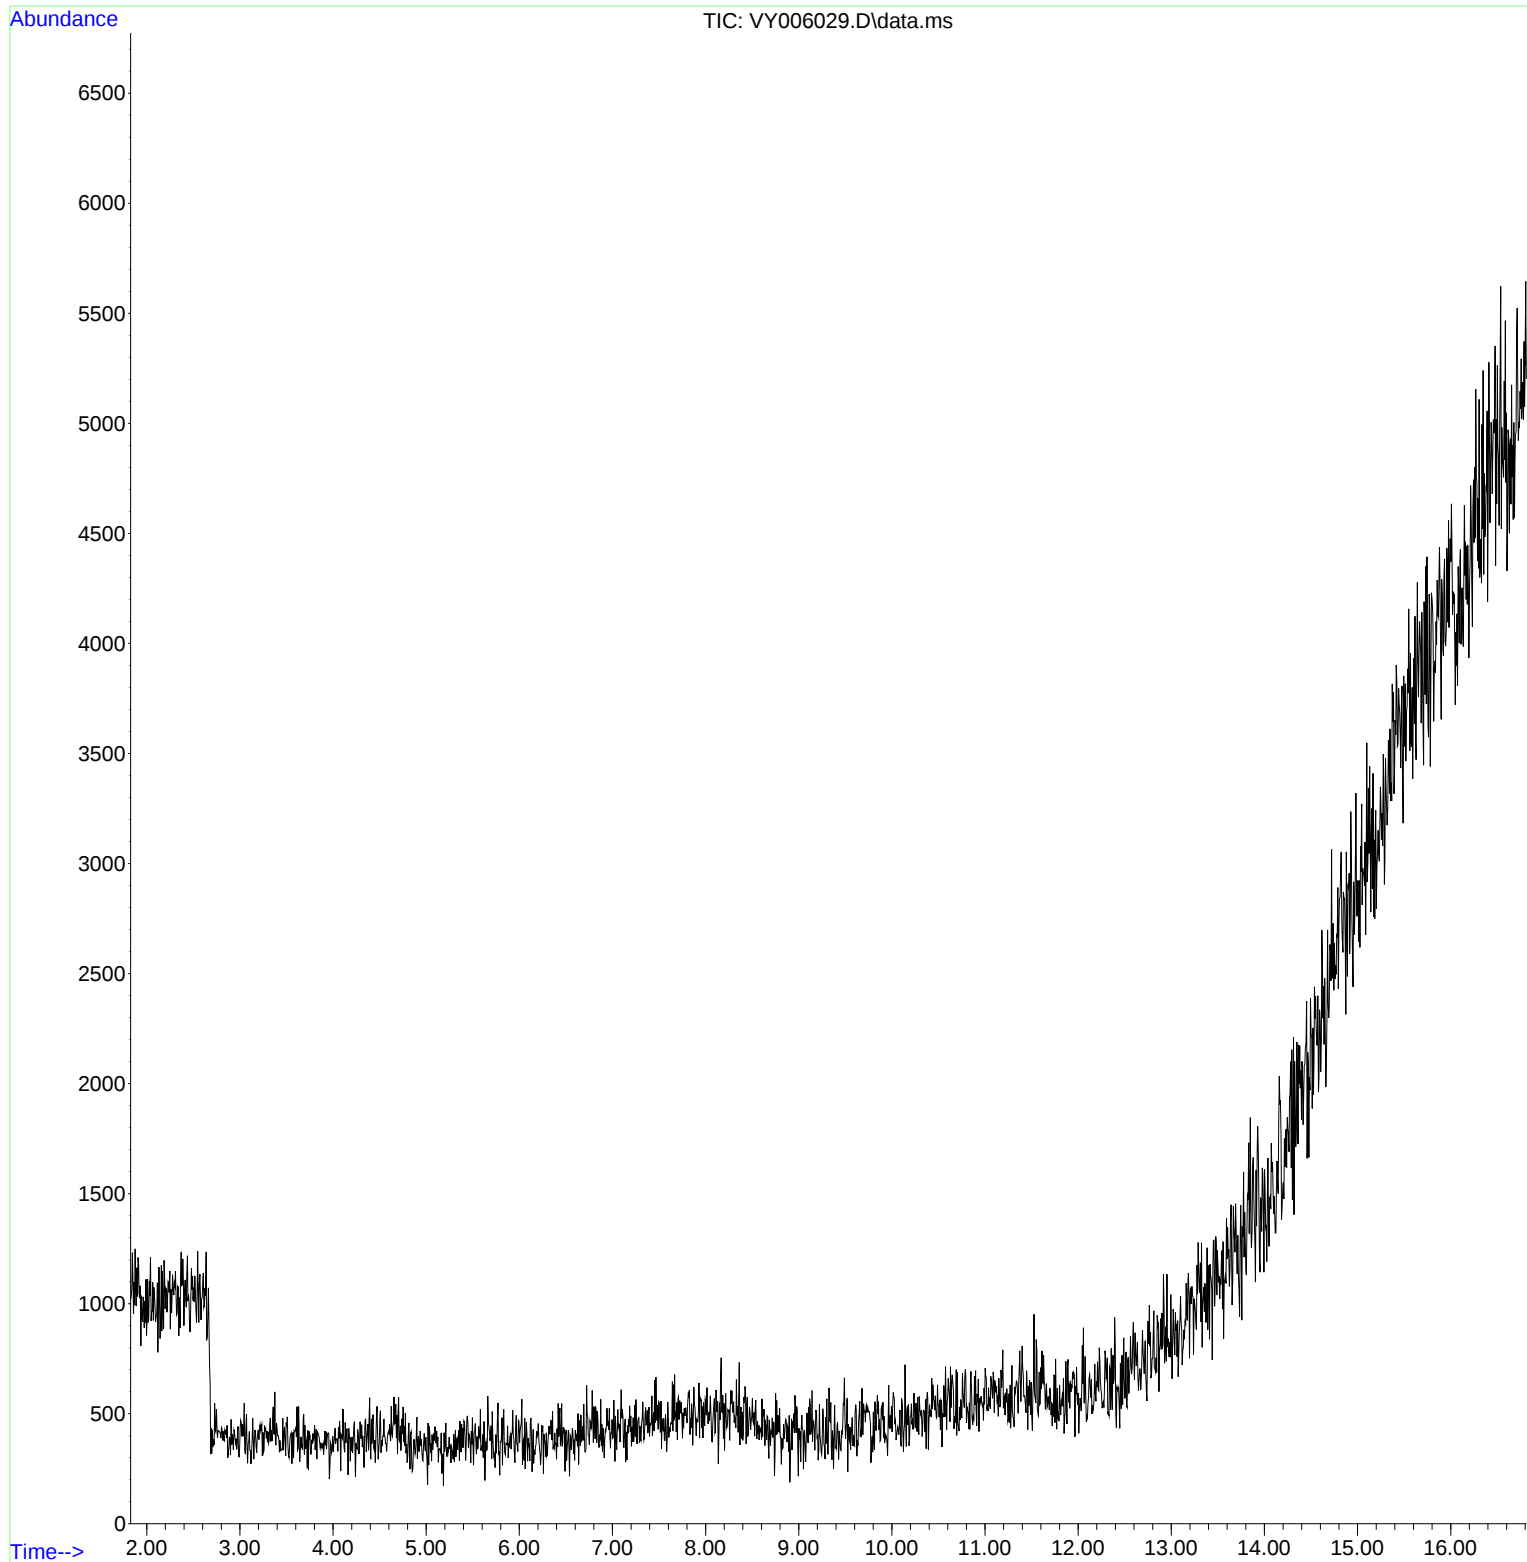


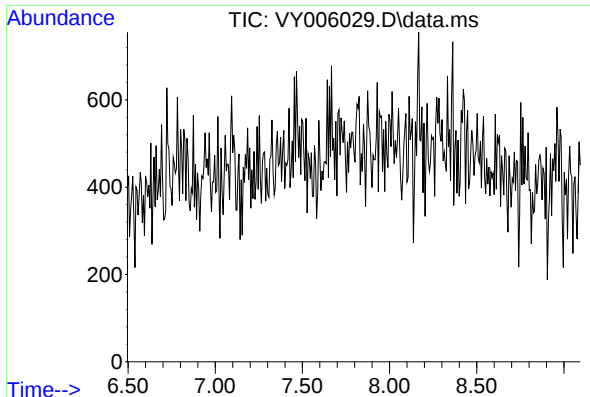


#1
Pentafluorobenzene
Concen: 0.000 ug/l
Expected RT: 7.79 min

Lab File: VY006029.D
Acq: 15 Sep 2021 17:13

Tgt Ion: 168
Sig Exp Ratio
168 100
99 58.6


Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-02-(5-8)

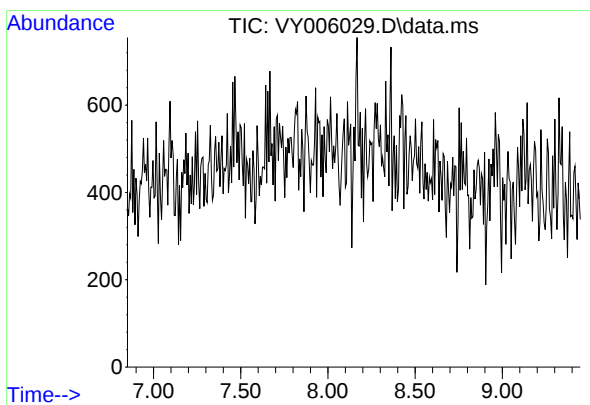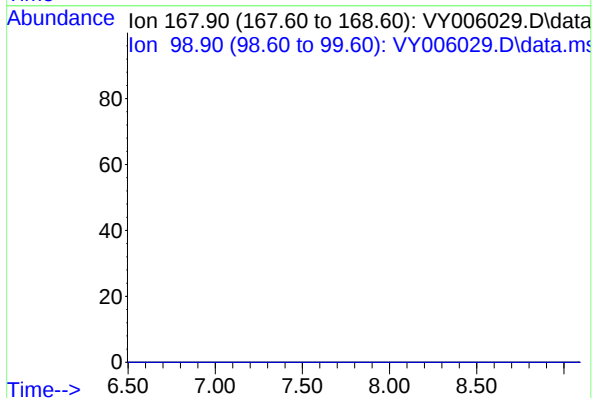


#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
Expected RT: 8.15 min

Lab File: VY006029.D
Acq: 15 Sep 2021 17:13

Tgt Ion: 65
Sig Exp Ratio
65 100
67 49.7

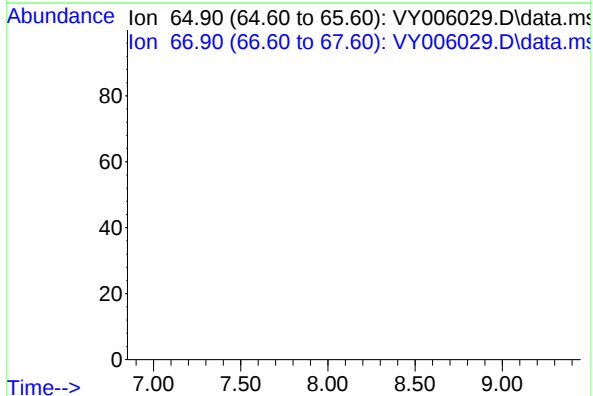


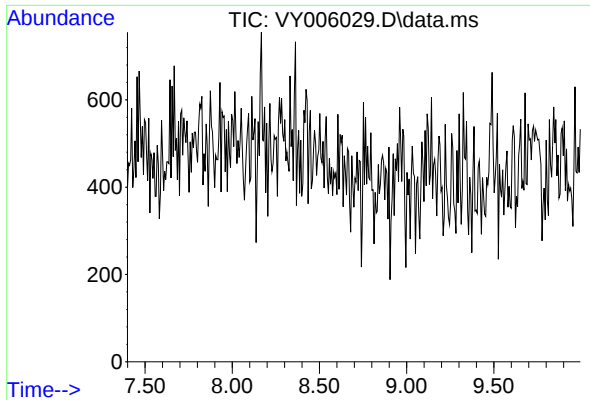


#34
1,4-Difluorobenzene
Concen: 0.000 ug/l
Expected RT: 8.70 min

Lab File: VY006029.D
Acq: 15 Sep 2021 17:13

Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-02-(5-8)


Tgt Ion: 114
Sig Exp Ratio
114 100
63 21.6
88 15.9

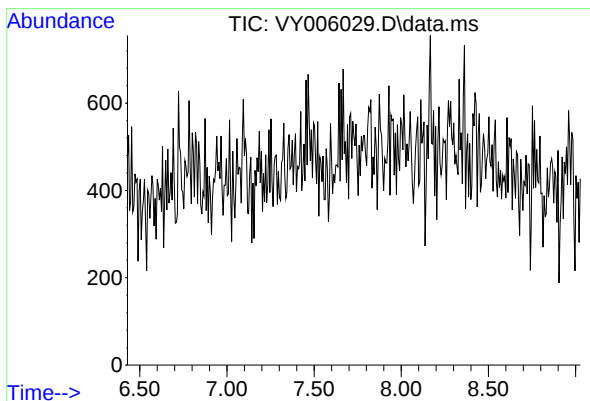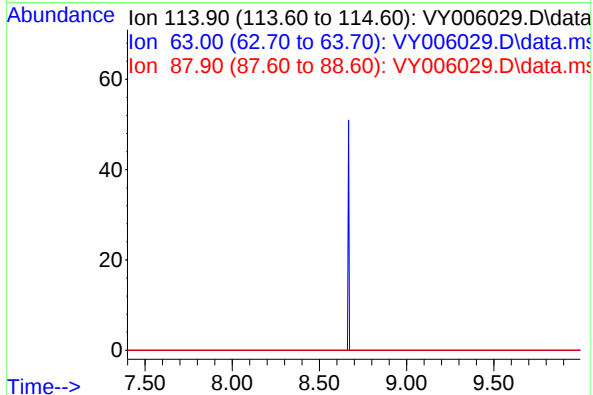


#35
Dibromofluoromethane
Concen: 0.000 ug/l
Expected RT: 7.73 min

Lab File: VY006029.D
Acq: 15 Sep 2021 17:13

Tgt Ion: 113
Sig Exp Ratio
113 100
111 103.3
192 22.0

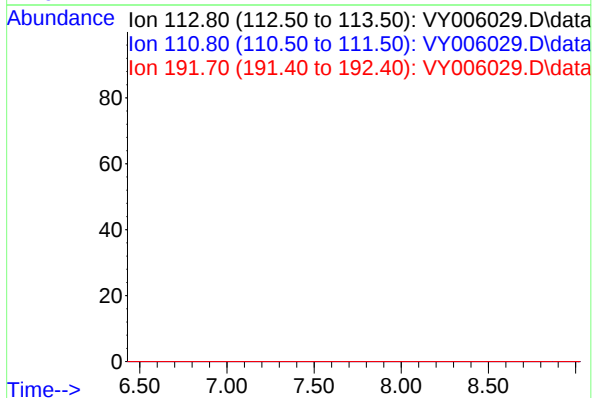


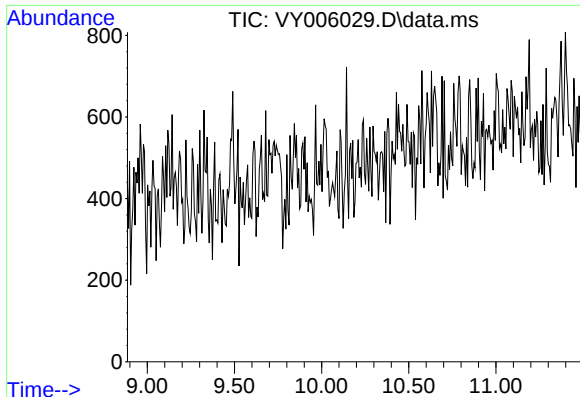


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.18 min

Lab File: VY006029.D
Acq: 15 Sep 2021 17:13

Tgt Ion: 98
Sig Exp Ratio
98 100
100 62.7


Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-02-(5-8)

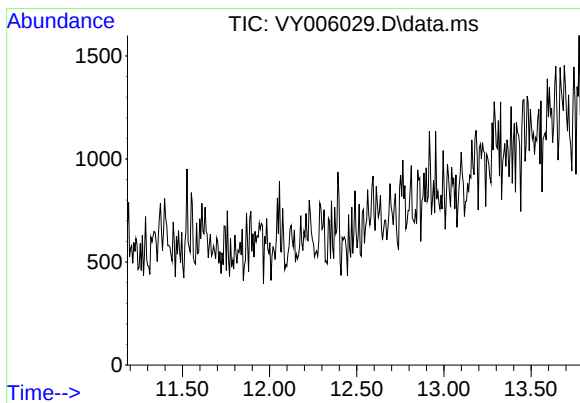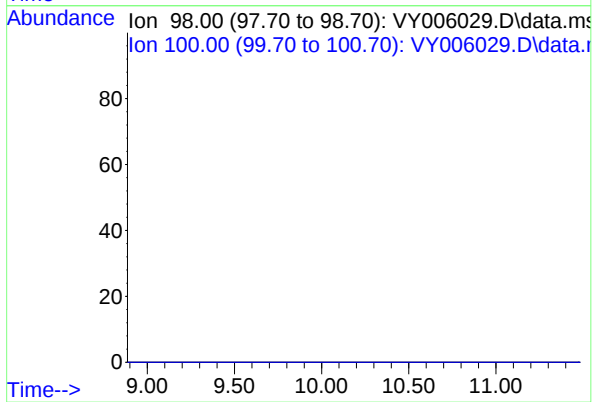


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.48 min

Lab File: VY006029.D
Acq: 15 Sep 2021 17:13

Tgt Ion: 95
Sig Exp Ratio
95 100
174 88.5
176 87.9

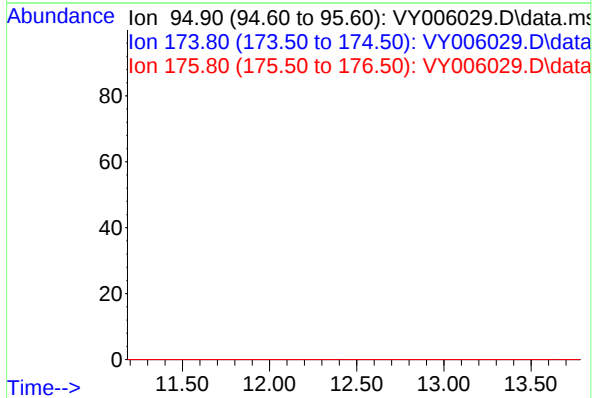


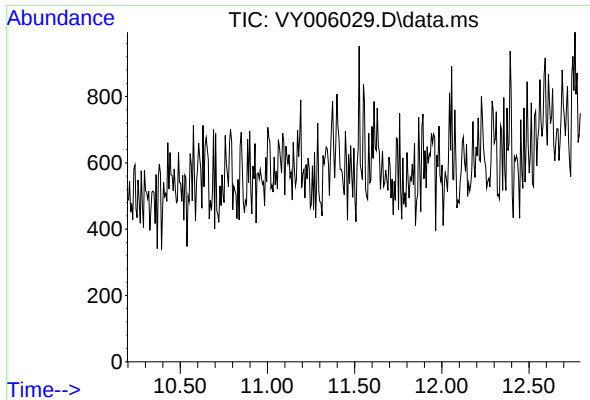


#63
Chlorobenzene-d5
Concen: 0.000 ug/l
Expected RT: 11.50 min

Lab File: VY006029.D
Acq: 15 Sep 2021 17:13

Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-02-(5-8)

Tgt Ion: 117
Sig Exp Ratio
117 100
82 53.7
119 31.7

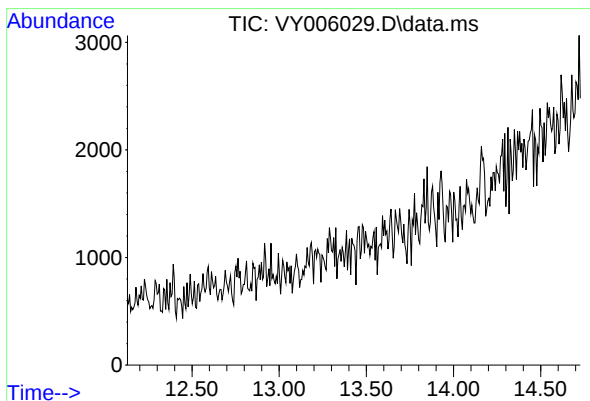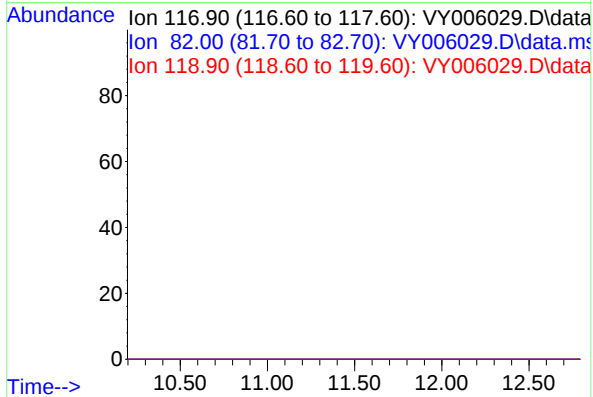

#72
1,4-Dichlorobenzene-d4
Concen: 0.000 ug/l
Expected RT: 13.43 min

Lab File: VY006029.D
Acq: 15 Sep 2021 17:13

Tgt Ion: 152
Sig Exp Ratio
152 100
115 56.5
150 173.8

