
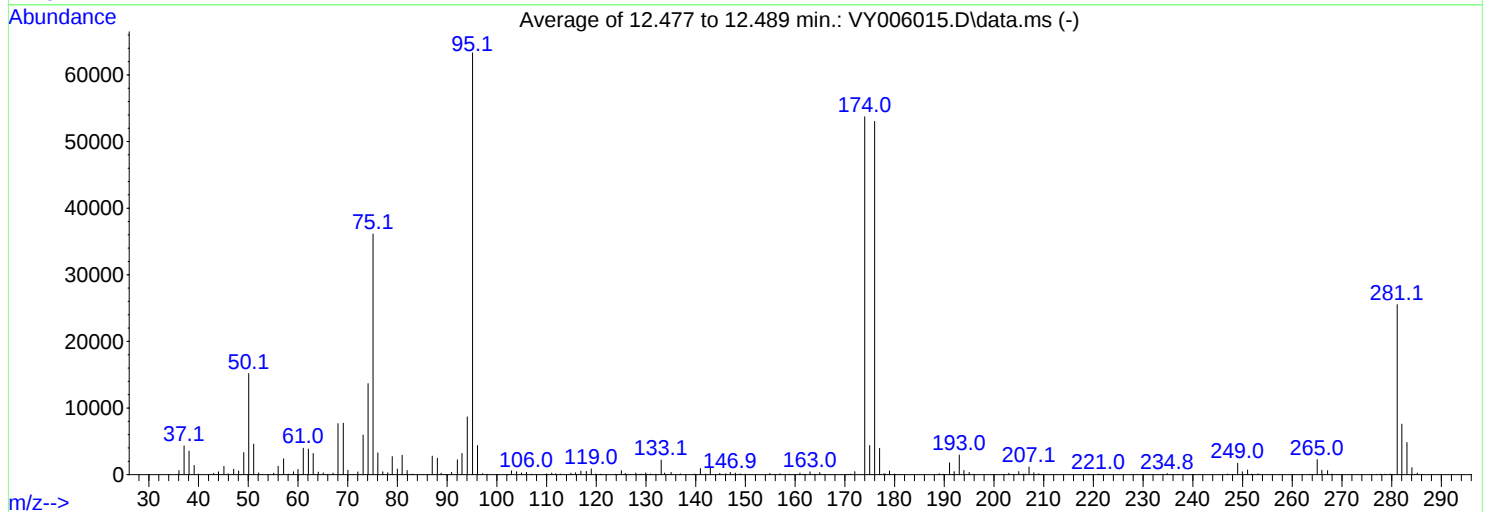


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091521\
 Data File : VY006015.D
 Acq On : 15 Sep 2021 08:51
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y0914215.M
 Title : SW846 8260
 Last Update : Wed Sep 15 05:01:47 2021

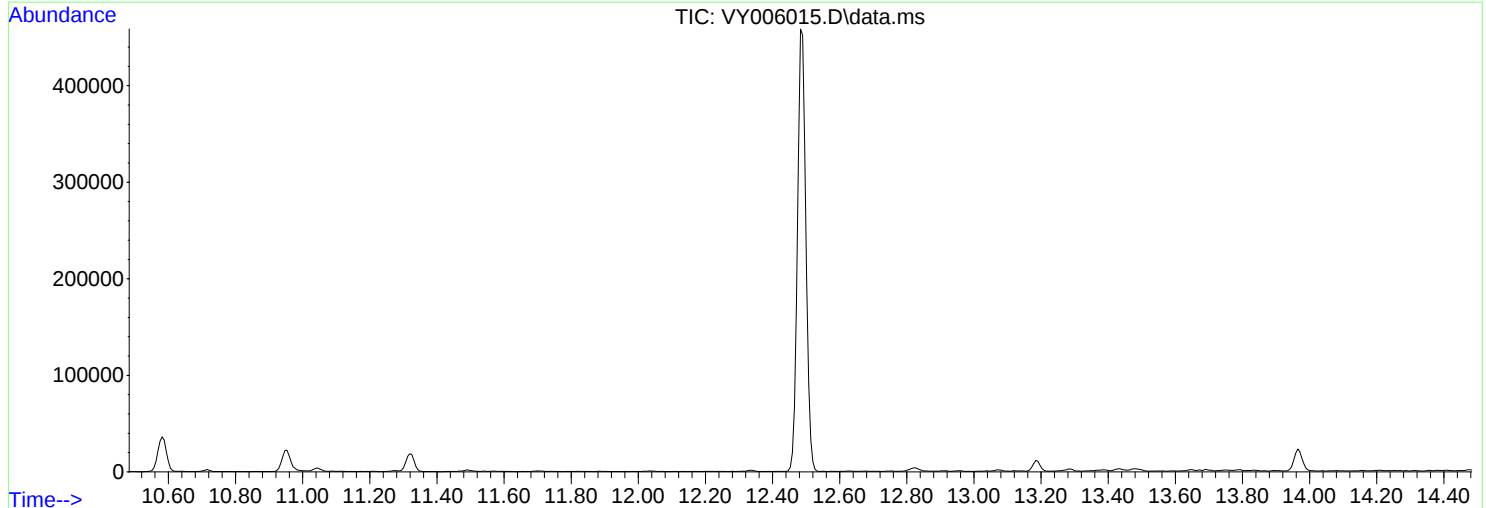

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	15172	PASS
75	95	30	60	57.0	36115	PASS
95	95	100	100	100.0	63315	PASS
96	95	5	9	6.9	4383	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.9	53736	PASS
175	174	5	9	8.1	4378	PASS
176	174	95	101	98.7	53032	PASS
177	176	5	9	7.4	3929	PASS