

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092024\
 Data File : VY019642.D
 Acq On : 20 Sep 2024 13:49
 Operator : SY/MD
 Sample : P4098-03
 Misc : 5.08g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Sep 20 15:23:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090924S.M
 Quant Title : SW846 8260
 QLast Update : Mon Sep 09 16:00:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.701	168	14509	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.616	114	25164	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	17026	50.000	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	13.341	152	3351	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	6549	48.746	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	97.500%
35) Dibromofluoromethane	7.628	113	6886	48.263	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	96.520%
50) Toluene-d8	10.103	98	27145	51.438	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	102.880%
62) 4-Bromofluorobenzene	12.402	95	5620	27.697	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	55.400%


Target Compounds			Qvalue			
3) Chloromethane	2.074	50	351	2.924	ug/l	94
5) Bromomethane	2.617	94	292	3.662	ug/l #	63
10) Methyl Iodide	4.013	142	288	1.678	ug/l #	92
11) Tert butyl alcohol	4.836	59	52	4.793	ug/l #	1
13) Acrolein	3.629	56	40	Below Cal	#	15
15) Acrylonitrile	5.049	53	85	2.714	ug/l #	18
16) Acetone	3.867	43	463	14.466	ug/l #	36
18) Methyl Acetate	4.373	43	114	1.312	ug/l #	46
20) Methylene Chloride	4.610	84	309	2.117	ug/l #	65
25) 2-Butanone	6.872	43	223	4.899	ug/l #	41
26) 2,2-Dichloropropane	6.872	77	364	1.517	ug/l #	51
31) Cyclohexane	7.707	56	552	2.296	ug/l #	34
36) 1,1-Dichloropropene	7.701	75	1301	6.701	ug/l #	49
38) Carbon Tetrachloride	7.713	117	1542	7.043	ug/l #	13
41) Methacrylonitrile	7.244	41	63	1.086	ug/l #	15
51) 4-Methyl-2-Pentanone	9.994	43	225	2.140	ug/l #	44
59) 2-Hexanone	10.749	43	220	2.854	ug/l #	19
74) N-amyl acetate	12.085	43	139	2.102	ug/l #	20
75) 1,1,2,2-Tetrachloroethane	12.438	83	48	1.112	ug/l #	83
76) 1,2,3-Trichloropropane	12.408	75	3128	99.591	ug/l #	100
78) n-propylbenzene	12.664	91	354	1.229	ug/l	98
80) 1,3,5-Trimethylbenzene	12.737	105	765	3.871	ug/l	93
81) trans-1,4-Dichloro-2-b...	12.408	75	3128	191.185	ug/l #	16
82) 4-Chlorotoluene	12.786	91	292	1.691	ug/l #	39
83) tert-Butylbenzene	13.237	119	326	1.822	ug/l	93
84) 1,2,4-Trimethylbenzene	13.042	105	1591	8.133	ug/l	90
85) sec-Butylbenzene	13.170	105	599	2.305	ug/l	86
86) p-Isopropyltoluene	13.286	119	261	1.227	ug/l #	37
89) n-Butylbenzene	13.621	91	476	2.341	ug/l #	79
90) Hexachloroethane	13.889	117	79	1.785	ug/l #	12
92) 1,2-Dibromo-3-Chloropr...	14.164	75	24	3.337	ug/l #	1
95) Naphthalene	15.151	128	594	5.216	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092024\
Data File : VY019642.D
Acq On : 20 Sep 2024 13:49
Operator : SY/MD
Sample : P4098-03
Misc : 5.08g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :

Quant Time: Sep 20 15:23:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090924S.M
Quant Title : SW846 8260
QLast Update : Mon Sep 09 16:00:30 2024
Response via : Initial Calibration




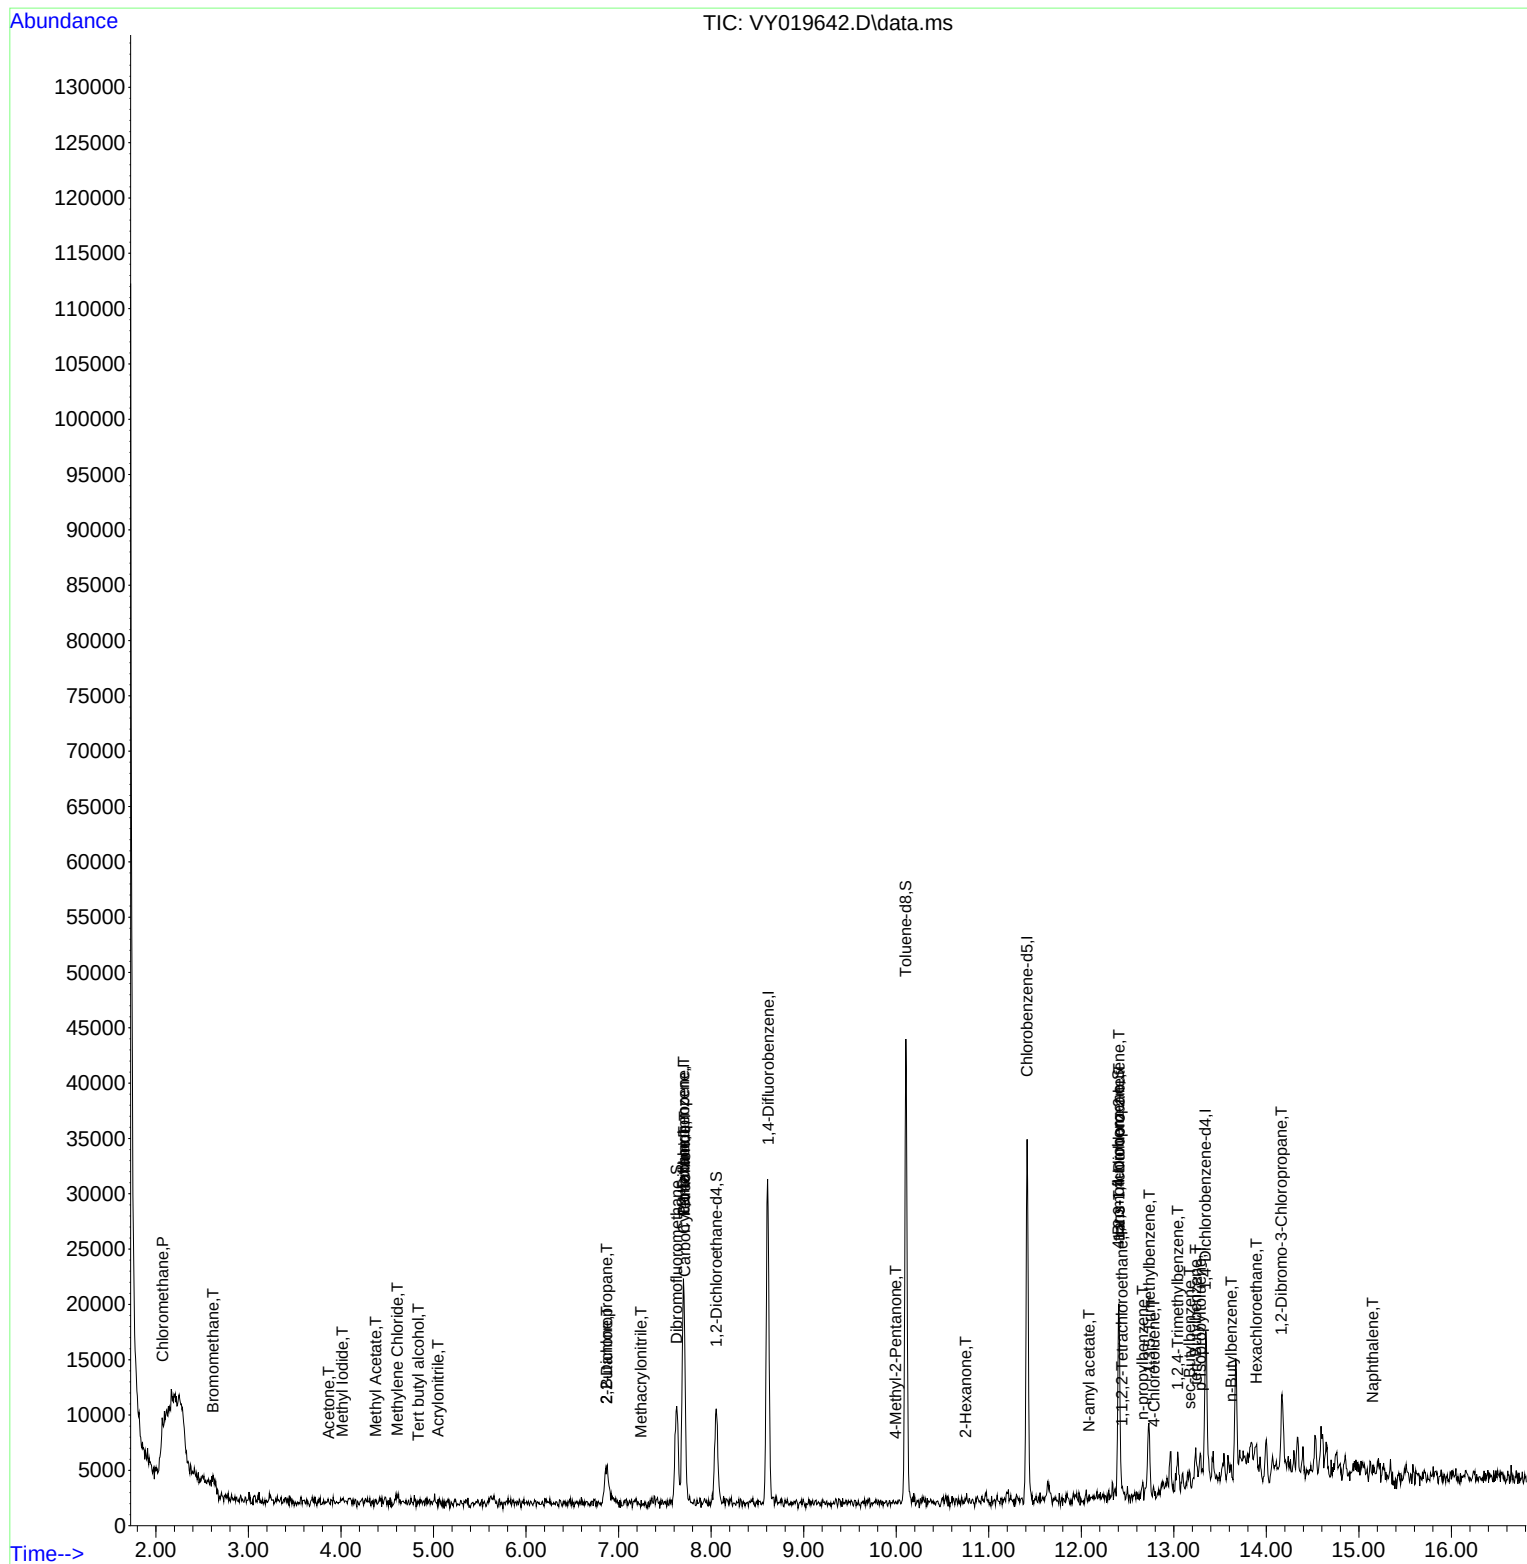




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.701 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:168 Resp: 14509
Ion Ratio Lower Upper
168 100
99 71.8 39.1 58.7#

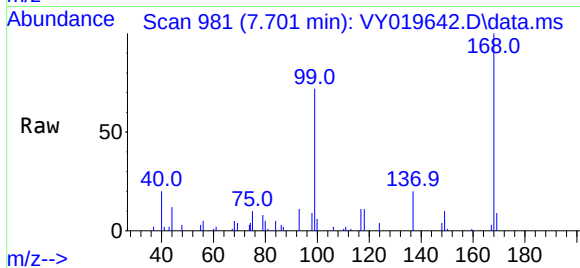

#3
Chloromethane
Concen: 2.924 ug/l
RT: 2.074 min Scan# 58
Delta R.T. 0.007 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Tgt Ion: 50 Resp: 351
Ion Ratio Lower Upper
50 100
52 35.3 25.6 38.4


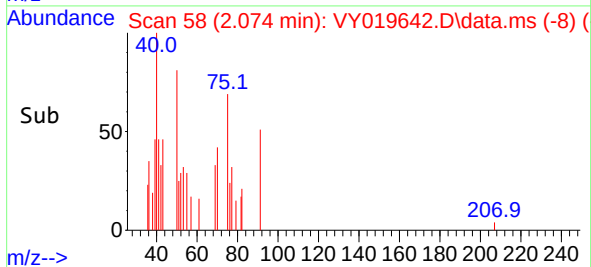

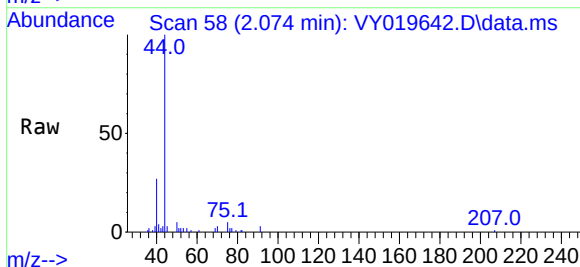


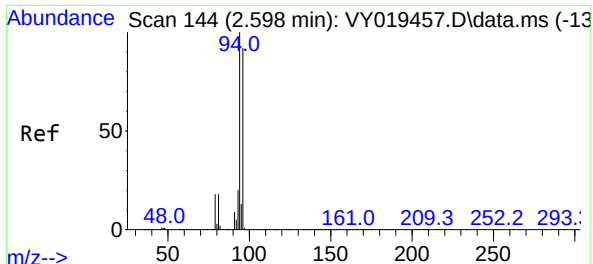

#5
Bromomethane
Concen: 3.662 ug/l
RT: 2.617 min Scan# 144
Delta R.T. 0.019 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 94 Resp: 292
Ion Ratio Lower Upper
94 100
96 56.9 74.1 111.1#

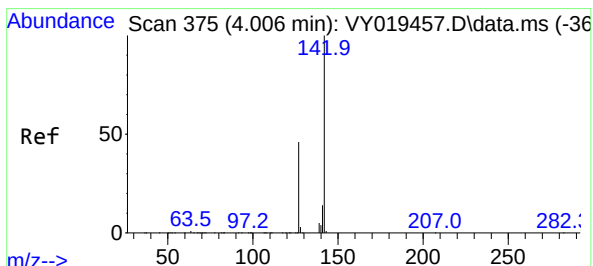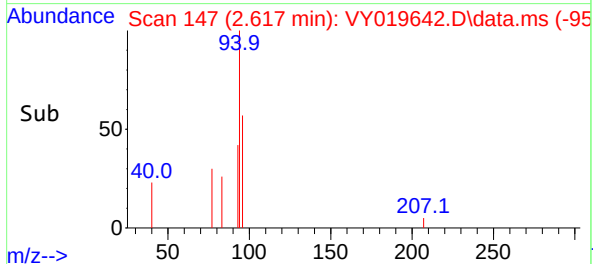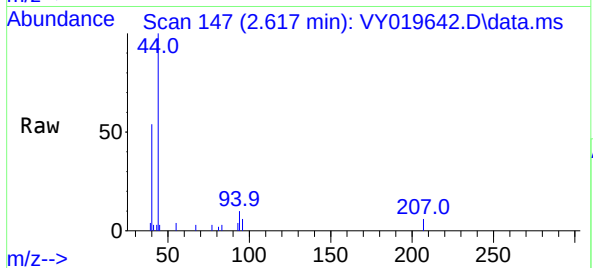

#10
Methyl Iodide
Concen: 1.678 ug/l
RT: 4.013 min Scan# 376
Delta R.T. 0.007 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Tgt Ion:142 Resp: 288
Ion Ratio Lower Upper
142 100
127 43.4 32.8 49.2
141 22.2 11.4 17.2#


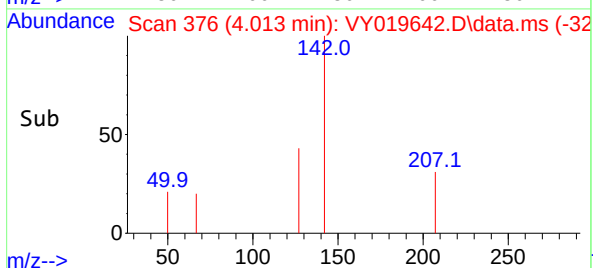

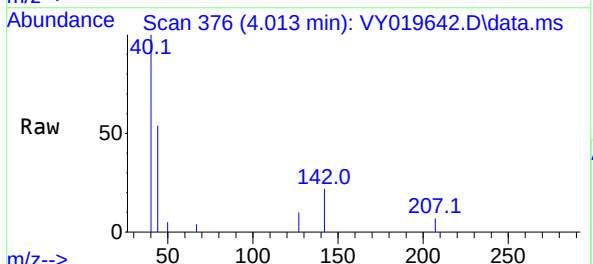




#11
Tert butyl alcohol
Concen: 4.793 ug/l
RT: 4.836 min Scan# 51
Delta R.T. -0.024 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 59 Resp: 52
Ion Ratio Lower Upper
59 100
57 44.2 3.0 4.6#

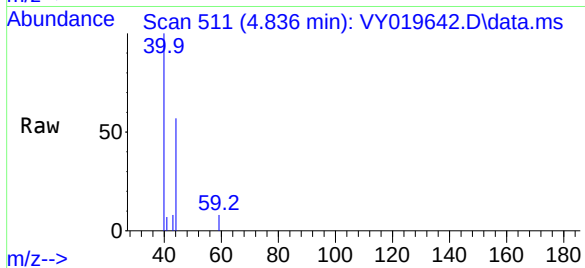

#13
Acrolein
Concen: Below Cal
RT: 3.629 min Scan# 313
Delta R.T. -0.024 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49


Tgt Ion: 56 Resp: 40
Ion Ratio Lower Upper
56 100
55 0.0 55.7 83.5#

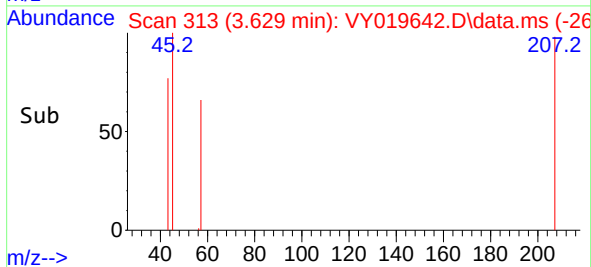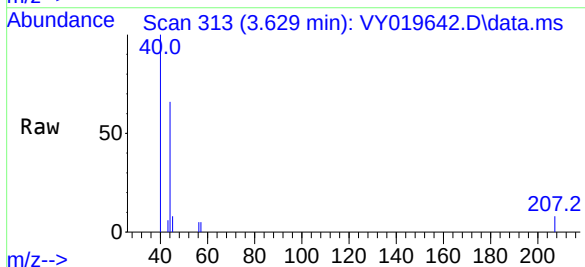






#15
Acrylonitrile
Concen: 2.714 ug/l
RT: 5.049 min Scan# 54
Delta R.T. -0.006 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion: 53 Resp: 85
Ion Ratio Lower Upper
53 100
52 0.0 64.7 97.1#
51 0.0 28.4 42.6#



#16
Acetone
Concen: 14.466 ug/l
RT: 3.867 min Scan# 352
Delta R.T. -0.006 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Tgt Ion: 43 Resp: 463
Ion Ratio Lower Upper
43 100
58 0.0 31.7 47.5#


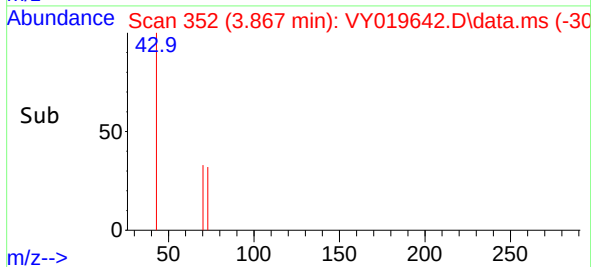

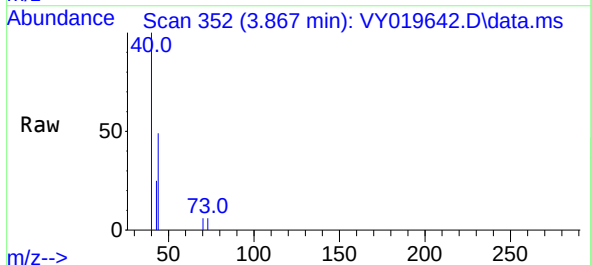




#18
Methyl Acetate
Concen: 1.312 ug/l
RT: 4.373 min Scan# 41
Delta R.T. -0.012 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 43 Resp: 114
Ion Ratio Lower Upper
43 100
74 0.0 23.3 34.9#



#20
Methylene Chloride
Concen: 2.117 ug/l
RT: 4.610 min Scan# 474
Delta R.T. -0.006 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49


Tgt Ion: 84 Resp: 309
Ion Ratio Lower Upper
84 100
49 61.2 84.4 126.6#
51 0.0 26.0 39.0#
86 54.1 49.5 74.3

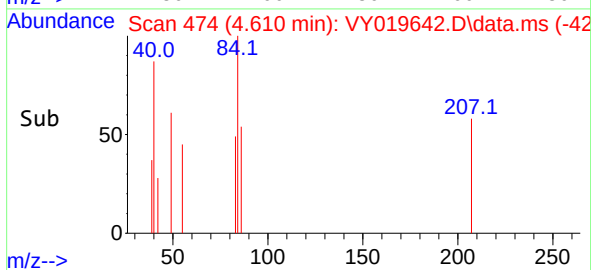



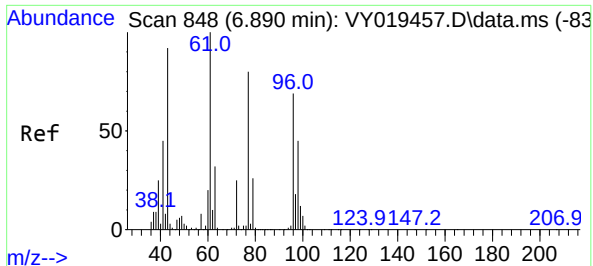


#25
2-Butanone
Concen: 4.899 ug/l
RT: 6.872 min Scan# 845
Delta R.T. -0.018 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Instrument :
MSVOA_Y
ClientSampleId :



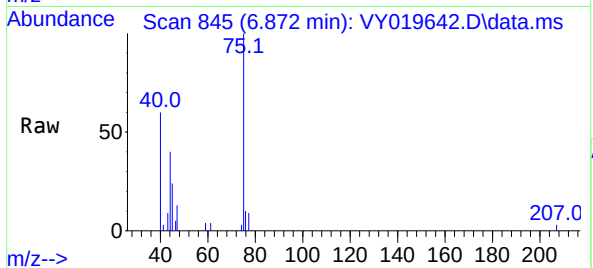



Tgt Ion: 43 Resp: 223
Ion Ratio Lower Upper
43 100
72 0.0 27.3 40.9#

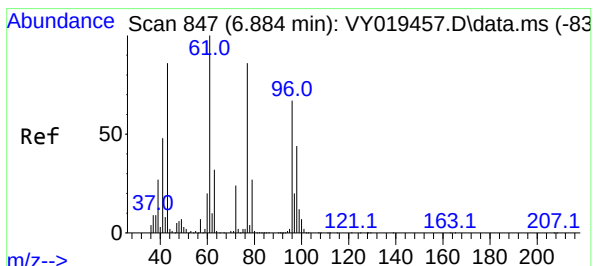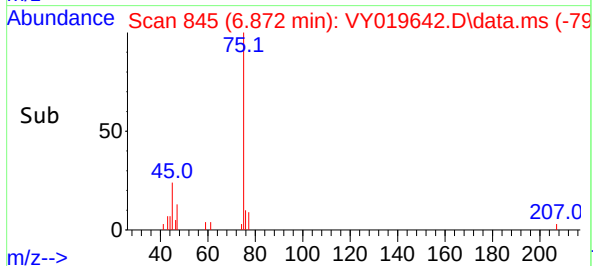

#26
2,2-Dichloropropane
Concen: 1.517 ug/l
RT: 6.872 min Scan# 845
Delta R.T. -0.012 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49


Tgt Ion: 77 Resp: 364
Ion Ratio Lower Upper
77 100
97 0.0 12.0 36.1#

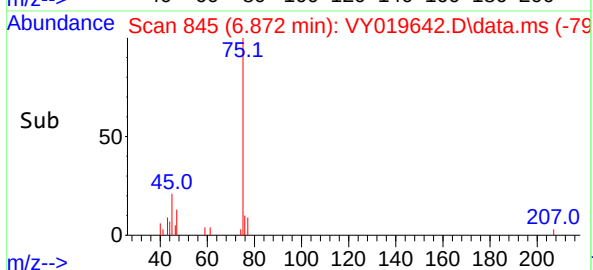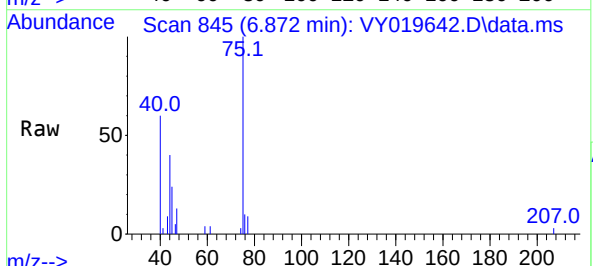






#31
Cyclohexane
Concen: 2.296 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.007 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49


Instrument :
MSVOA_Y
ClientSampleId :





Tgt Ion: 56 Resp: 552
Ion Ratio Lower Upper
56 100
69 114.6 28.7 43.1#
84 138.0 77.7 116.5#




#33
1,2-Dichloroethane-d4
Concen: 48.746 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. -0.006 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

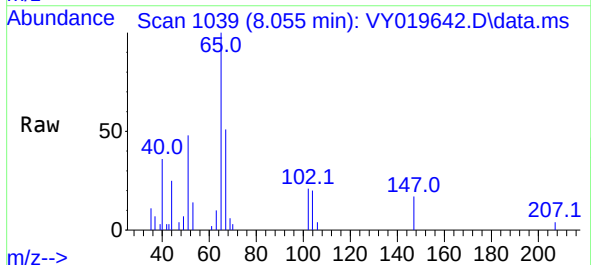

Tgt Ion: 65 Resp: 6549
Ion Ratio Lower Upper
65 100
67 54.8 0.0 109.6

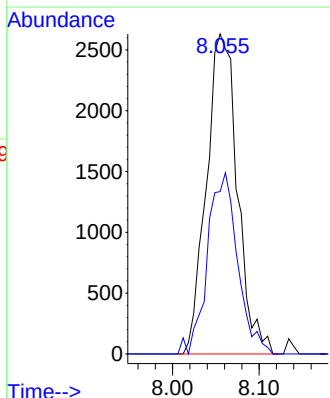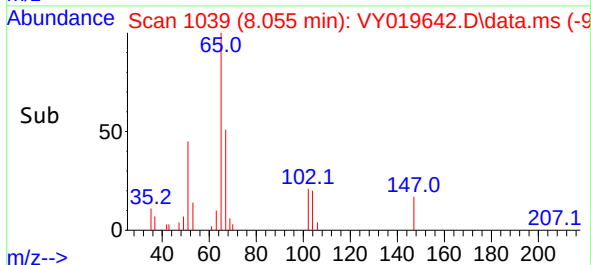



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. 0.000 min

Lab File: VY019642.D





Acq: 20 Sep 2024 13:49

Instrument :

MSVOA_Y

ClientSampleId :

Tgt Ion:	114	Resp:	25164
Ion	Ratio	Lower	Upper
114	100		
63	17.8	0.0	35.0
88	15.1	0.0	27.2



#35

Dibromofluoromethane

Concen: 48.263 ug/l




RT: 7.628 min Scan# 969


Delta R.T. -0.006 min

Lab File: VY019642.D

Acq: 20 Sep 2024 13:49

Tgt Ion:	113	Resp:	6886
Ion	Ratio	Lower	Upper
113	100		
111	102.1	82.2	123.4
192	19.6	15.9	23.9


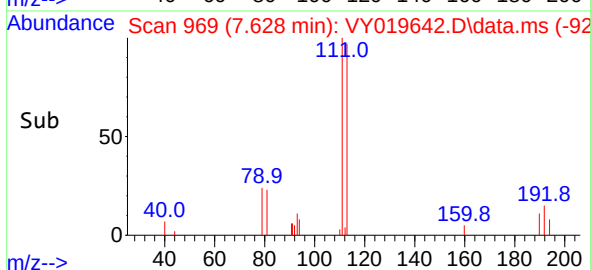




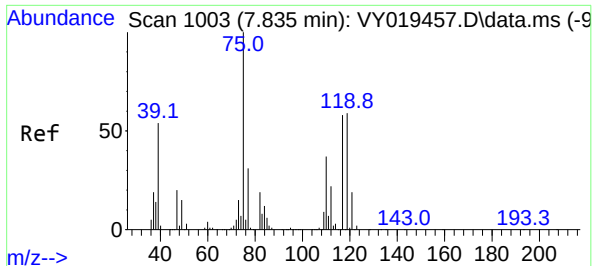

#36
1,1-Dichloropropene
Concen: 6.701 ug/l
RT: 7.701 min Scan# 91
Delta R.T. -0.134 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 75 Resp: 1301
Ion Ratio Lower Upper
75 100
110 9.8 19.0 57.0#
77 0.0 25.3 37.9#

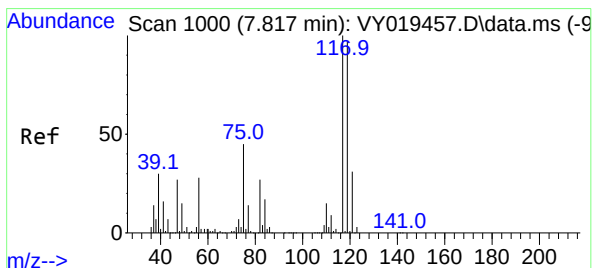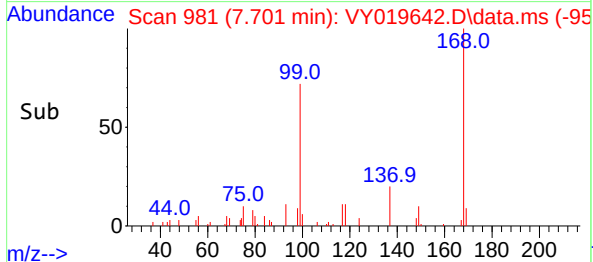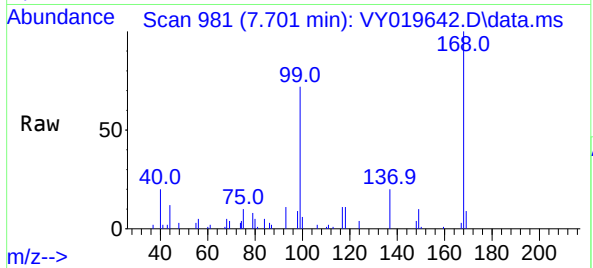

#38
Carbon Tetrachloride
Concen: 7.043 ug/l
RT: 7.713 min Scan# 983
Delta R.T. -0.103 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49


Tgt Ion: 117 Resp: 1542
Ion Ratio Lower Upper
117 100
119 0.0 75.8 113.6#
121 0.0 24.0 36.0#

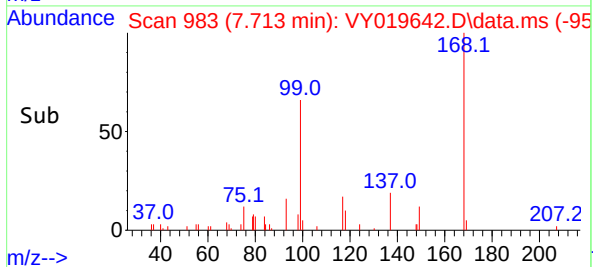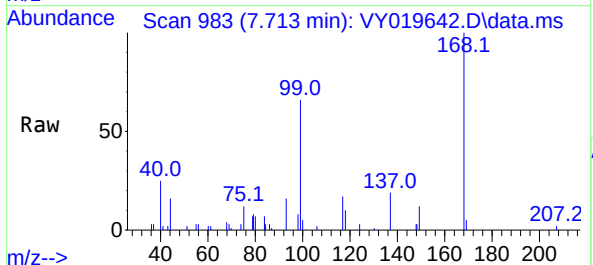






#41
Methacrylonitrile
Concen: 1.086 ug/l
RT: 7.244 min Scan# 90
Delta R.T. 0.025 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion: 41 Resp: 63
Ion Ratio Lower Upper
41 100
39 0.0 48.0 72.0#
67 0.0 75.1 112.7#
52 0.0 29.8 44.6#

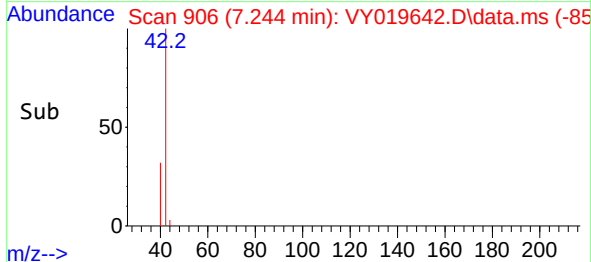

#50
Toluene-d8
Concen: 51.438 ug/l
RT: 10.103 min Scan# 1375
Delta R.T. -0.006 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Tgt Ion: 98 Resp: 27145
Ion Ratio Lower Upper
98 100
100 63.9 52.0 78.0


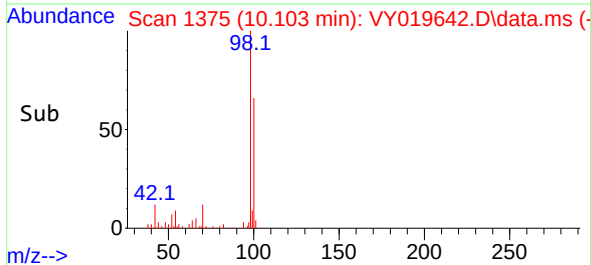

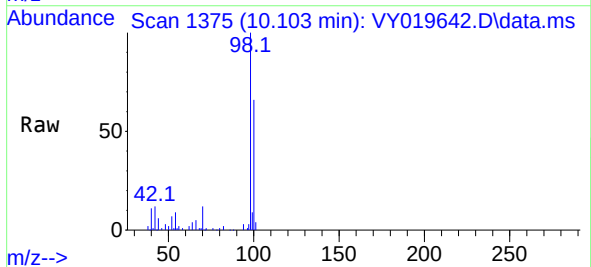


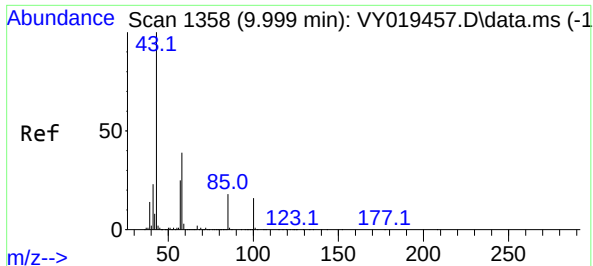

#51
4-Methyl-2-Pentanone
Concen: 2.140 ug/l
RT: 9.994 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 43 Resp: 225
Ion Ratio Lower Upper
43 100
58 8.4 35.7 53.5#

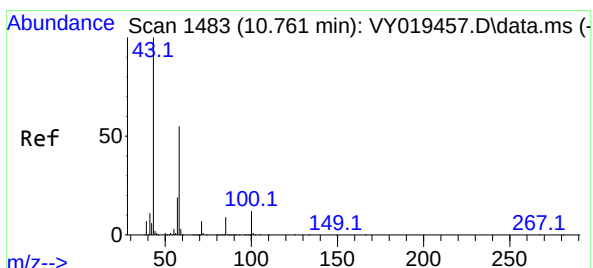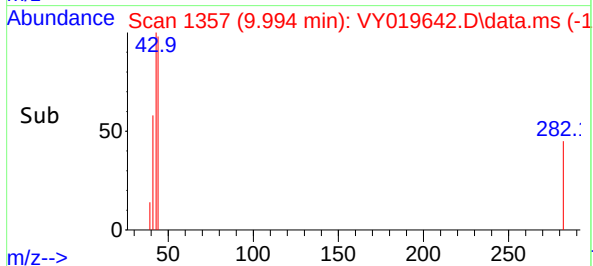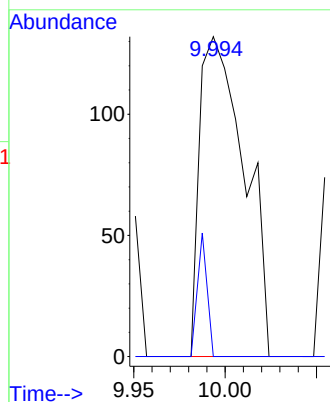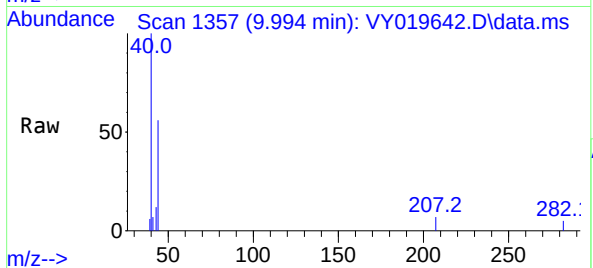

#59
2-Hexanone
Concen: 2.854 ug/l
RT: 10.749 min Scan# 1481
Delta R.T. -0.012 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Tgt Ion: 43 Resp: 220
Ion Ratio Lower Upper
43 100
58 0.0 31.4 94.0#


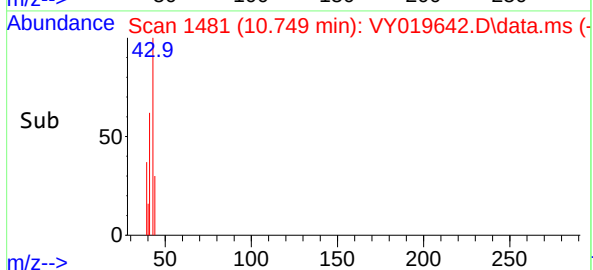

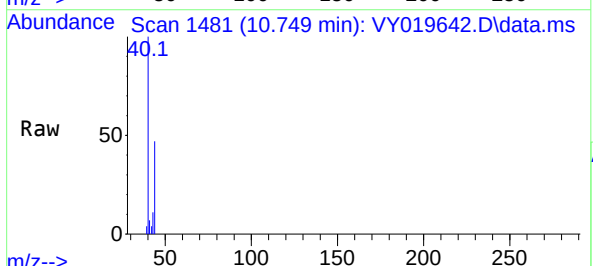




#62
4-Bromofluorobenzene
Concen: 27.697 ug/l
RT: 12.402 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 95 Resp: 5620
Ion Ratio Lower Upper
95 100
174 70.9 0.0 175.6
176 73.8 0.0 171.4

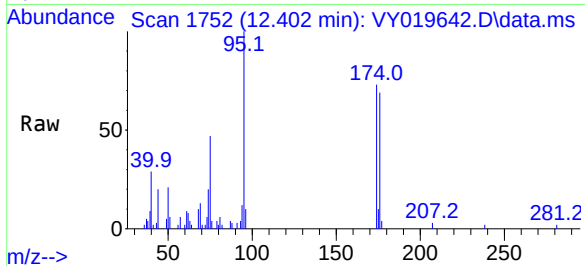

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 1590
Delta R.T. -0.006 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Tgt Ion: 117 Resp: 17026
Ion Ratio Lower Upper
117 100
82 64.0 42.4 63.6#
119 32.6 25.9 38.9


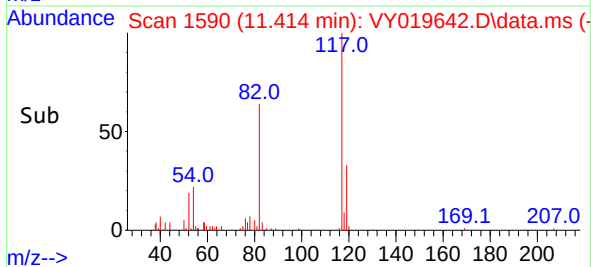

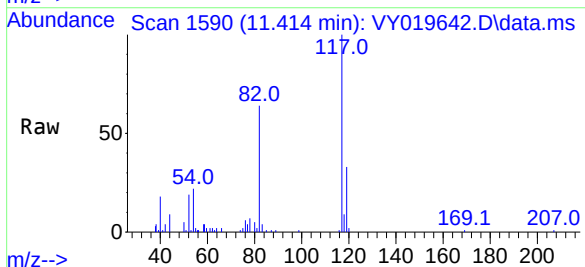




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.341 min Scan# 1907
Delta R.T. -0.006 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:152 Resp: 3351
Ion Ratio Lower Upper
152 100
115 58.4 28.2 84.7
150 154.2 0.0 345.6

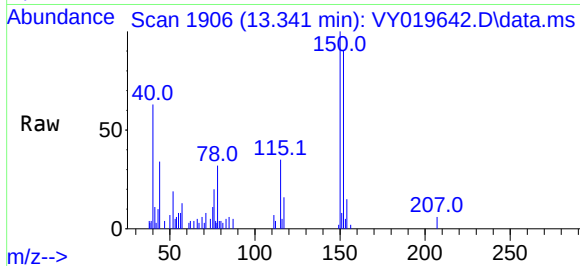

#74
N-ethyl acetate
Concen: 2.102 ug/l
RT: 12.085 min Scan# 1700
Delta R.T. 0.013 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Tgt Ion: 43 Resp: 139
Ion Ratio Lower Upper
43 100
70 0.0 41.4 62.2#
55 91.4 23.3 34.9#
61 0.0 22.6 33.8#


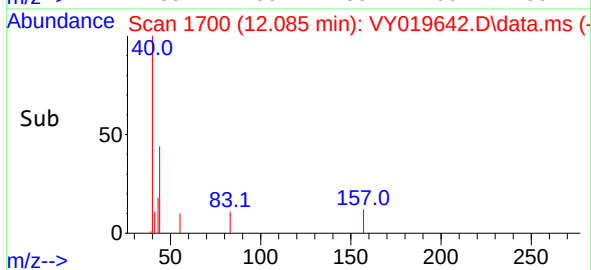

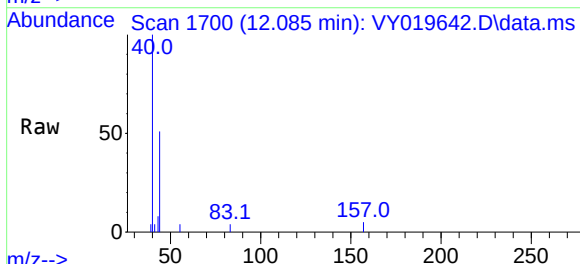




#75
1,1,2,2-Tetrachloroethane
Concen: 1.112 ug/l
RT: 12.438 min Scan# 1753
Delta R.T. -0.073 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 83 Resp: 48
Ion Ratio Lower Upper
83 100
131 0.0 5.0 14.9#
85 52.1 32.0 96.0

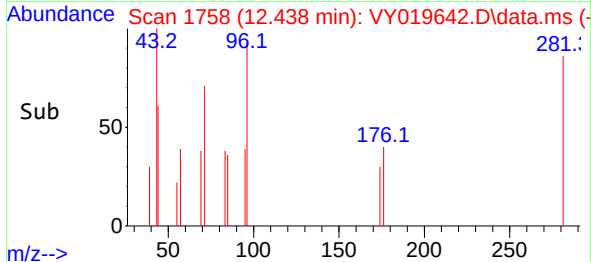

#76
1,2,3-Trichloropropane
Concen: 99.591 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. -0.152 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Tgt Ion: 75 Resp: 3128
Ion Ratio Lower Upper
75 100
77 0.0 0.0 0.0


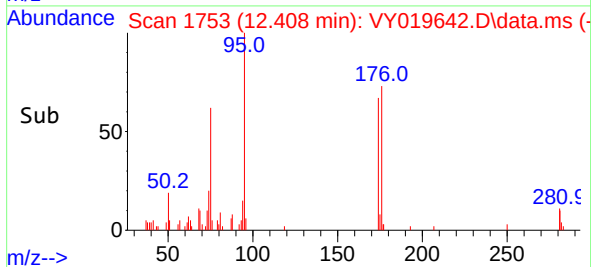

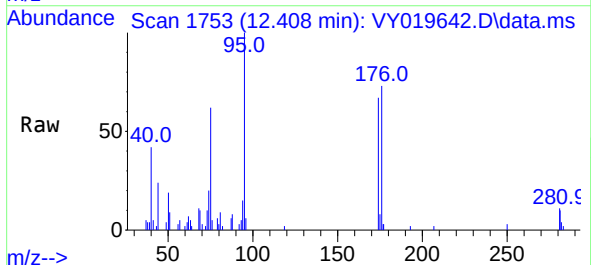




#78
n-propylbenzene
Concen: 1.229 ug/l
RT: 12.664 min Scan# 1784
Delta R.T. 0.068 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 91 Resp: 354
Ion Ratio Lower Upper
91 100
120 21.8 11.5 34.4

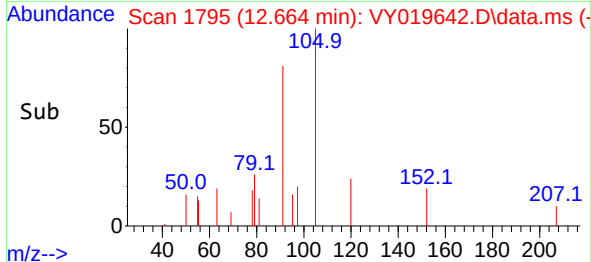

#80
1,3,5-Trimethylbenzene
Concen: 3.871 ug/l
RT: 12.737 min Scan# 1807
Delta R.T. 0.000 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Tgt Ion: 105 Resp: 765
Ion Ratio Lower Upper
105 100
120 45.1 25.1 75.2


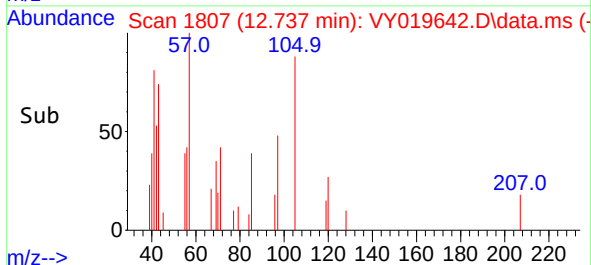
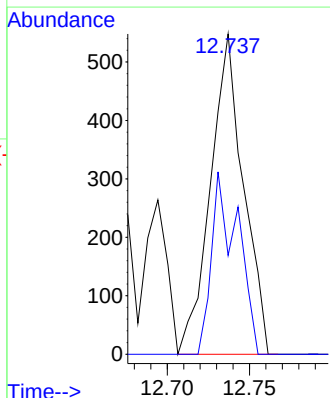
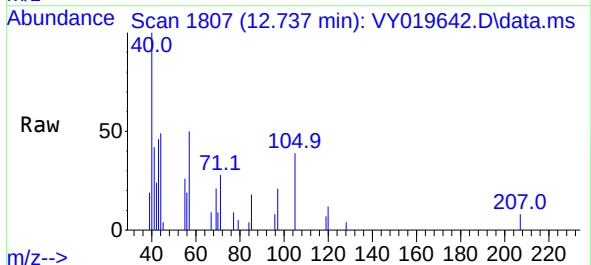




#81
trans-1,4-Dichloro-2-butene
Concen: 191.185 ug/l
RT: 12.408 min Scan# 11
Delta R.T. 0.104 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 75 Resp: 3128
Ion Ratio Lower Upper
75 100
53 0.0 66.8 100.2#
89 0.0 35.8 53.6#

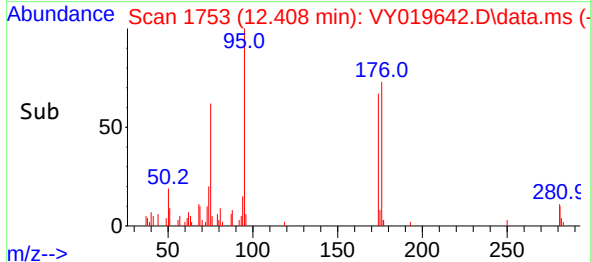

#82
4-Chlorotoluene
Concen: 1.691 ug/l
RT: 12.786 min Scan# 1815
Delta R.T. 0.007 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Tgt Ion: 91 Resp: 292
Ion Ratio Lower Upper
91 100
126 0.0 17.6 52.9#


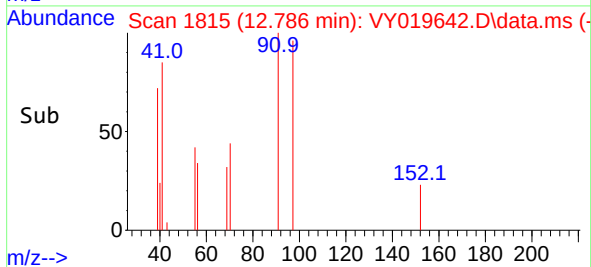

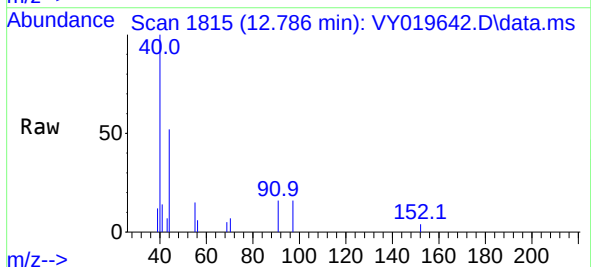




#83
tert-Butylbenzene
Concen: 1.822 ug/l
RT: 13.237 min Scan# 1889
Delta R.T. 0.238 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:	119	Resp:	326
Ion	Ratio	Lower	Upper
119	100		
91	57.4	31.3	93.8
134	30.1	13.4	40.1

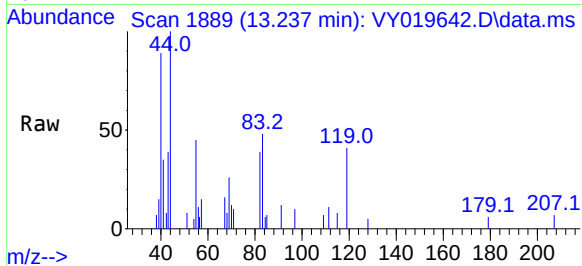

#84
1,2,4-Trimethylbenzene
Concen: 8.133 ug/l
RT: 13.042 min Scan# 1857
Delta R.T. -0.006 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Tgt Ion:	105	Resp:	1591
Ion	Ratio	Lower	Upper
105	100		
120	39.8	23.2	69.6



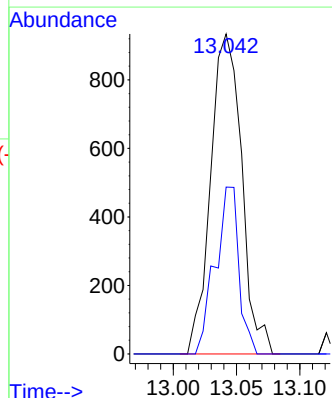
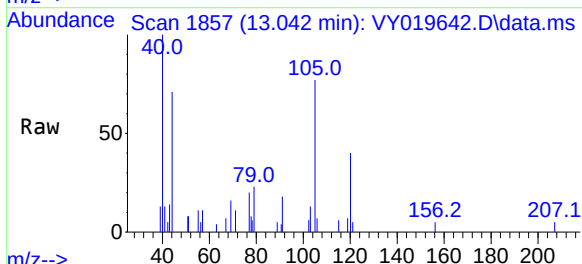




#85
sec-Butylbenzene
Concen: 2.305 ug/l
RT: 13.170 min Scan# 1879
Delta R.T. -0.006 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:105 Resp: 599
Ion Ratio Lower Upper
105 100
134 13.5 10.1 30.1



#86
p-Isopropyltoluene
Concen: 1.227 ug/l
RT: 13.286 min Scan# 1897
Delta R.T. -0.006 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Tgt Ion:119 Resp: 261
Ion Ratio Lower Upper
119 100
134 64.8 13.1 39.3#
91 43.7 10.7 32.1#

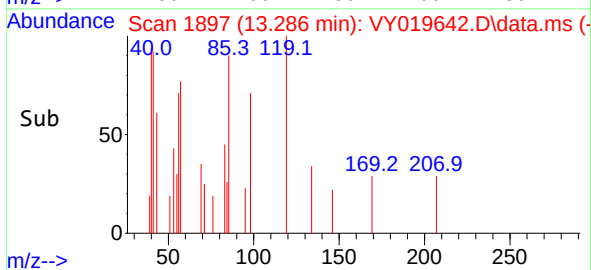



#89

n-Butylbenzene

Concen: 2.341 ug/l

RT: 13.621 min Scan# 1952

Delta R.T. 0.000 min

Lab File: VY019642.D





Acq: 20 Sep 2024 13:49

Instrument :

MSVOA_Y

ClientSampleId :

Tgt Ion:	91	Resp:	476
Ion	Ratio	Lower	Upper
91	100		
92	48.7	26.6	79.7
134	0.0	12.9	38.7#

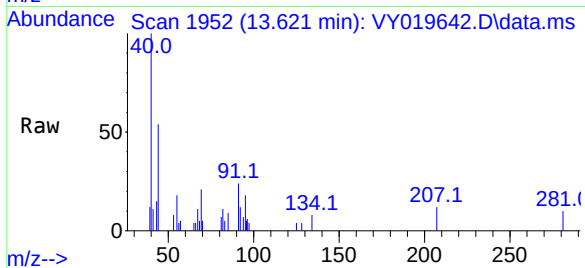

#90

Hexachloroethane

Concen: 1.785 ug/l




RT: 13.889 min Scan# 1996


Delta R.T. 0.007 min

Lab File: VY019642.D

Acq: 20 Sep 2024 13:49

Tgt Ion:	117	Resp:	79
Ion	Ratio	Lower	Upper
117	100		
201	0.0	37.4	112.2#


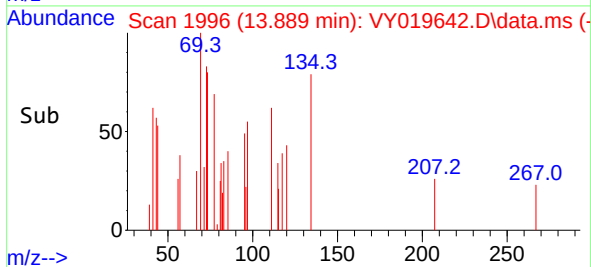

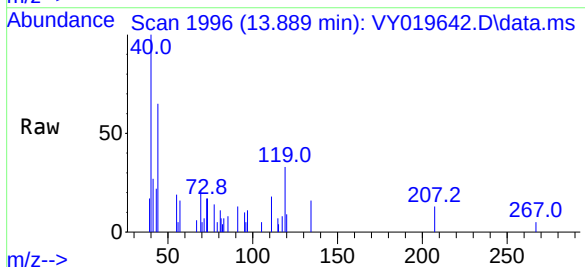




#92
1,2-Dibromo-3-Chloropropane
Concen: 3.337 ug/l
RT: 14.164 min Scan# 2059
Delta R.T. -0.109 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Instrument :
MSVOA_Y
ClientSampleId :

Tgt Ion: 75 Resp: 24
Ion Ratio Lower Upper
75 100
155 0.0 48.6 145.8#
157 0.0 62.7 188.2#



#95
Naphthalene
Concen: 5.216 ug/l
RT: 15.151 min Scan# 2203
Delta R.T. 0.007 min
Lab File: VY019642.D
Acq: 20 Sep 2024 13:49

Tgt Ion:128 Resp: 594
Ion Ratio Lower Upper
128 100
127 0.0 10.6 16.0#
129 0.0 8.6 13.0#

