
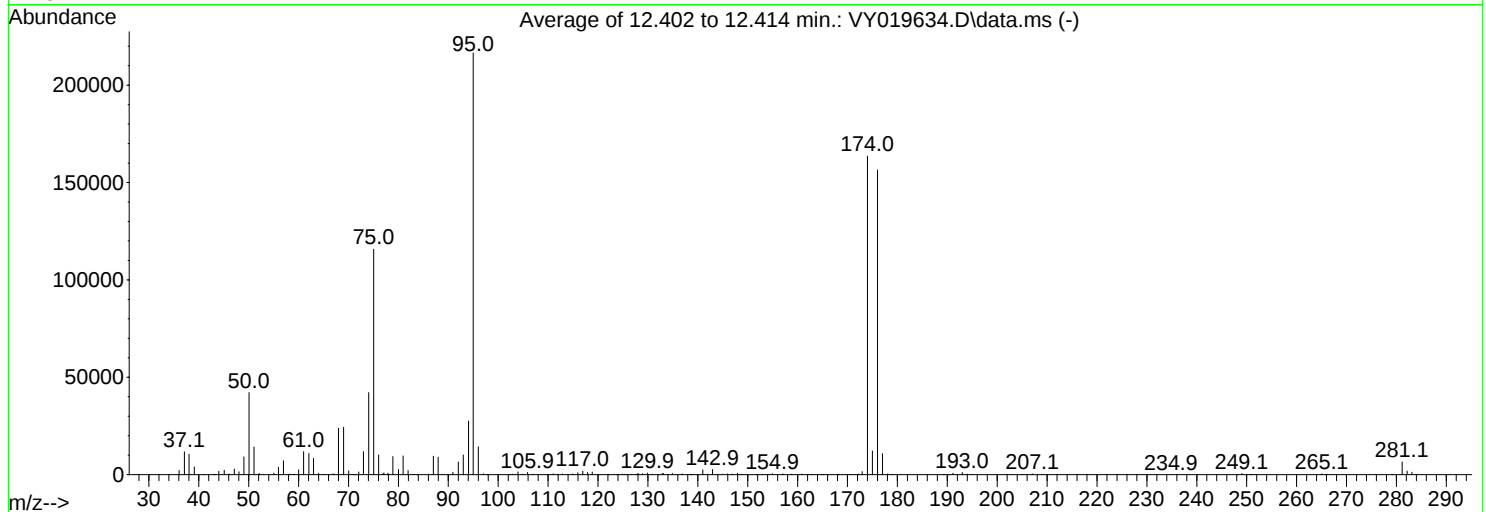


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092024\
Data File : VY019634.D
Acq On : 20 Sep 2024 08:52
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090924S.M
Title : SW846 8260
Last Update : Mon Sep 09 16:00:30 2024

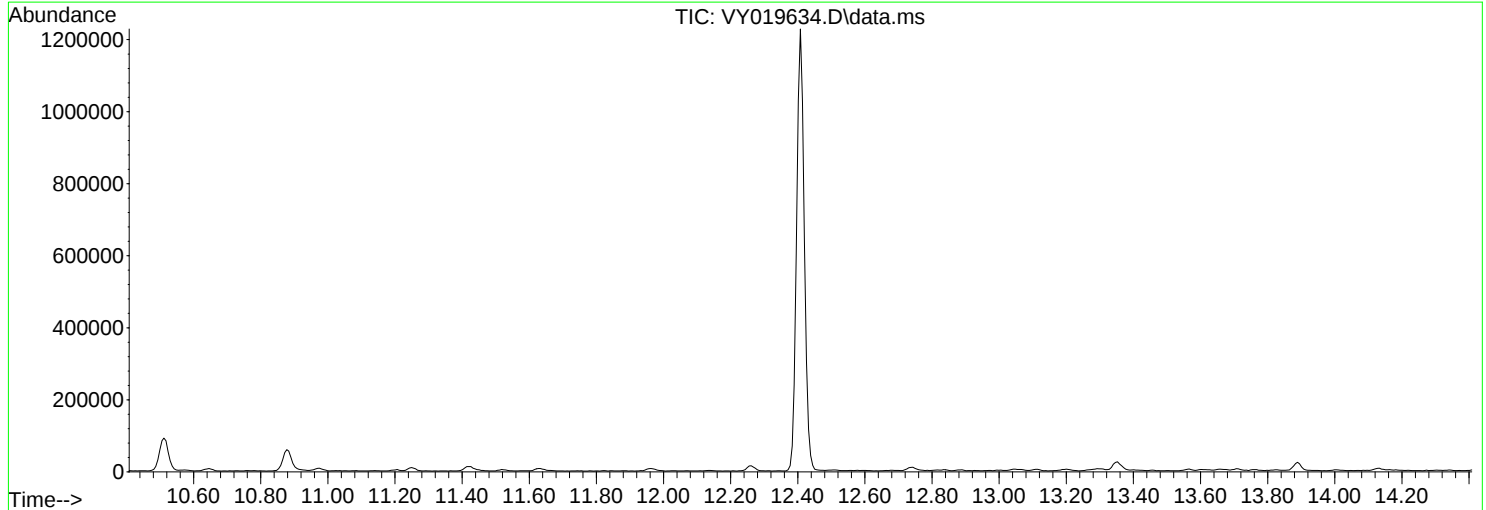

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.5	42131	PASS
75	95	30	60	53.4	115768	PASS
95	95	100	100	100.0	216597	PASS
96	95	5	9	6.6	14337	PASS
173	174	0.00	2	1.0	1588	PASS
174	95	50	100	75.5	163627	PASS
175	174	5	9	7.4	12137	PASS
176	174	95	101	95.6	156416	PASS
177	176	5	9	6.9	10790	PASS