

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092222\
 Data File : VY010630.D
 Acq On : 22 Sep 2022 18:13
 Operator : KP/MD
 Sample : N4723-09
 Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-15-6.5-7.0

Quant Time: Sep 23 09:04:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091922S.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 20 01:02:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	184674	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	354182	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	366987	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	171483	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	95834	54.255	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	108.500%
35) Dibromofluoromethane	7.716	113	87813	38.849	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	77.700%
50) Toluene-d8	10.179	98	332735	40.465	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	80.920%
62) 4-Bromofluorobenzene	12.483	95	109590	34.511	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	69.020%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092222\
Data File : VY010630.D
Acq On : 22 Sep 2022 18:13
Operator : KP/MD
Sample : N4723-09
Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-15-6.5-7.0

Quant Time: Sep 23 09:04:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091922S.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 01:02:44 2022
Response via : Initial Calibration




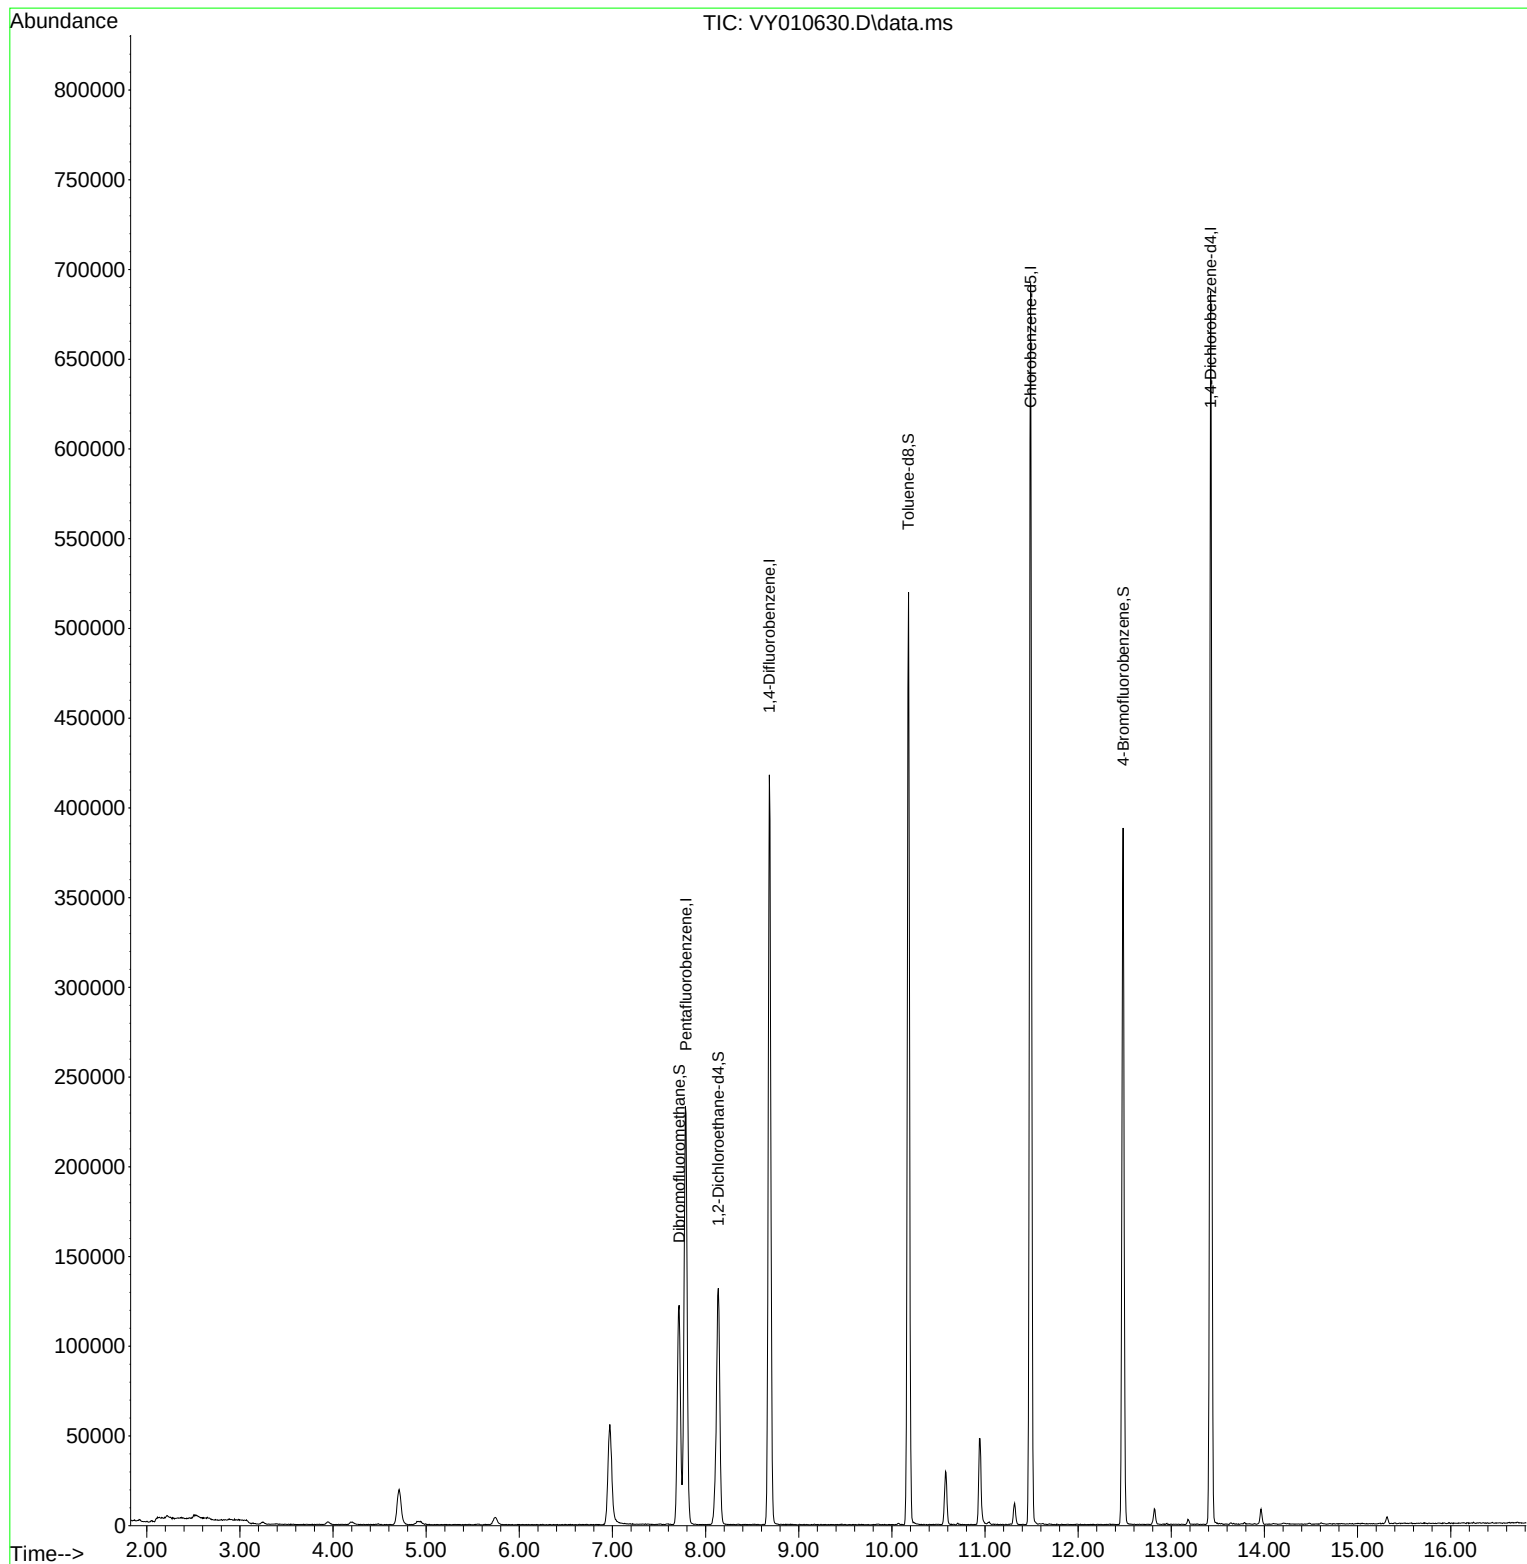


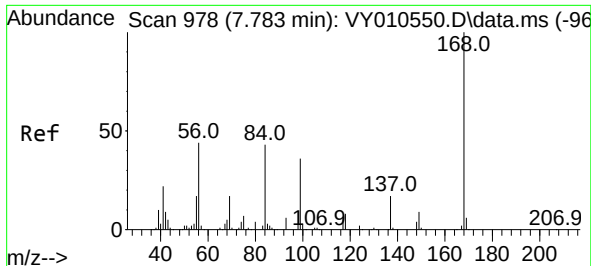

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY010630.D
Acq: 22 Sep 2022 18:13




Instrument :
MSVOA_Y
ClientSampleId :
SB-15-6.5-7.0


Tgt Ion:168 Resp: 184674
Ion Ratio Lower Upper
168 100
99 52.3 46.9 70.3

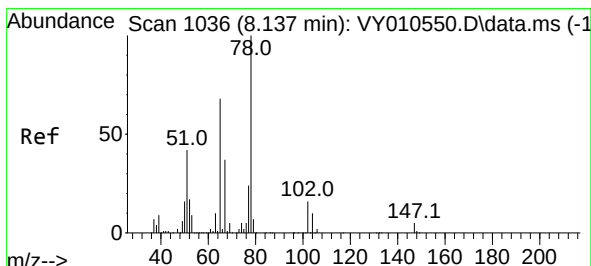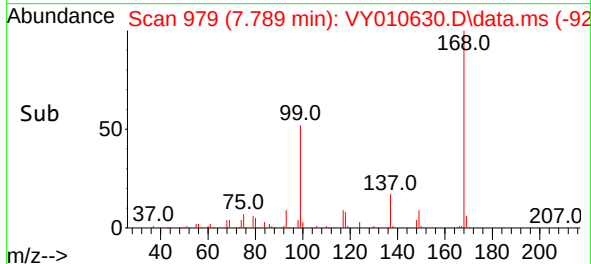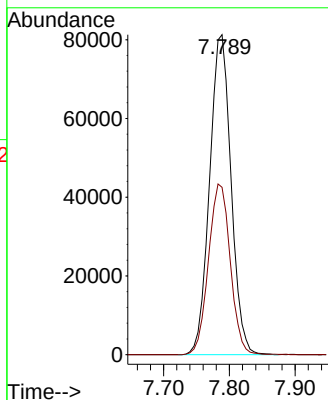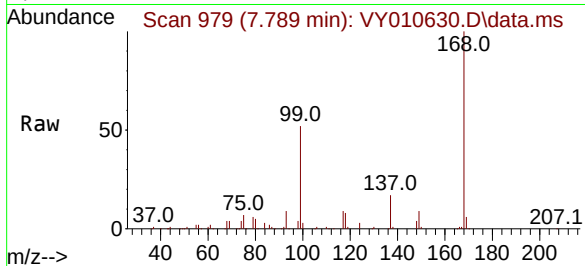

#33
1,2-Dichloroethane-d4
Concen: 54.255 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.001 min
Lab File: VY010630.D
Acq: 22 Sep 2022 18:13

Tgt Ion: 65 Resp: 95834
Ion Ratio Lower Upper
65 100
67 53.1 0.0 99.4

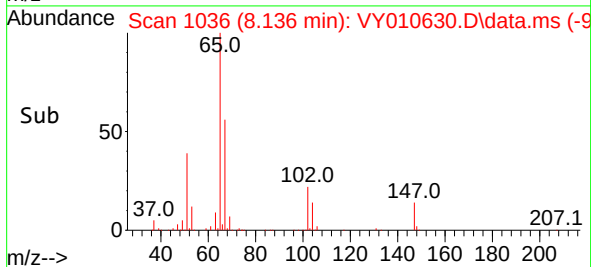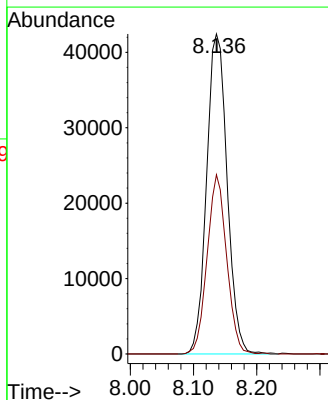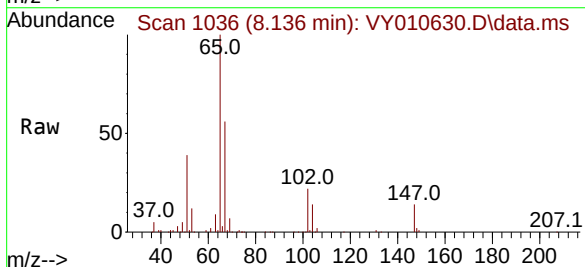

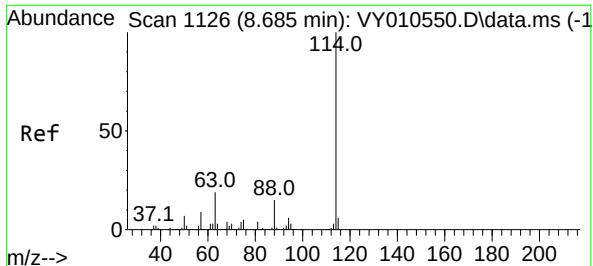

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VY010630.D

Acq: 22 Sep 2022 18:13

Instrument :

MSVOA_Y

ClientSampleId :

SB-15-6.5-7.0





Tgt Ion:114 Resp: 354182

Ion Ratio Lower Upper

114 100

63 19.0 0.0 43.2

88 15.0 0.0 31.8

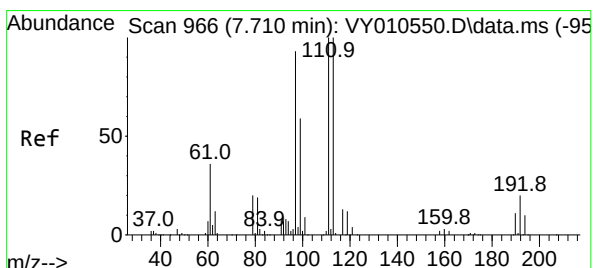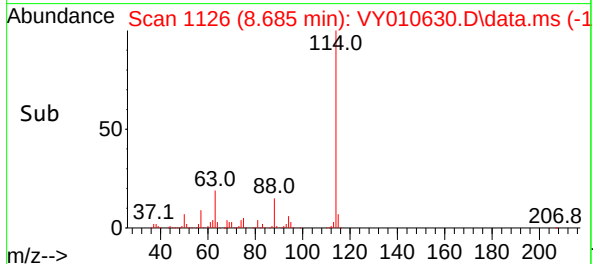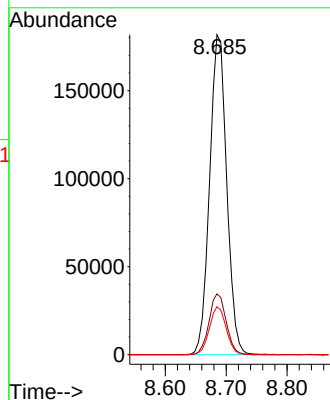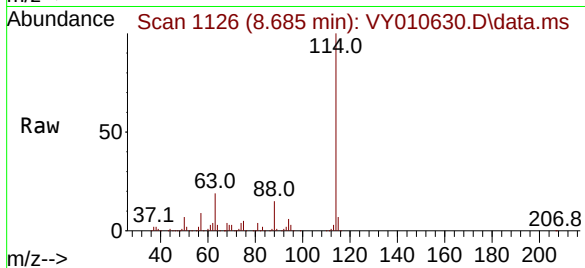

#35

Dibromofluoromethane

Concen: 38.849 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.006 min

Lab File: VY010630.D

Acq: 22 Sep 2022 18:13




Tgt Ion:113 Resp: 87813


Ion Ratio Lower Upper

113 100

111 103.0 82.6 124.0

192 19.3 17.6 26.4


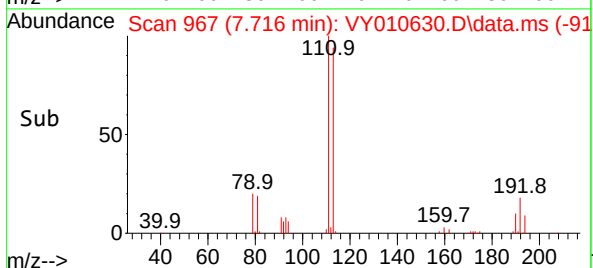
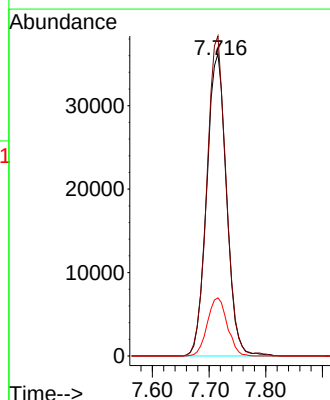
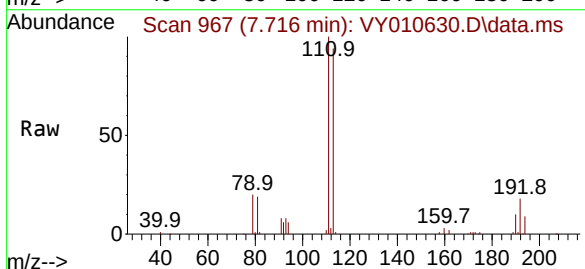


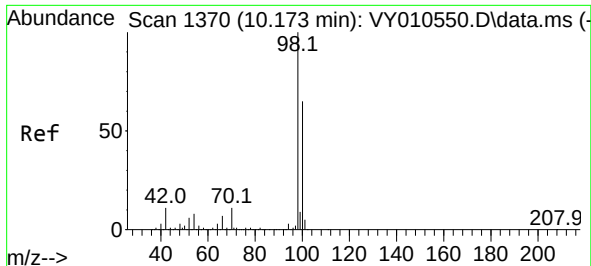

#50
Toluene-d8
Concen: 40.465 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY010630.D
Acq: 22 Sep 2022 18:13




Instrument :
MSVOA_Y
ClientSampleId :
SB-15-6.5-7.0


Tgt Ion: 98 Resp: 332735
Ion Ratio Lower Upper
98 100
100 64.6 50.2 75.2

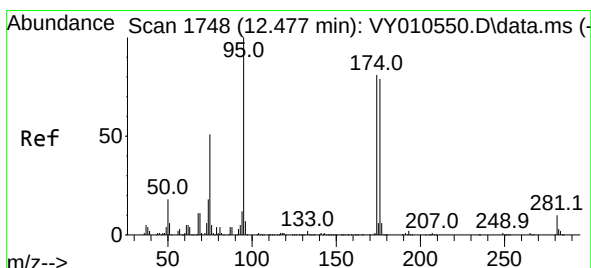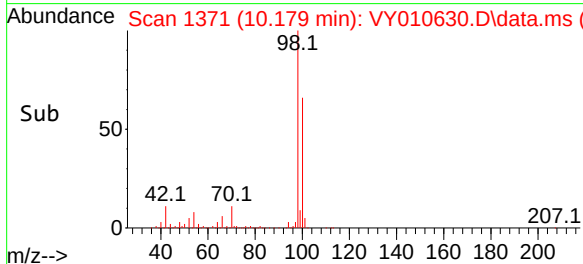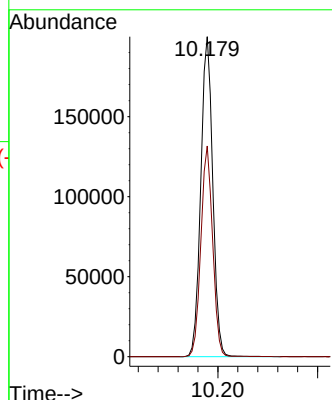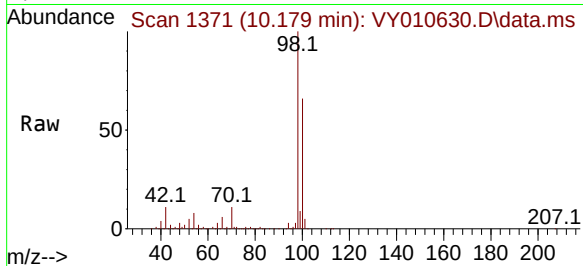

#62
4-Bromofluorobenzene
Concen: 34.511 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY010630.D
Acq: 22 Sep 2022 18:13

Tgt Ion: 95 Resp: 109590
Ion Ratio Lower Upper
95 100
174 88.3 0.0 177.0
176 83.0 0.0 175.8


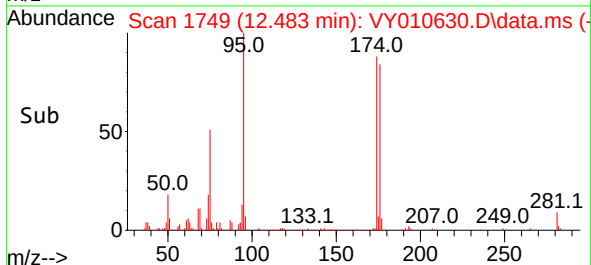
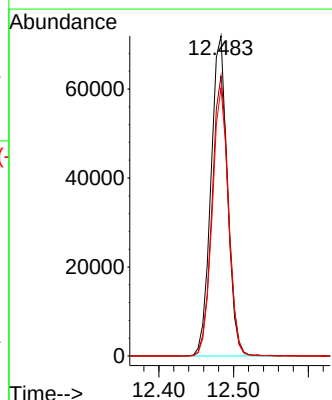
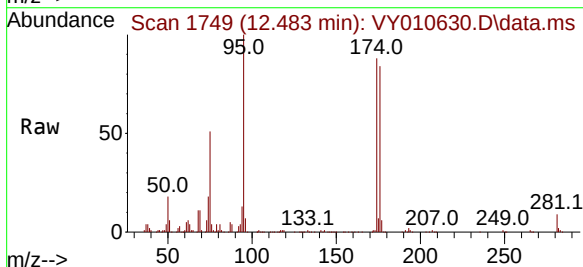


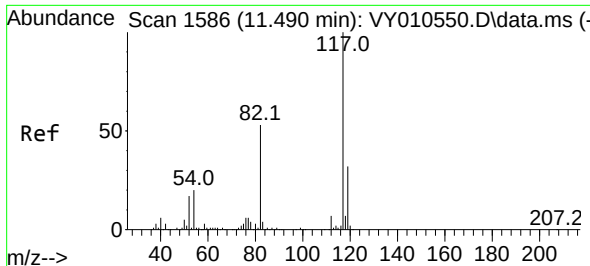

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY010630.D
Acq: 22 Sep 2022 18:13

Instrument :
MSVOA_Y
ClientSampleId :
SB-15-6.5-7.0

Tgt Ion:117 Resp: 366987
Ion Ratio Lower Upper
117 100
82 53.0 43.0 64.4
119 31.9 25.4 38.0

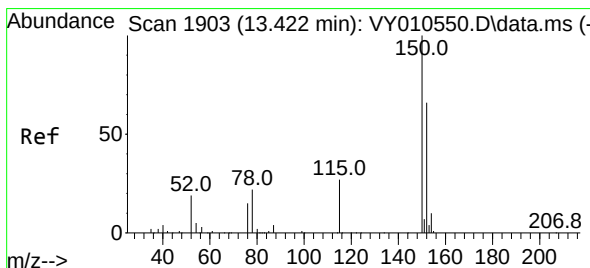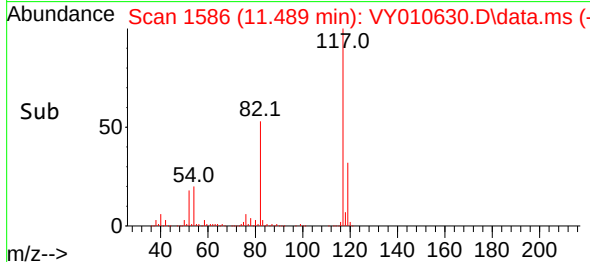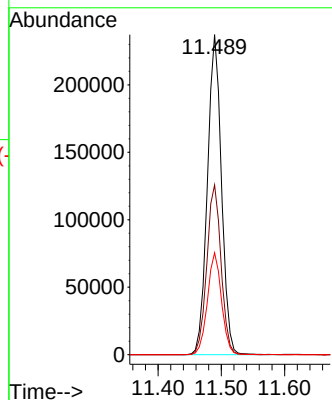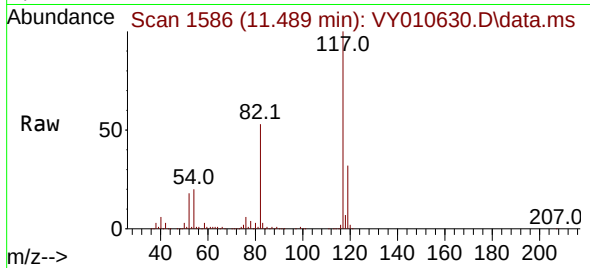

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY010630.D
Acq: 22 Sep 2022 18:13

Tgt Ion:152 Resp: 171483
Ion Ratio Lower Upper
152 100
115 57.8 28.2 84.7
150 157.0 0.0 347.6

