

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092322\
 Data File : VY010654.D
 Acq On : 23 Sep 2022 17:20
 Operator : KP/MD
 Sample : N4724-07
 Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-01-8.5-9.0

Quant Time: Sep 24 01:22:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091922S.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 20 01:02:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	199164	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	390657	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	416059	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	196888	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	95287	50.021	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	100.040%
35) Dibromofluoromethane	7.715	113	88652	35.558	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	71.120%
50) Toluene-d8	10.178	98	347635	38.494	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	76.980%
62) 4-Bromofluorobenzene	12.483	95	113737	32.304	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	64.600%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092322\
Data File : VY010654.D
Acq On : 23 Sep 2022 17:20
Operator : KP/MD
Sample : N4724-07
Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-01-8.5-9.0

Quant Time: Sep 24 01:22:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091922S.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 01:02:44 2022
Response via : Initial Calibration




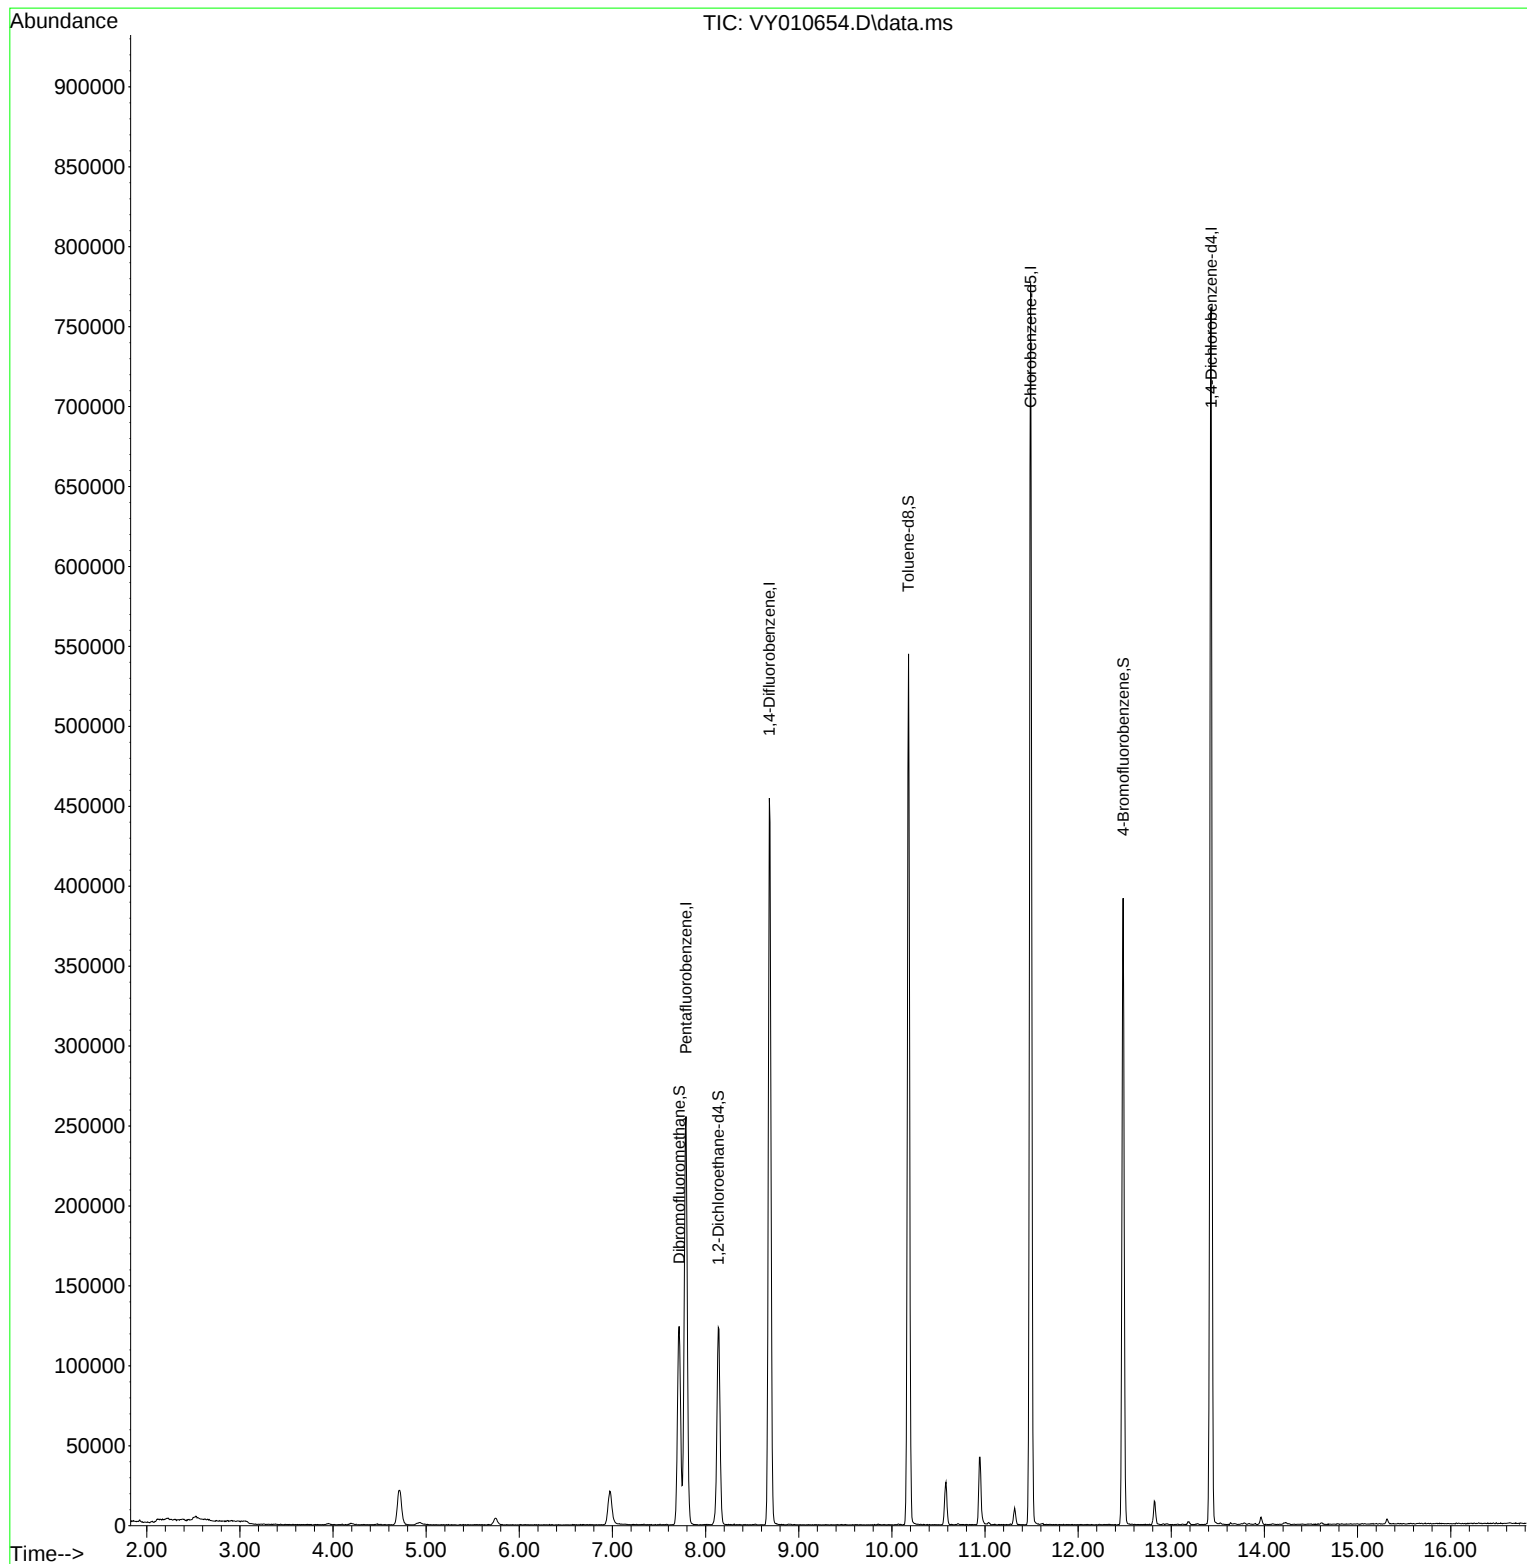


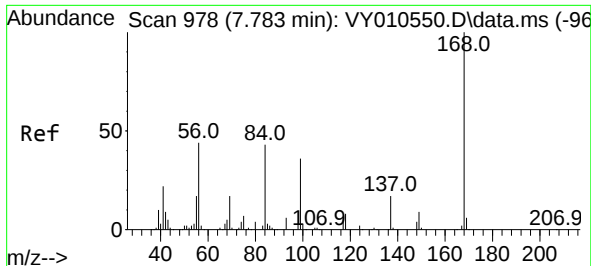

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY010654.D
Acq: 23 Sep 2022 17:20




Instrument :
MSVOA_Y
ClientSampleId :
SB-01-8.5-9.0


Tgt Ion:168 Resp: 199164
Ion Ratio Lower Upper
168 100
99 54.5 46.9 70.3

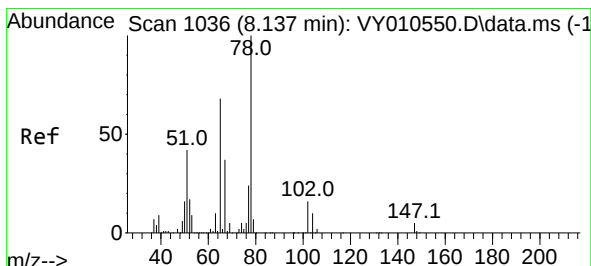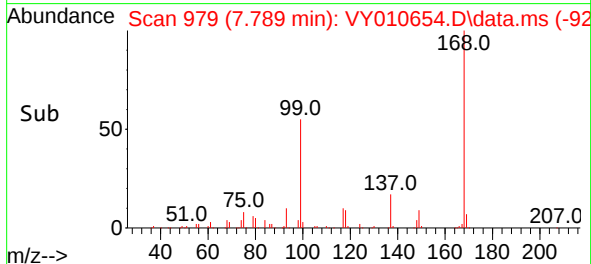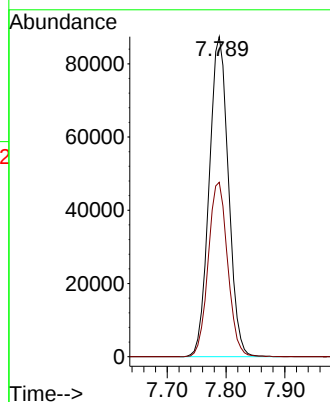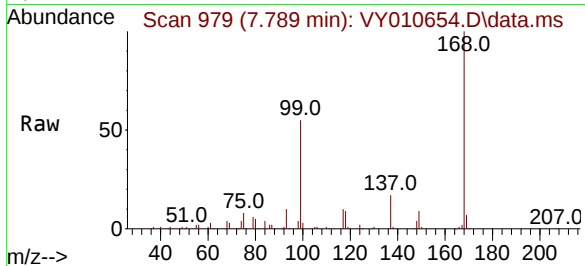

#33
1,2-Dichloroethane-d4
Concen: 50.021 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.001 min
Lab File: VY010654.D
Acq: 23 Sep 2022 17:20

Tgt Ion: 65 Resp: 95287
Ion Ratio Lower Upper
65 100
67 52.3 0.0 99.4

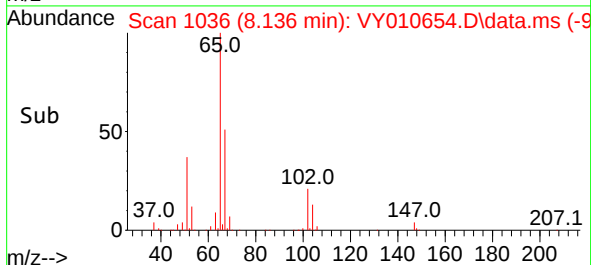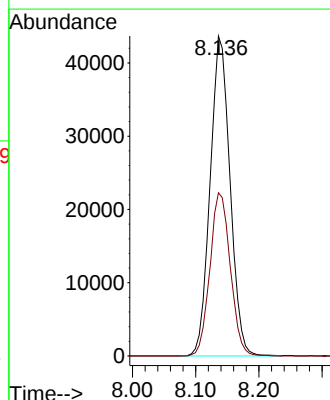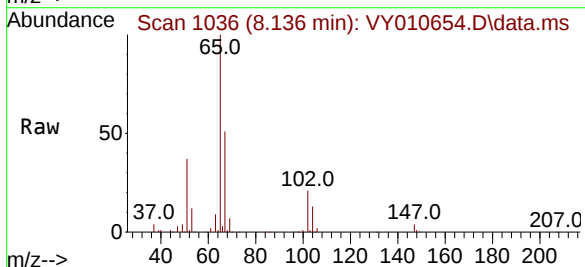

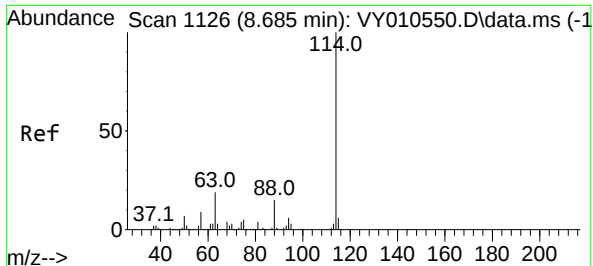

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VY010654.D

Acq: 23 Sep 2022 17:20

Instrument :

MSVOA_Y

ClientSampleId :

SB-01-8.5-9.0





Tgt Ion:114 Resp: 390657

Ion Ratio Lower Upper

114 100

63 19.7 0.0 43.2

88 14.9 0.0 31.8

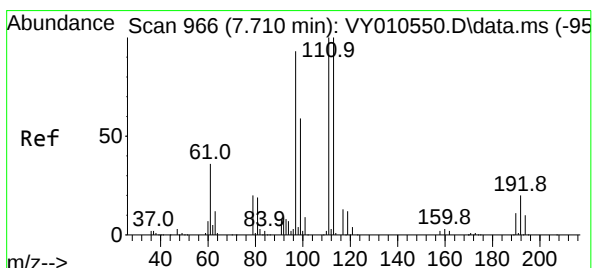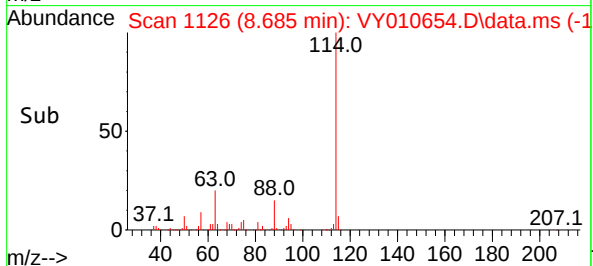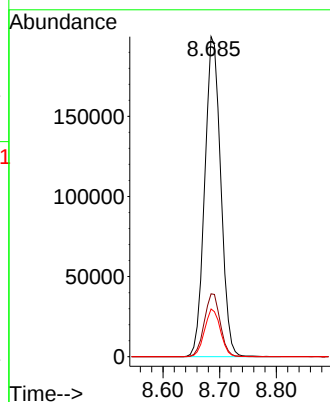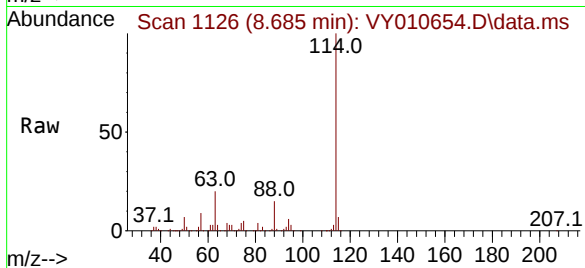

#35

Dibromofluoromethane

Concen: 35.558 ug/l

RT: 7.715 min Scan# 967

Delta R.T. 0.005 min

Lab File: VY010654.D

Acq: 23 Sep 2022 17:20




Tgt Ion:113 Resp: 88652


Ion Ratio Lower Upper

113 100

111 103.7 82.6 124.0

192 19.9 17.6 26.4


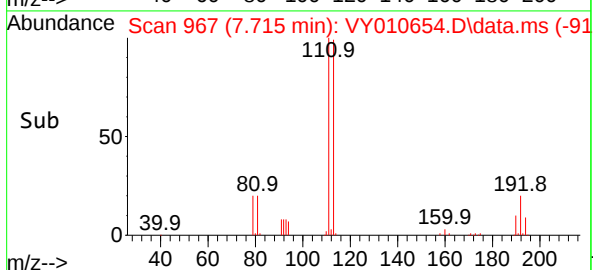
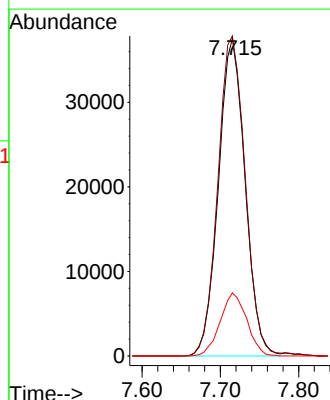
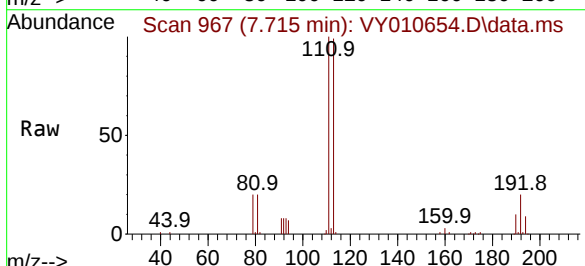


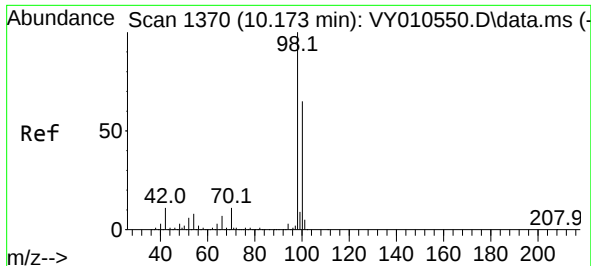

#50
Toluene-d8
Concen: 38.494 ug/l
RT: 10.178 min Scan# 11
Delta R.T. 0.005 min
Lab File: VY010654.D
Acq: 23 Sep 2022 17:20




Instrument :
MSVOA_Y
ClientSampleId :
SB-01-8.5-9.0


Tgt Ion: 98 Resp: 347635
Ion Ratio Lower Upper
98 100
100 64.9 50.2 75.2

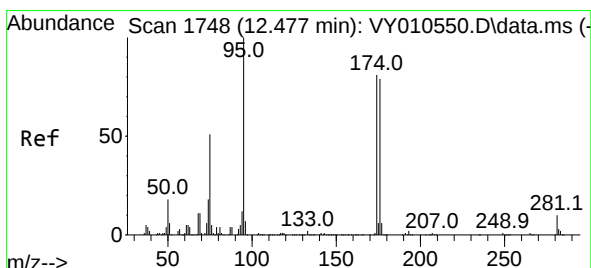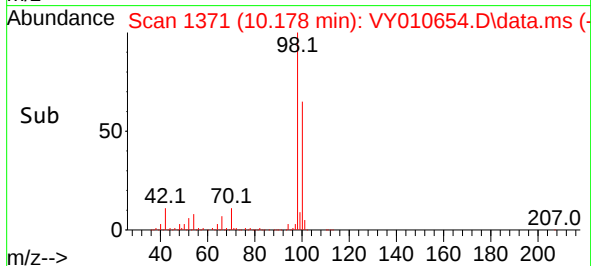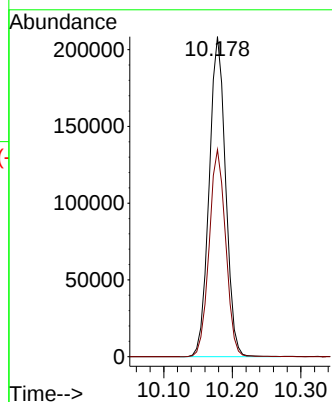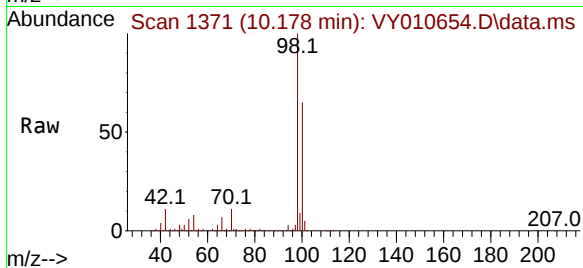

#62
4-Bromofluorobenzene
Concen: 32.304 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY010654.D
Acq: 23 Sep 2022 17:20

Tgt Ion: 95 Resp: 113737
Ion Ratio Lower Upper
95 100
174 86.1 0.0 177.0
176 82.9 0.0 175.8


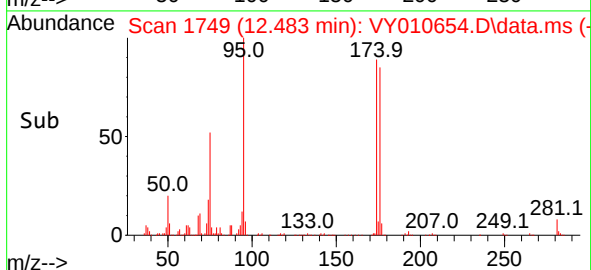
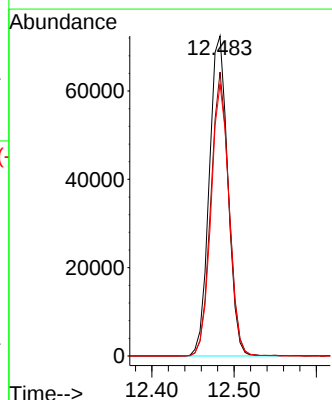
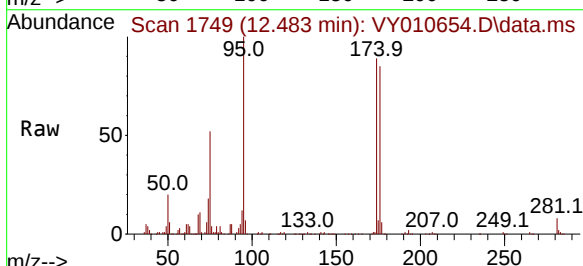


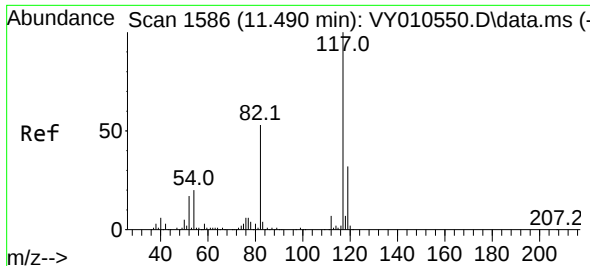

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY010654.D
Acq: 23 Sep 2022 17:20

Instrument :
MSVOA_Y
ClientSampleId :
SB-01-8.5-9.0

Tgt Ion:117 Resp: 416059
Ion Ratio Lower Upper
117 100
82 54.2 43.0 64.4
119 31.7 25.4 38.0

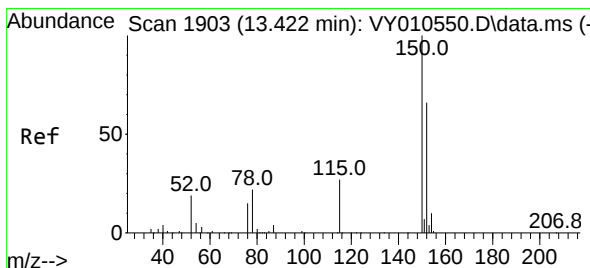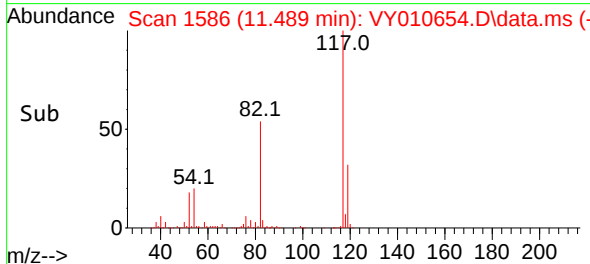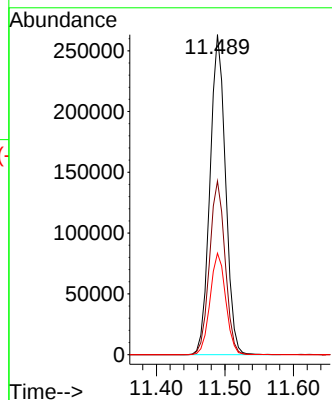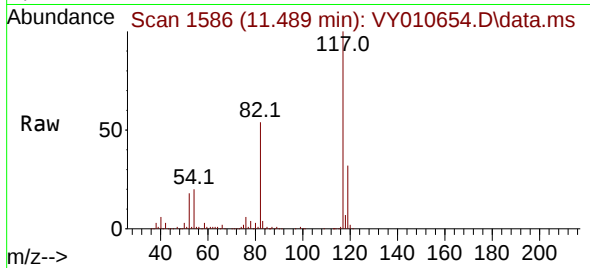

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY010654.D
Acq: 23 Sep 2022 17:20

Tgt Ion:152 Resp: 196888
Ion Ratio Lower Upper
152 100
115 57.6 28.2 84.7
150 155.8 0.0 347.6

