


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092322\
Data File : VY010637.D
Acq On : 23 Sep 2022 09:05
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091922S.M
Title : SW846 8260
Last Update : Tue Sep 20 01:02:44 2022

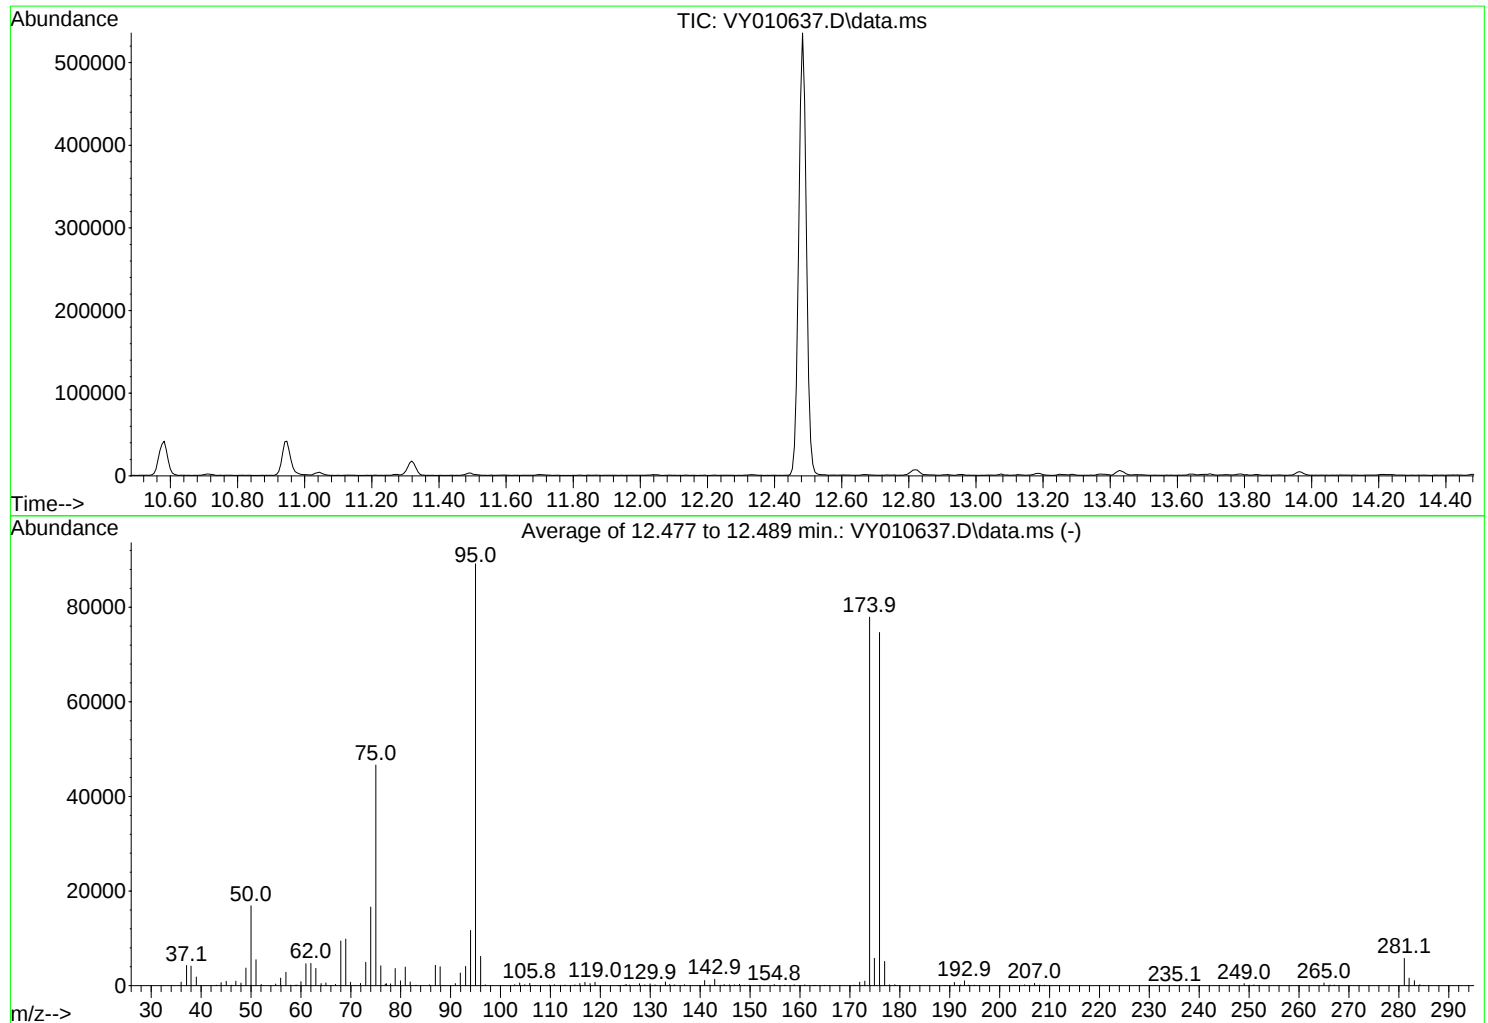

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	16895	PASS
75	95	30	60	52.3	46651	PASS
95	95	100	100	100.0	89179	PASS
96	95	5	9	7.0	6206	PASS
173	174	0.00	2	1.2	953	PASS
174	95	50	100	87.4	77899	PASS
175	174	5	9	7.4	5776	PASS
176	174	95	101	95.9	74672	PASS
177	176	5	9	6.9	5125	PASS