


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092324\
Data File : VY019657.D
Acq On : 23 Sep 2024 09:02
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090924S.M
Title : SW846 8260
Last Update : Mon Sep 09 16:00:30 2024

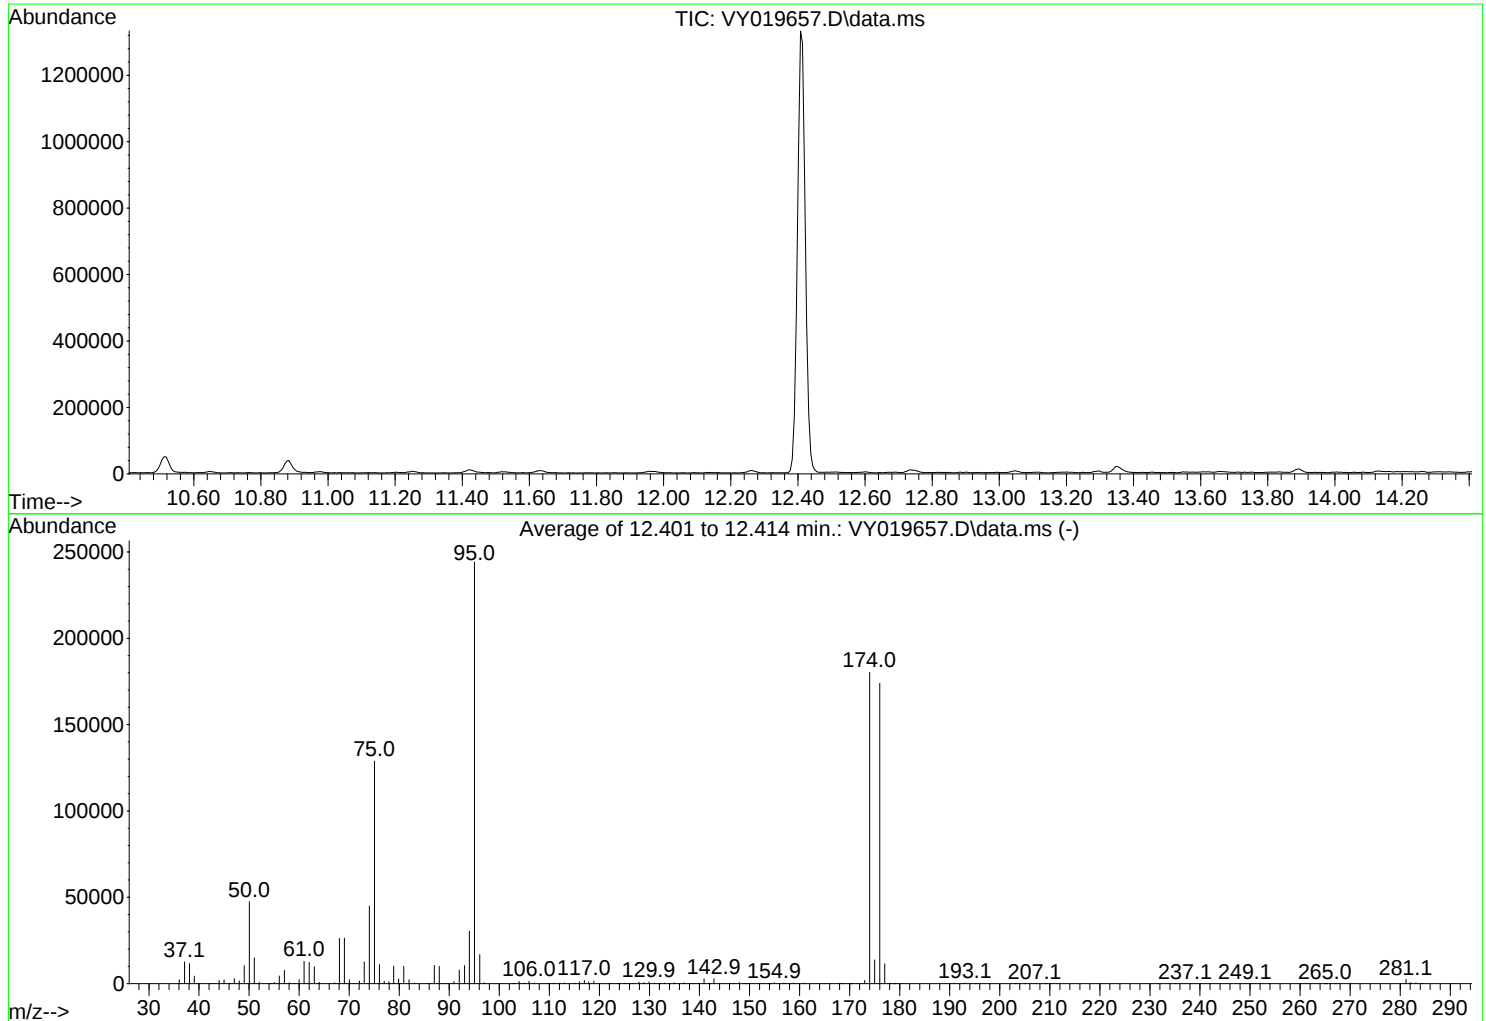

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	47477	PASS
75	95	30	60	52.7	128819	PASS
95	95	100	100	100.0	244267	PASS
96	95	5	9	6.9	16737	PASS
173	174	0.00	2	1.0	1834	PASS
174	95	50	100	73.8	180309	PASS
175	174	5	9	7.6	13748	PASS
176	174	95	101	96.5	173920	PASS
177	176	5	9	6.6	11467	PASS