

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092525\
 Data File : VY023378.D
 Acq On : 25 Sep 2025 16:53
 Operator : SY/MD
 Sample : Q3206-01
 Misc : 5.02g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TR-06-092525

Quant Time: Sep 26 04:27:00 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090825S.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 10 01:44:33 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	66269	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	106279	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	87708	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	30581	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	30416	52.233	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	104.460%
35) Dibromofluoromethane	7.634	113	37625	57.916	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	115.840%
50) Toluene-d8	10.109	98	119646	48.773	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.540%
62) 4-Bromofluorobenzene	12.402	95	30127	39.025	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	78.060%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092525\
Data File : VY023378.D
Acq On : 25 Sep 2025 16:53
Operator : SY/MD
Sample : Q3206-01
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TR-06-092525

Quant Time: Sep 26 04:27:00 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090825S.M
Quant Title : SW846 8260
QLast Update : Wed Sep 10 01:44:33 2025
Response via : Initial Calibration




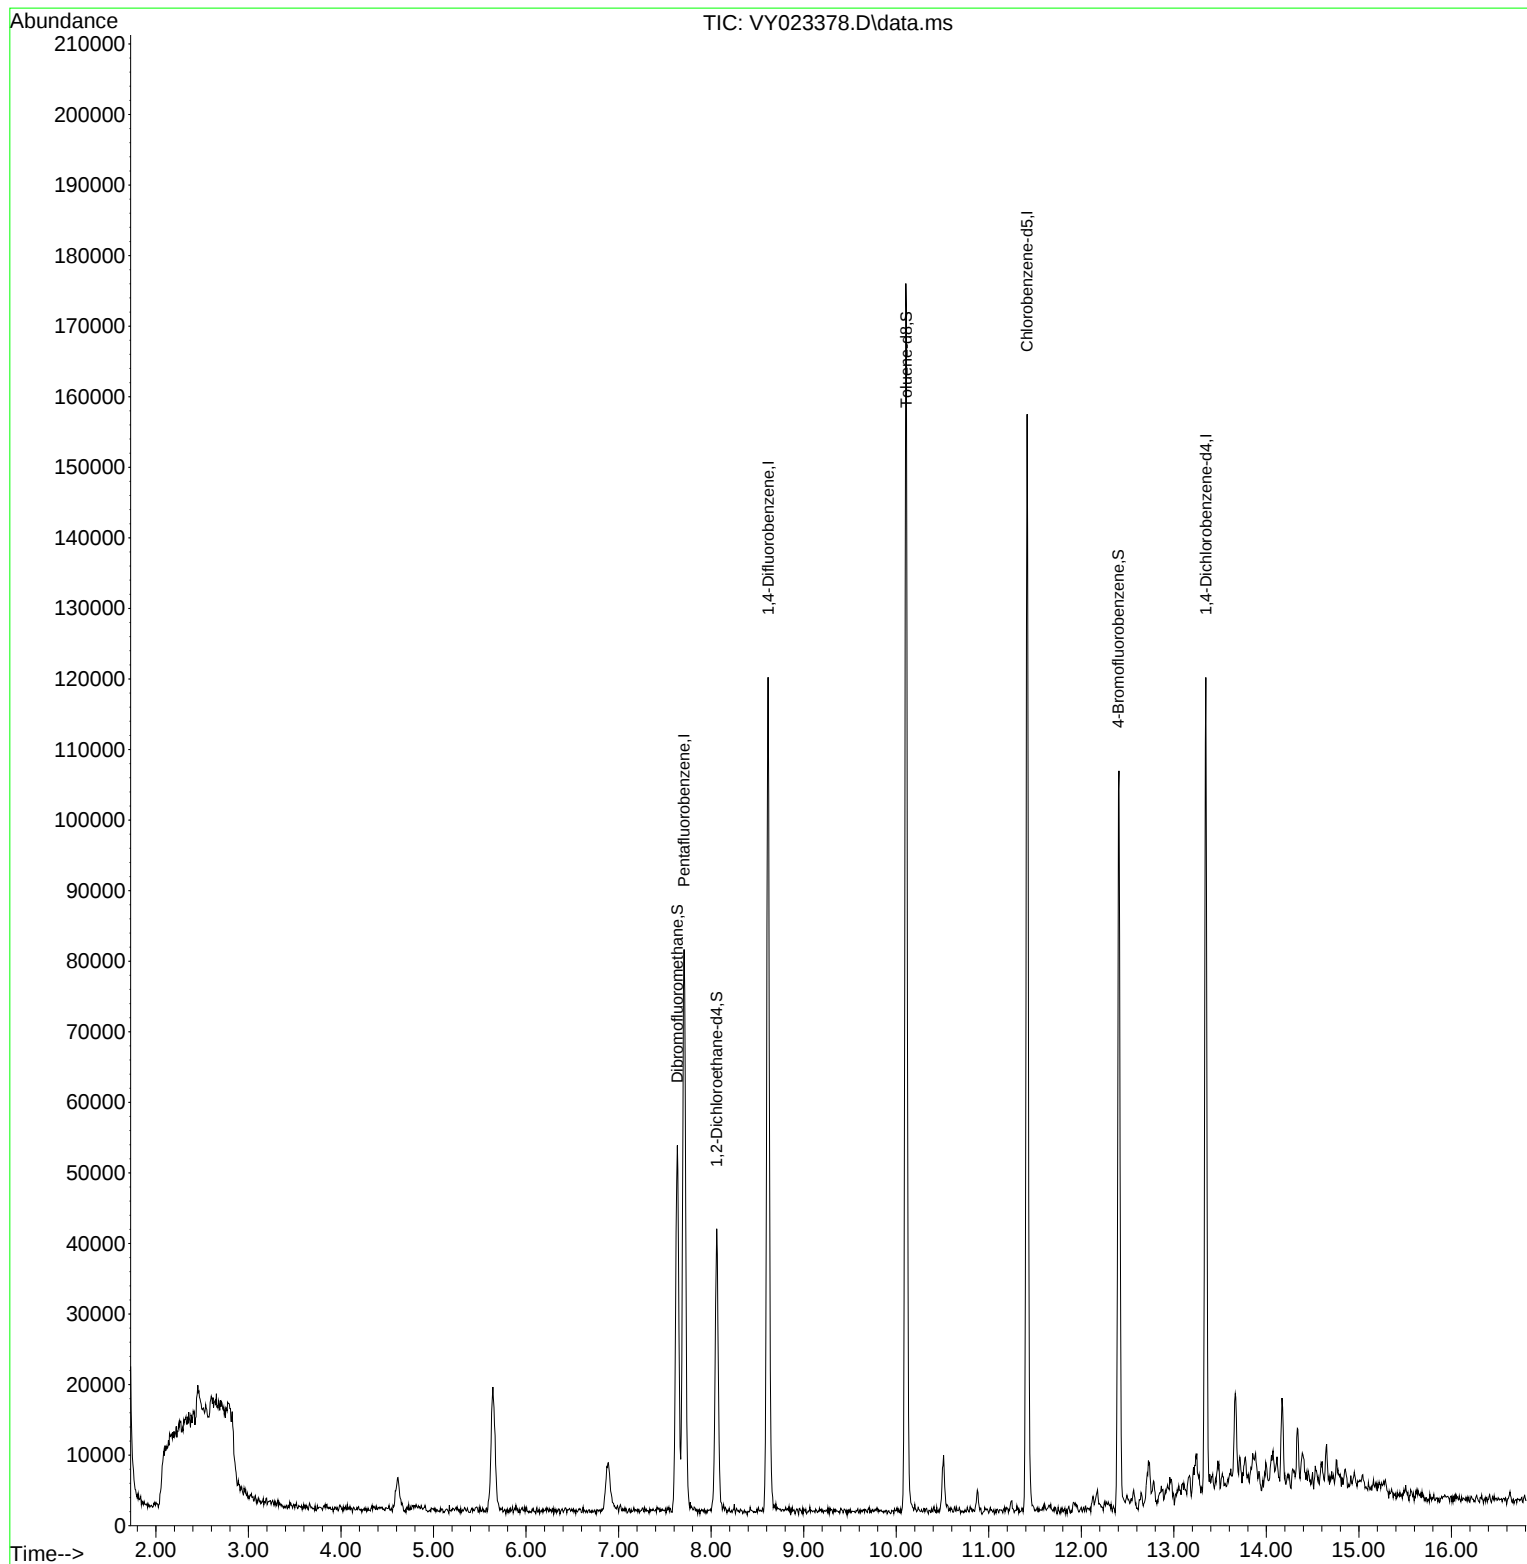


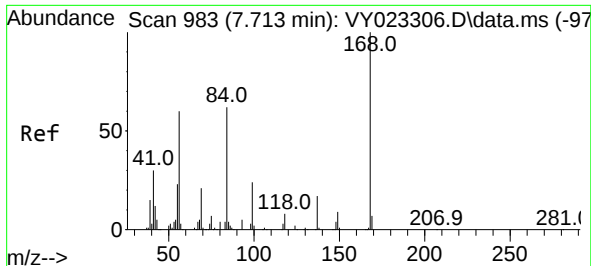

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY023378.D
Acq: 25 Sep 2025 16:53




Instrument :
MSVOA_Y
ClientSampleId :
TR-06-092525


Tgt Ion:168 Resp: 66269
Ion Ratio Lower Upper
168 100
99 48.4 42.8 64.2

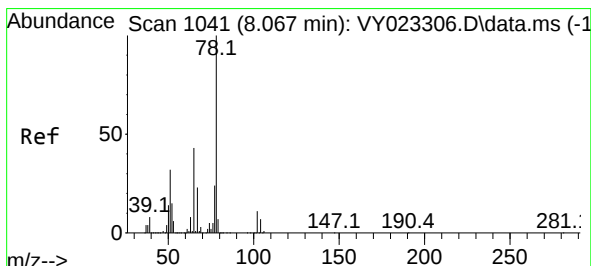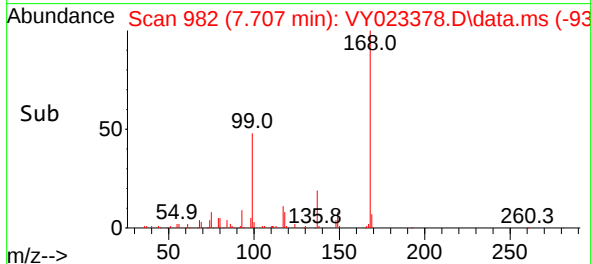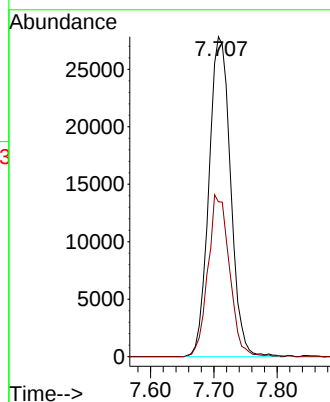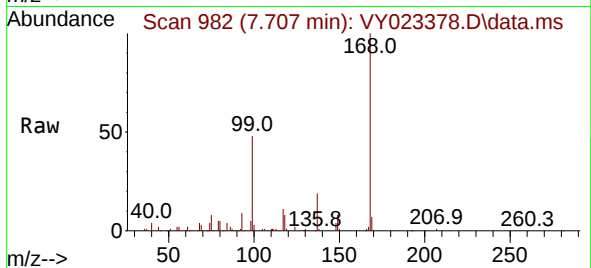

#33
1,2-Dichloroethane-d4
Concen: 52.233 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VY023378.D
Acq: 25 Sep 2025 16:53

Tgt Ion: 65 Resp: 30416
Ion Ratio Lower Upper
65 100
67 53.9 0.0 106.8


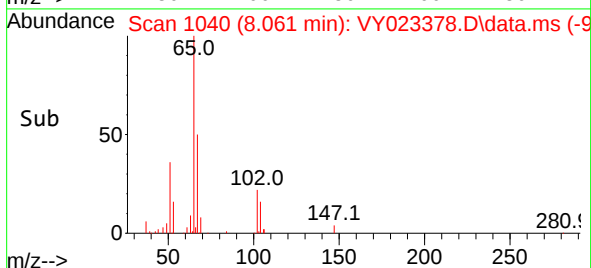
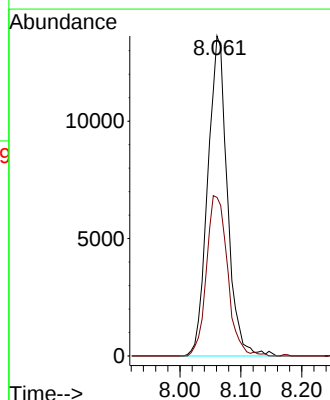
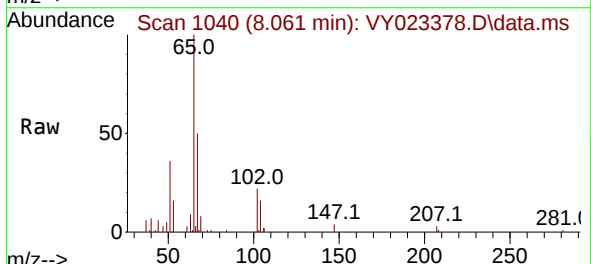


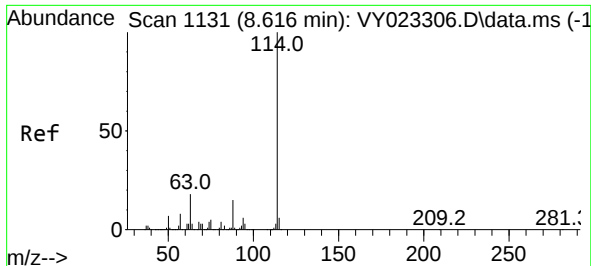

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.006 min
Lab File: VY023378.D
Acq: 25 Sep 2025 16:53




Instrument :
MSVOA_Y
ClientSampleId :
TR-06-092525


Tgt Ion:114 Resp: 106279
Ion Ratio Lower Upper
114 100
63 18.6 0.0 38.4
88 16.8 0.0 30.0

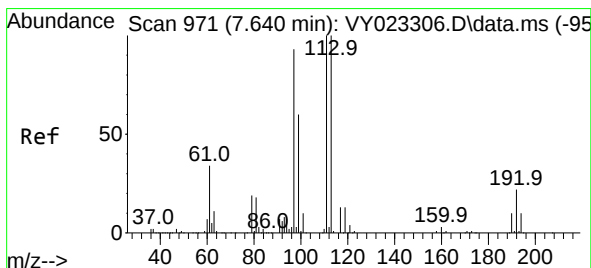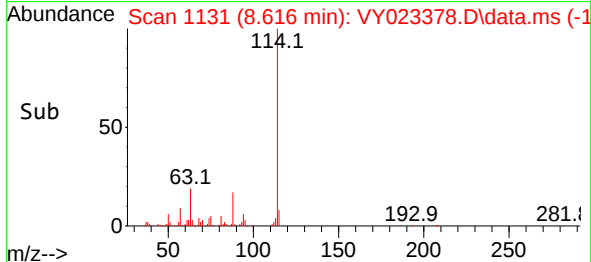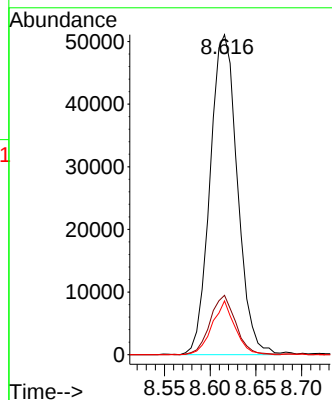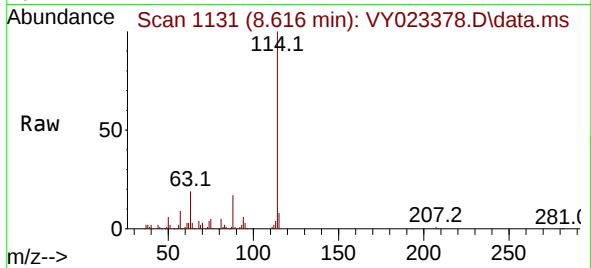

#35
Dibromofluoromethane
Concen: 57.916 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.006 min
Lab File: VY023378.D
Acq: 25 Sep 2025 16:53

Tgt Ion:113 Resp: 37625
Ion Ratio Lower Upper
113 100
111 100.9 81.1 121.7
192 21.7 16.2 24.4


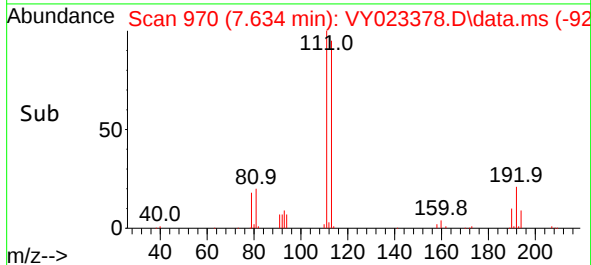
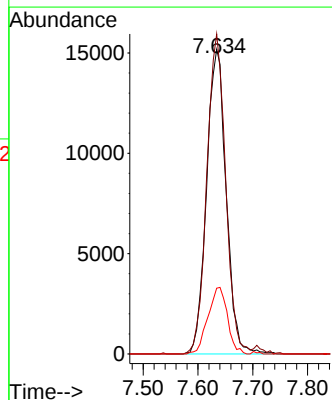
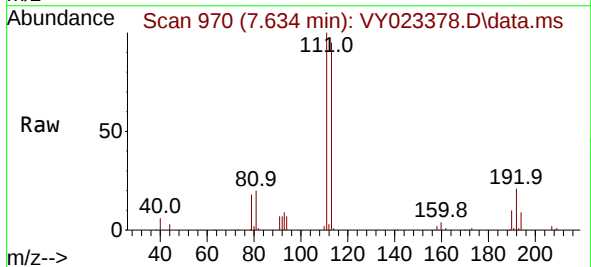


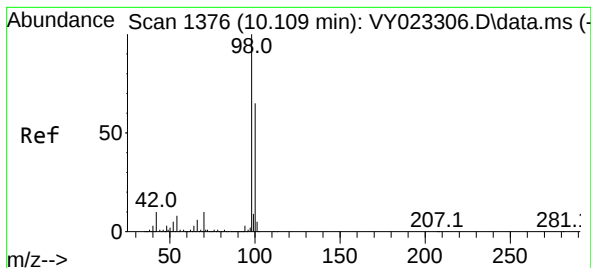

#50
Toluene-d8
Concen: 48.773 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY023378.D
Acq: 25 Sep 2025 16:53




Instrument :
MSVOA_Y
ClientSampleId :
TR-06-092525


Tgt Ion: 98 Resp: 119646
Ion Ratio Lower Upper
98 100
100 65.0 52.3 78.5

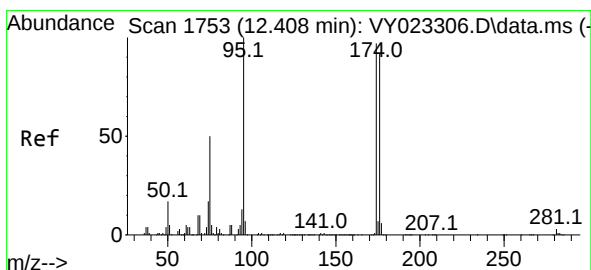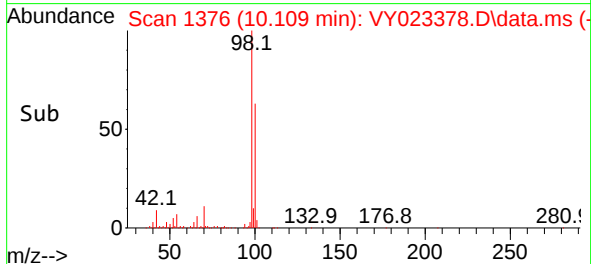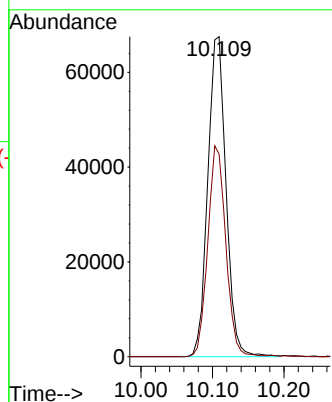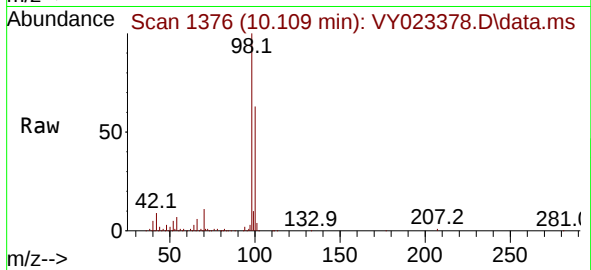

#62
4-Bromofluorobenzene
Concen: 39.025 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. 0.000 min
Lab File: VY023378.D
Acq: 25 Sep 2025 16:53

Tgt Ion: 95 Resp: 30127
Ion Ratio Lower Upper
95 100
174 92.1 0.0 171.6
176 91.0 0.0 167.6

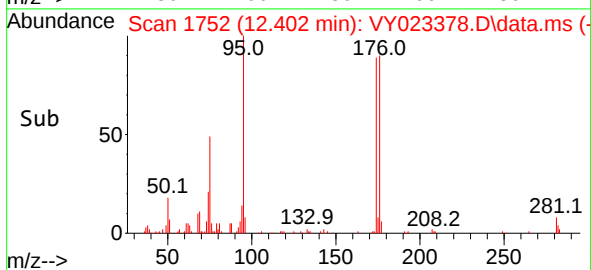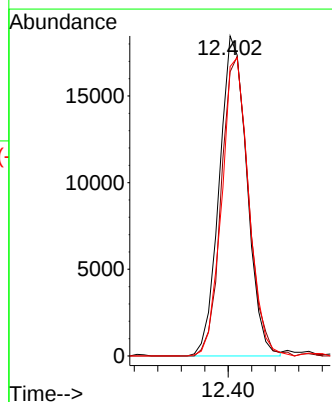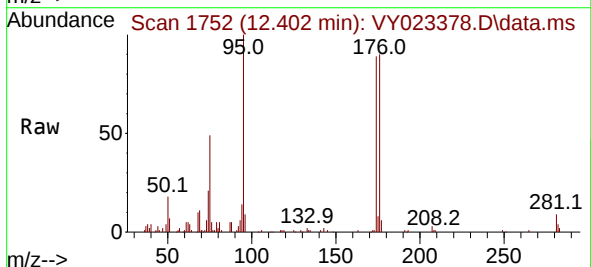

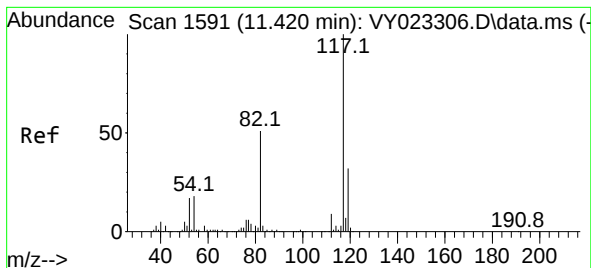

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY023378.D

Acq: 25 Sep 2025 16:53

Instrument :

MSVOA_Y

ClientSampleId :

TR-06-092525





Tgt Ion:117 Resp: 87708

Ion Ratio Lower Upper

117 100

82 55.5 43.4 65.0

119 32.3 25.6 38.4

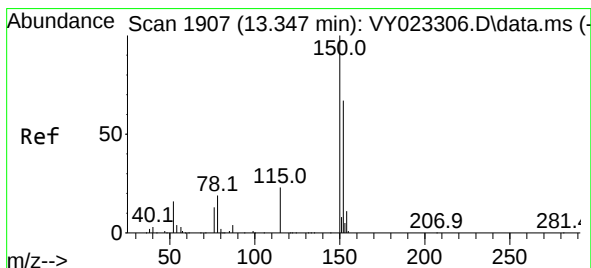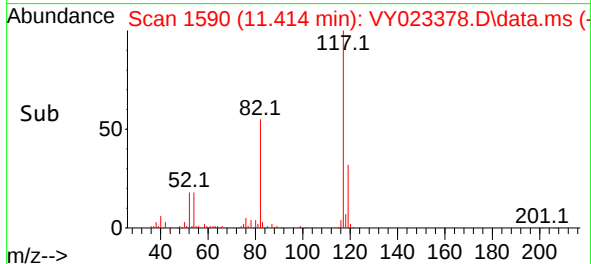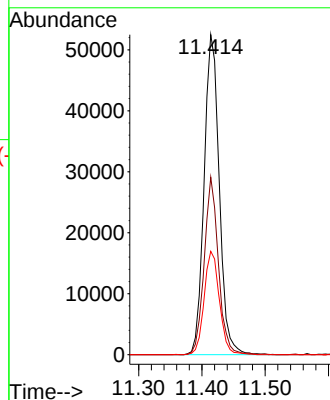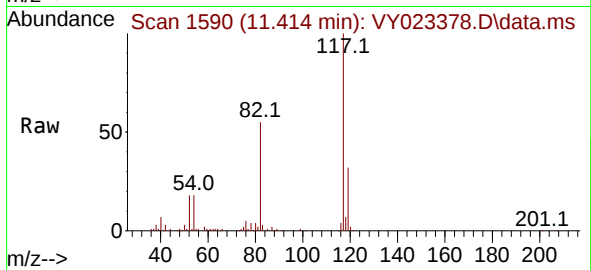

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. 0.006 min

Lab File: VY023378.D

Acq: 25 Sep 2025 16:53

Tgt Ion:152 Resp: 30581

Ion Ratio Lower Upper

152 100

115 58.4 28.2 84.6

150 159.2 0.0 348.0

