

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092622\
 Data File : VY010683.D
 Acq On : 26 Sep 2022 19:51
 Operator : KP/MD
 Sample : N4765-01
 Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OK-01-092222

Quant Time: Sep 27 06:29:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091922S.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 20 01:02:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	205246	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	351987	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	316320	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	142794	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	111286	56.688	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	113.380%
35) Dibromofluoromethane	7.716	113	108623	48.355	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	96.700%
50) Toluene-d8	10.179	98	351487	42.815	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	85.640%
62) 4-Bromofluorobenzene	12.477	95	120692	38.553	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	77.100%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092622\
Data File : VY010683.D
Acq On : 26 Sep 2022 19:51
Operator : KP/MD
Sample : N4765-01
Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OK-01-092222

Quant Time: Sep 27 06:29:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091922S.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 01:02:44 2022
Response via : Initial Calibration




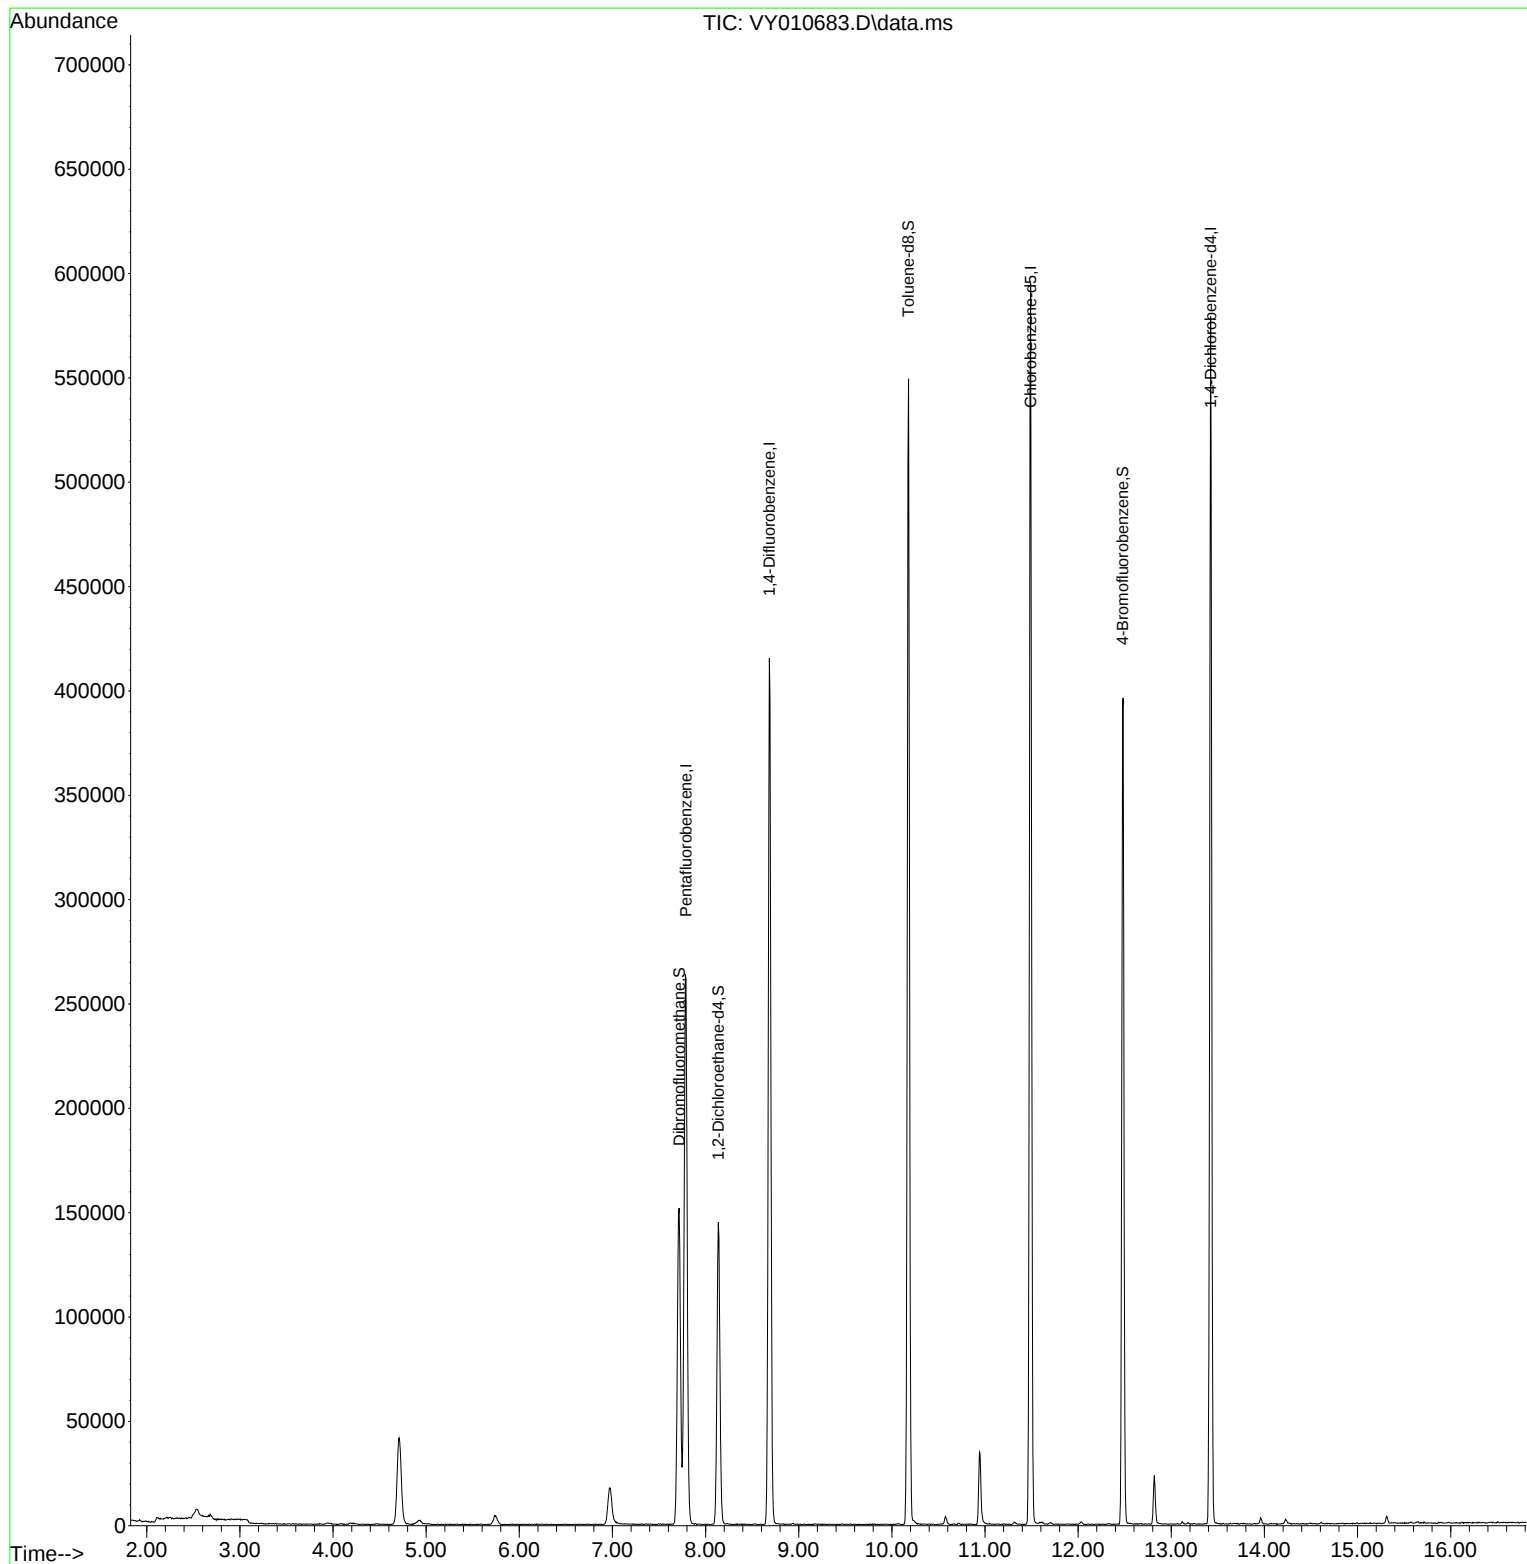


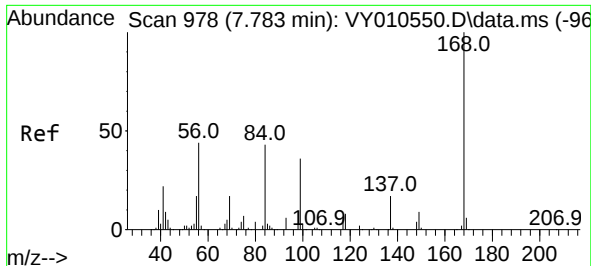

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY010683.D
Acq: 26 Sep 2022 19:51




Instrument :
MSVOA_Y
ClientSampleId :
OK-01-092222


Tgt Ion:168 Resp: 205246
Ion Ratio Lower Upper
168 100
99 55.9 46.9 70.3

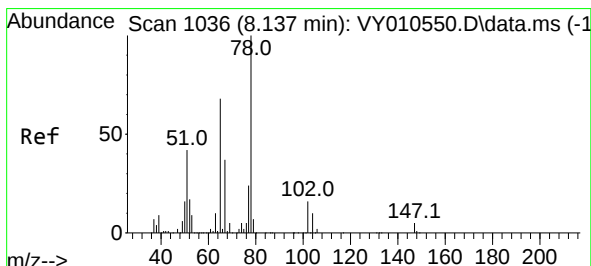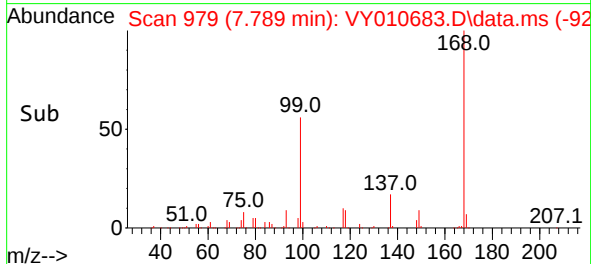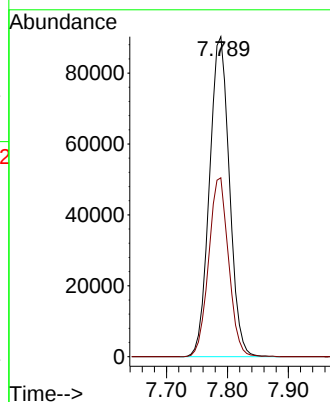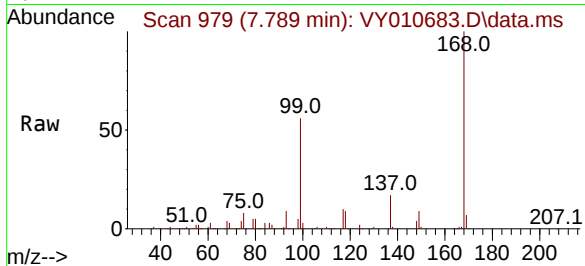

#33
1,2-Dichloroethane-d4
Concen: 56.688 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.001 min
Lab File: VY010683.D
Acq: 26 Sep 2022 19:51

Tgt Ion: 65 Resp: 111286
Ion Ratio Lower Upper
65 100
67 52.8 0.0 99.4

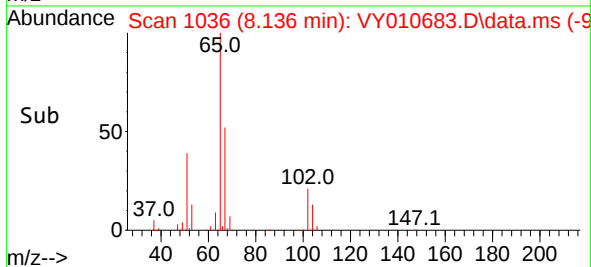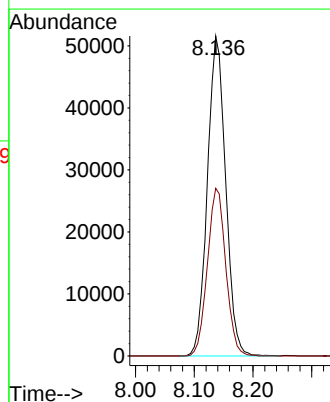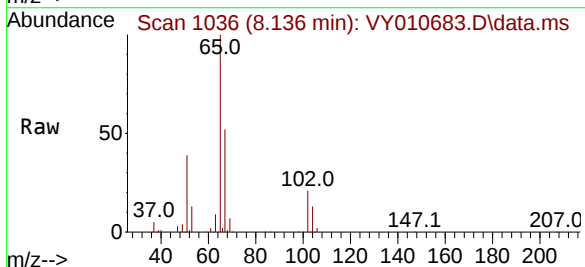

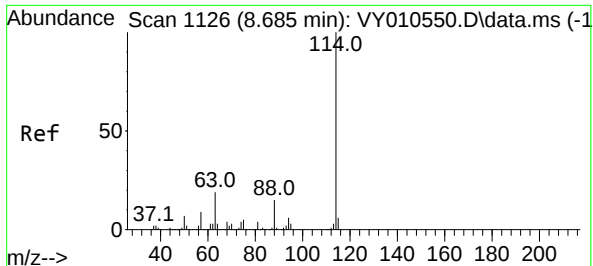

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY010683.D

Acq: 26 Sep 2022 19:51

Instrument :

MSVOA_Y

ClientSampleId :

OK-01-092222





Tgt Ion:114 Resp: 351987

Ion Ratio Lower Upper

114 100

63 20.7 0.0 43.2

88 15.2 0.0 31.8

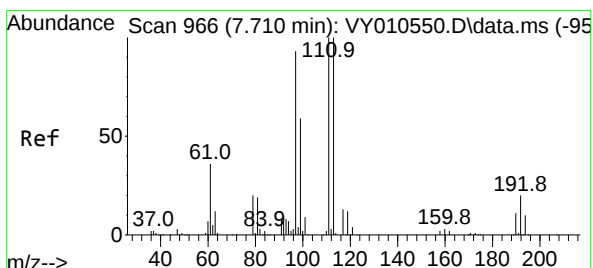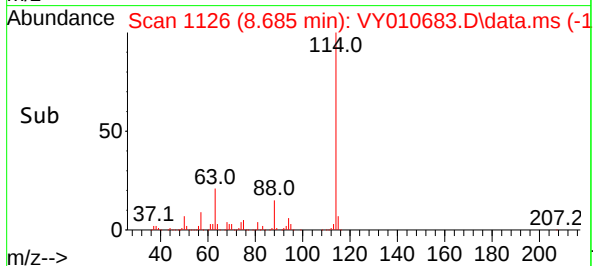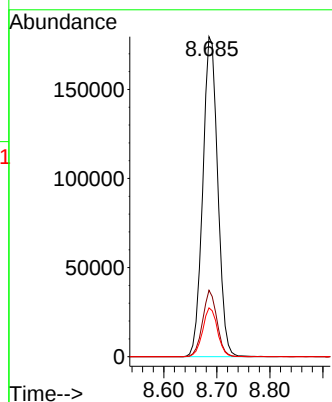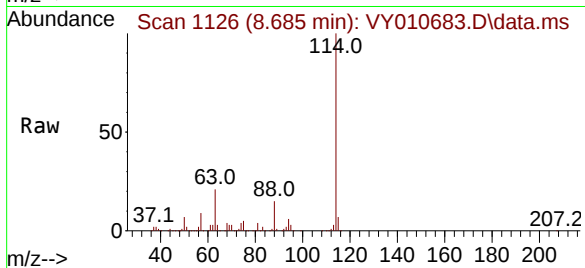

#35

Dibromofluoromethane

Concen: 48.355 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.006 min

Lab File: VY010683.D

Acq: 26 Sep 2022 19:51




Tgt Ion:113 Resp: 108623


Ion Ratio Lower Upper

113 100

111 102.1 82.6 124.0

192 19.1 17.6 26.4


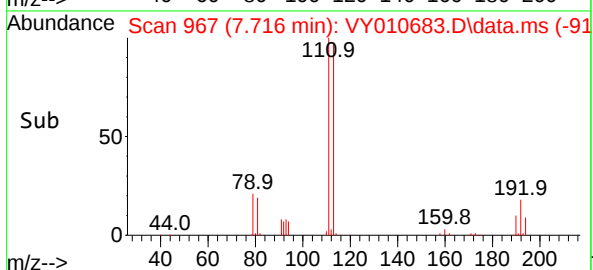
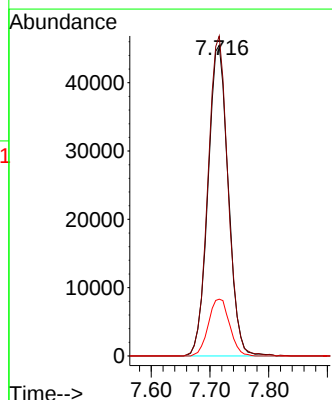
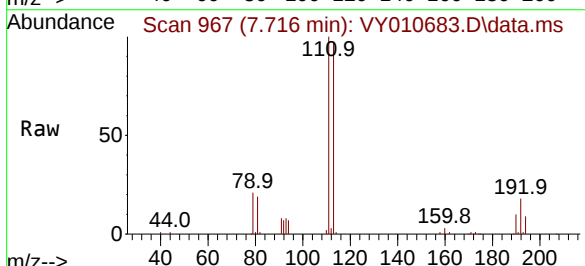


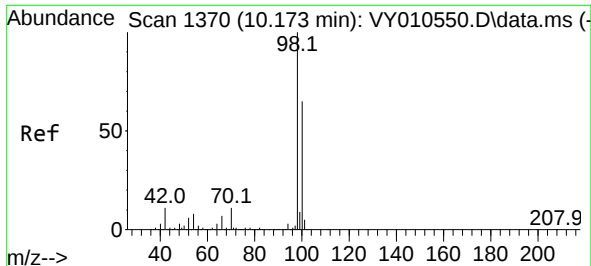

#50
Toluene-d8
Concen: 42.815 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY010683.D
Acq: 26 Sep 2022 19:51




Instrument :
MSVOA_Y
ClientSampleId :
OK-01-092222


Tgt Ion: 98 Resp: 351487
Ion Ratio Lower Upper
98 100
100 64.5 50.2 75.2

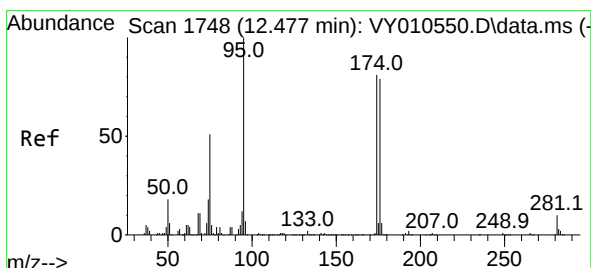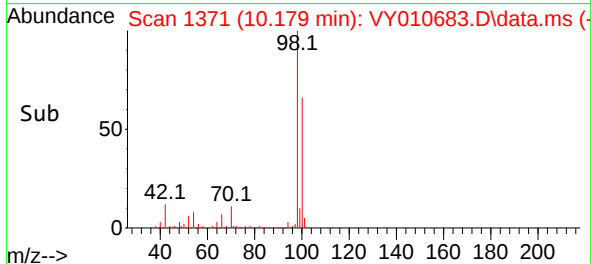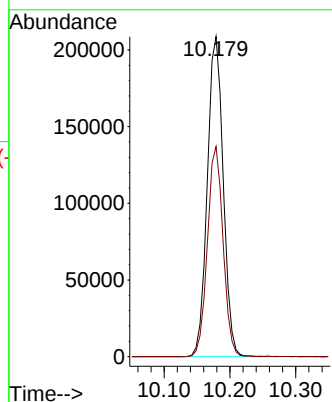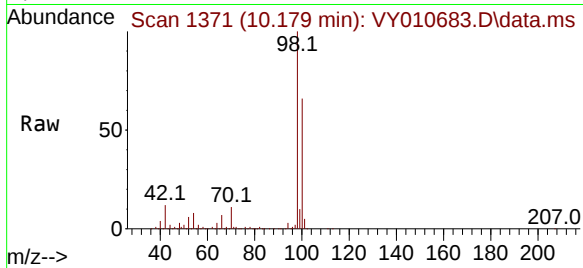

#62
4-Bromofluorobenzene
Concen: 38.553 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY010683.D
Acq: 26 Sep 2022 19:51

Tgt Ion: 95 Resp: 120692
Ion Ratio Lower Upper
95 100
174 83.3 0.0 177.0
176 81.3 0.0 175.8


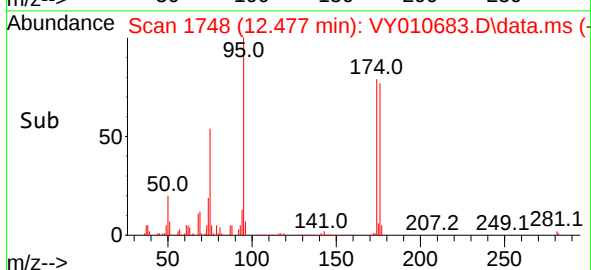
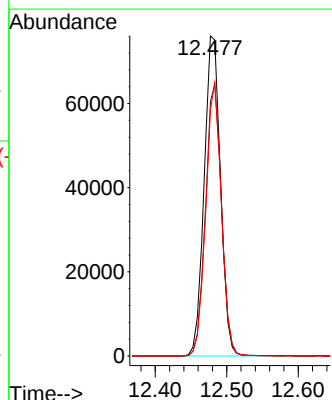
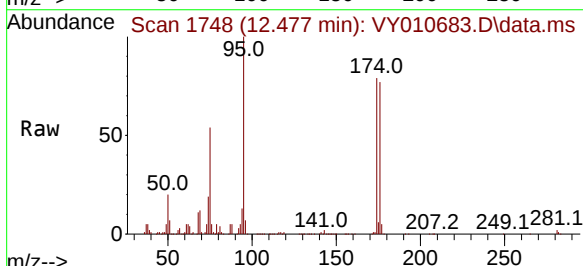


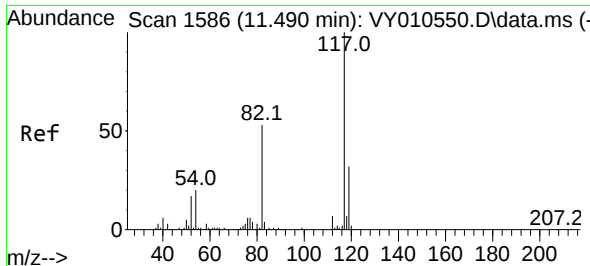

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY010683.D
Acq: 26 Sep 2022 19:51

Instrument :
MSVOA_Y
ClientSampleId :
OK-01-092222

Tgt Ion:117 Resp: 316320
Ion Ratio Lower Upper
117 100
82 54.0 43.0 64.4
119 32.1 25.4 38.0

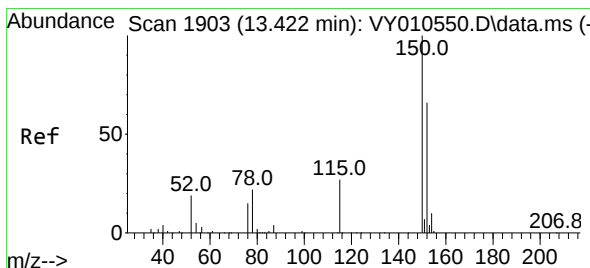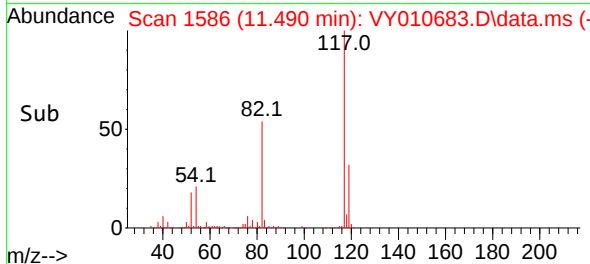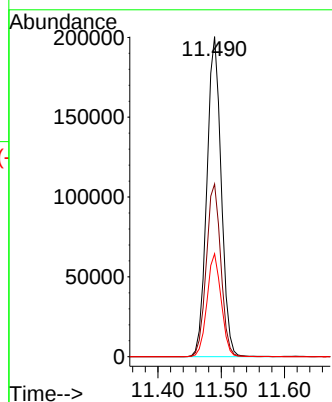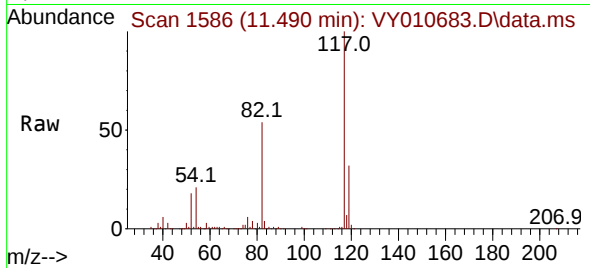

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY010683.D
Acq: 26 Sep 2022 19:51

Tgt Ion:152 Resp: 142794
Ion Ratio Lower Upper
152 100
115 58.3 28.2 84.7
150 157.6 0.0 347.6

