
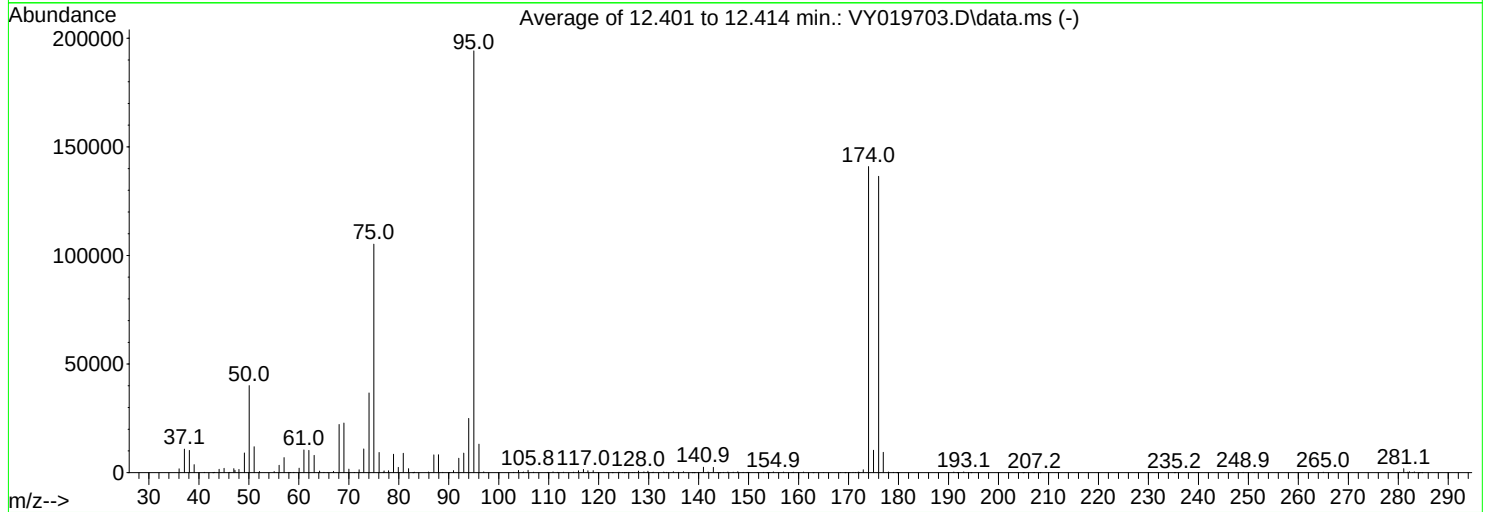


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092624\
Data File : VY019703.D
Acq On : 26 Sep 2024 09:02
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090924S.M
Title : SW846 8260
Last Update : Mon Sep 09 16:00:30 2024

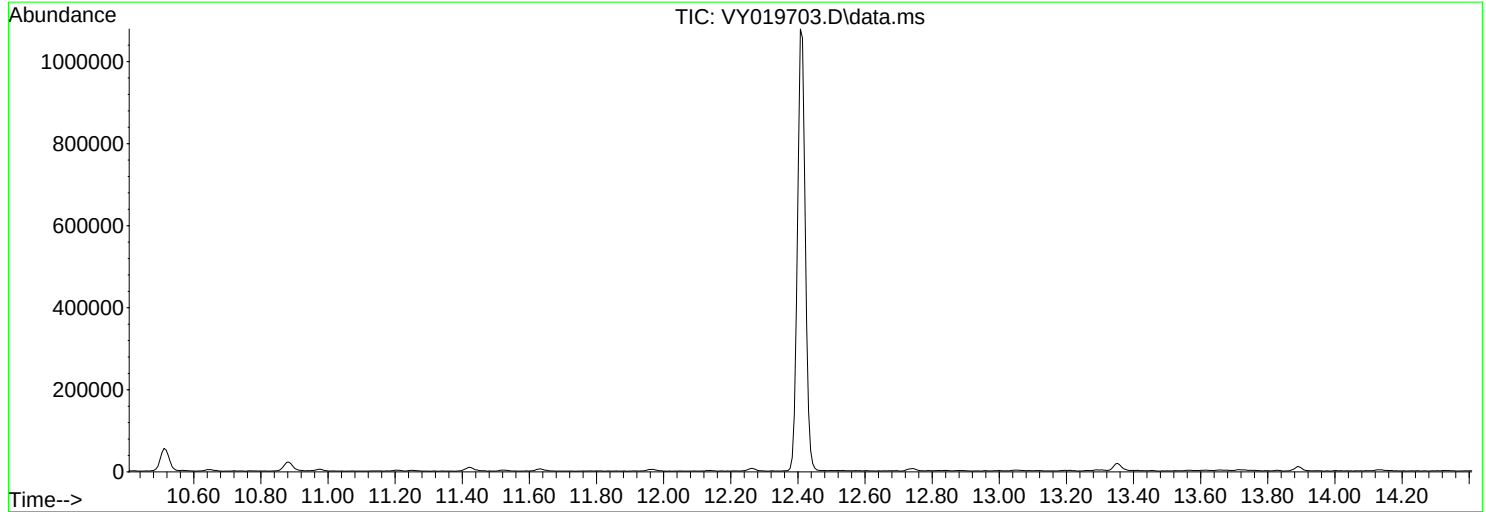

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	40067	PASS
75	95	30	60	54.2	105227	PASS
95	95	100	100	100.0	194219	PASS
96	95	5	9	6.8	13147	PASS
173	174	0.00	2	1.0	1358	PASS
174	95	50	100	72.6	140968	PASS
175	174	5	9	7.3	10348	PASS
176	174	95	101	96.8	136461	PASS
177	176	5	9	6.8	9333	PASS