
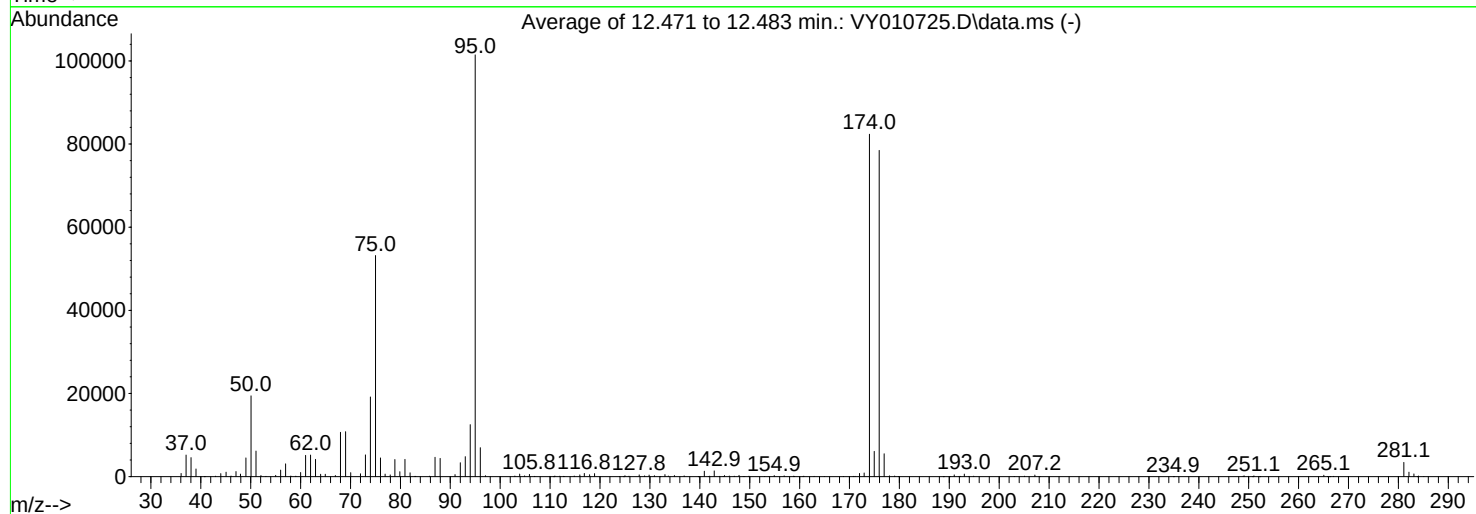


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092922\
 Data File : VY010725.D
 Acq On : 29 Sep 2022 09:16
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091922S.M
 Title : SW846 8260
 Last Update : Tue Sep 20 01:02:44 2022

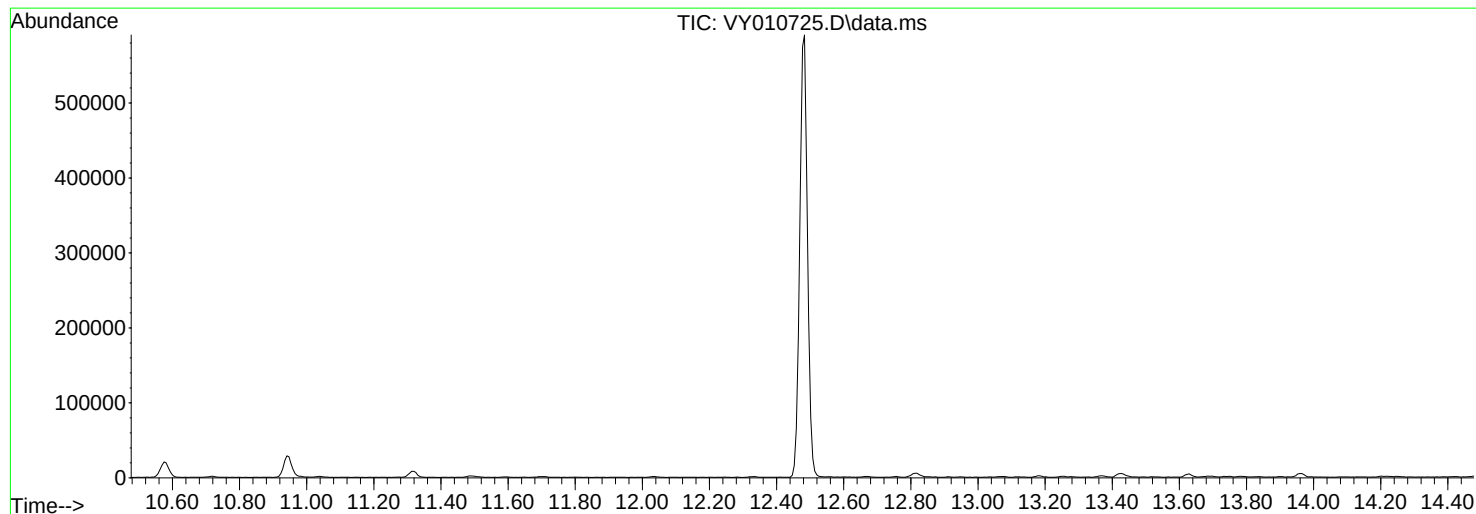

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	19434	PASS
75	95	30	60	52.4	53192	PASS
95	95	100	100	100.0	101461	PASS
96	95	5	9	6.9	6983	PASS
173	174	0.00	2	1.1	885	PASS
174	95	50	100	81.2	82381	PASS
175	174	5	9	7.4	6070	PASS
176	174	95	101	95.2	78467	PASS
177	176	5	9	7.0	5499	PASS