
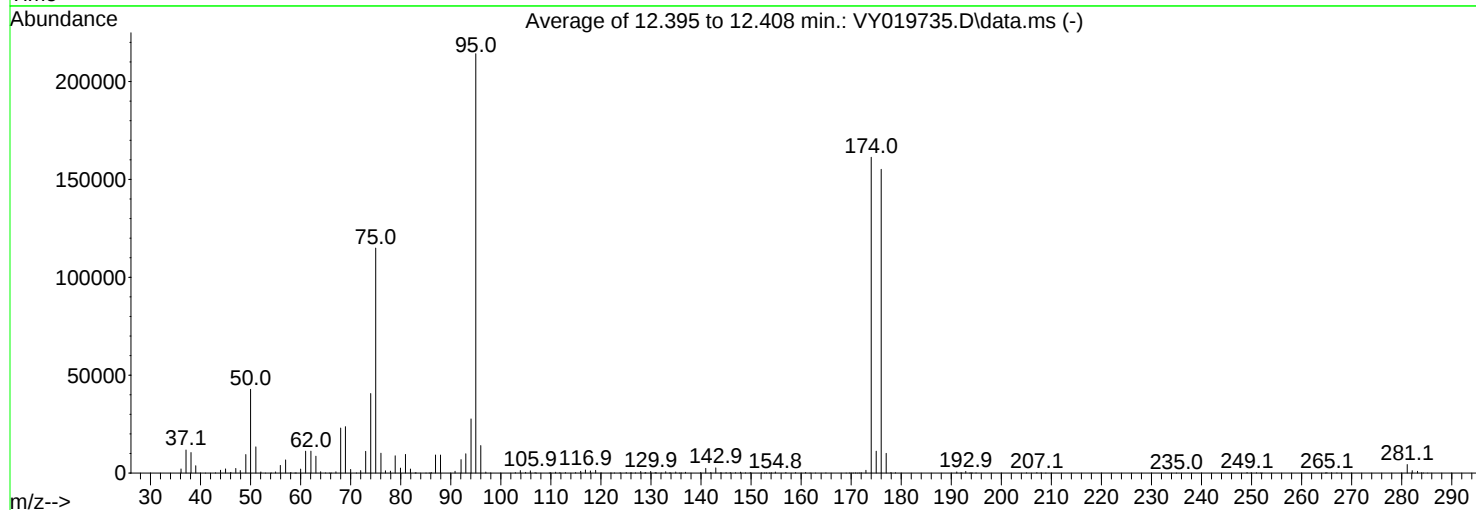


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100124\
Data File : VY019735.D
Acq On : 01 Oct 2024 09:24
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090924S.M
Title : SW846 8260
Last Update : Mon Sep 09 16:00:30 2024

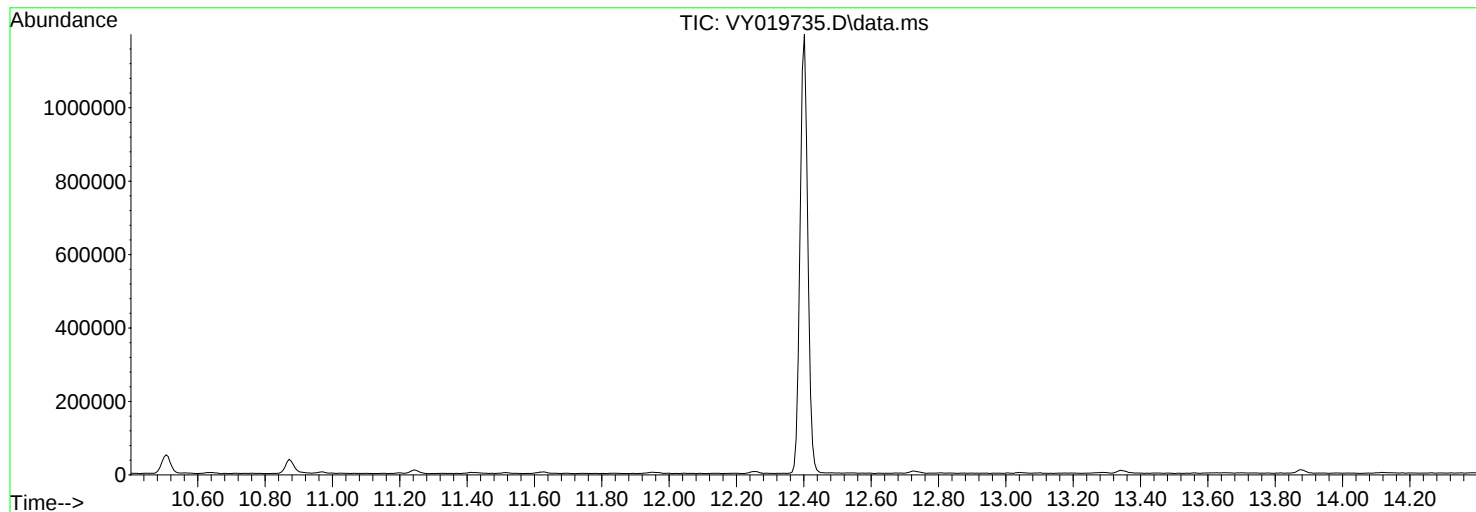

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1742

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	42787	PASS
75	95	30	60	53.6	114912	PASS
95	95	100	100	100.0	214208	PASS
96	95	5	9	6.6	14056	PASS
173	174	0.00	2	0.9	1417	PASS
174	95	50	100	75.3	161323	PASS
175	174	5	9	6.9	11195	PASS
176	174	95	101	96.2	155157	PASS
177	176	5	9	6.5	10093	PASS