
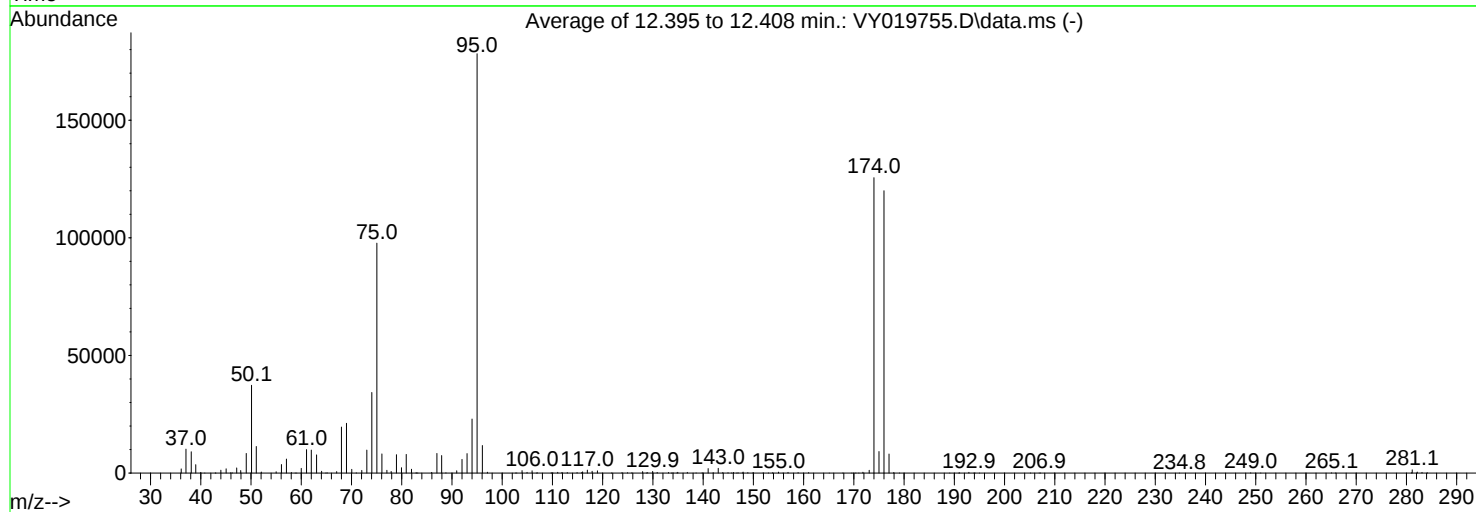


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY100224\  
Data File : VY019755.D  
Acq On : 02 Oct 2024 08:37  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y090924S.M  
Title : SW846 8260  
Last Update : Mon Sep 09 16:00:30 2024

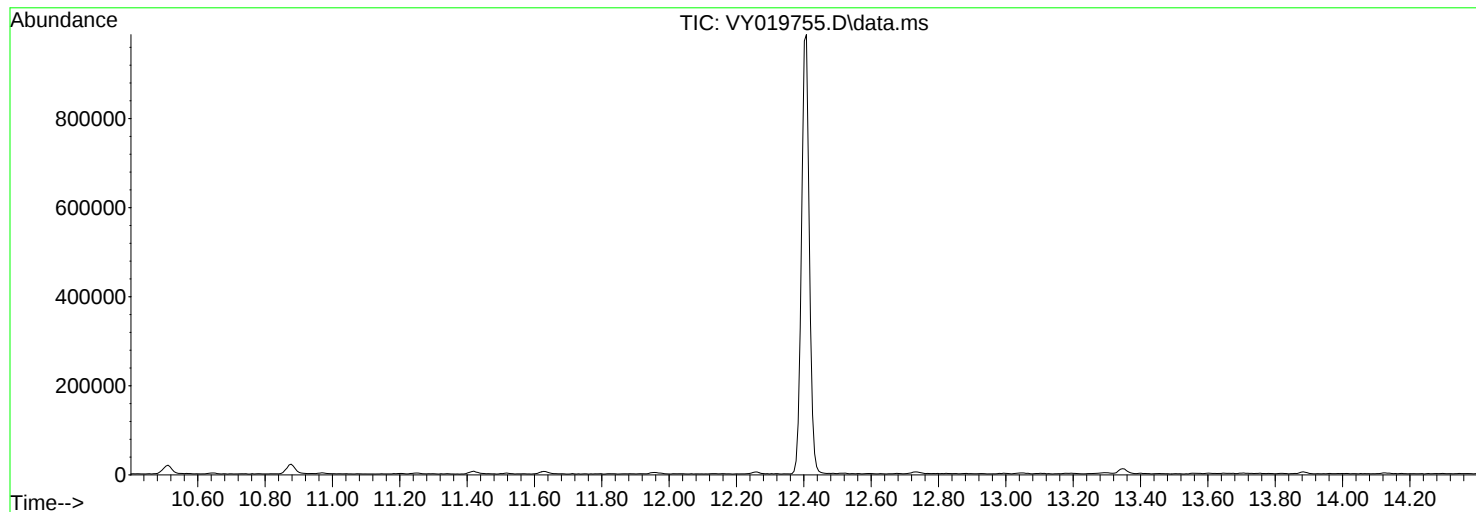

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 20.9         | 37323      | PASS                |
| 75             | 95              | 30              | 60              | 54.8         | 97728      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 178261     | PASS                |
| 96             | 95              | 5               | 9               | 6.6          | 11727      | PASS                |
| 173            | 174             | 0.00            | 2               | 0.9          | 1182       | PASS                |
| 174            | 95              | 50              | 100             | 70.4         | 125565     | PASS                |
| 175            | 174             | 5               | 9               | 7.3          | 9167       | PASS                |
| 176            | 174             | 95              | 101             | 95.6         | 120029     | PASS                |
| 177            | 176             | 5               | 9               | 6.8          | 8104       | PASS                |