


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100422\
Data File : VY010780.D
Acq On : 04 Oct 2022 08:32
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100322S.M
Title : SW846 8260
Last Update : Tue Oct 04 07:26:22 2022

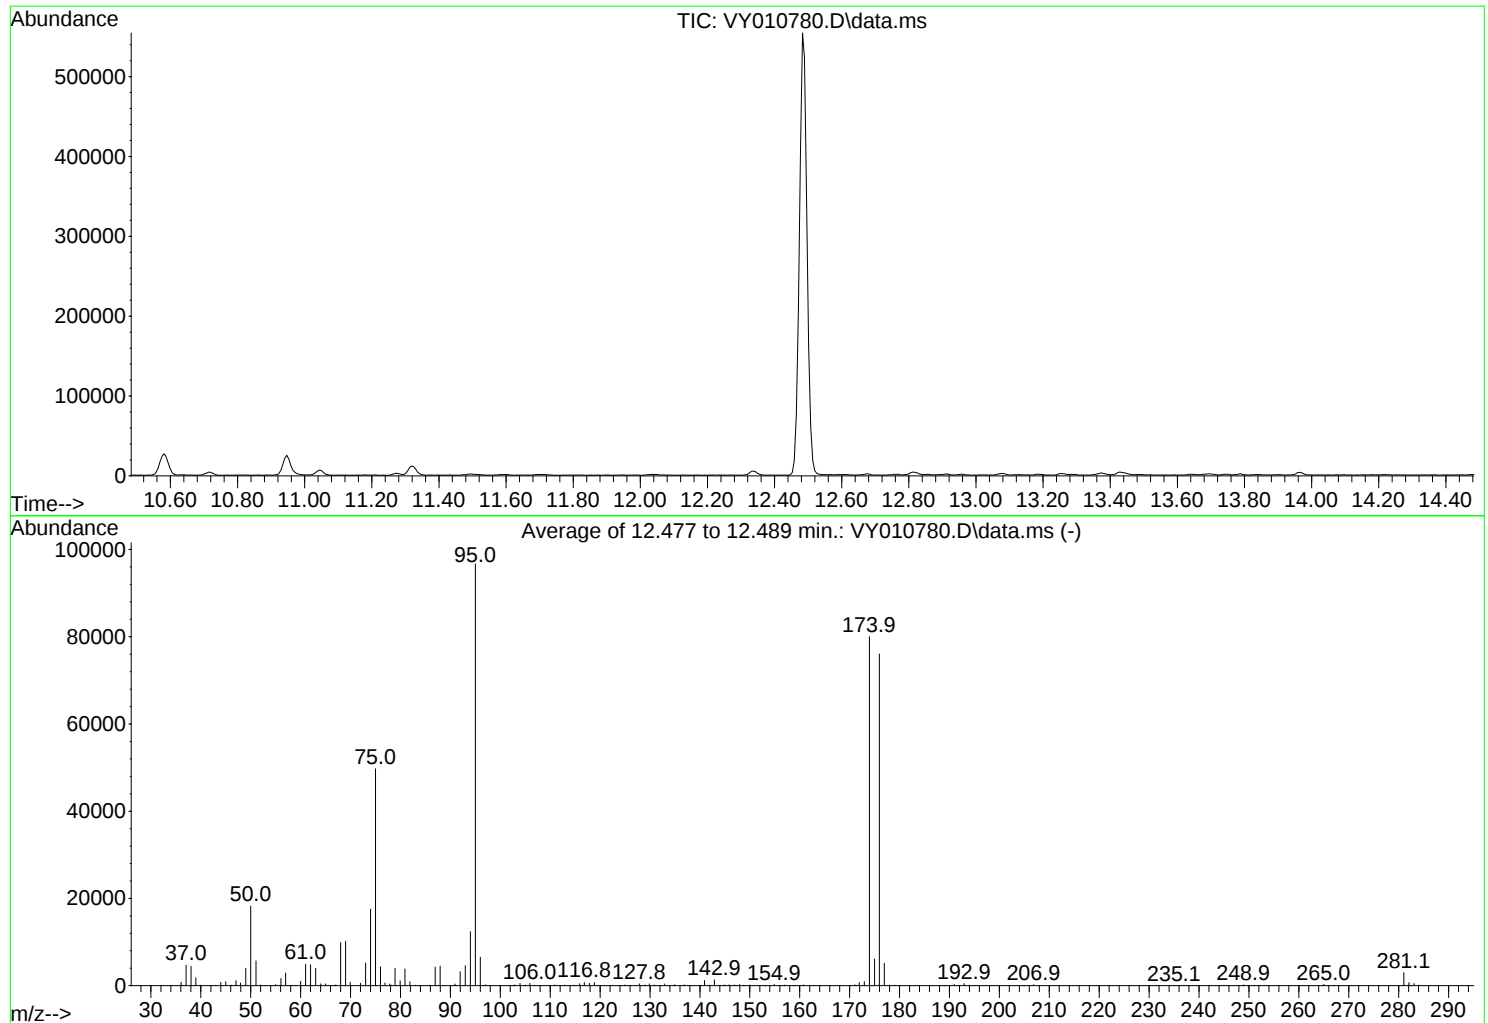

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	18229	PASS
75	95	30	60	51.4	49712	PASS
95	95	100	100	100.0	96717	PASS
96	95	5	9	6.7	6501	PASS
173	174	0.00	2	1.2	935	PASS
174	95	50	100	82.7	80000	PASS
175	174	5	9	7.6	6081	PASS
176	174	95	101	95.1	76069	PASS
177	176	5	9	6.8	5147	PASS