
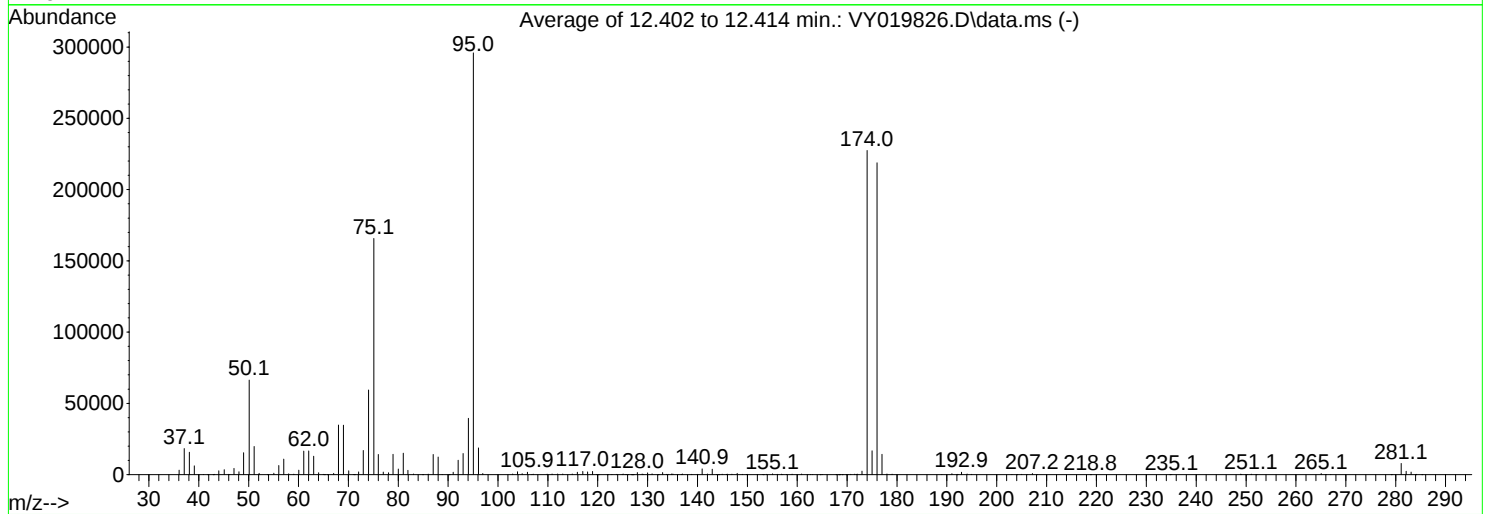


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100924\
Data File : VY019826.D
Acq On : 09 Oct 2024 09:33
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
Title : SW846 8260
Last Update : Thu Oct 10 05:30:07 2024

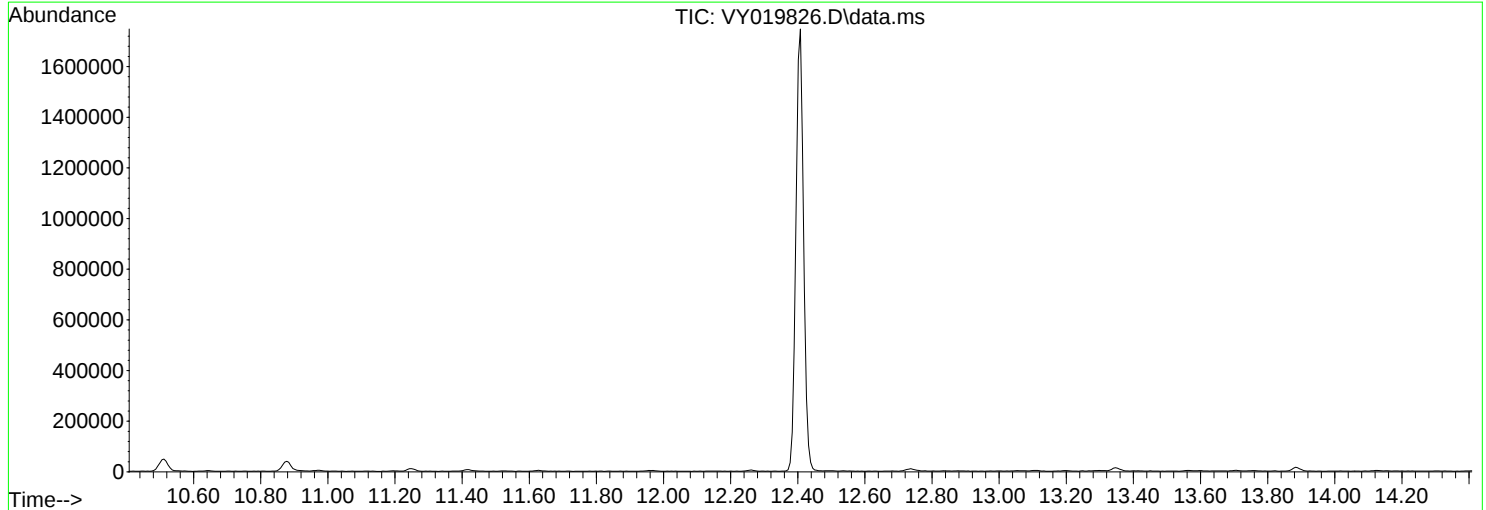

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	66352	PASS
75	95	30	60	56.0	165725	PASS
95	95	100	100	100.0	295936	PASS
96	95	5	9	6.3	18775	PASS
173	174	0.00	2	1.1	2529	PASS
174	95	50	100	76.9	227477	PASS
175	174	5	9	7.3	16688	PASS
176	174	95	101	96.2	218837	PASS
177	176	5	9	6.5	14261	PASS