

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100925\
 Data File : VY023414.D
 Acq On : 09 Oct 2025 11:47
 Operator : SY/MD
 Sample : Q3318-01
 Misc : 5.15g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VNJ-207

Quant Time: Oct 10 04:24:32 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.713	168	619900	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	1205387	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	1186929	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	518747	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.067	65	320385	61.806	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	123.620%
35) Dibromofluoromethane	7.640	113	401363	54.190	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	108.380%
50) Toluene-d8	10.109	98	1438063	52.137	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	104.280%
62) 4-Bromofluorobenzene	12.408	95	478158	52.508	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	105.020%
Target Compounds						
					Qvalue	
16) Acetone	3.866	43	9110	7.382	ug/l #	87
52) Toluene	10.170	92	68841	3.414	ug/l	99
67) Ethyl Benzene	11.517	91	43167	1.033	ug/l	98
68) m/p-Xylenes	11.627	106	57903	3.455	ug/l	100
69) o-Xylene	11.956	106	27838	1.771	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100925\
Data File : VY023414.D
Acq On : 09 Oct 2025 11:47
Operator : SY/MD
Sample : Q3318-01
Misc : 5.15g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VNJ-207

Quant Time: Oct 10 04:24:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration




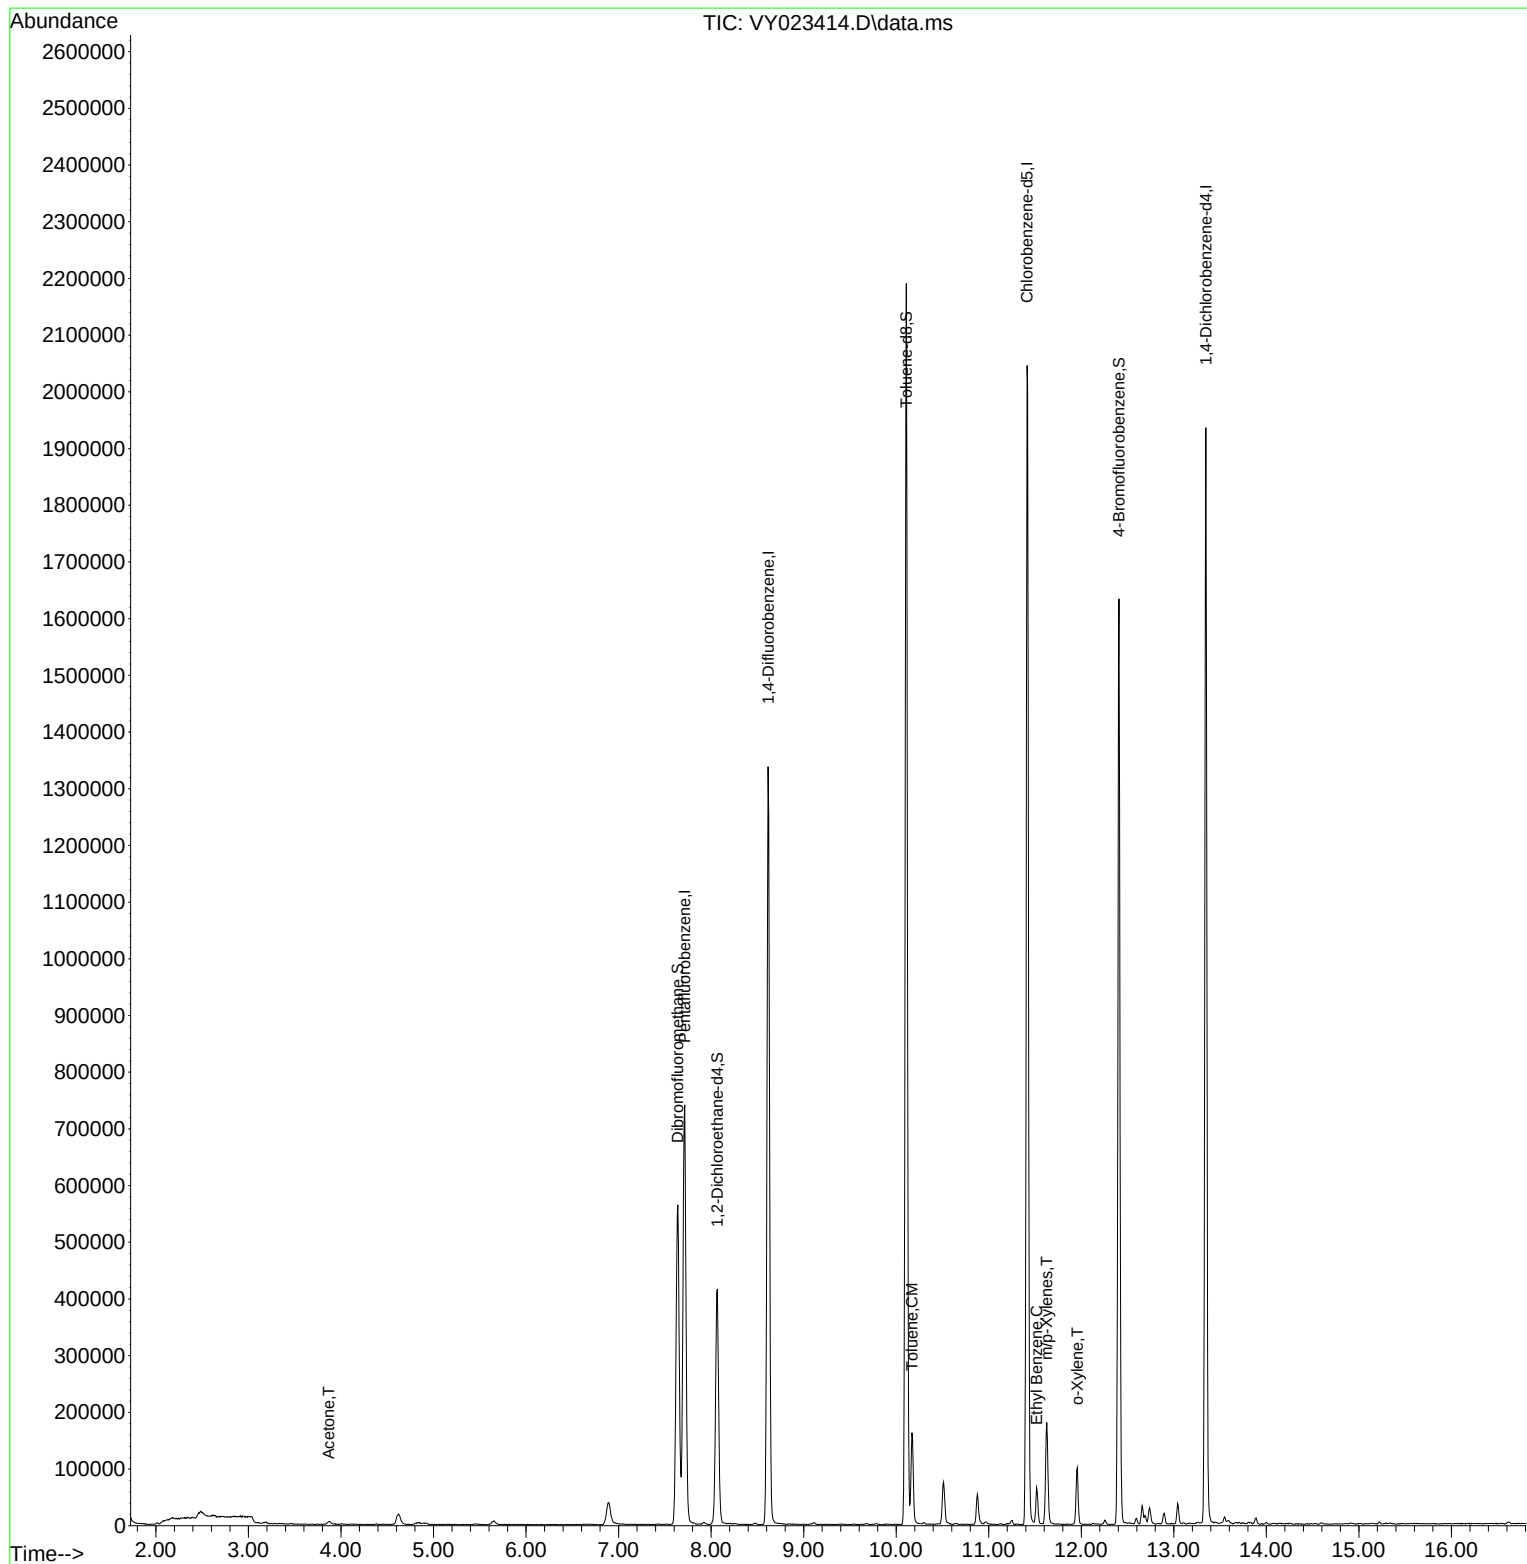


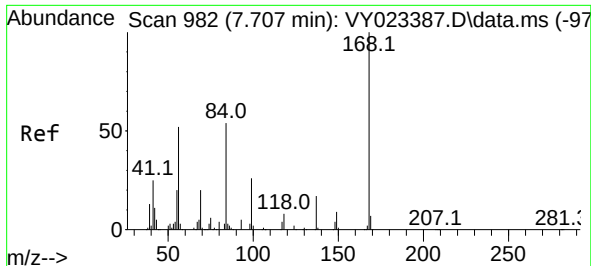

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY023414.D
Acq: 09 Oct 2025 11:47




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-207


Tgt Ion:168 Resp: 619900
Ion Ratio Lower Upper
168 100
99 48.2 39.7 59.5

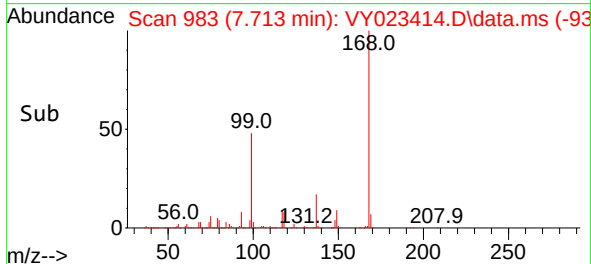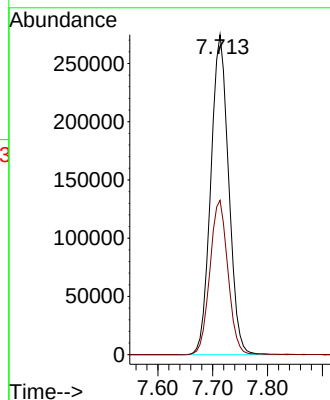

#16
Acetone
Concen: 7.382 ug/l
RT: 3.866 min Scan# 352
Delta R.T. -0.000 min
Lab File: VY023414.D
Acq: 09 Oct 2025 11:47

Tgt Ion: 43 Resp: 9110
Ion Ratio Lower Upper
43 100
58 26.9 27.7 41.5#

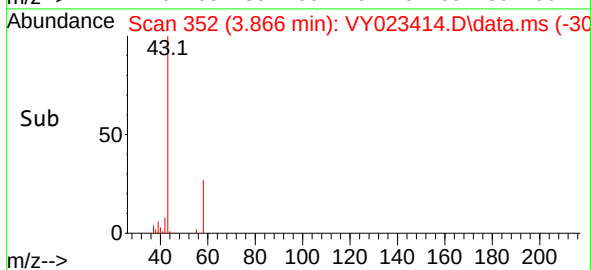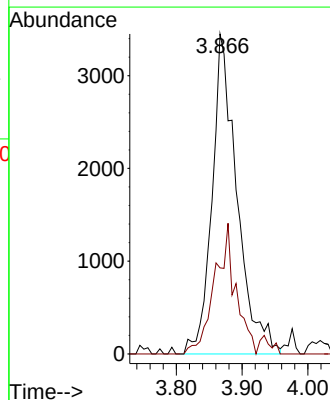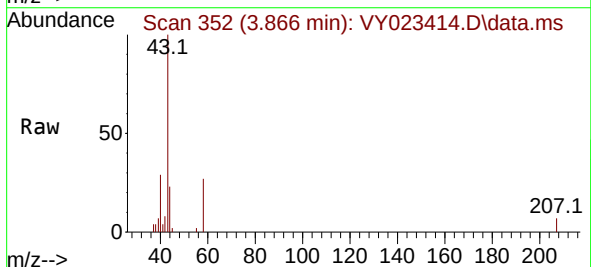

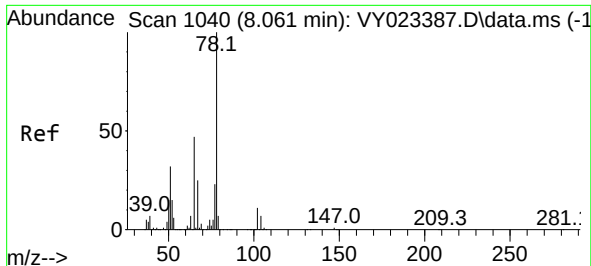

#33

1,2-Dichloroethane-d4

Concen: 61.806 ug/l

RT: 8.067 min Scan# 1

Delta R.T. 0.006 min

Lab File: VY023414.D

Acq: 09 Oct 2025 11:47

Instrument :

MSVOA_Y

ClientSampleId :





VNJ-207

Tgt Ion: 65 Resp: 320385

Ion Ratio Lower Upper

65 100

67 52.8 0.0 105.8

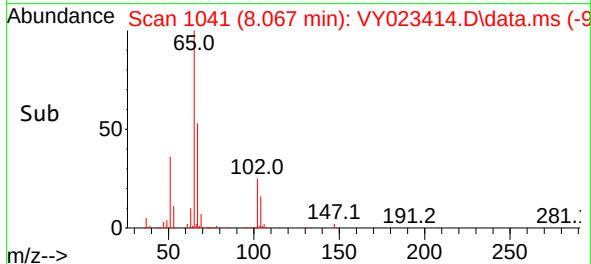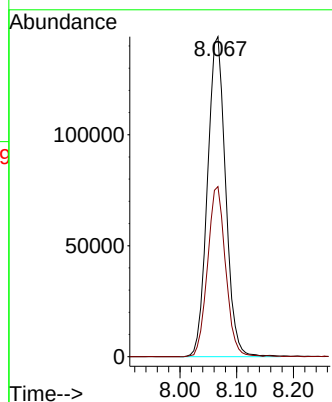

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. -0.000 min

Lab File: VY023414.D

Acq: 09 Oct 2025 11:47




Tgt Ion:114 Resp: 1205387


Ion Ratio Lower Upper

114 100

63 16.6 0.0 34.2

88 14.4 0.0 28.4


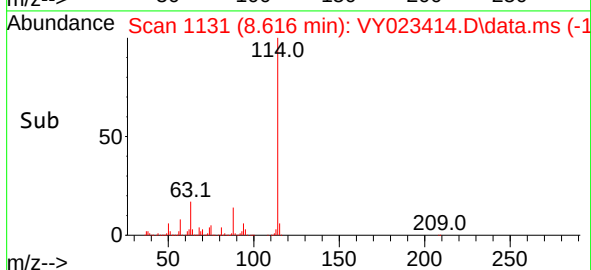
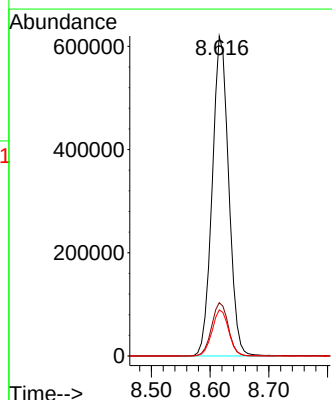
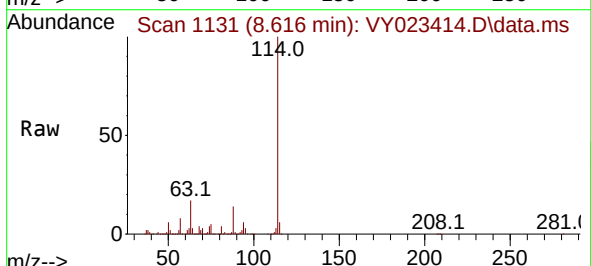


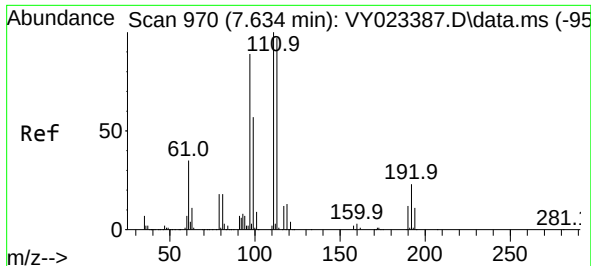

#35
Dibromofluoromethane
Concen: 54.190 ug/l
RT: 7.640 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY023414.D
Acq: 09 Oct 2025 11:47




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-207


Tgt Ion:113 Resp: 401363
Ion Ratio Lower Upper
113 100
111 103.4 81.8 122.6
192 22.5 18.0 27.0

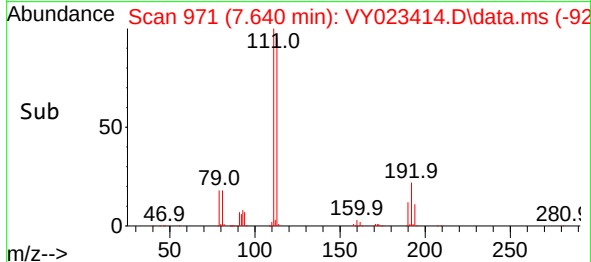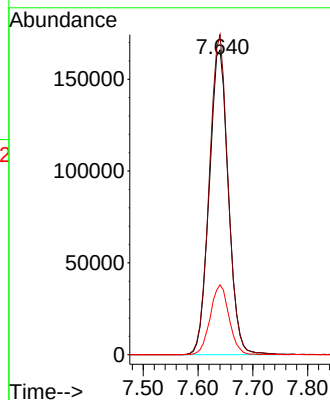

#50
Toluene-d8
Concen: 52.137 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.006 min
Lab File: VY023414.D
Acq: 09 Oct 2025 11:47

Tgt Ion: 98 Resp: 1438063
Ion Ratio Lower Upper
98 100
100 65.6 53.0 79.4

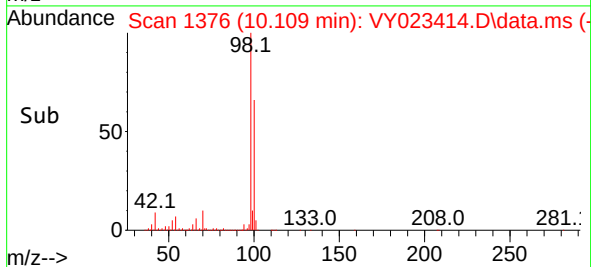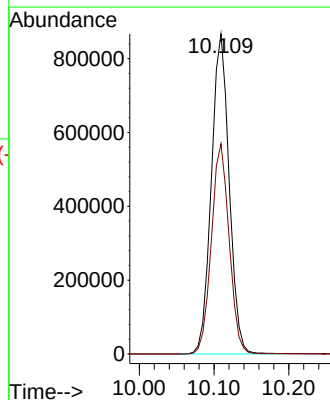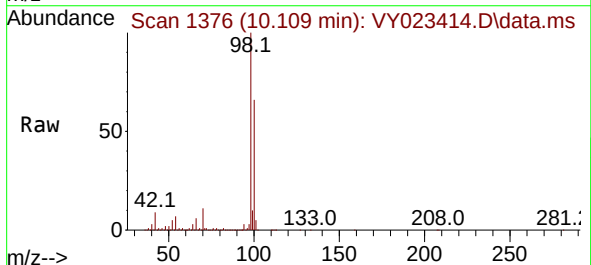

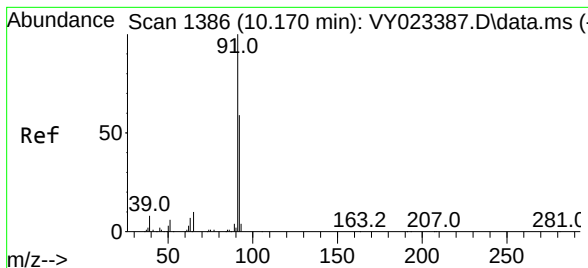

#52

Toluene

Concen: 3.414 ug/l

RT: 10.170 min Scan# 1

Delta R.T. -0.000 min

Lab File: VY023414.D

Acq: 09 Oct 2025 11:47

Instrument :

MSVOA_Y

ClientSampleId :





VNJ-207

Tgt Ion: 92 Resp: 68841

Ion Ratio Lower Upper

92 100

91 168.7 136.4 204.6

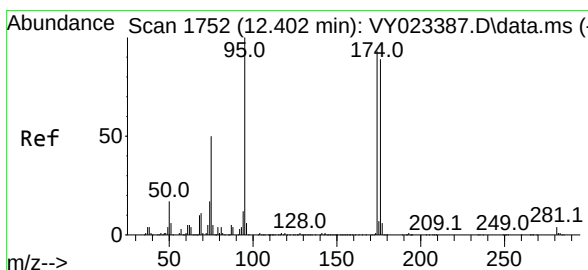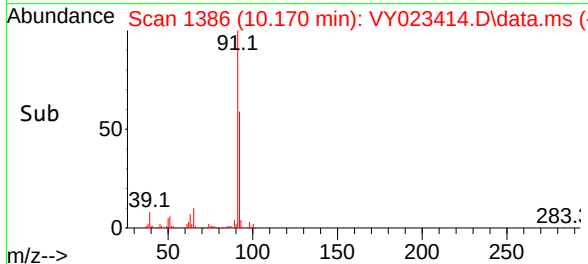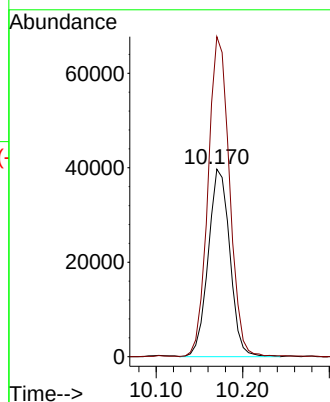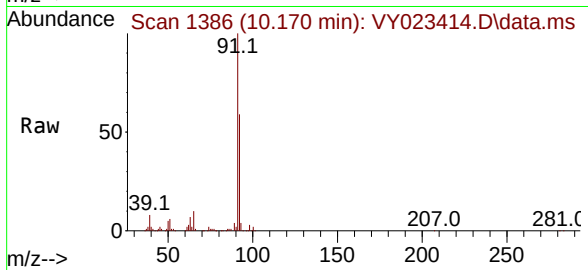

#62

4-Bromofluorobenzene

Concen: 52.508 ug/l

RT: 12.408 min Scan# 1753

Delta R.T. 0.006 min

Lab File: VY023414.D

Acq: 09 Oct 2025 11:47




Tgt Ion: 95 Resp: 478158


Ion Ratio Lower Upper

95 100

174 96.6 0.0 192.8

176 93.4 0.0 187.6

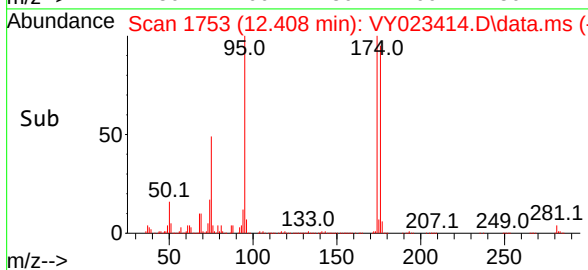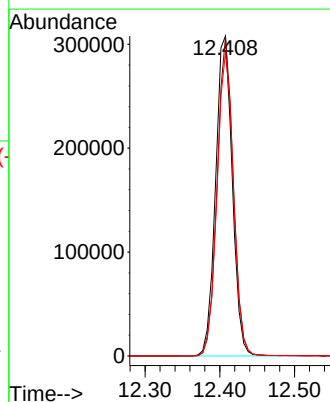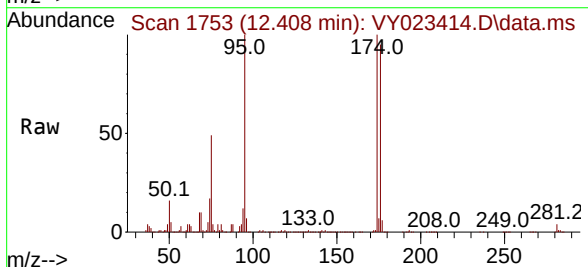



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY023414.D

Acq: 09 Oct 2025 11:47

Instrument :

MSVOA_Y

ClientSampleId :

VNJ-207





Tgt Ion:117 Resp: 1186929

Ion Ratio Lower Upper

117 100

82 51.0 41.0 61.4

119 32.0 25.6 38.4

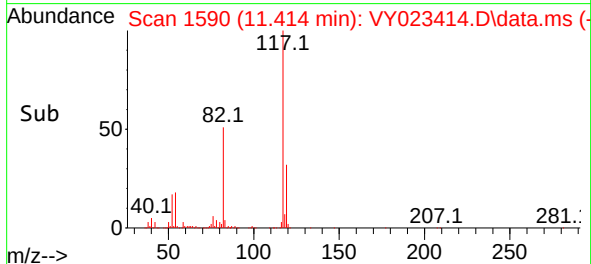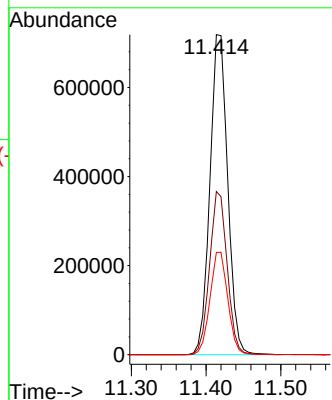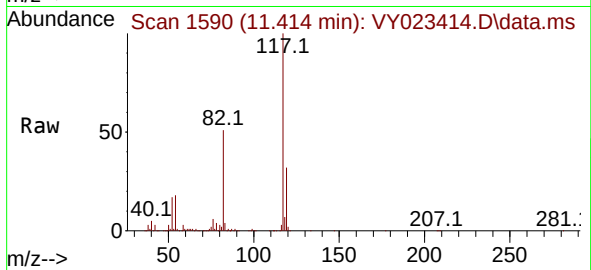

#67

Ethyl Benzene

Concen: 1.033 ug/l

RT: 11.517 min Scan# 1607

Delta R.T. -0.000 min

Lab File: VY023414.D




Acq: 09 Oct 2025 11:47


Tgt Ion: 91 Resp: 43167

Ion Ratio Lower Upper

91 100

106 31.3 25.8 38.8


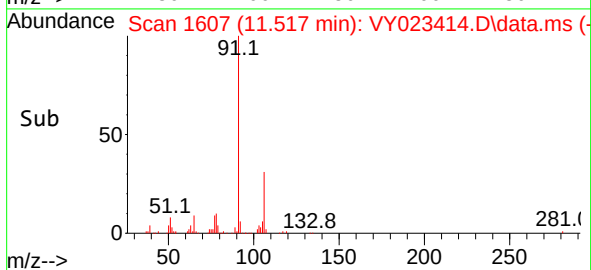
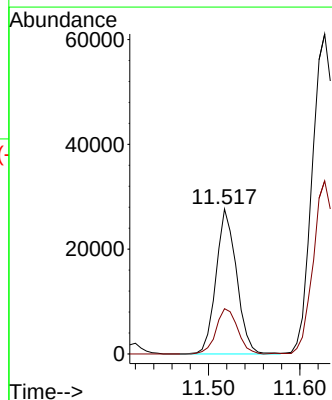
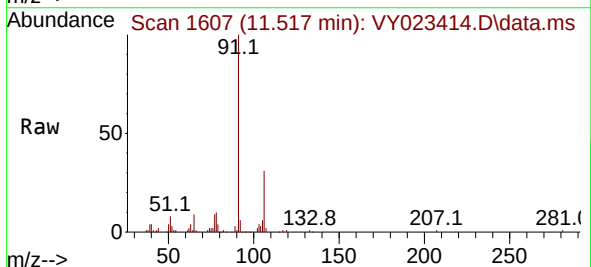


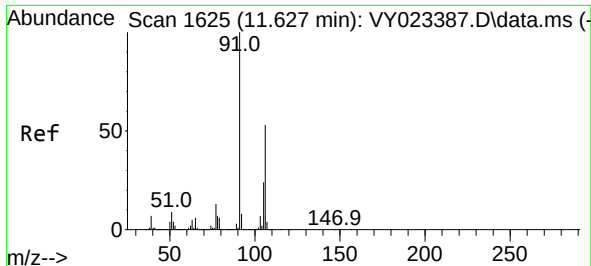

#68
m/p-Xylenes
Concen: 3.455 ug/l
RT: 11.627 min Scan# 1625
Delta R.T. -0.000 min
Lab File: VY023414.D
Acq: 09 Oct 2025 11:47




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-207


Tgt Ion:106 Resp: 57903
Ion Ratio Lower Upper
106 100
91 190.1 152.6 229.0

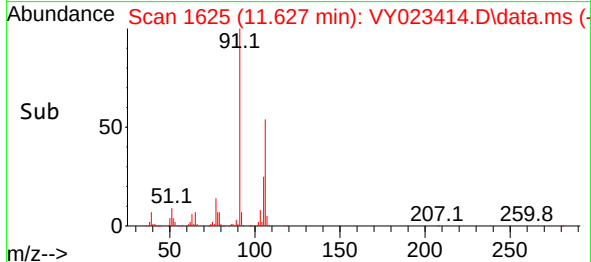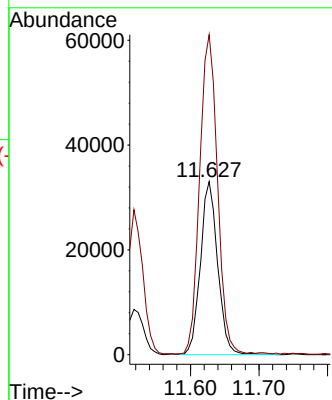

#69
o-Xylene
Concen: 1.771 ug/l
RT: 11.956 min Scan# 1679
Delta R.T. 0.006 min
Lab File: VY023414.D
Acq: 09 Oct 2025 11:47

Tgt Ion:106 Resp: 27838
Ion Ratio Lower Upper
106 100
91 207.6 101.4 304.1

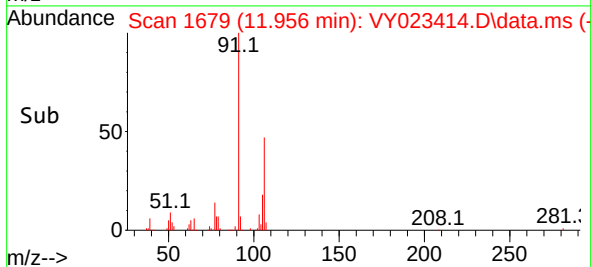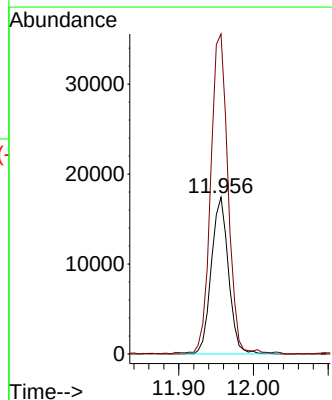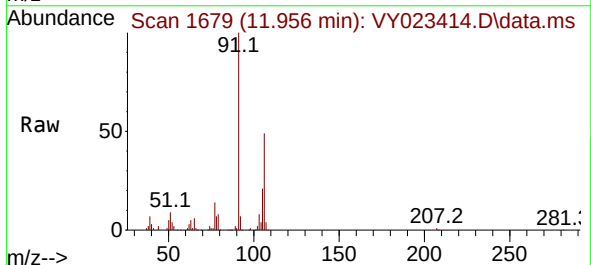



#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.346 min Scan# 1907
 Delta R.T. -0.000 min
 Lab File: VY023414.D
 Acq: 09 Oct 2025 11:47

Instrument :
 MSVOA_Y
 ClientSampleId :
 VNJ-207

Tgt Ion:152 Resp: 518747
 Ion Ratio Lower Upper
 152 100
 115 54.3 27.1 81.2
 150 155.9 0.0 347.4

