
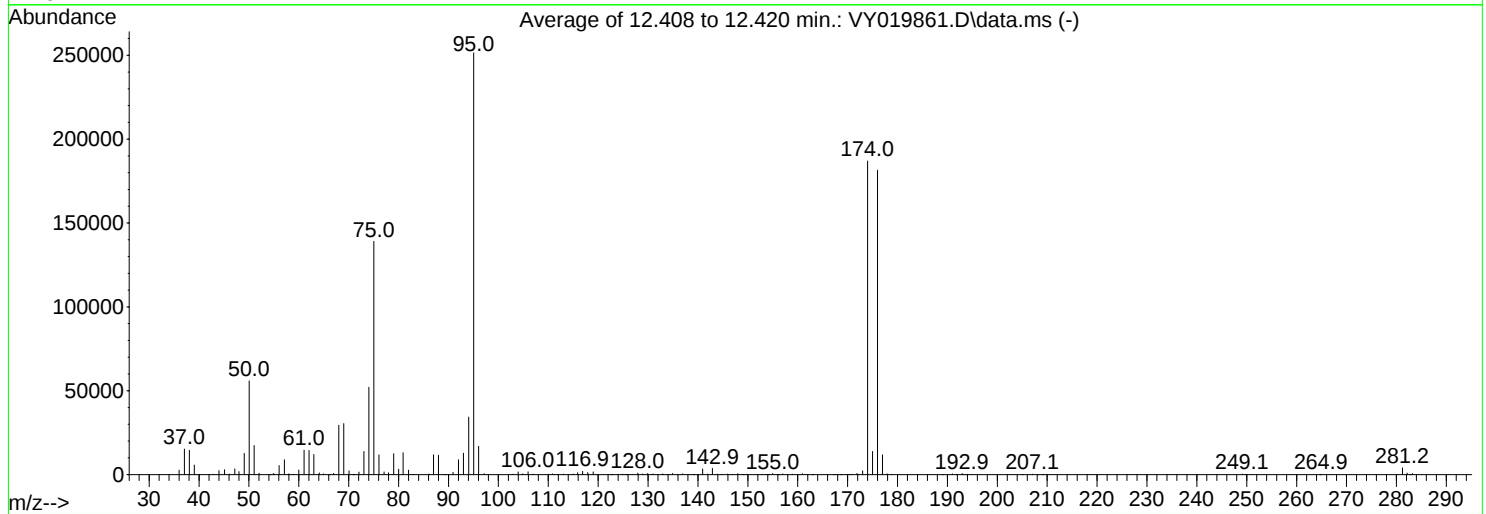


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101124\
Data File : VY019861.D
Acq On : 11 Oct 2024 08:22
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
Title : SW846 8260
Last Update : Thu Oct 10 05:30:07 2024

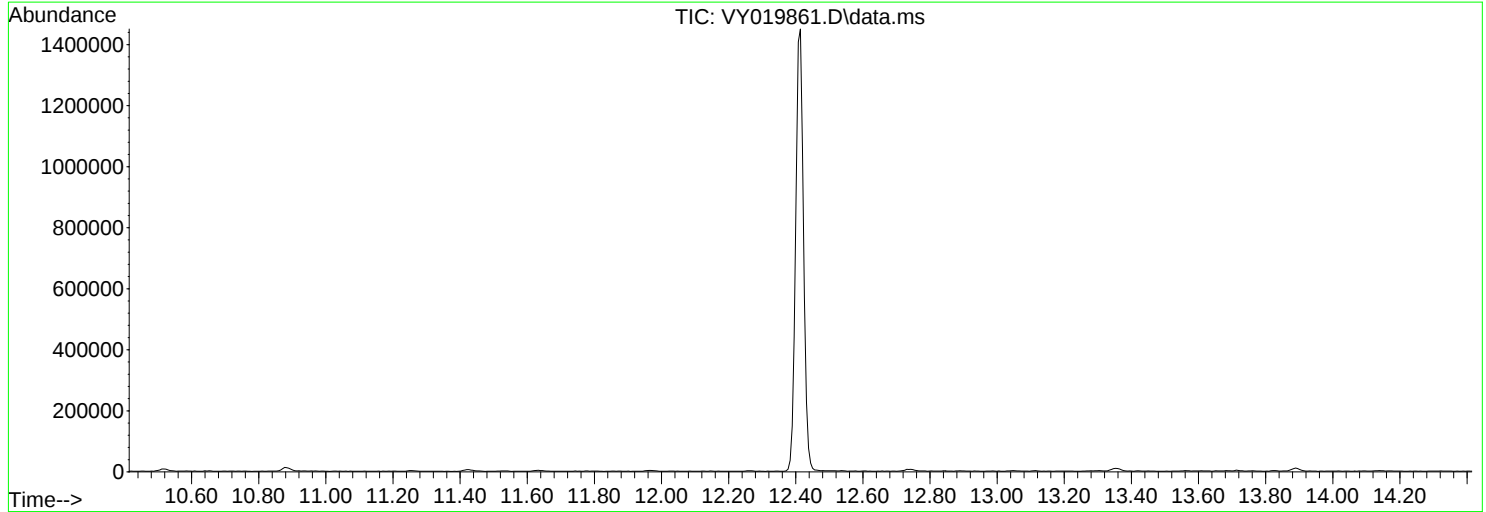

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	55939	PASS
75	95	30	60	55.3	139053	PASS
95	95	100	100	100.0	251435	PASS
96	95	5	9	6.7	16898	PASS
173	174	0.00	2	1.2	2327	PASS
174	95	50	100	74.3	186901	PASS
175	174	5	9	7.4	13866	PASS
176	174	95	101	97.1	181461	PASS
177	176	5	9	6.6	11886	PASS