


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv101419\
Data File : VY000290.D
Acq On : 14 Oct 2019 09:23
Operator : SY/MD
Sample : BFB
Misc : 5.00q/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y101119S.M
Title : SW846 8260
Last Update : Mon Oct 14 08:10:23 2019

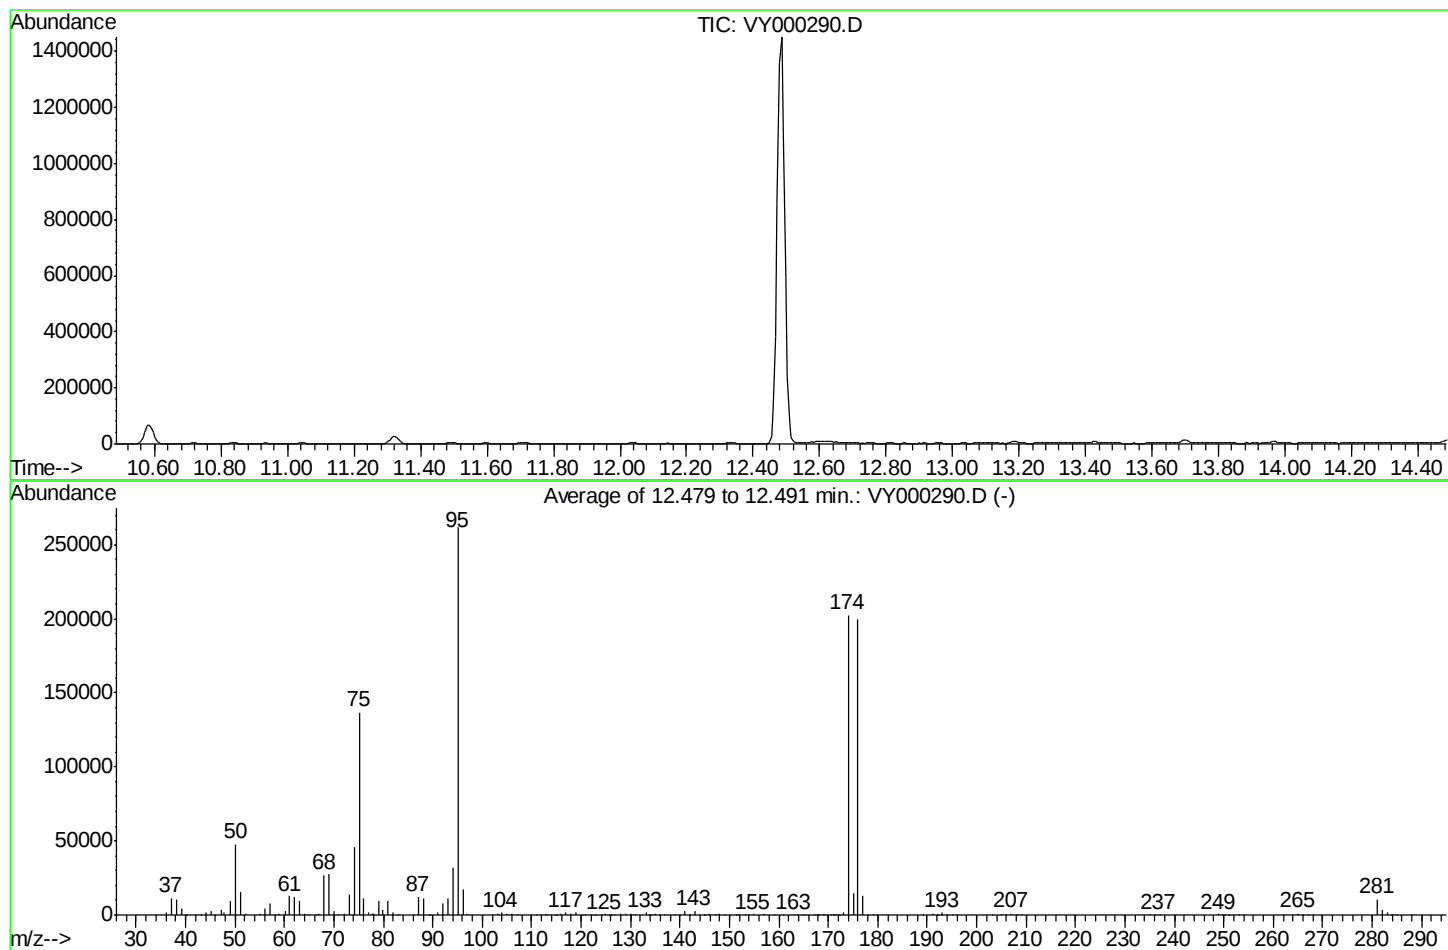

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	47621	PASS
75	95	30	60	52.2	136541	PASS
95	95	100	100	100.0	261674	PASS
96	95	5	9	6.7	17515	PASS
173	174	0.00	2	0.8	1573	PASS
174	95	50	100	77.4	202560	PASS
175	174	5	9	7.1	14476	PASS
176	174	95	101	98.6	199722	PASS
177	176	5	9	6.6	13108	PASS