

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101424\
 Data File : VY019887.D
 Acq On : 14 Oct 2024 13:21
 Operator : SY/MD
 Sample : P4385-11
 Misc : 6.09g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Oct 15 01:36:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 10 05:30:07 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.713	168	255373	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.616	114	522145	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	475654	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	169983	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	179341	57.035	ug/l	0.00
Spiked Amount	50.000	Range 50 - 163	Recovery	= 114.080%		
35) Dibromofluoromethane	7.634	113	173376	50.318	ug/l	0.00
Spiked Amount	50.000	Range 54 - 147	Recovery	= 100.640%		
50) Toluene-d8	10.109	98	639012	50.221	ug/l	0.00
Spiked Amount	50.000	Range 58 - 134	Recovery	= 100.440%		
62) 4-Bromofluorobenzene	12.408	95	200799	43.675	ug/l	0.00
Spiked Amount	50.000	Range 29 - 146	Recovery	= 87.340%		
Target Compounds						
						Qvalue
20) Methylene Chloride	4.616	84	7241	1.614	ug/l	85
31) Cyclohexane	7.713	56	7670	1.460	ug/l #	56
36) 1,1-Dichloropropene	7.713	75	25809	5.199	ug/l #	47
38) Carbon Tetrachloride	7.713	117	28601	5.375	ug/l #	15
76) 1,2,3-Trichloropropane	12.402	75	115680	34.739	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.402	75	115680	140.221	ug/l #	16

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101424\
Data File : VY019887.D
Acq On : 14 Oct 2024 13:21
Operator : SY/MD
Sample : P4385-11
Misc : 6.09g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :

Quant Time: Oct 15 01:36:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 10 05:30:07 2024
Response via : Initial Calibration




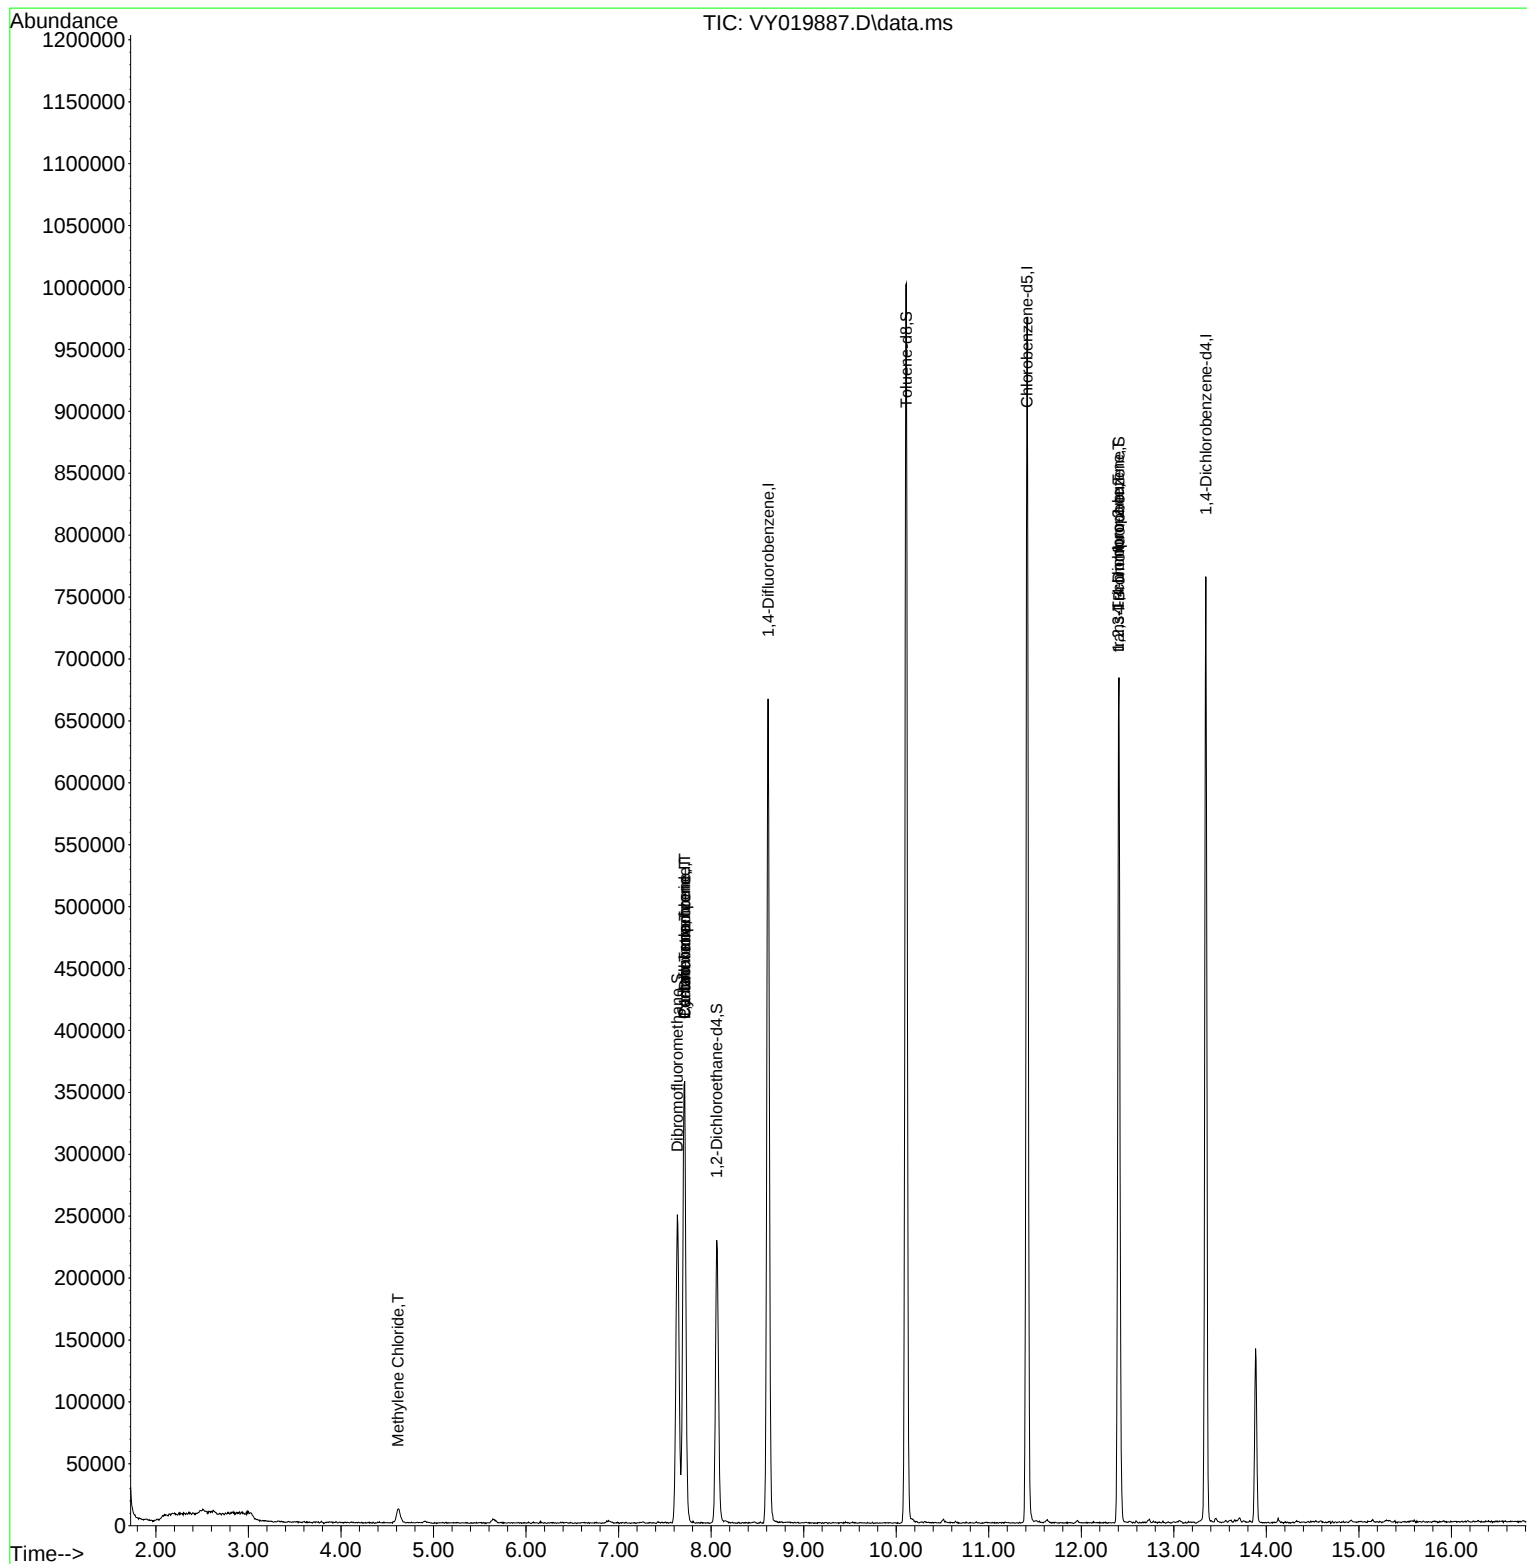




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY019887.D
Acq: 14 Oct 2024 13:21




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:168 Resp: 255373
Ion Ratio Lower Upper
168 100
99 60.5 39.1 58.7#

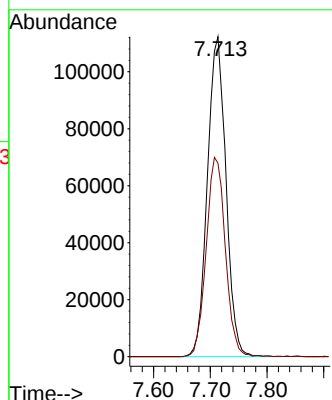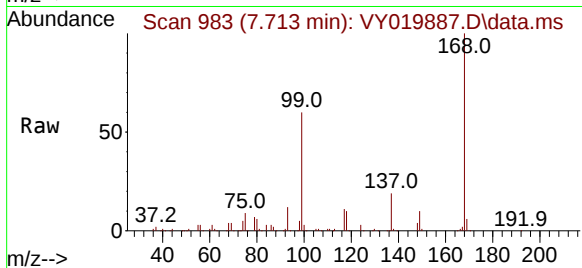

#20
Methylene Chloride
Concen: 1.614 ug/l
RT: 4.616 min Scan# 475
Delta R.T. 0.000 min
Lab File: VY019887.D
Acq: 14 Oct 2024 13:21


Tgt Ion: 84 Resp: 7241
Ion Ratio Lower Upper
84 100
49 126.6 84.4 126.6
51 29.4 26.0 39.0
86 53.1 49.5 74.3

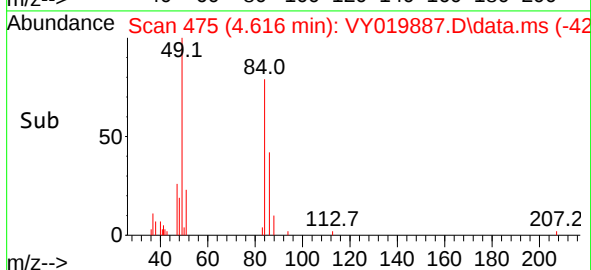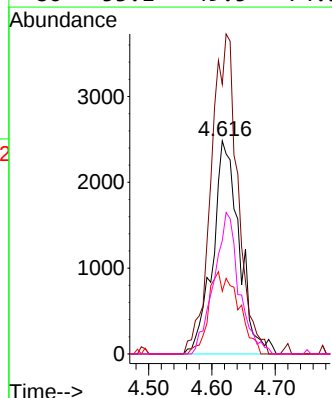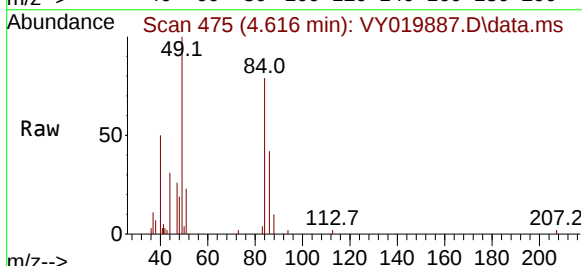






#31
Cyclohexane
Concen: 1.460 ug/l
RT: 7.713 min Scan# 981
Delta R.T. 0.013 min
Lab File: VY019887.D
Acq: 14 Oct 2024 13:21


Instrument :
MSVOA_Y
ClientSampleId :





Tgt Ion: 56 Resp: 7670
Ion Ratio Lower Upper
56 100
69 127.5 28.7 43.1#
84 99.1 77.7 116.5

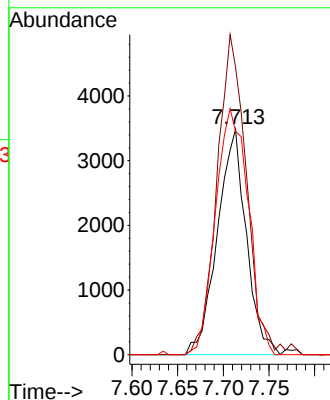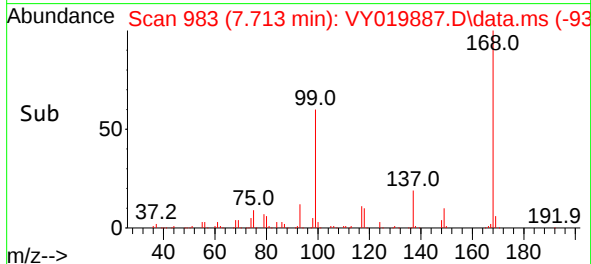


#33
1,2-Dichloroethane-d4
Concen: 57.035 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY019887.D
Acq: 14 Oct 2024 13:21

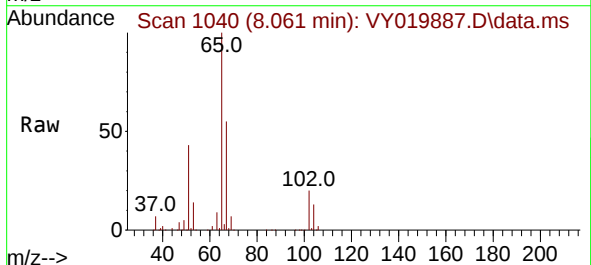


Tgt Ion: 65 Resp: 179341
Ion Ratio Lower Upper
65 100
67 52.5 0.0 109.6

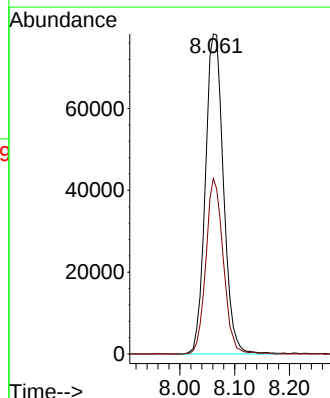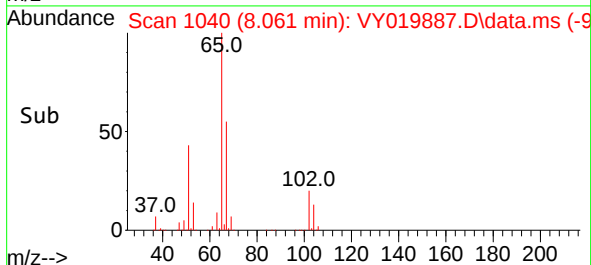






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY019887.D
Acq: 14 Oct 2024 13:21

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion:114 Resp: 522145
Ion Ratio Lower Upper
114 100
63 22.6 0.0 35.0
88 16.0 0.0 27.2

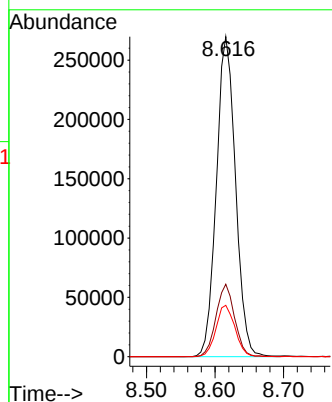

#35
Dibromofluoromethane
Concen: 50.318 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY019887.D
Acq: 14 Oct 2024 13:21


Tgt Ion:113 Resp: 173376
Ion Ratio Lower Upper
113 100
111 104.2 82.2 123.4
192 17.1 15.9 23.9

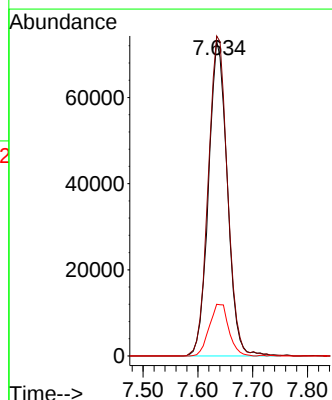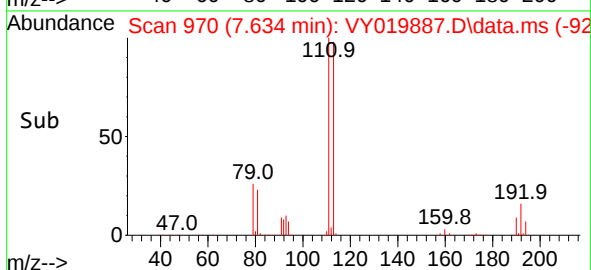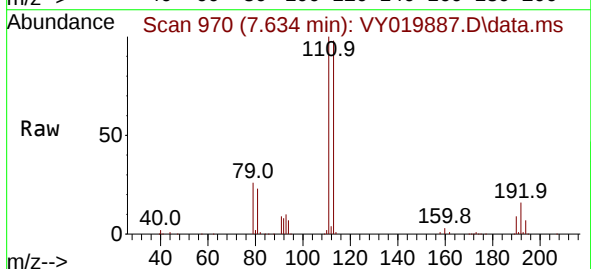






#36
1,1-Dichloropropene
Concen: 5.199 ug/l
RT: 7.713 min Scan# 983
Delta R.T. -0.121 min
Lab File: VY019887.D
Acq: 14 Oct 2024 13:21

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion: 75 Resp: 25809
Ion Ratio Lower Upper
75 100
110 8.3 19.0 57.0#
77 0.0 25.3 37.9#

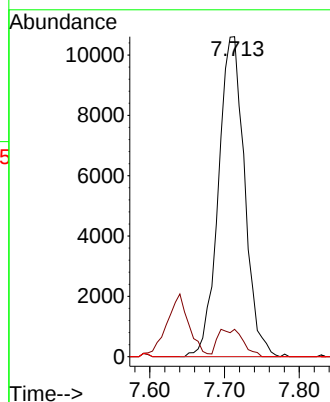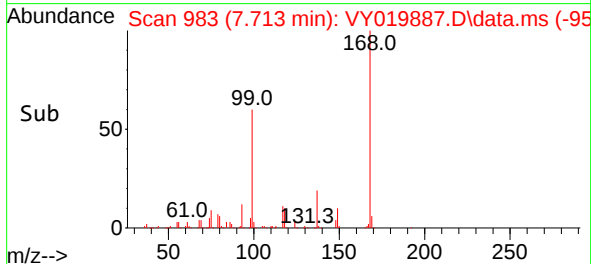

#38
Carbon Tetrachloride
Concen: 5.375 ug/l
RT: 7.713 min Scan# 983
Delta R.T. -0.103 min
Lab File: VY019887.D
Acq: 14 Oct 2024 13:21

Tgt Ion: 117 Resp: 28601
Ion Ratio Lower Upper
117 100
119 2.8 75.8 113.6#
121 0.0 24.0 36.0#


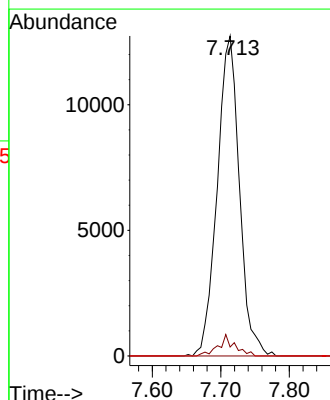

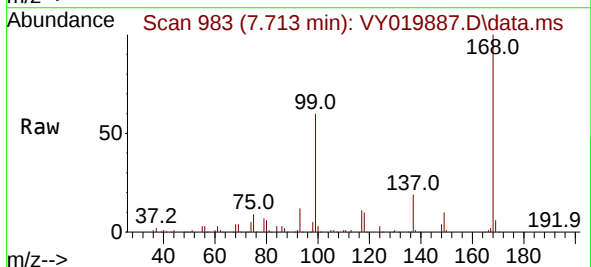




#50
Toluene-d8
Concen: 50.221 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY019887.D
Acq: 14 Oct 2024 13:21




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 98 Resp: 639012
Ion Ratio Lower Upper
98 100
100 64.9 52.0 78.0

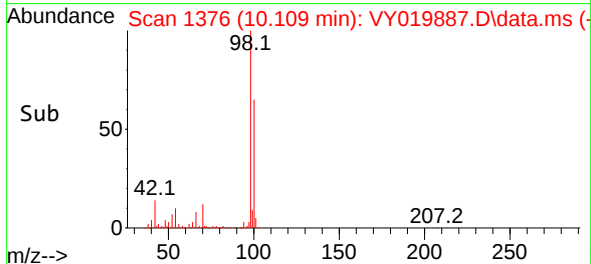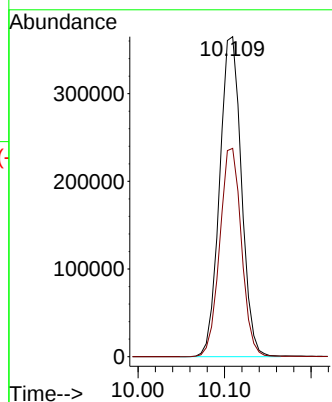

#62
4-Bromofluorobenzene
Concen: 43.675 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.000 min
Lab File: VY019887.D
Acq: 14 Oct 2024 13:21

Tgt Ion: 95 Resp: 200799
Ion Ratio Lower Upper
95 100
174 74.2 0.0 175.6
176 70.0 0.0 171.4

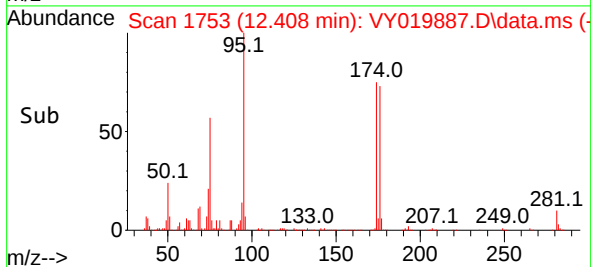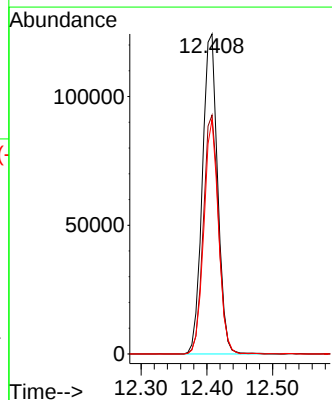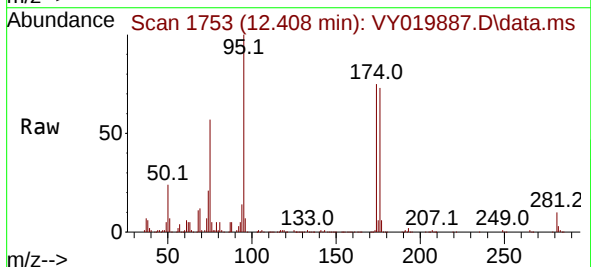



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.006 min


Lab File: VY019887.D

Acq: 14 Oct 2024 13:21

Instrument :

MSVOA_Y

ClientSampleId :






Tgt Ion:117 Resp: 475654

Ion Ratio Lower Upper

117 100

82 60.7 42.4 63.6

119 32.6 25.9 38.9

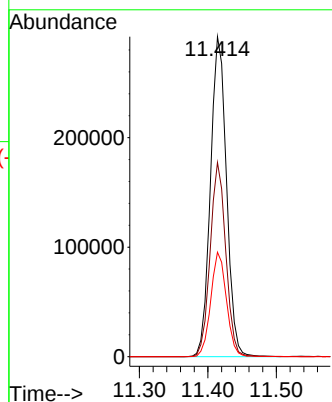

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY019887.D

Acq: 14 Oct 2024 13:21




Tgt Ion:152 Resp: 169983


Ion Ratio Lower Upper

152 100

115 63.4 28.2 84.7

150 160.4 0.0 345.6


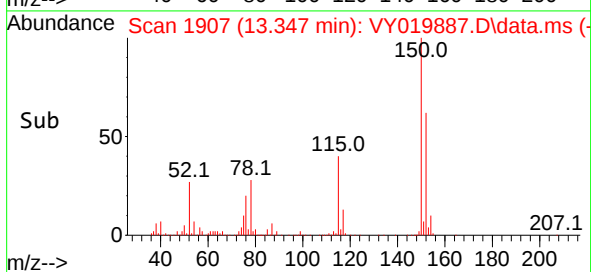

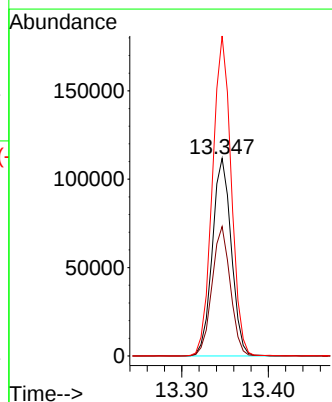




#76
1,2,3-Trichloropropane
Concen: 34.739 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. -0.158 min
Lab File: VY019887.D
Acq: 14 Oct 2024 13:21

Instrument :
MSVOA_Y
ClientSampleId :

Tgt Ion: 75 Resp: 115680
Ion Ratio Lower Upper
75 100
77 1.5 0.0 0.0#

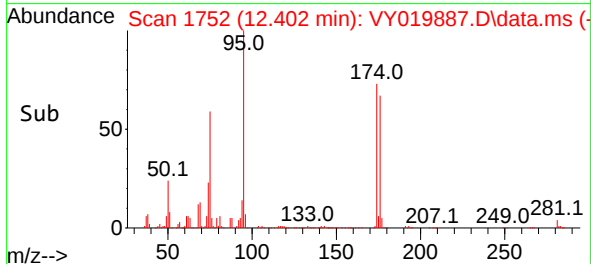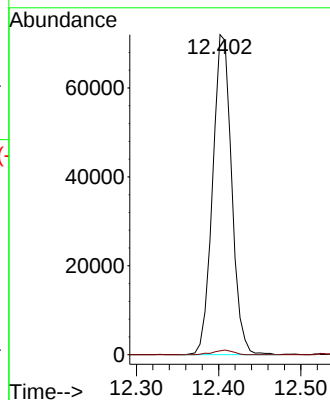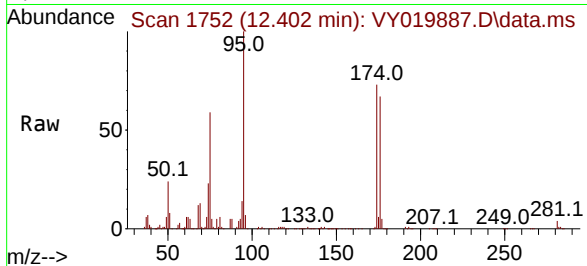

#81
trans-1,4-Dichloro-2-butene
Concen: 140.221 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. 0.098 min
Lab File: VY019887.D
Acq: 14 Oct 2024 13:21

Tgt Ion: 75 Resp: 115680
Ion Ratio Lower Upper
75 100
53 0.1 66.8 100.2#
89 0.2 35.8 53.6#

