

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101424\
 Data File : VY019892.D
 Acq On : 14 Oct 2024 15:22
 Operator : SY/MD
 Sample : P4403-01
 Misc : 4.16g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 Hawthorne TP Soil

Quant Time: Oct 15 01:38:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 10 05:30:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	297149	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.616	114	612839	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	548156	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	198699	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	190268	52.003	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	104.000%
35) Dibromofluoromethane	7.634	113	196503	48.590	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	97.180%
50) Toluene-d8	10.109	98	744580	49.857	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	99.720%
62) 4-Bromofluorobenzene	12.408	95	232289	43.047	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	86.100%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101424\
Data File : VY019892.D
Acq On : 14 Oct 2024 15:22
Operator : SY/MD
Sample : P4403-01
Misc : 4.16g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
Hawthorne TP Soil

Quant Time: Oct 15 01:38:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 10 05:30:07 2024
Response via : Initial Calibration




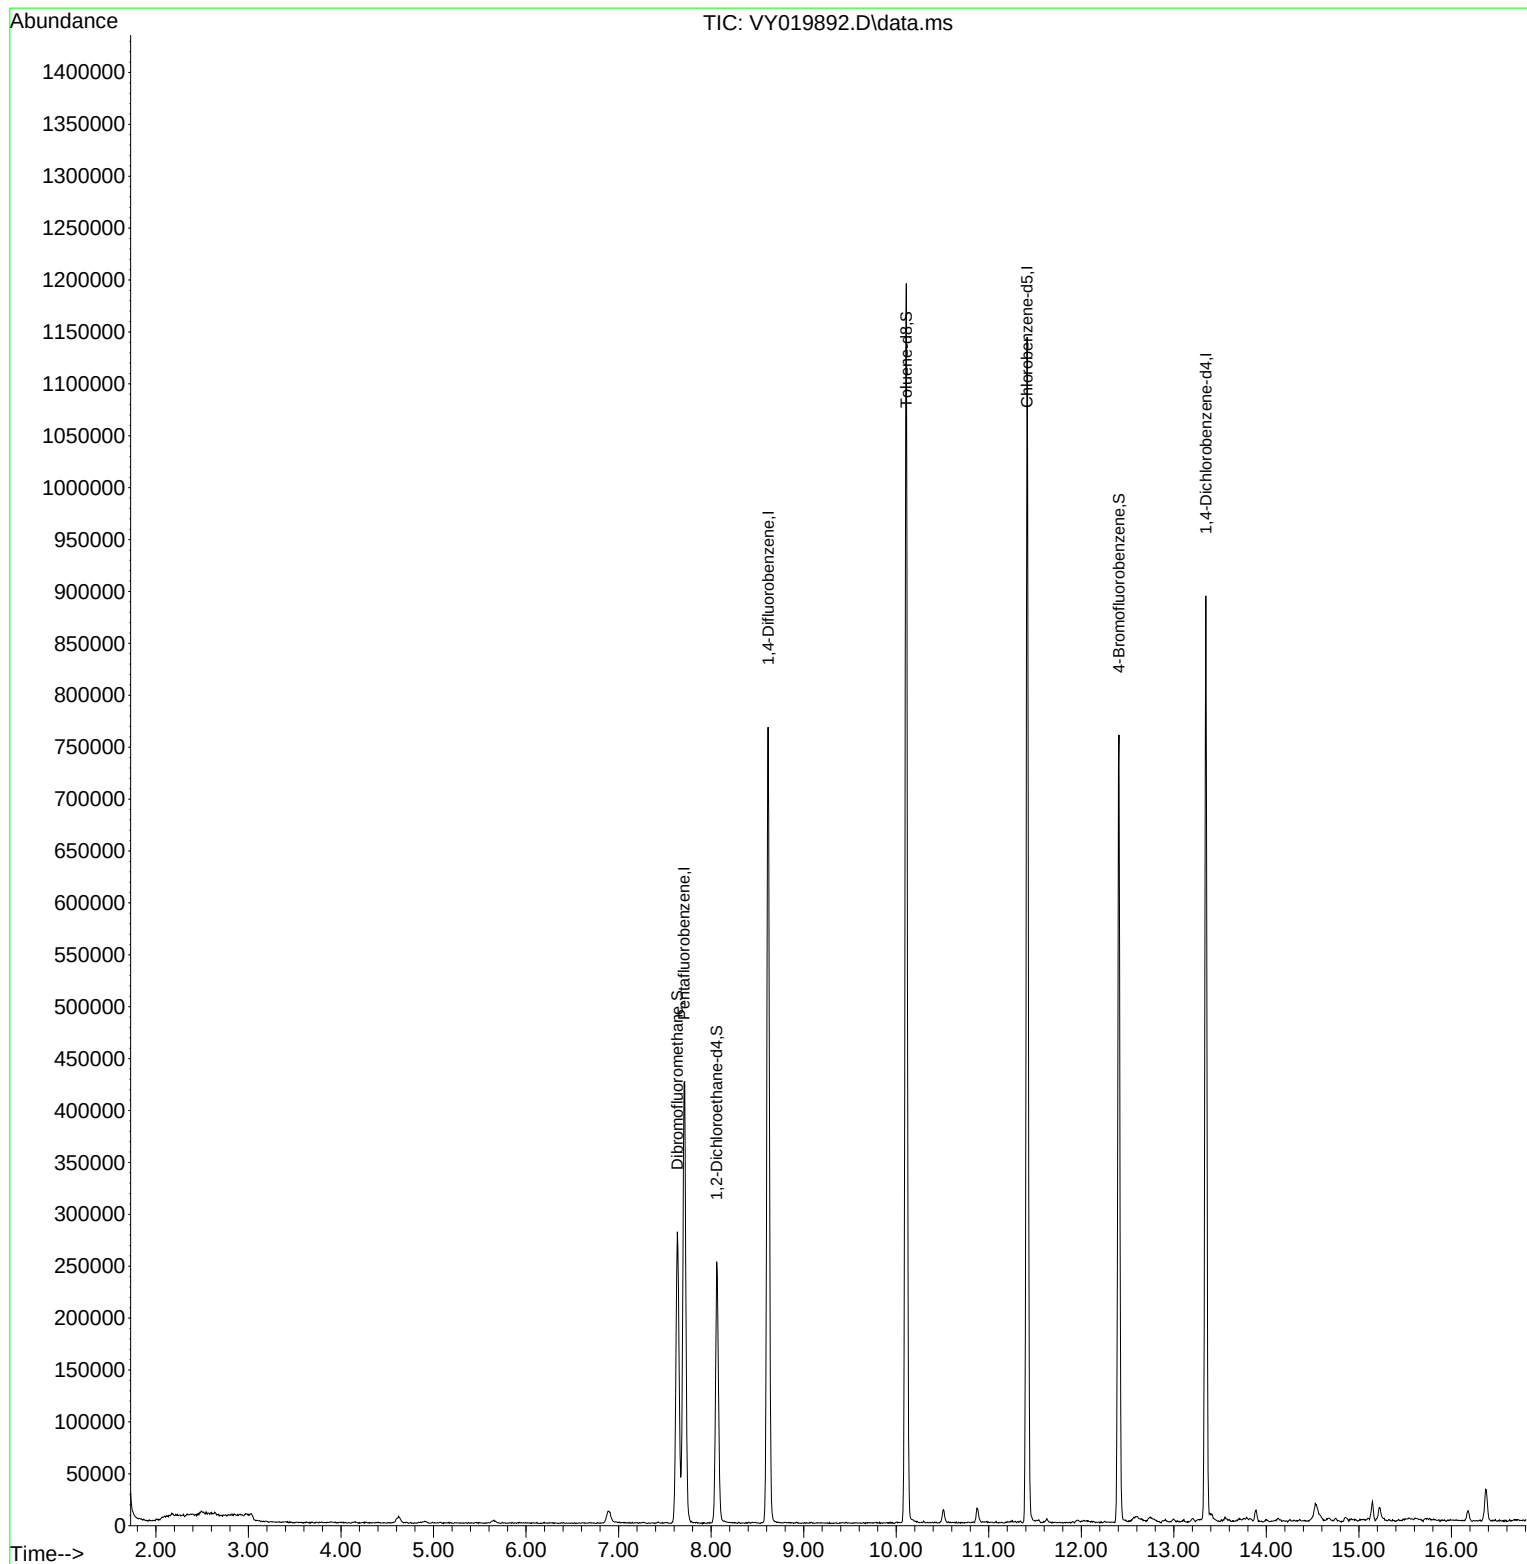


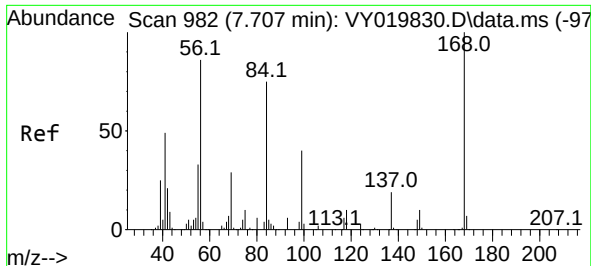

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY019892.D
Acq: 14 Oct 2024 15:22




Instrument :
MSVOA_Y
ClientSampleId :
Hawthorne TP Soil


Tgt Ion:168 Resp: 297149
Ion Ratio Lower Upper
168 100
99 66.1 39.1 58.7#

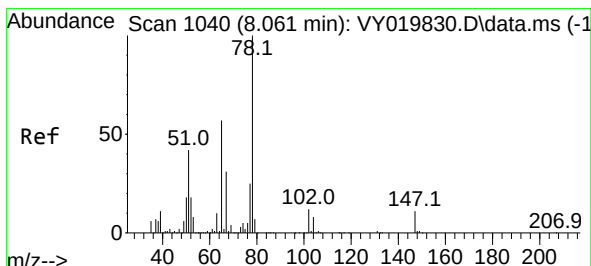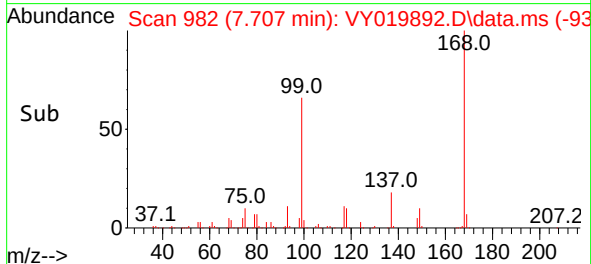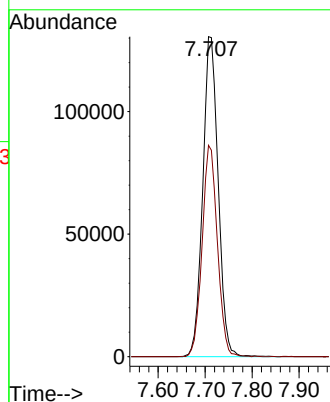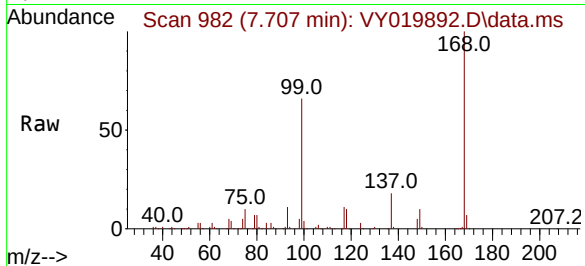

#33
1,2-Dichloroethane-d4
Concen: 52.003 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY019892.D
Acq: 14 Oct 2024 15:22

Tgt Ion: 65 Resp: 190268
Ion Ratio Lower Upper
65 100
67 51.8 0.0 109.6


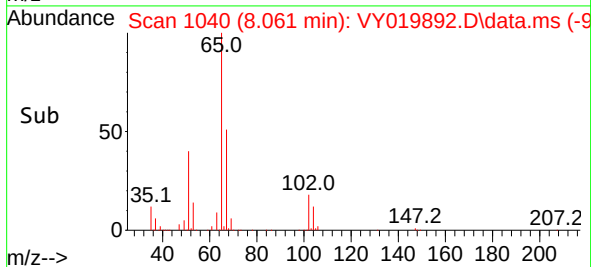
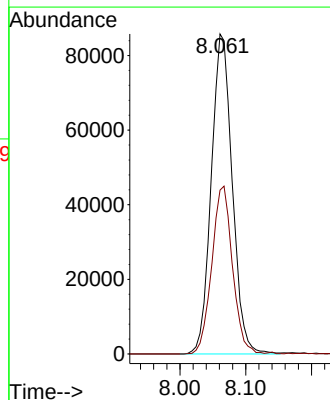
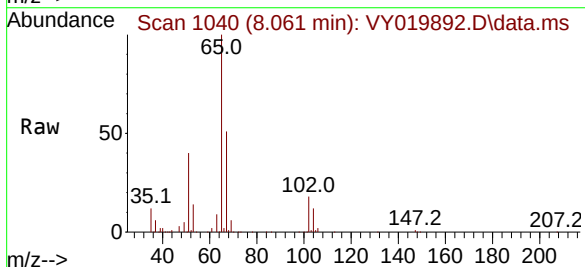


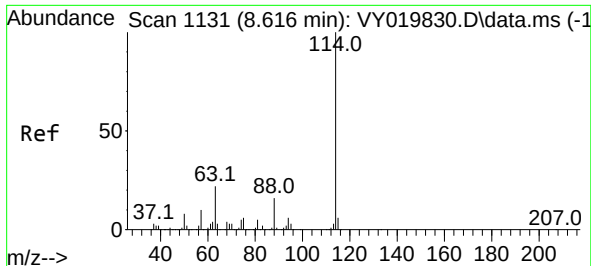

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY019892.D
Acq: 14 Oct 2024 15:22




Instrument :
MSVOA_Y
ClientSampleId :
Hawthorne TP Soil


Tgt Ion:114 Resp: 612839
Ion Ratio Lower Upper
114 100
63 22.2 0.0 35.0
88 16.1 0.0 27.2

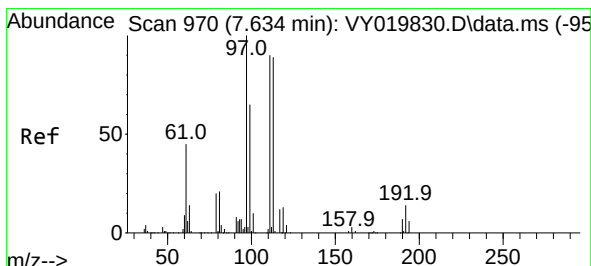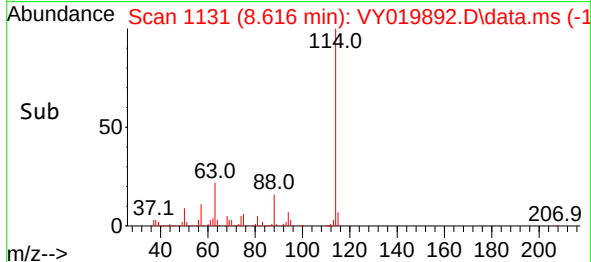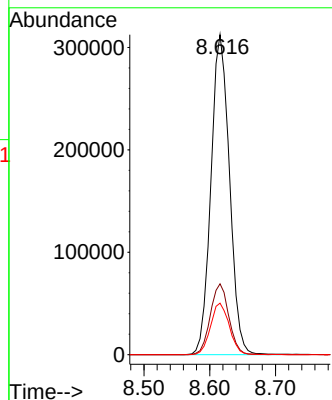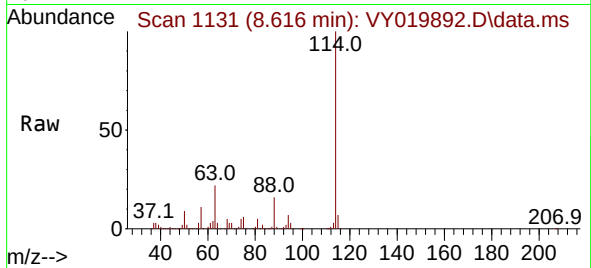

#35
Dibromofluoromethane
Concen: 48.590 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY019892.D
Acq: 14 Oct 2024 15:22

Tgt Ion:113 Resp: 196503
Ion Ratio Lower Upper
113 100
111 102.5 82.2 123.4
192 16.7 15.9 23.9


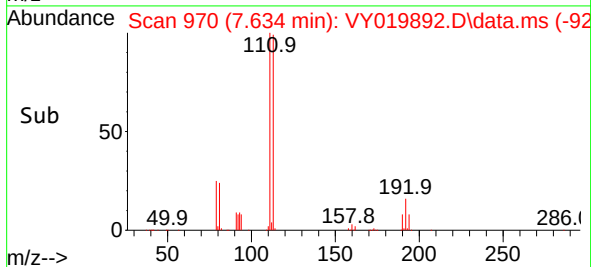
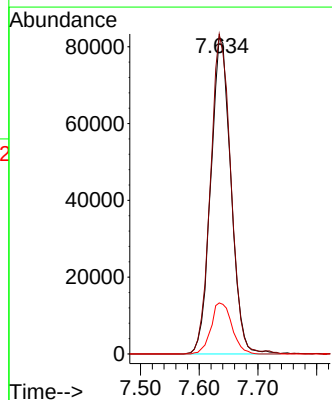
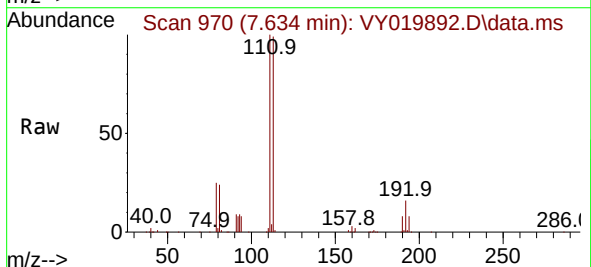


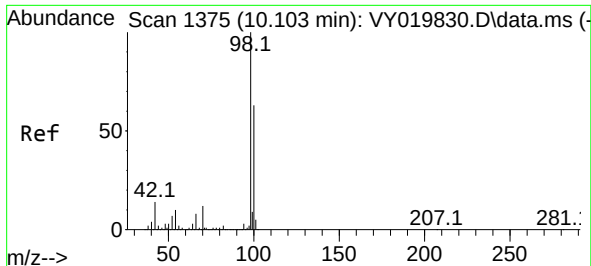

#50
Toluene-d8
Concen: 49.857 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY019892.D
Acq: 14 Oct 2024 15:22




Instrument :
MSVOA_Y
ClientSampleId :
Hawthorne TP Soil


Tgt Ion: 98 Resp: 744580
Ion Ratio Lower Upper
98 100
100 64.0 52.0 78.0

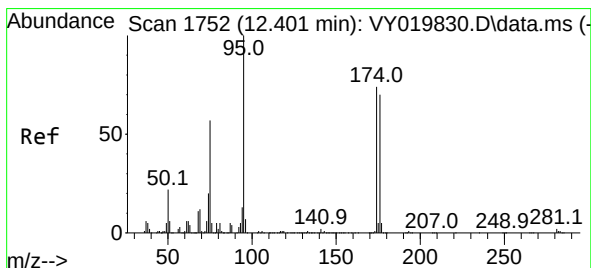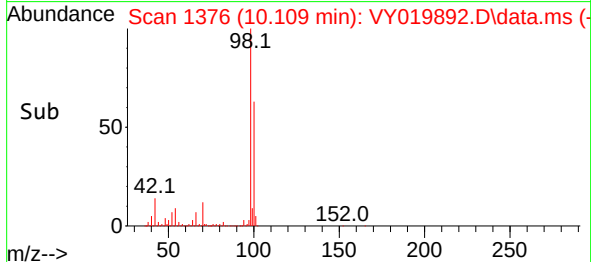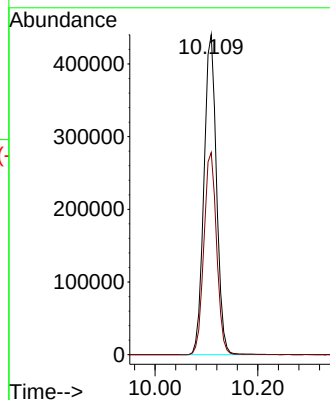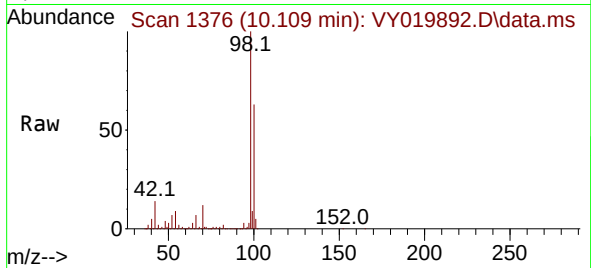

#62
4-Bromofluorobenzene
Concen: 43.047 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.000 min
Lab File: VY019892.D
Acq: 14 Oct 2024 15:22

Tgt Ion: 95 Resp: 232289
Ion Ratio Lower Upper
95 100
174 72.7 0.0 175.6
176 69.6 0.0 171.4

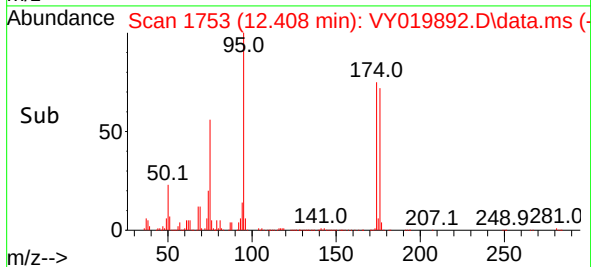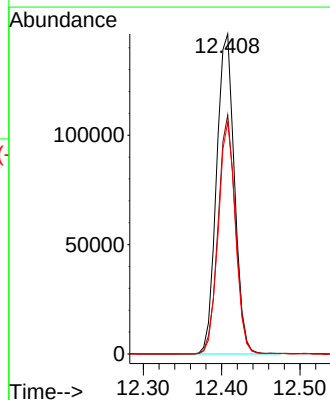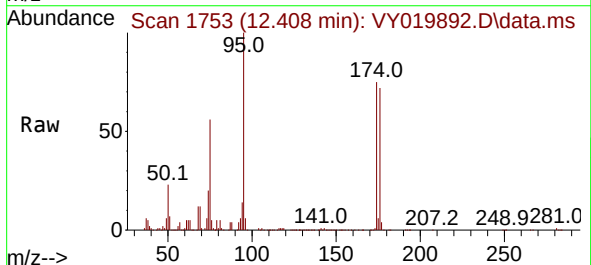

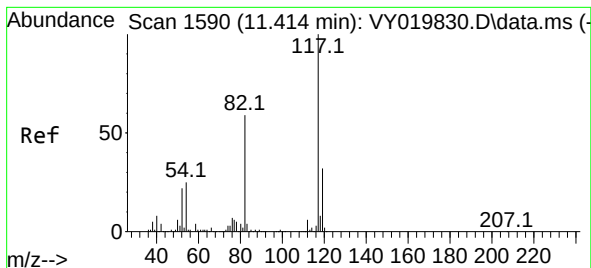

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY019892.D

Acq: 14 Oct 2024 15:22

Instrument :

MSVOA_Y

ClientSampleId :

Hawthorne TP Soil





Tgt Ion:117 Resp: 548156

Ion Ratio Lower Upper

117 100

82 60.2 42.4 63.6

119 32.1 25.9 38.9

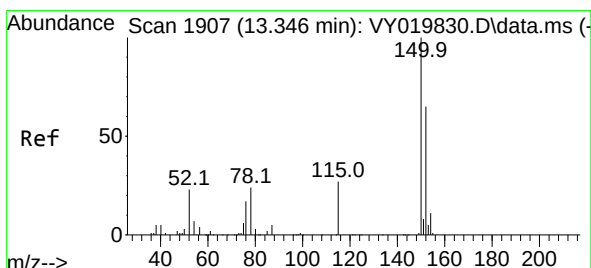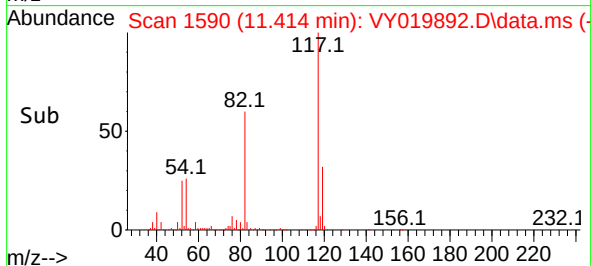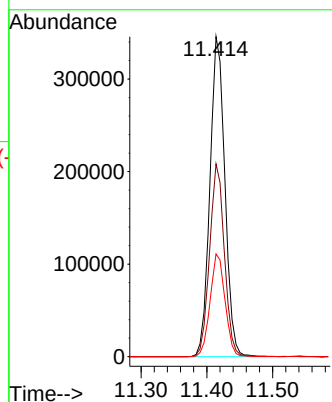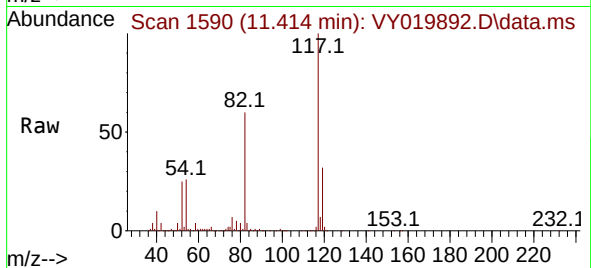

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY019892.D

Acq: 14 Oct 2024 15:22

Tgt Ion:152 Resp: 198699

Ion Ratio Lower Upper

152 100

115 63.2 28.2 84.7

150 159.5 0.0 345.6

