
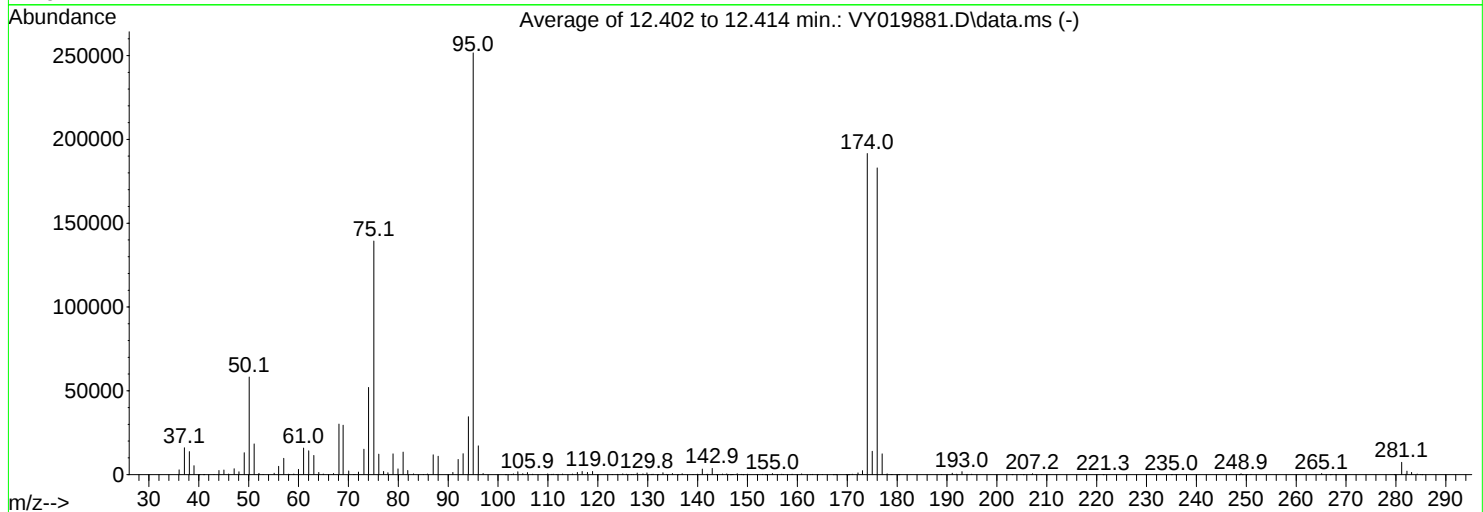


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY0101424\
Data File : VY019881.D
Acq On : 14 Oct 2024 09:19
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
Title : SW846 8260
Last Update : Thu Oct 10 05:30:07 2024

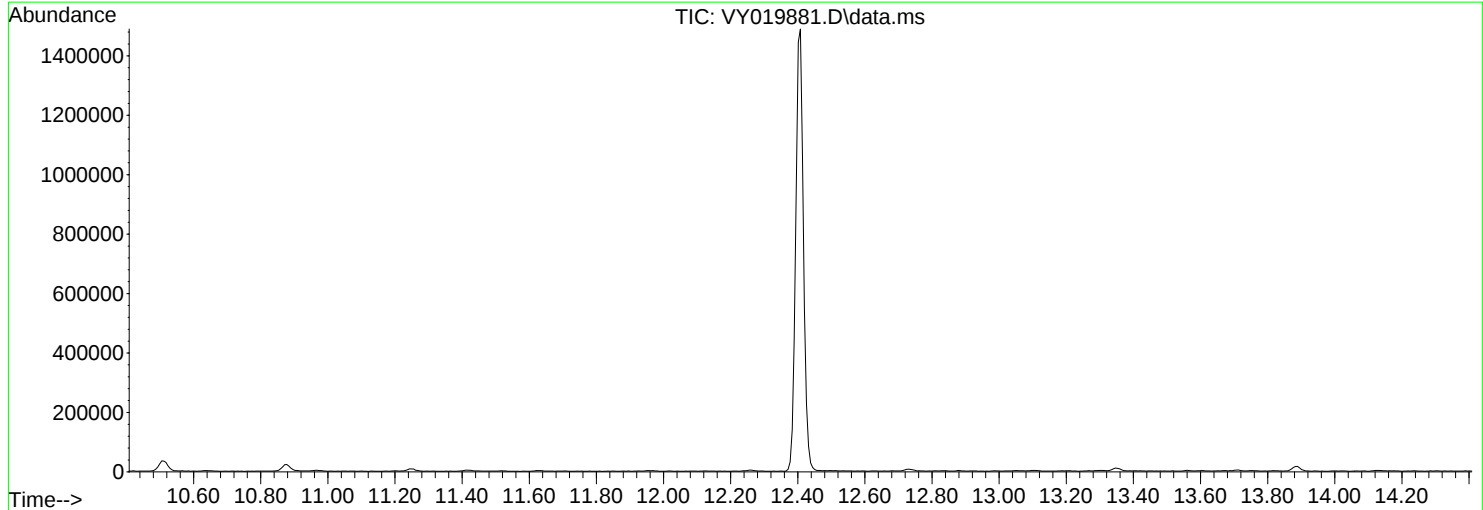

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	58240	PASS
75	95	30	60	55.4	139389	PASS
95	95	100	100	100.0	251627	PASS
96	95	5	9	6.8	17153	PASS
173	174	0.00	2	1.2	2378	PASS
174	95	50	100	76.1	191573	PASS
175	174	5	9	7.3	13966	PASS
176	174	95	101	95.5	182955	PASS
177	176	5	9	6.8	12416	PASS