
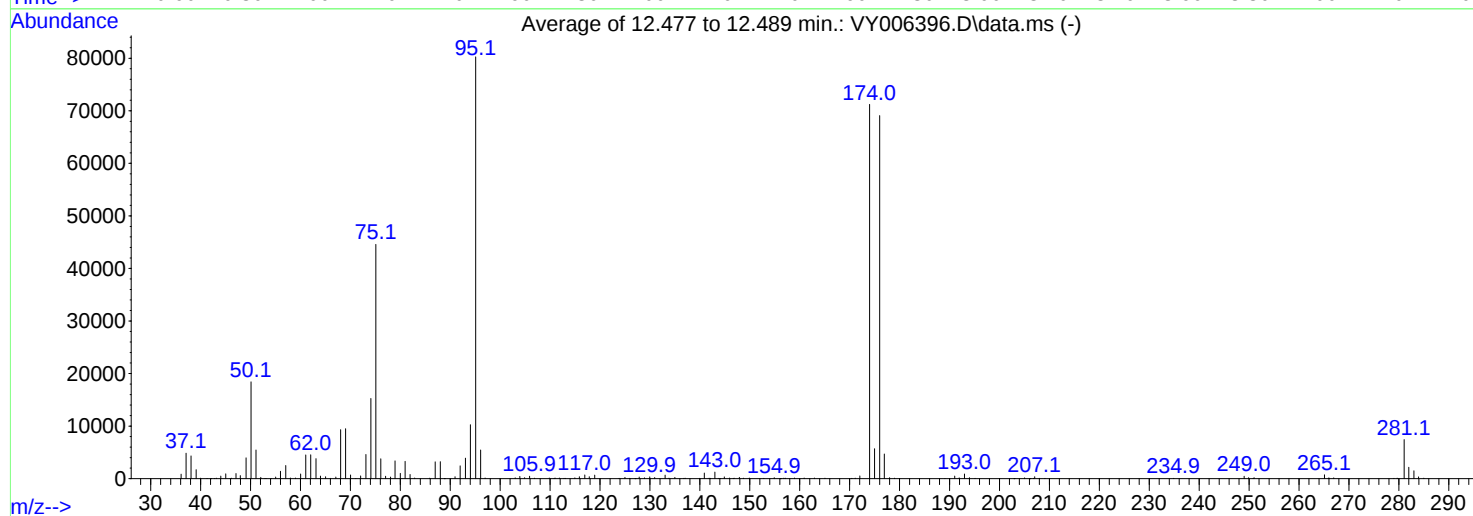


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY101521\  
Data File : VY006396.D  
Acq On : 15 Oct 2021 08:48  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00G/5ML/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y092821S.M  
Title : SW846 8260  
Last Update : Tue Sep 28 17:44:36 2021

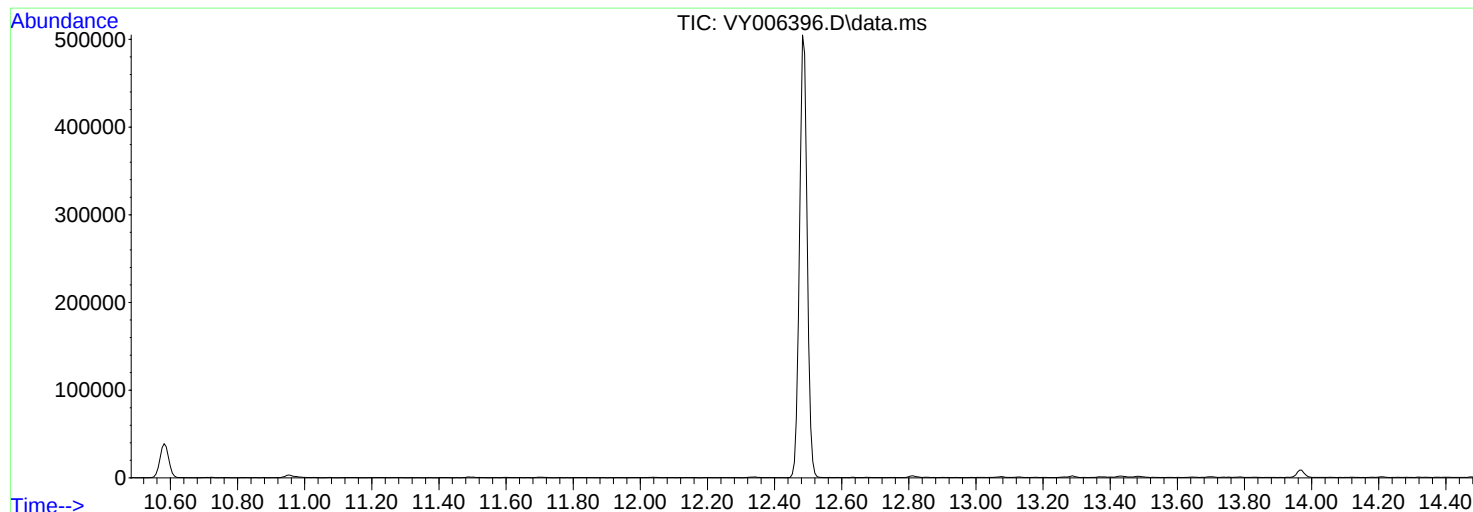

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 22.9         | 18410      | PASS                |
| 75             | 95              | 30              | 60              | 55.5         | 44576      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 80267      | PASS                |
| 96             | 95              | 5               | 9               | 6.8          | 5439       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 174            | 95              | 50              | 100             | 88.7         | 71208      | PASS                |
| 175            | 174             | 5               | 9               | 8.0          | 5700       | PASS                |
| 176            | 174             | 95              | 101             | 97.0         | 69088      | PASS                |
| 177            | 176             | 5               | 9               | 6.8          | 4697       | PASS                |