

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102224\
 Data File : VY019970.D
 Acq On : 22 Oct 2024 10:36
 Operator : SY/MD
 Sample : VY1022SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1022SBL01

Quant Time: Oct 23 01:24:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 16 05:44:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	219150	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.616	114	450425	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	395647	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	132931	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	150698	55.848	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	111.700%
35) Dibromofluoromethane	7.634	113	145305	48.886	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	97.780%
50) Toluene-d8	10.109	98	554994	50.563	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	101.120%
62) 4-Bromofluorobenzene	12.408	95	159930	40.325	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	80.640%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102224\
Data File : VY019970.D
Acq On : 22 Oct 2024 10:36
Operator : SY/MD
Sample : VY1022SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1022SBL01

Quant Time: Oct 23 01:24:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 16 05:44:48 2024
Response via : Initial Calibration




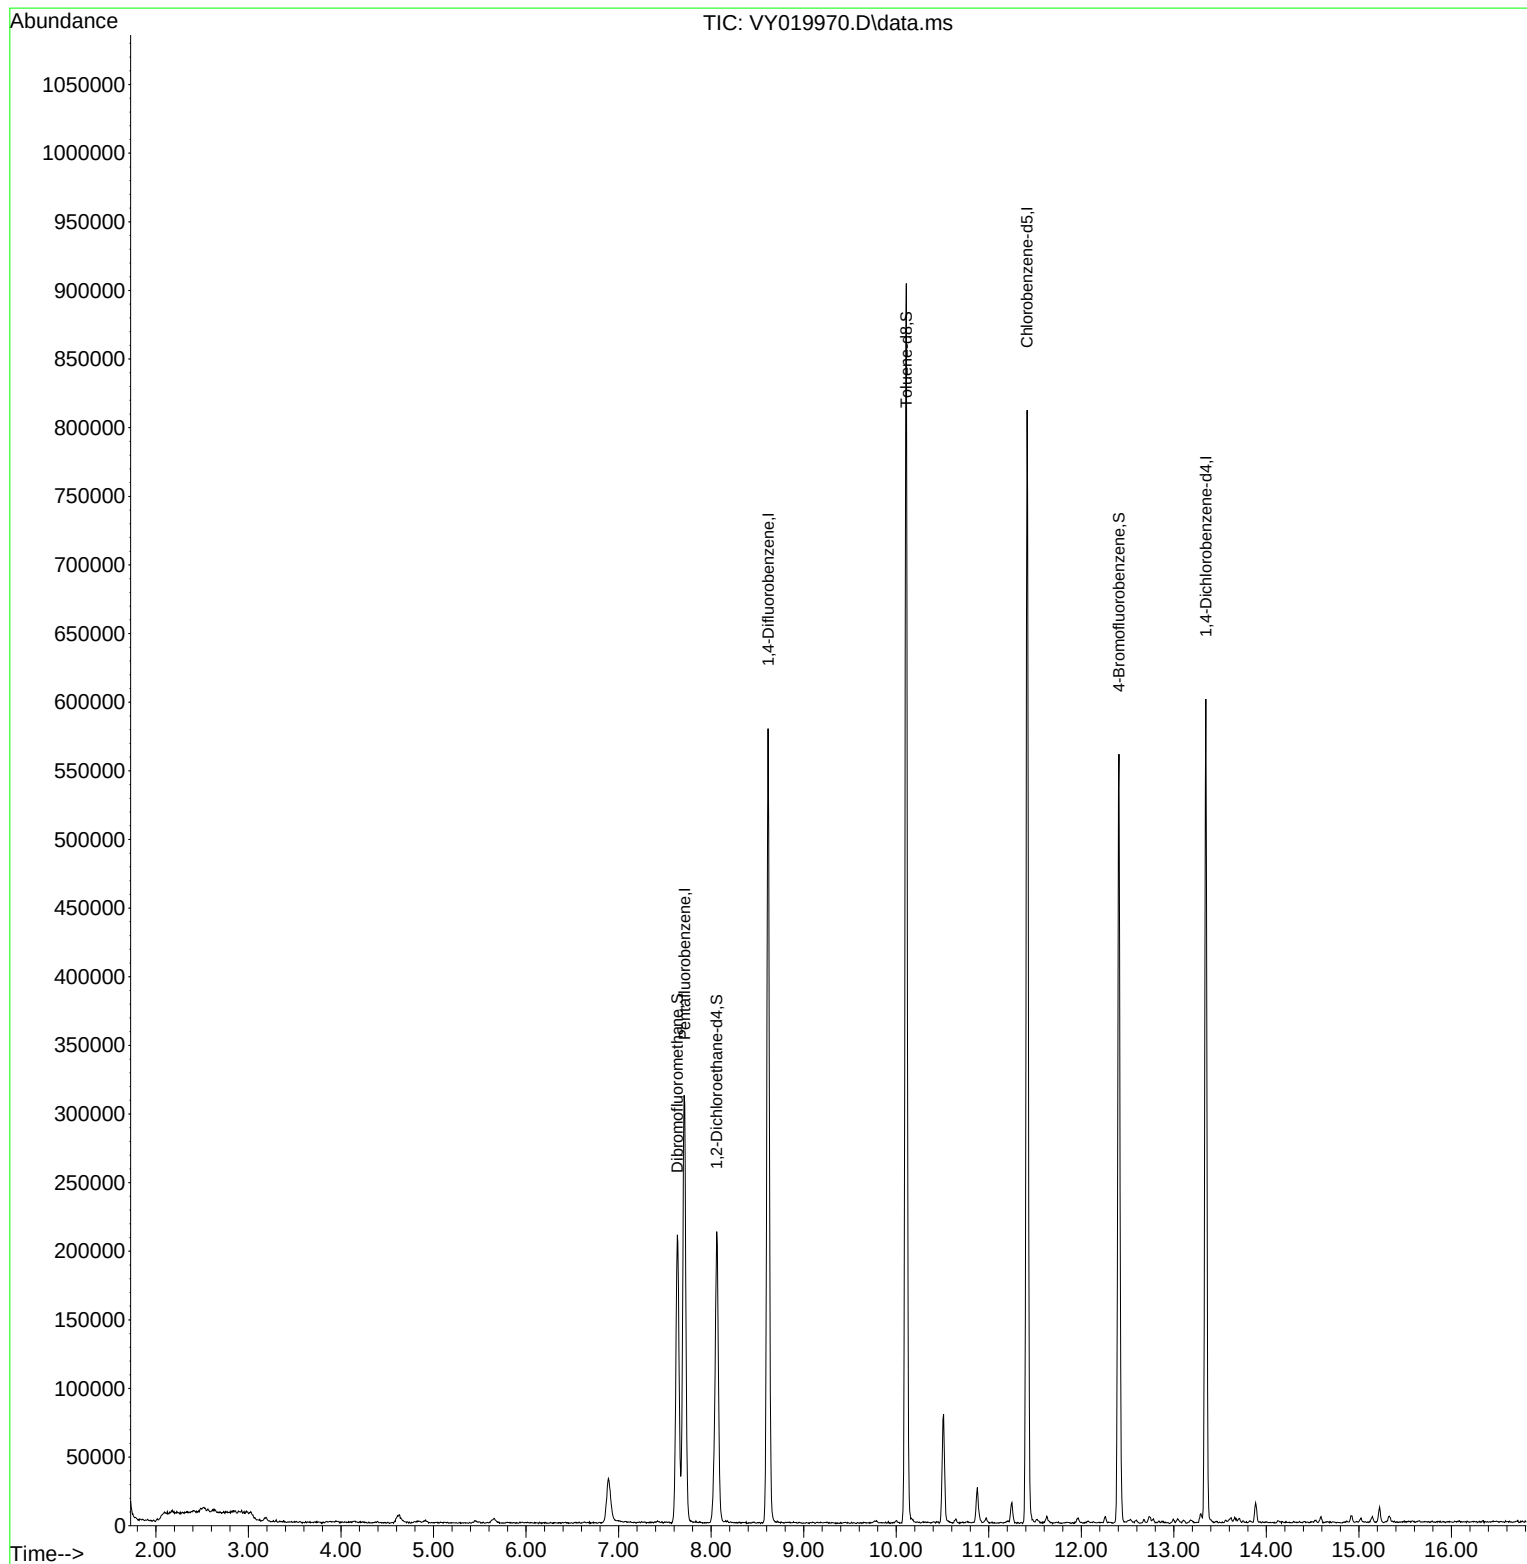


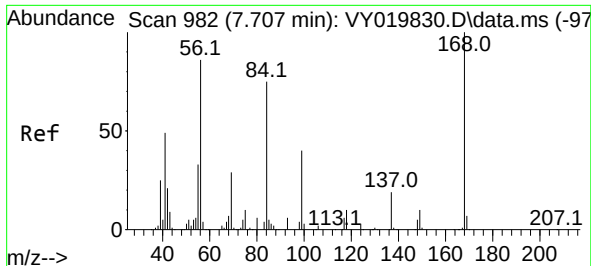

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY019970.D
Acq: 22 Oct 2024 10:36




Instrument :
MSVOA_Y
ClientSampleId :
VY1022SBL01


Tgt Ion:168 Resp: 219150
Ion Ratio Lower Upper
168 100
99 64.0 39.1 58.7#

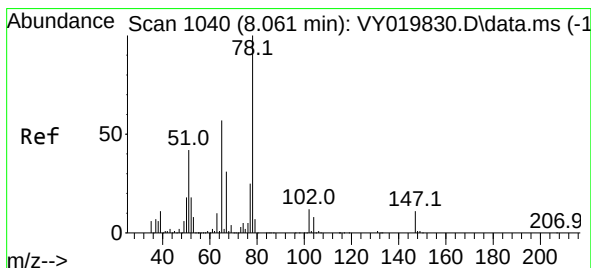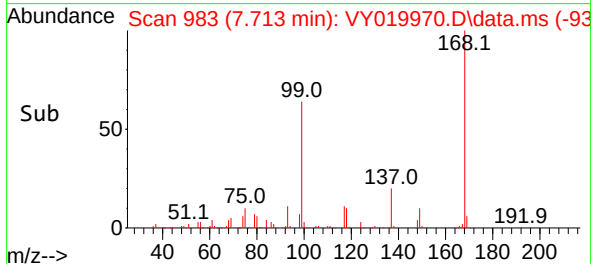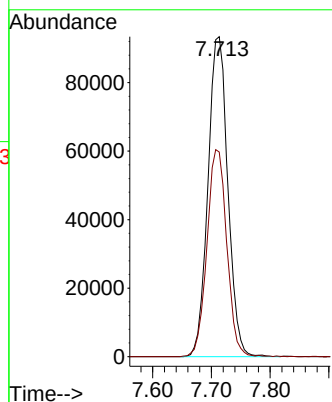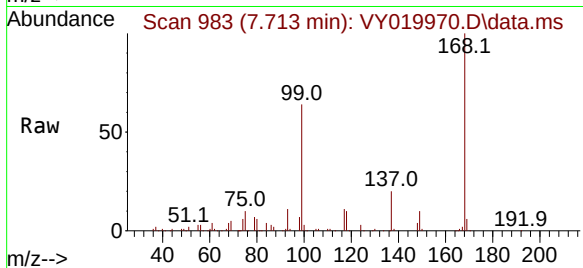

#33
1,2-Dichloroethane-d4
Concen: 55.848 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY019970.D
Acq: 22 Oct 2024 10:36

Tgt Ion: 65 Resp: 150698
Ion Ratio Lower Upper
65 100
67 51.0 0.0 109.6


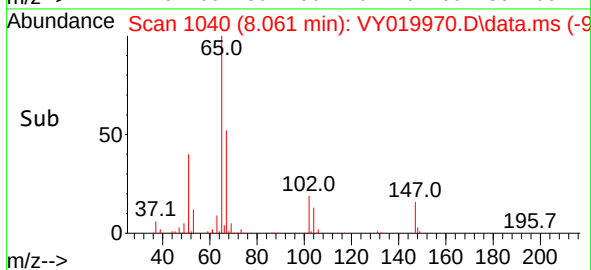
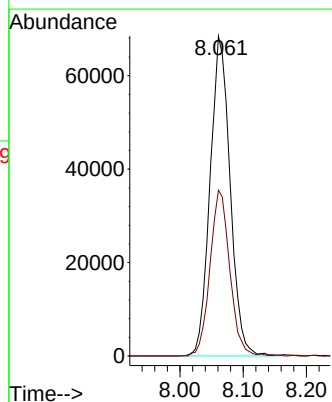
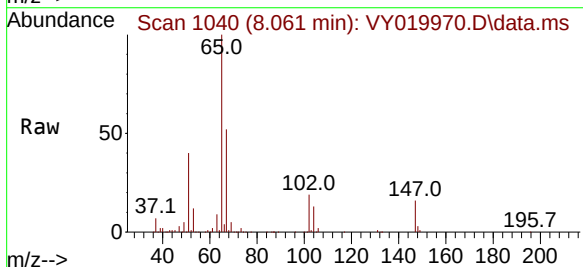


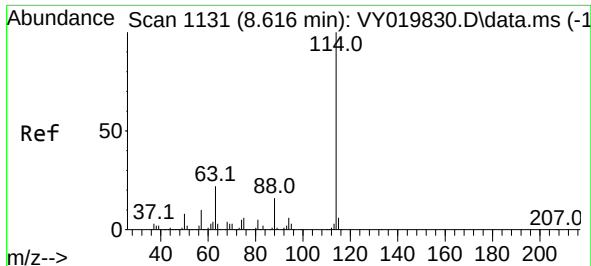

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY019970.D
Acq: 22 Oct 2024 10:36




Instrument :
MSVOA_Y
ClientSampleId :
VY1022SBL01


Tgt Ion:114 Resp: 450425
Ion Ratio Lower Upper
114 100
63 21.4 0.0 35.0
88 15.5 0.0 27.2

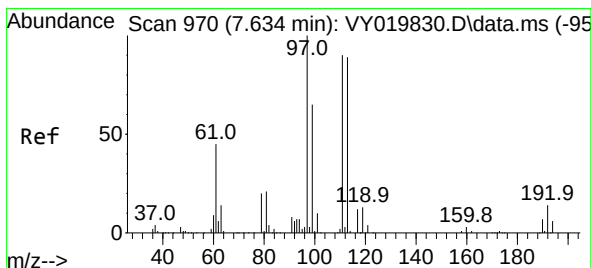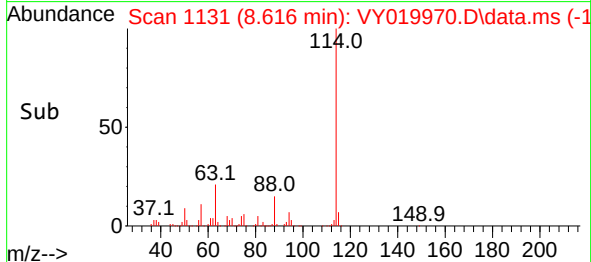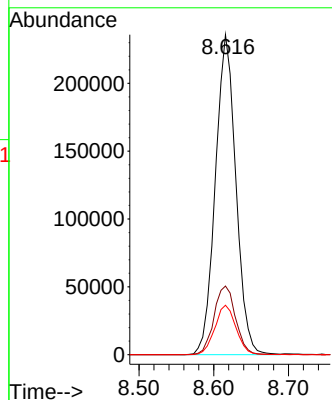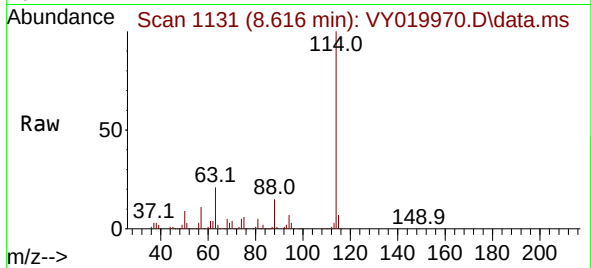

#35
Dibromofluoromethane
Concen: 48.886 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY019970.D
Acq: 22 Oct 2024 10:36

Tgt Ion:113 Resp: 145305
Ion Ratio Lower Upper
113 100
111 103.8 82.2 123.4
192 17.1 15.9 23.9


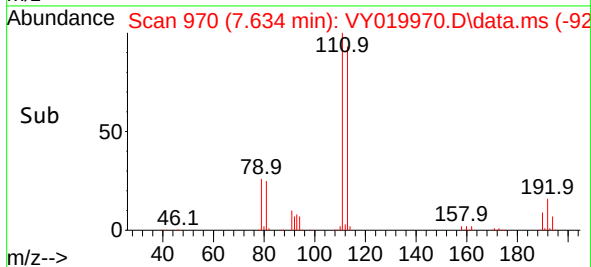
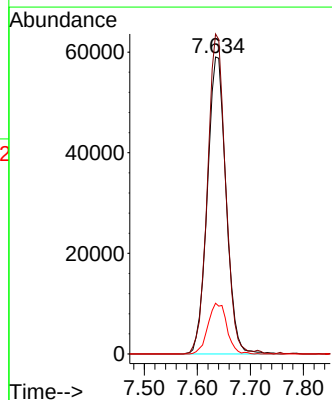
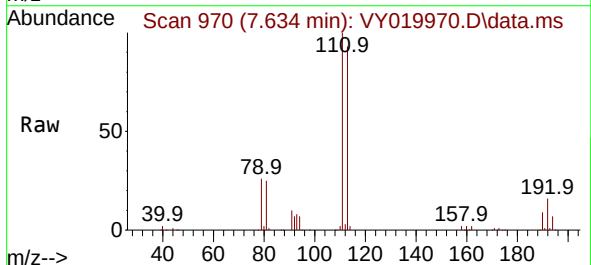


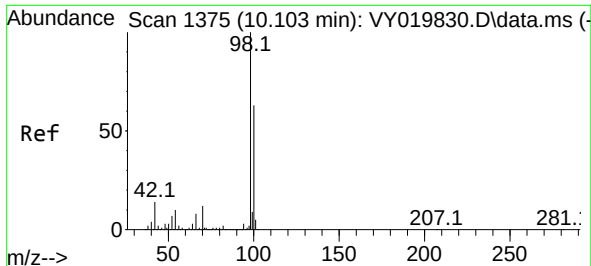

#50
Toluene-d8
Concen: 50.563 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY019970.D
Acq: 22 Oct 2024 10:36




Instrument :
MSVOA_Y
ClientSampleId :
VY1022SBL01


Tgt Ion: 98 Resp: 554994
Ion Ratio Lower Upper
98 100
100 64.2 52.0 78.0

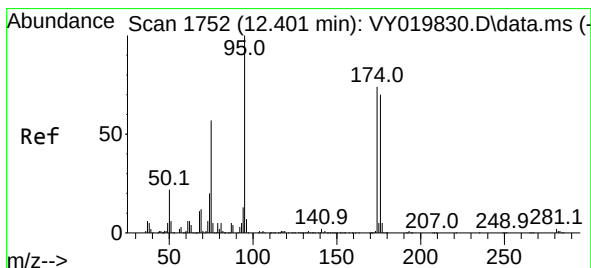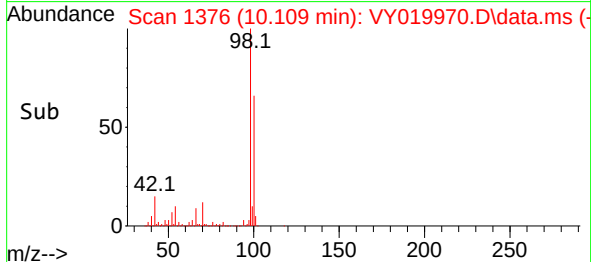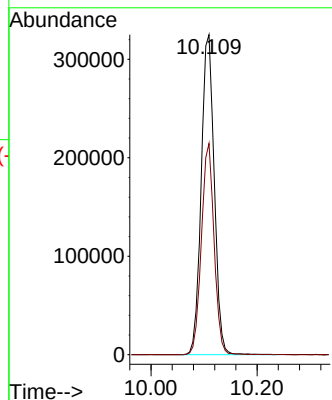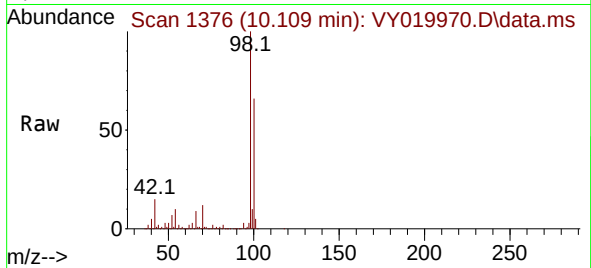

#62
4-Bromofluorobenzene
Concen: 40.325 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.000 min
Lab File: VY019970.D
Acq: 22 Oct 2024 10:36

Tgt Ion: 95 Resp: 159930
Ion Ratio Lower Upper
95 100
174 74.1 0.0 175.6
176 71.3 0.0 171.4


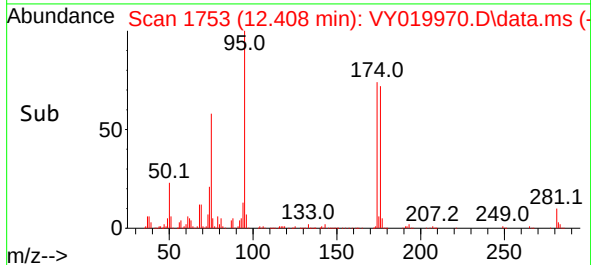
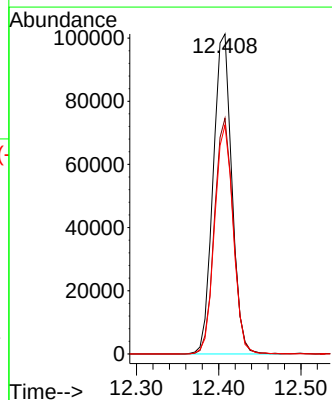
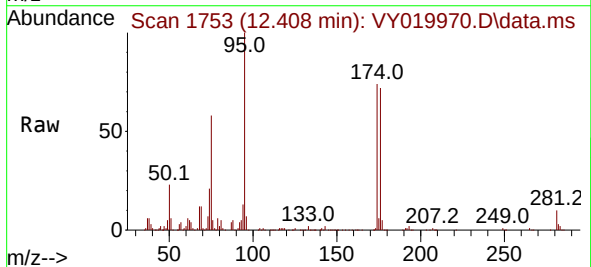


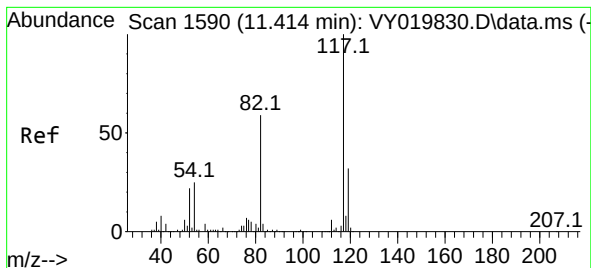

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY019970.D
Acq: 22 Oct 2024 10:36

Instrument :
MSVOA_Y
ClientSampleId :
VY1022SBL01

Tgt Ion:117 Resp: 395647
Ion Ratio Lower Upper
117 100
82 62.6 42.4 63.6
119 31.9 25.9 38.9

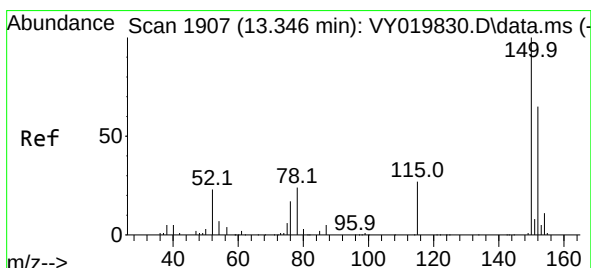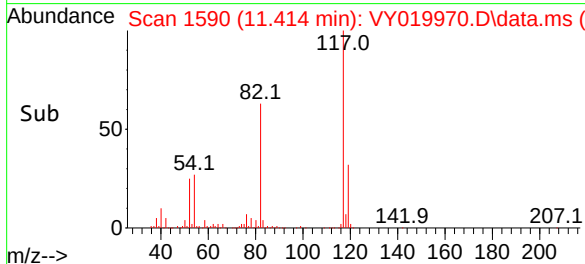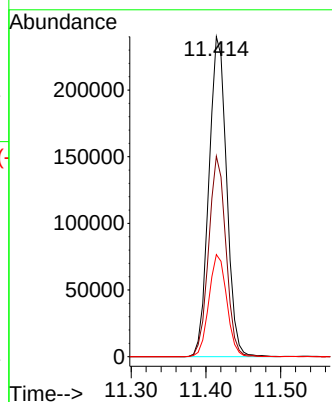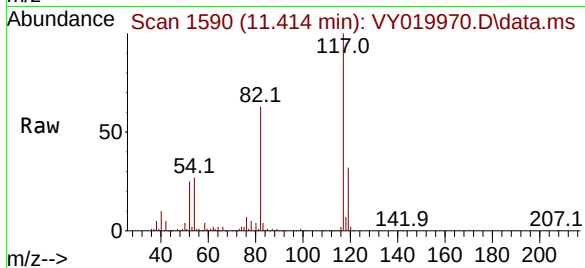

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.347 min Scan# 1907
Delta R.T. 0.000 min
Lab File: VY019970.D
Acq: 22 Oct 2024 10:36

Tgt Ion:152 Resp: 132931
Ion Ratio Lower Upper
152 100
115 62.3 28.2 84.7
150 158.7 0.0 345.6

