

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102425\
 Data File : VY023573.D
 Acq On : 24 Oct 2025 15:15
 Operator : SY/MD
 Sample : Q3451-03
 Misc : 4.50g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-11-VOC

Quant Time: Oct 25 00:36:36 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.713	168	822757	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.621	114	1341741	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	1118358	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	461240	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.067	65	339287	49.315	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	98.620%
35) Dibromofluoromethane	7.640	113	414977	50.335	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.660%
50) Toluene-d8	10.109	98	1491119	48.566	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.140%
62) 4-Bromofluorobenzene	12.407	95	419419	41.377	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	82.760%
Target Compounds						
16) Acetone	3.866	43	9753	5.955	ug/l	Qvalue # 83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102425\
Data File : VY023573.D
Acq On : 24 Oct 2025 15:15
Operator : SY/MD
Sample : Q3451-03
Misc : 4.50g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-11-VOC

Quant Time: Oct 25 00:36:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration




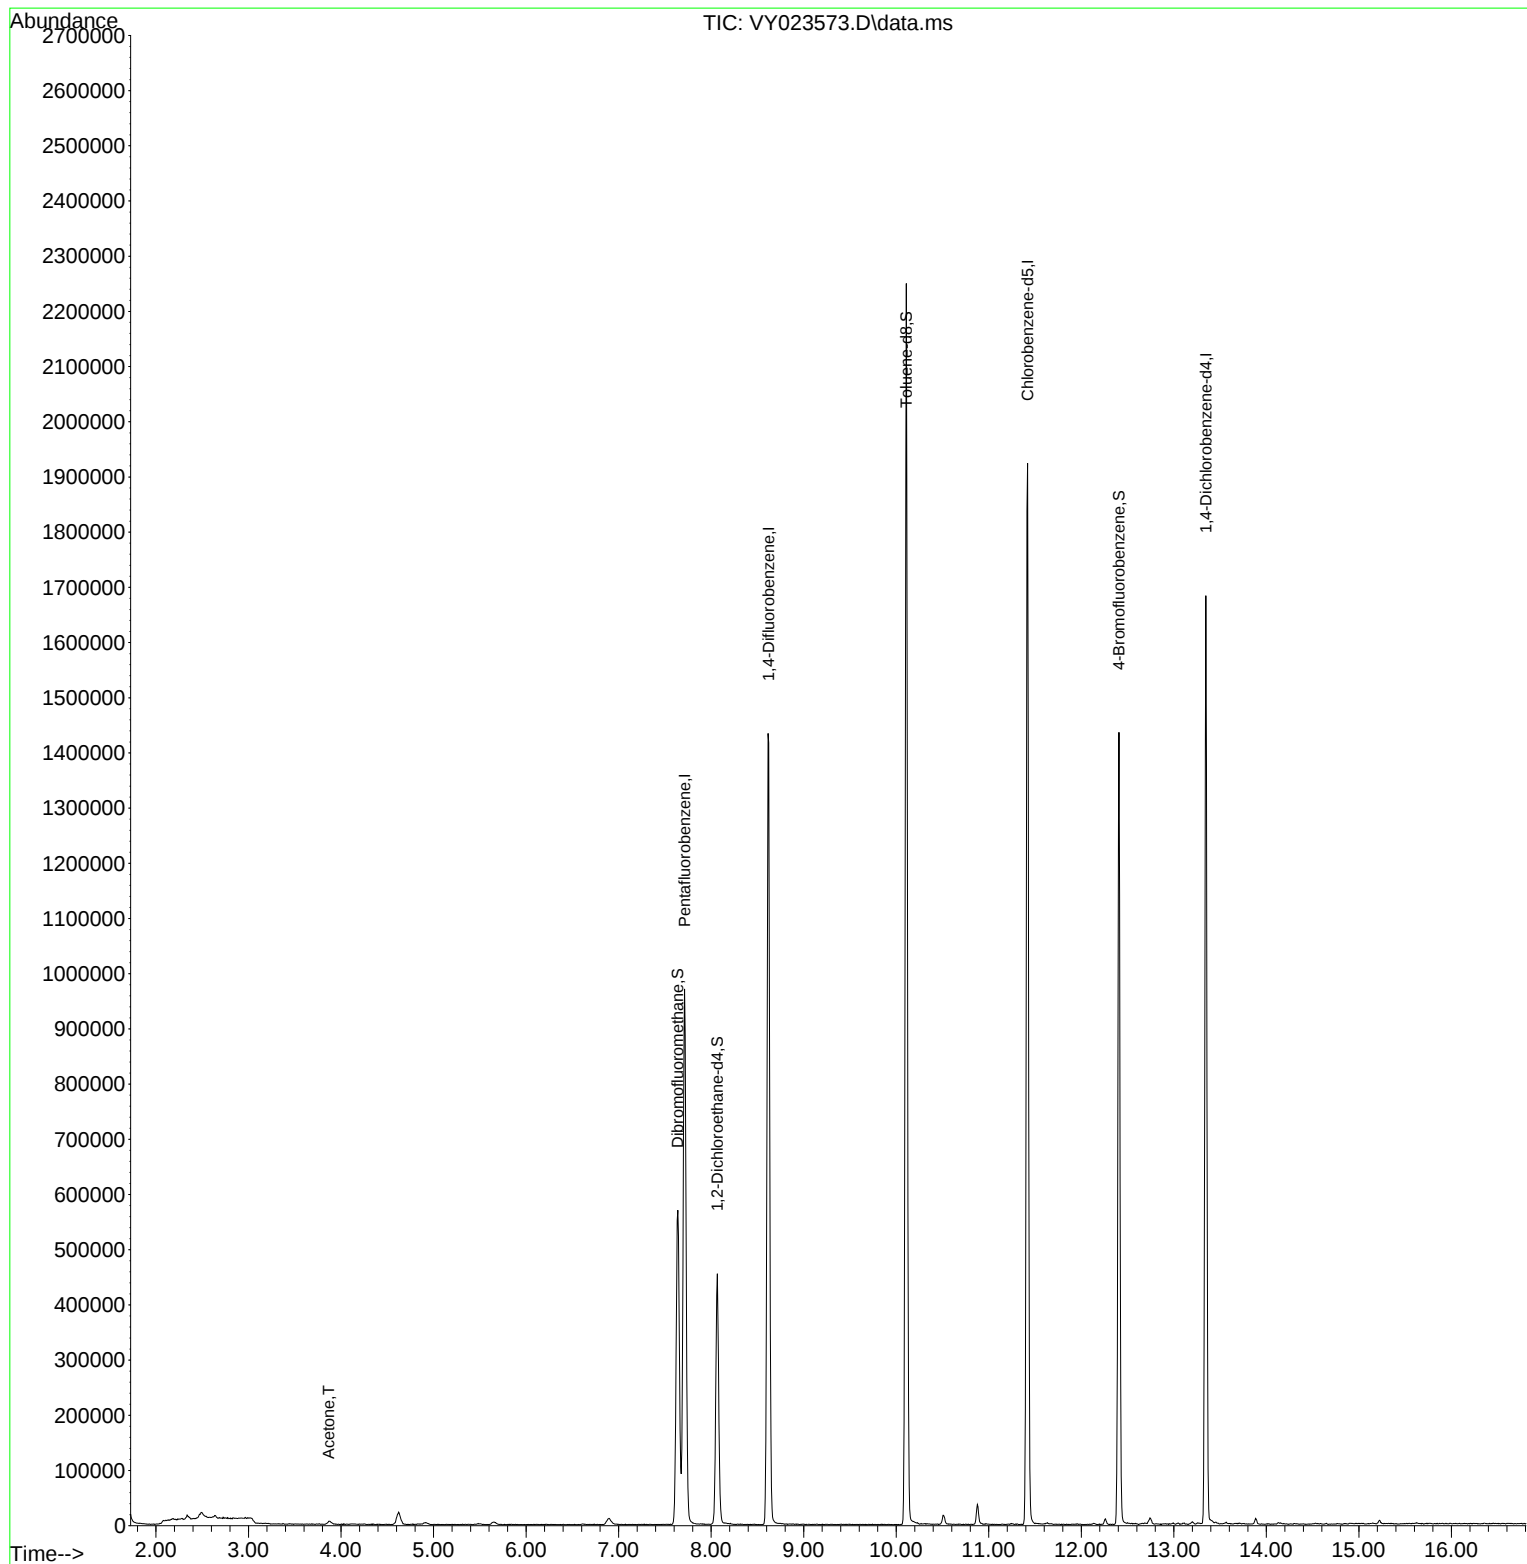




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY023573.D
Acq: 24 Oct 2025 15:15




Instrument :
MSVOA_Y
ClientSampleId :
TP-11-VOC


Tgt Ion:168 Resp: 822757
Ion Ratio Lower Upper
168 100
99 47.4 39.7 59.5

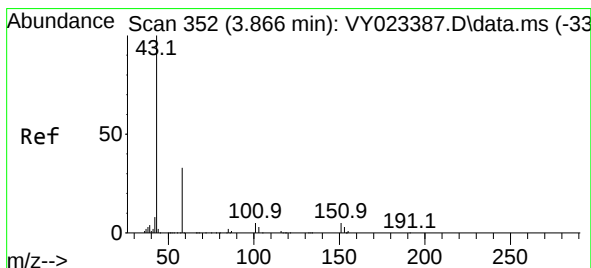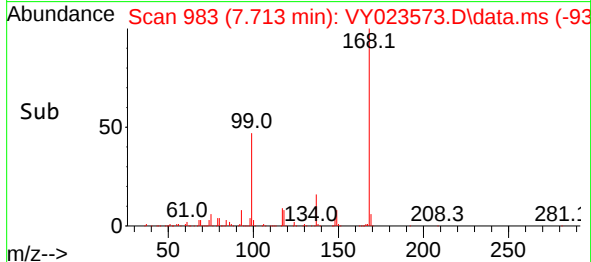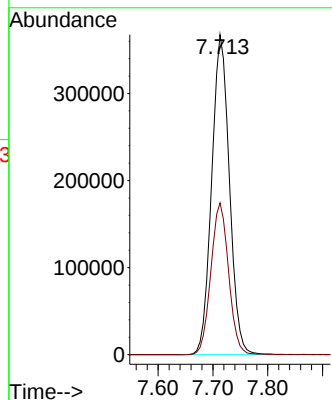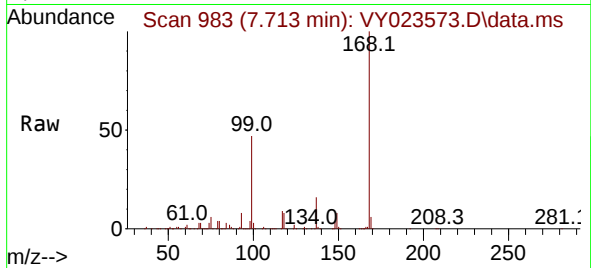

#16
Acetone
Concen: 5.955 ug/l
RT: 3.866 min Scan# 352
Delta R.T. -0.000 min
Lab File: VY023573.D
Acq: 24 Oct 2025 15:15

Tgt Ion: 43 Resp: 9753
Ion Ratio Lower Upper
43 100
58 44.3 27.7 41.5#

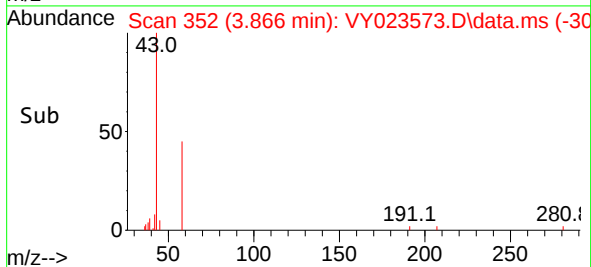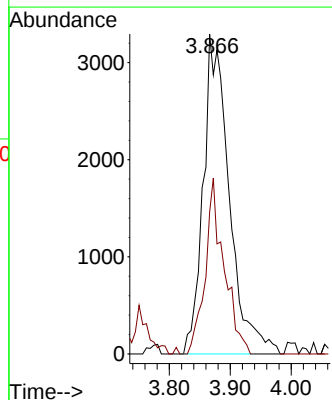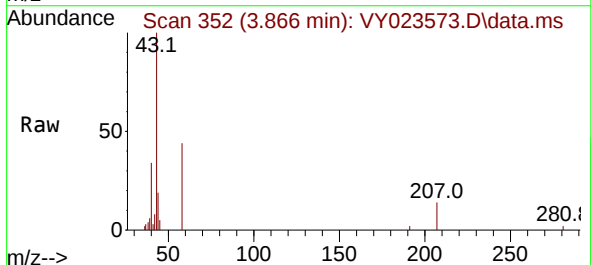

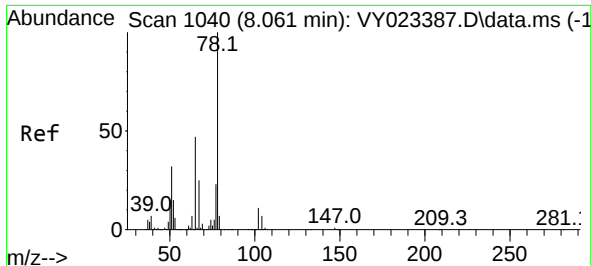

#33

1,2-Dichloroethane-d4

Concen: 49.315 ug/l

RT: 8.067 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VY023573.D

Acq: 24 Oct 2025 15:15

Instrument :

MSVOA_Y

ClientSampleId :





TP-11-VOC

Tgt Ion: 65 Resp: 339287

Ion Ratio Lower Upper

65 100

67 53.6 0.0 105.8

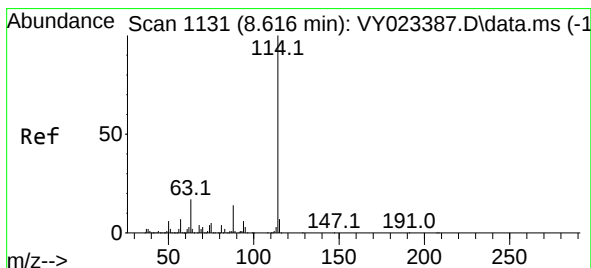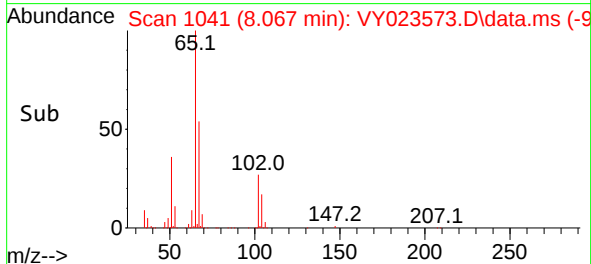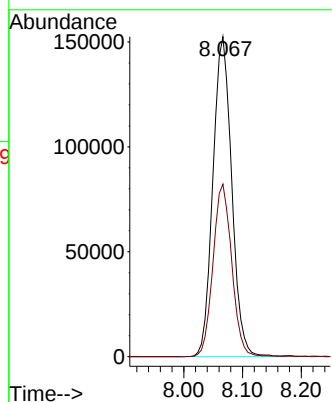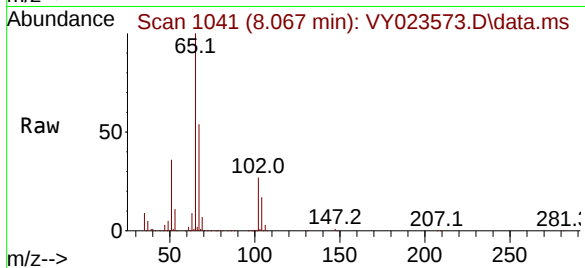

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.621 min Scan# 1132

Delta R.T. 0.006 min

Lab File: VY023573.D

Acq: 24 Oct 2025 15:15




Tgt Ion:114 Resp: 1341741


Ion Ratio Lower Upper

114 100

63 15.4 0.0 34.2

88 13.7 0.0 28.4


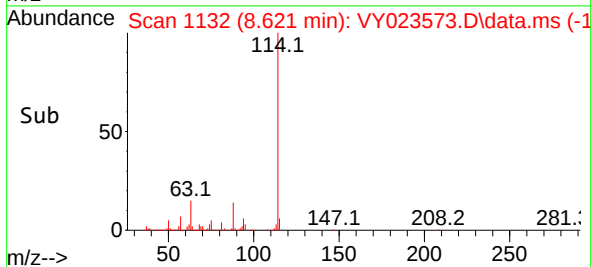
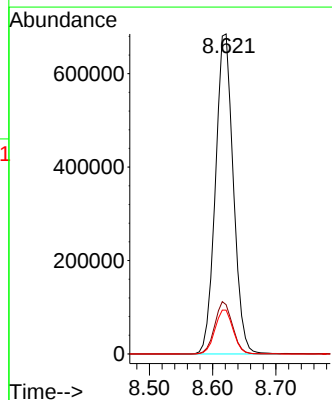
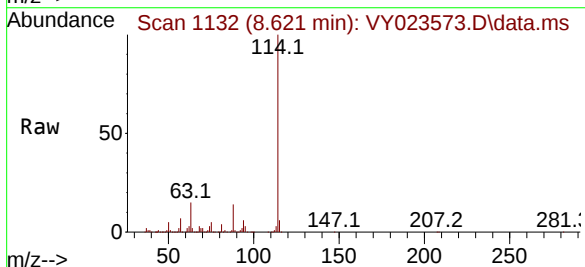


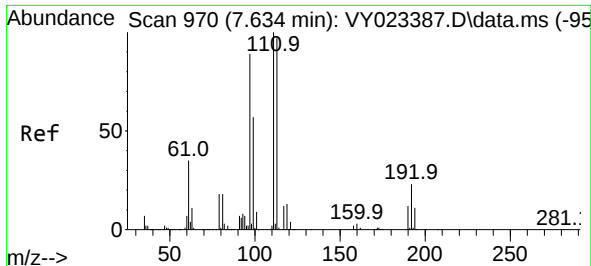

#35
Dibromofluoromethane
Concen: 50.335 ug/l
RT: 7.640 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY023573.D
Acq: 24 Oct 2025 15:15




Instrument :
MSVOA_Y
ClientSampleId :
TP-11-VOC


Tgt Ion:113 Resp: 414977
Ion Ratio Lower Upper
113 100
111 101.7 81.8 122.6
192 23.1 18.0 27.0

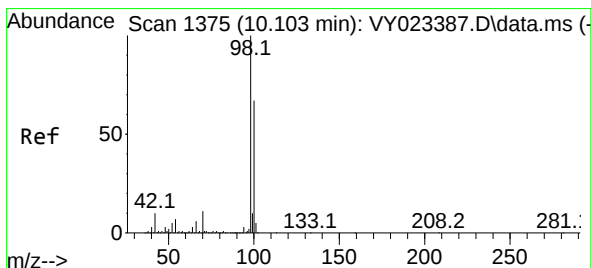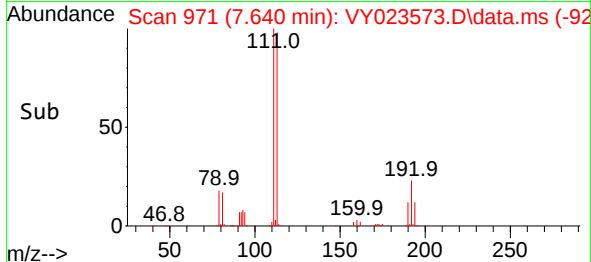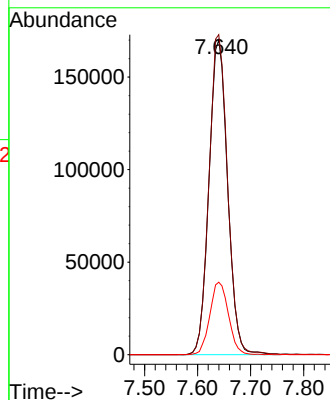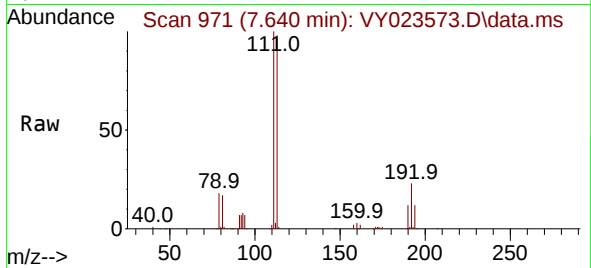

#50
Toluene-d8
Concen: 48.566 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.006 min
Lab File: VY023573.D
Acq: 24 Oct 2025 15:15

Tgt Ion: 98 Resp: 1491119
Ion Ratio Lower Upper
98 100
100 65.6 53.0 79.4


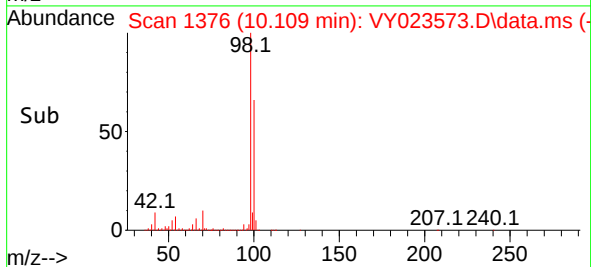
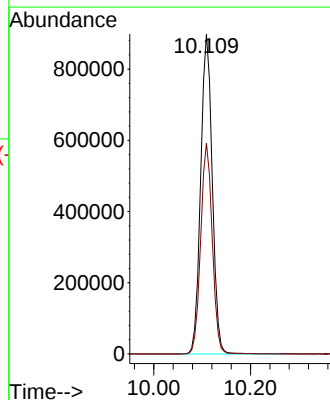
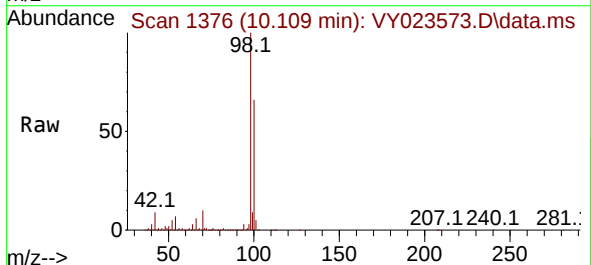


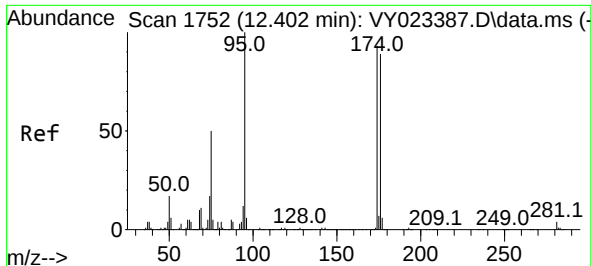

#62
4-Bromofluorobenzene
Concen: 41.377 ug/l
RT: 12.407 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY023573.D
Acq: 24 Oct 2025 15:15




Instrument :
MSVOA_Y
ClientSampleId :
TP-11-VOC


Tgt Ion: 95 Resp: 419419
Ion Ratio Lower Upper
95 100
174 98.9 0.0 192.8
176 96.7 0.0 187.6

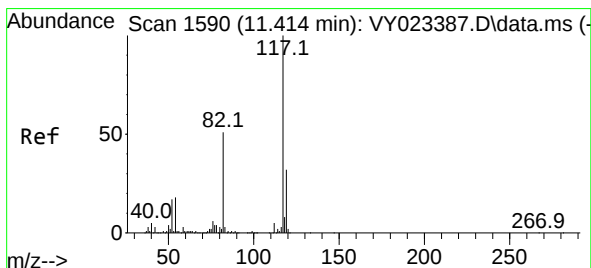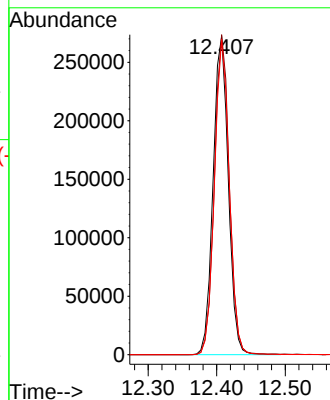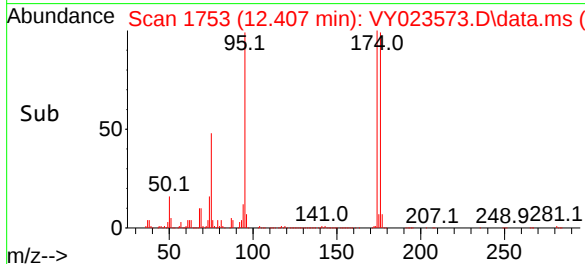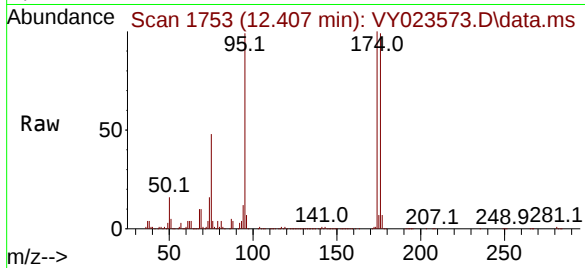

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.420 min Scan# 1591
Delta R.T. 0.006 min
Lab File: VY023573.D
Acq: 24 Oct 2025 15:15


Tgt Ion: 117 Resp: 1118358
Ion Ratio Lower Upper
117 100
82 48.9 41.0 61.4
119 32.8 25.6 38.4

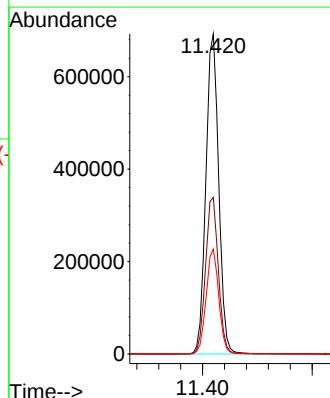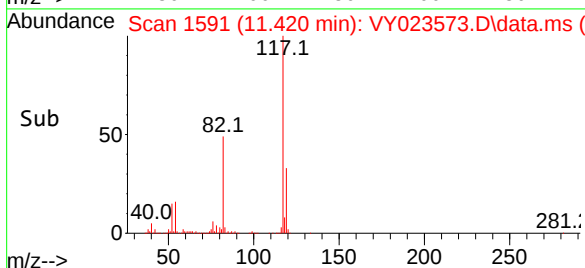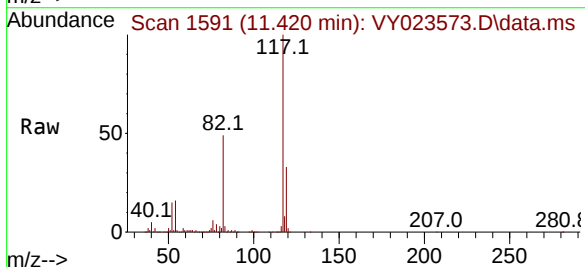

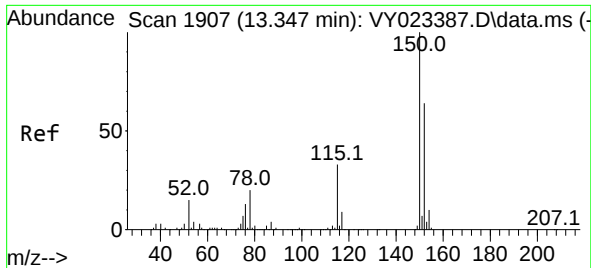

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.346 min Scan# 1907
 Delta R.T. -0.000 min
 Lab File: VY023573.D
 Acq: 24 Oct 2025 15:15

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-11-VOC

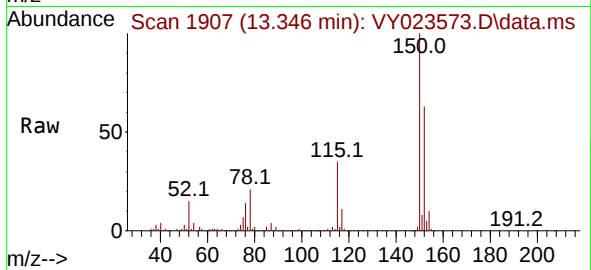

Tgt Ion:152 Resp: 461240
 Ion Ratio Lower Upper
 152 100
 115 54.2 27.1 81.2
 150 156.9 0.0 347.4

