

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102524\
 Data File : VY020024.D
 Acq On : 25 Oct 2024 14:12
 Operator : SY/MD
 Sample : P4547-07
 Misc : 3.56g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Oct 26 00:22:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 16 05:44:48 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	186942	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.615	114	400396	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	374696	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	141592	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.060	65	151114	65.650	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 131.300%	
35) Dibromofluoromethane	7.634	113	135472	51.273	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 102.540%	
50) Toluene-d8	10.109	98	499836	51.227	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 102.460%	
62) 4-Bromofluorobenzene	12.407	95	156865	44.494	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	= 88.980%	
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	4.884	59	225	Below Cal	#	88
16) Acetone	3.884	43	3736	6.235	ug/l	92
25) 2-Butanone	6.908	43	1417	1.767	ug/l	100
31) Cyclohexane	7.713	56	5750	1.495	ug/l	# 38
36) 1,1-Dichloropropene	7.707	75	19576	5.143	ug/l	# 47
38) Carbon Tetrachloride	7.713	117	21554	5.282	ug/l	# 16
76) 1,2,3-Trichloropropane	12.401	75	92825	33.465	ug/l	# 100
81) trans-1,4-Dichloro-2-b...	12.401	75	92825	135.078	ug/l	# 16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102524\
Data File : VY020024.D
Acq On : 25 Oct 2024 14:12
Operator : SY/MD
Sample : P4547-07
Misc : 3.56g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :


Quant Time: Oct 26 00:22:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 16 05:44:48 2024
Response via : Initial Calibration

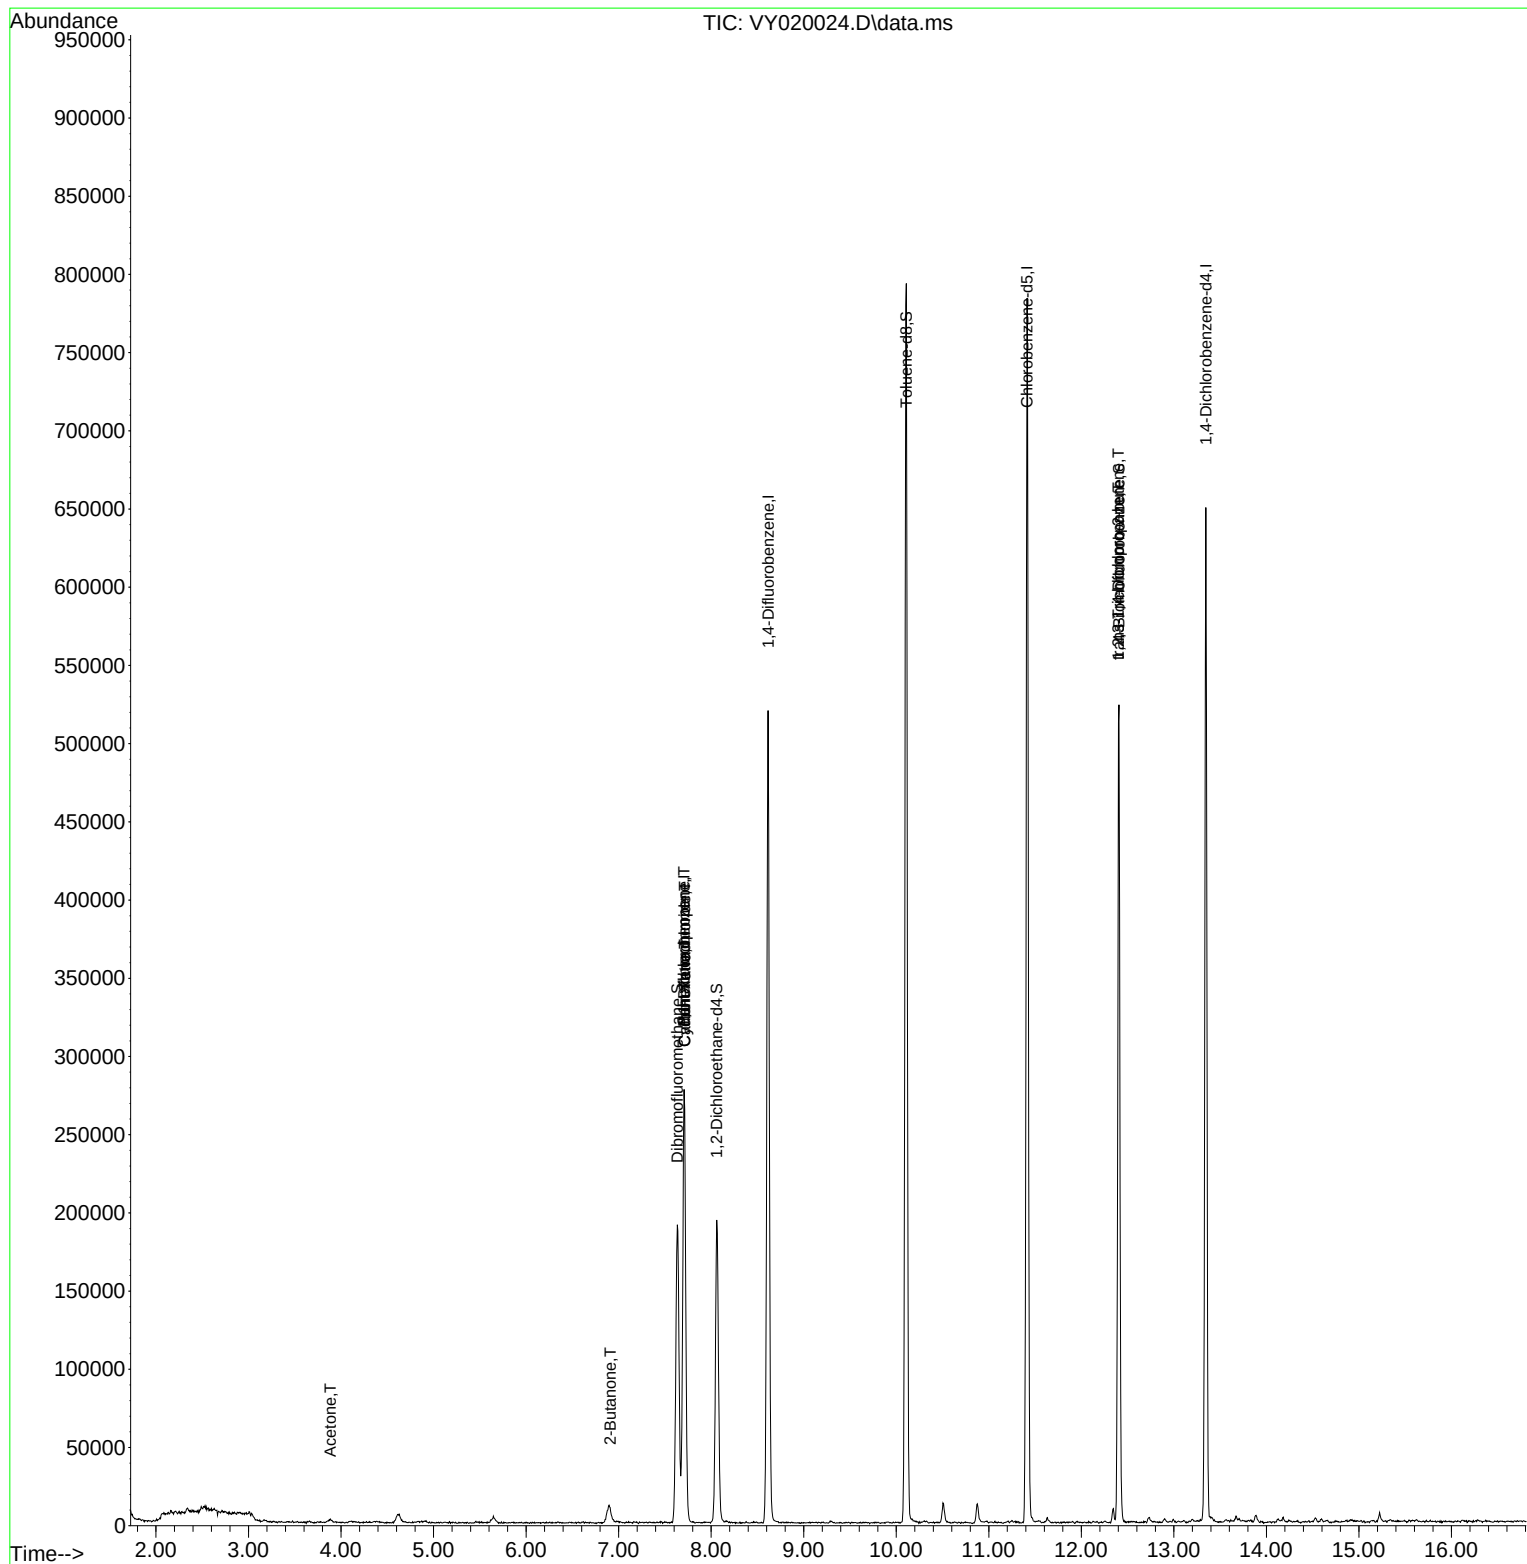






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY020024.D
Acq: 25 Oct 2024 14:12

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion:168 Resp: 186942
Ion Ratio Lower Upper
168 100
99 62.2 39.1 58.7#

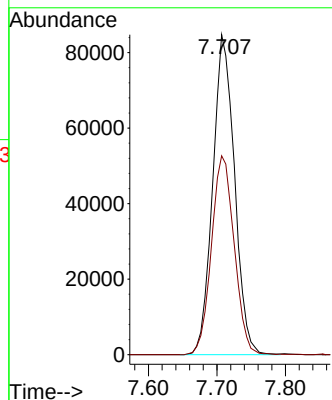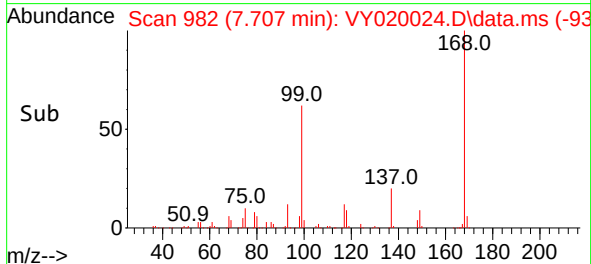

#11
Tert butyl alcohol
Concen: Below Cal
RT: 4.884 min Scan# 519
Delta R.T. 0.024 min
Lab File: VY020024.D
Acq: 25 Oct 2024 14:12

Tgt Ion: 59 Resp: 225
Ion Ratio Lower Upper
59 100
57 0.0 3.0 4.6#


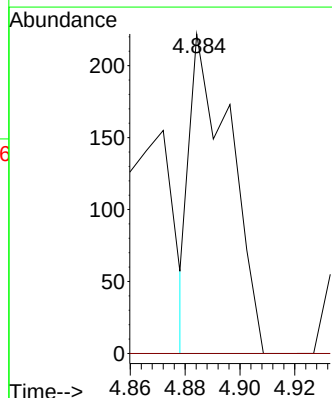
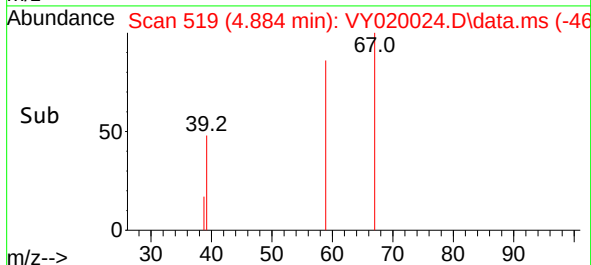
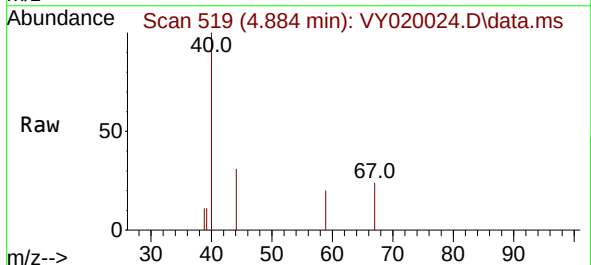




#16
Acetone
Concen: 6.235 ug/l
RT: 3.884 min Scan# 31
Delta R.T. 0.012 min
Lab File: VY020024.D
Acq: 25 Oct 2024 14:12




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 43 Resp: 3736
Ion Ratio Lower Upper
43 100
58 34.8 31.7 47.5

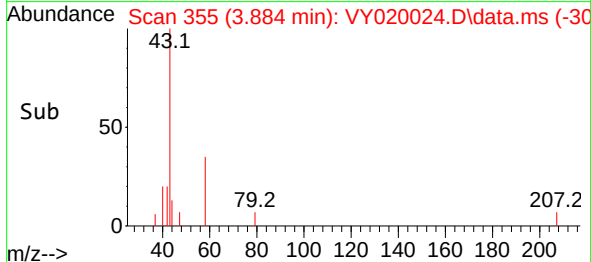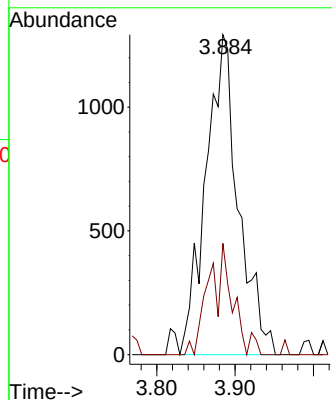

#25
2-Butanone
Concen: 1.767 ug/l
RT: 6.908 min Scan# 851
Delta R.T. 0.018 min
Lab File: VY020024.D
Acq: 25 Oct 2024 14:12

Tgt Ion: 43 Resp: 1417
Ion Ratio Lower Upper
43 100
72 33.9 27.3 40.9


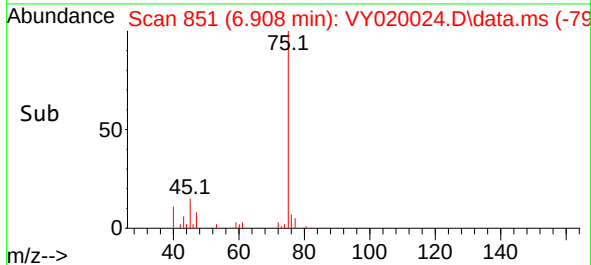
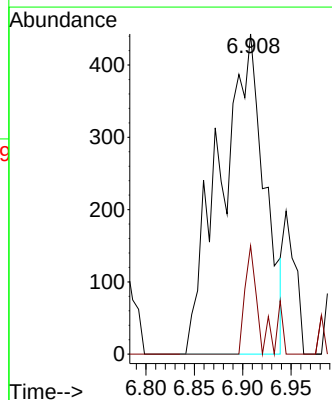
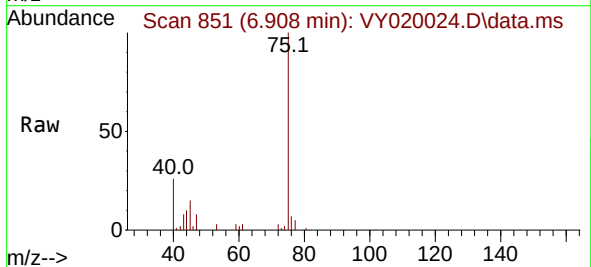




#31
Cyclohexane
Concen: 1.495 ug/l
RT: 7.713 min Scan# 981
Delta R.T. 0.012 min
Lab File: VY020024.D
Acq: 25 Oct 2024 14:12




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 56 Resp: 5750
Ion Ratio Lower Upper
56 100
69 148.4 28.7 43.1#
84 111.5 77.7 116.5

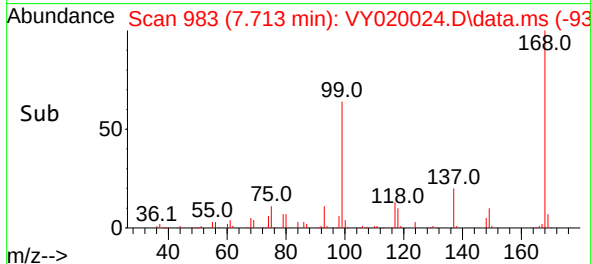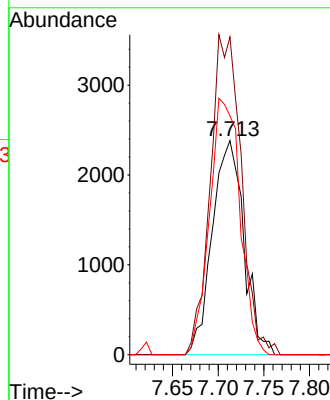

#33
1,2-Dichloroethane-d4
Concen: 65.650 ug/l
RT: 8.060 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY020024.D
Acq: 25 Oct 2024 14:12


Tgt Ion: 65 Resp: 151114
Ion Ratio Lower Upper
65 100
67 50.9 0.0 109.6

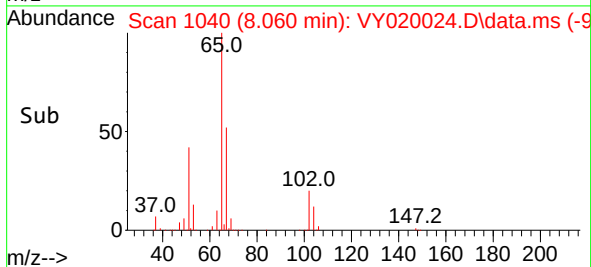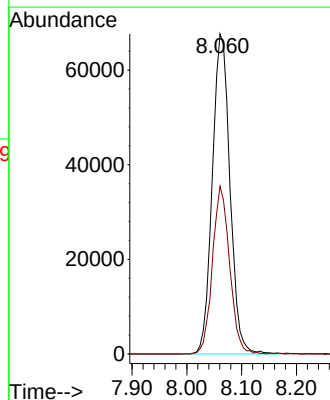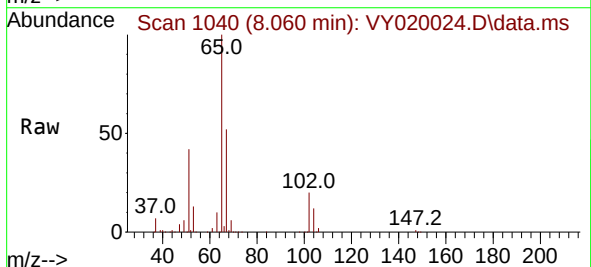






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.615 min Scan# 1131
Delta R.T. -0.000 min
Lab File: VY020024.D
Acq: 25 Oct 2024 14:12

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion:114 Resp: 400396
Ion Ratio Lower Upper
114 100
63 23.5 0.0 35.0
88 16.0 0.0 27.2

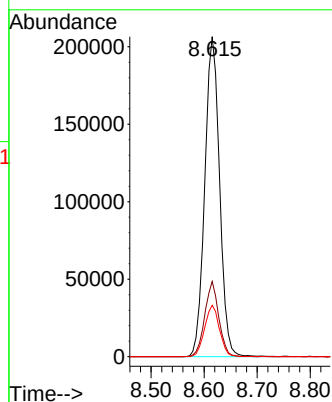

#35
Dibromofluoromethane
Concen: 51.273 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.000 min
Lab File: VY020024.D
Acq: 25 Oct 2024 14:12

Tgt Ion:113 Resp: 135472
Ion Ratio Lower Upper
113 100
111 102.7 82.2 123.4
192 17.0 15.9 23.9

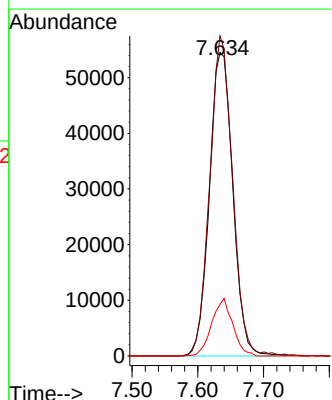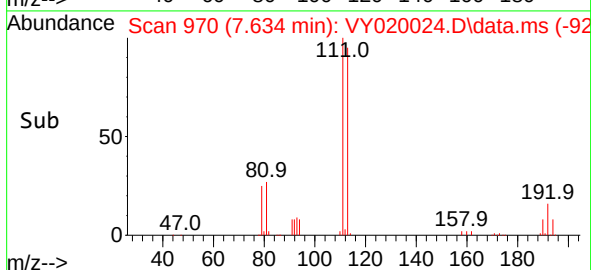

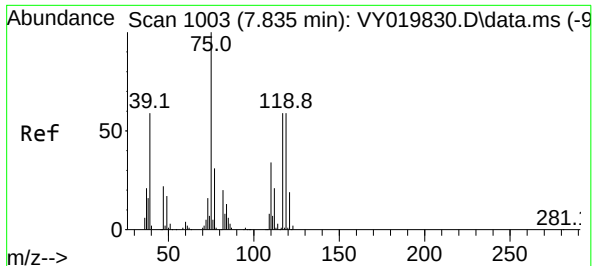

#36

1,1-Dichloropropene

Concen: 5.143 ug/l

RT: 7.707 min Scan# 982

Delta R.T. -0.128 min


Lab File: VY020024.D

Acq: 25 Oct 2024 14:12

Instrument :

MSVOA_Y

ClientSampleId :

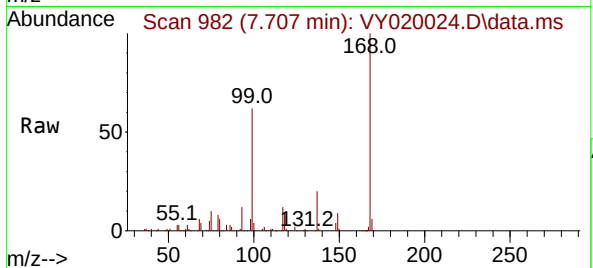




Tgt Ion: 75 Resp: 19576

Ion Ratio Lower Upper

75 100

110 7.9 19.0 57.0#

77 0.0 25.3 37.9#

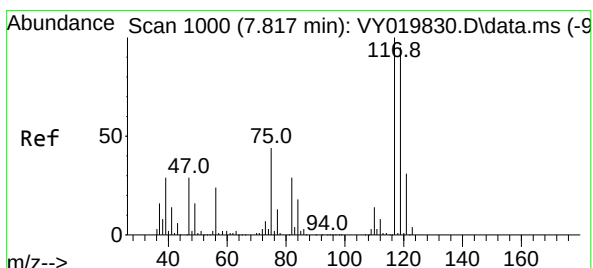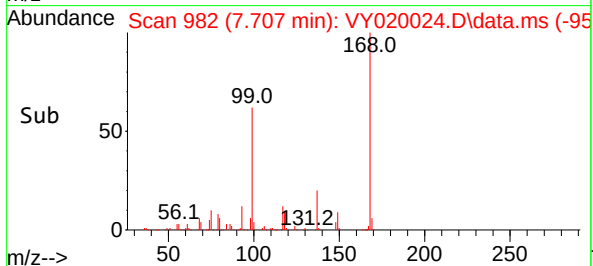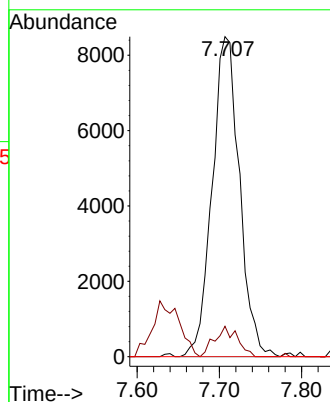

#38

Carbon Tetrachloride

Concen: 5.282 ug/l

RT: 7.713 min Scan# 983

Delta R.T. -0.104 min

Lab File: VY020024.D

Acq: 25 Oct 2024 14:12




Tgt Ion: 117 Resp: 21554


Ion Ratio Lower Upper

117 100

119 4.5 75.8 113.6#

121 0.0 24.0 36.0#


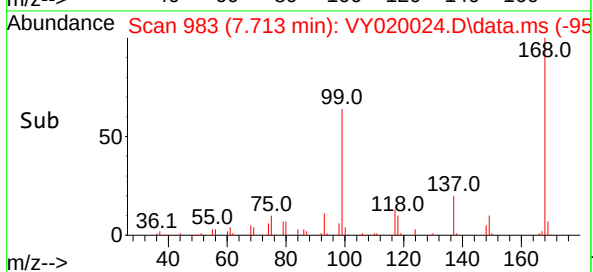
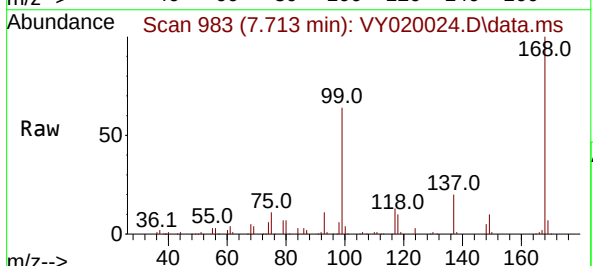
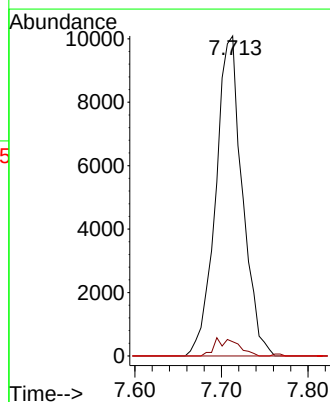




#50
Toluene-d8
Concen: 51.227 ug/l
RT: 10.109 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY020024.D
Acq: 25 Oct 2024 14:12




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 98 Resp: 499836
Ion Ratio Lower Upper
98 100
100 62.8 52.0 78.0

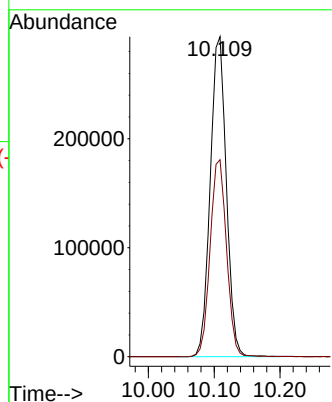

#62
4-Bromofluorobenzene
Concen: 44.494 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. -0.000 min
Lab File: VY020024.D
Acq: 25 Oct 2024 14:12

Tgt Ion: 95 Resp: 156865
Ion Ratio Lower Upper
95 100
174 74.1 0.0 175.6
176 70.2 0.0 171.4

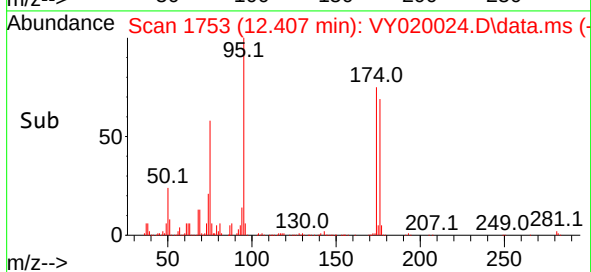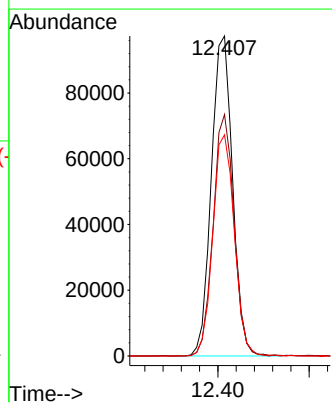



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY020024.D

Acq: 25 Oct 2024 14:12

Instrument :

MSVOA_Y

ClientSampleId :





Tgt Ion:117 Resp: 374696

Ion Ratio Lower Upper

117 100

82 60.2 42.4 63.6

119 31.3 25.9 38.9

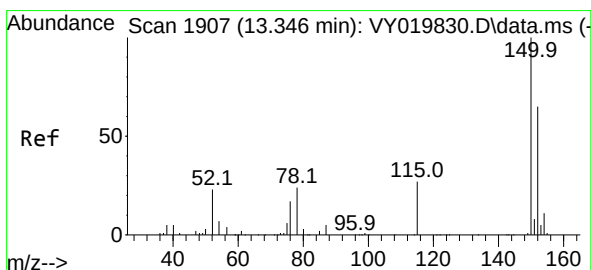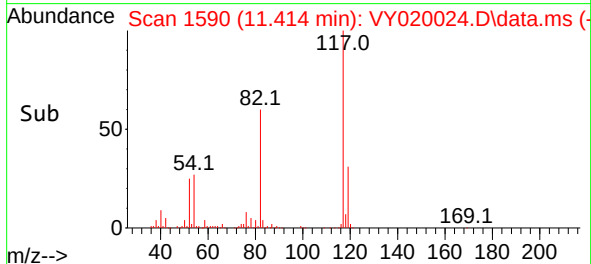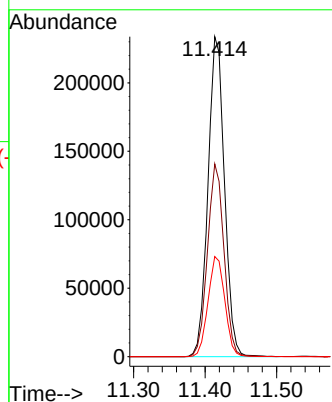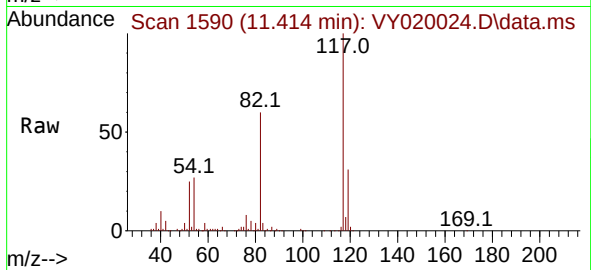

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. -0.000 min

Lab File: VY020024.D

Acq: 25 Oct 2024 14:12




Tgt Ion:152 Resp: 141592


Ion Ratio Lower Upper

152 100

115 62.7 28.2 84.7

150 157.7 0.0 345.6



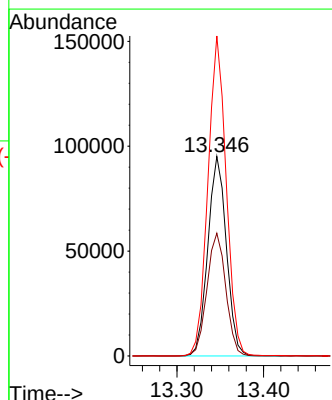
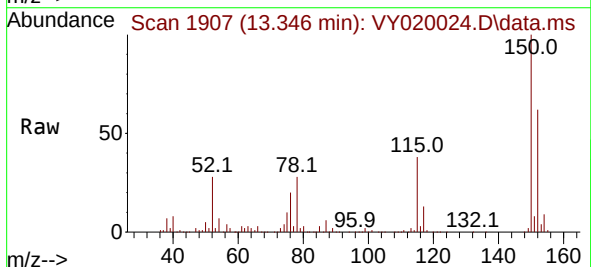




#76
1,2,3-Trichloropropane
Concen: 33.465 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. -0.159 min
Lab File: VY020024.D
Acq: 25 Oct 2024 14:12

Instrument :
MSVOA_Y
ClientSampleId :

Tgt Ion: 75 Resp: 92825
Ion Ratio Lower Upper
75 100
77 1.4 0.0 0.0#

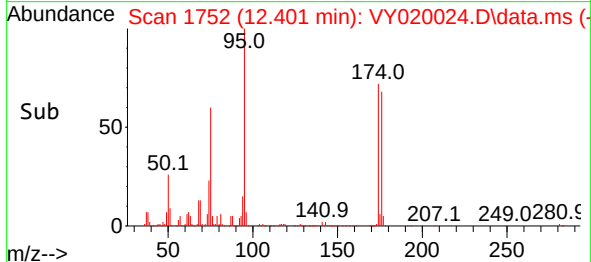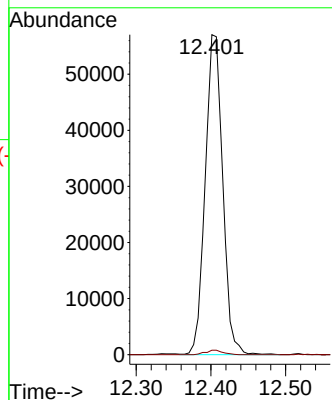

#81
trans-1,4-Dichloro-2-butene
Concen: 135.078 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. 0.098 min
Lab File: VY020024.D
Acq: 25 Oct 2024 14:12

Tgt Ion: 75 Resp: 92825
Ion Ratio Lower Upper
75 100
53 0.0 66.8 100.2#
89 0.1 35.8 53.6#

