

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102622\
 Data File : VY011115.D
 Acq On : 26 Oct 2022 14:50
 Operator : KP/MD
 Sample : N5281-04
 Misc : 6.08g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-4

Quant Time: Oct 27 04:39:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101722S.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 18 01:42:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	320968	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	572592	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	509600	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	228537	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	126466	42.774	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	85.540%
35) Dibromofluoromethane	7.710	113	136483	42.435	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	84.860%
50) Toluene-d8	10.179	98	440418	36.837	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	73.680%
62) 4-Bromofluorobenzene	12.477	95	159519	36.859	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	73.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102622\
Data File : VY011115.D
Acq On : 26 Oct 2022 14:50
Operator : KP/MD
Sample : N5281-04
Misc : 6.08g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-4

Quant Time: Oct 27 04:39:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101722S.M
Quant Title : SW846 8260
QLast Update : Tue Oct 18 01:42:42 2022
Response via : Initial Calibration




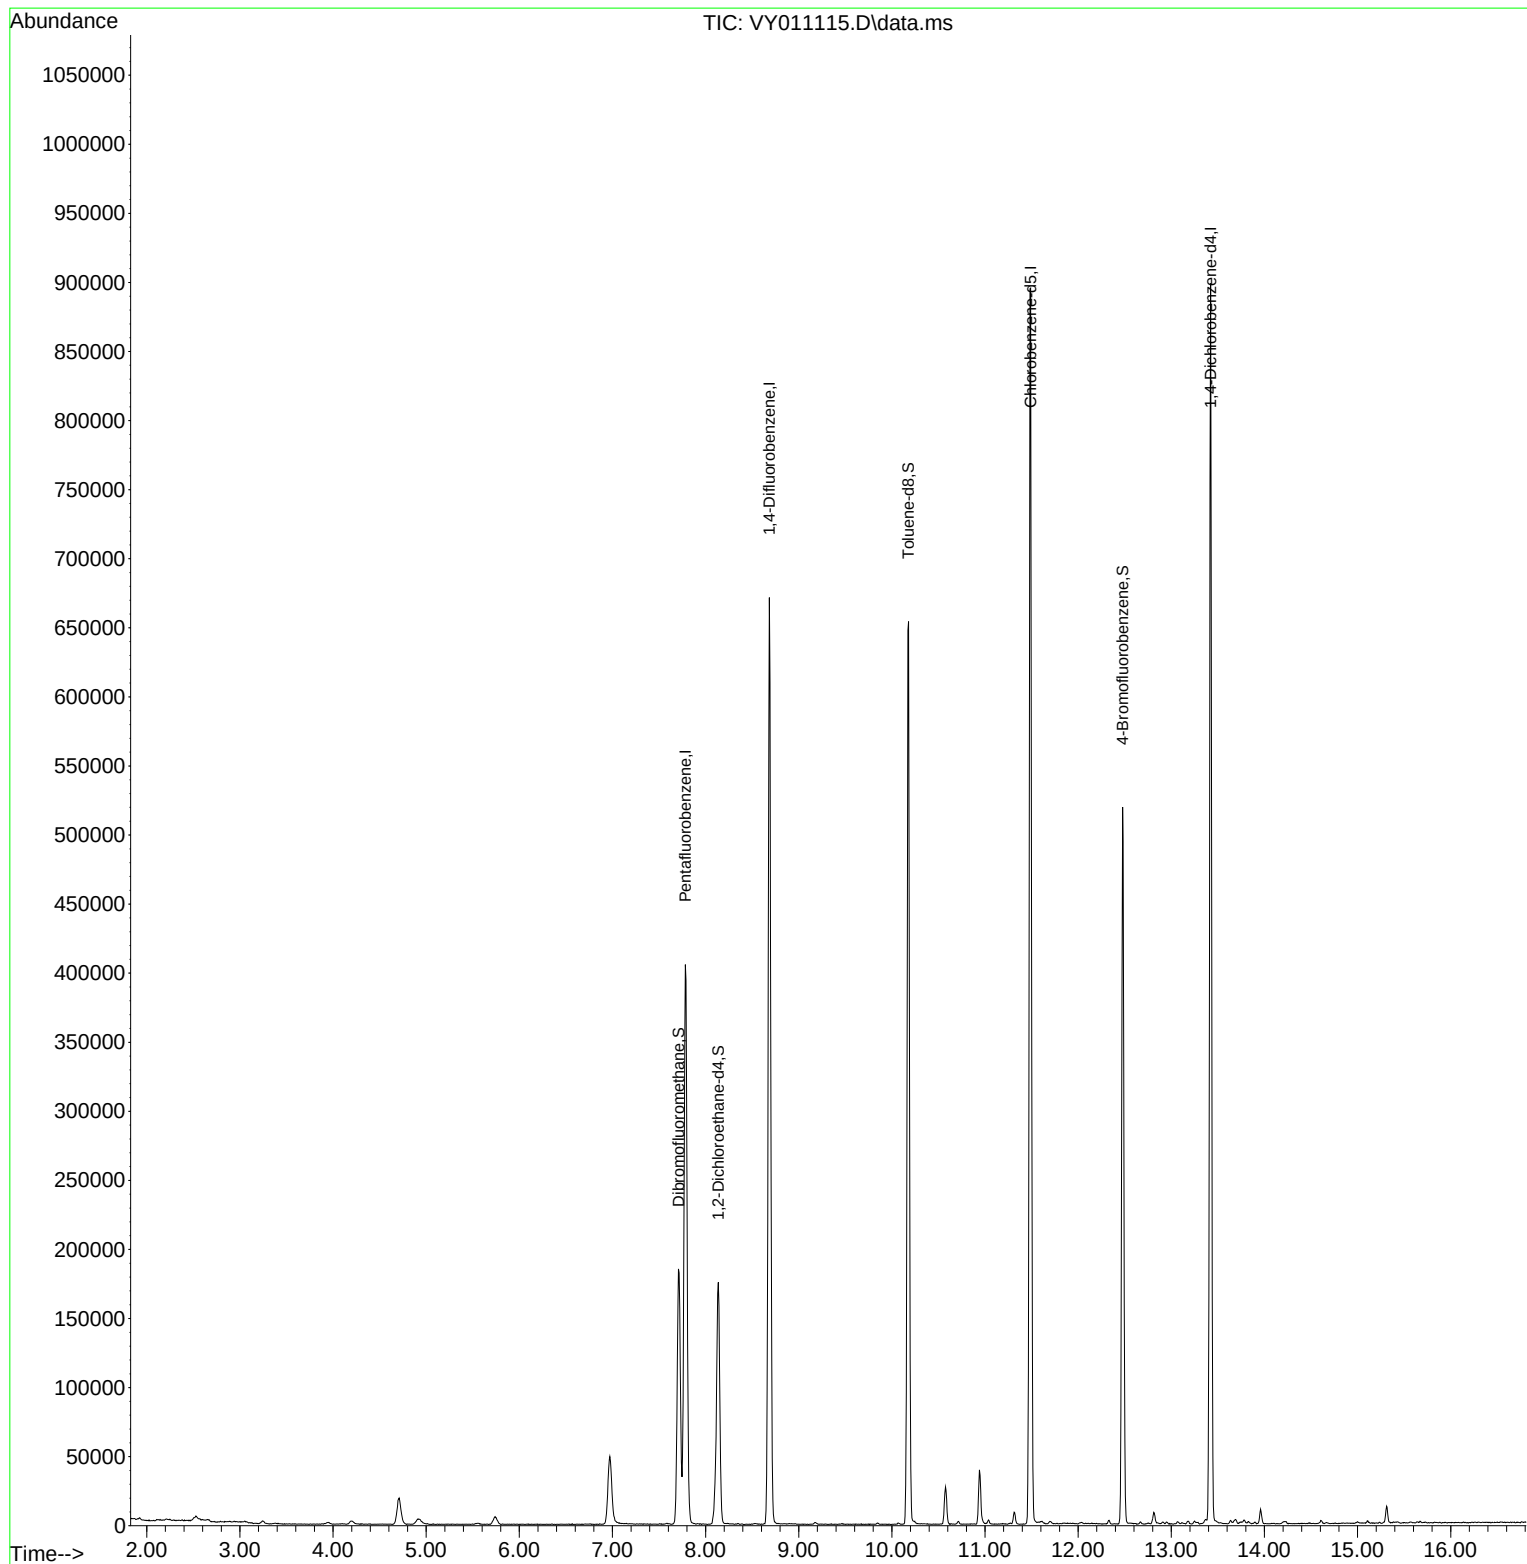


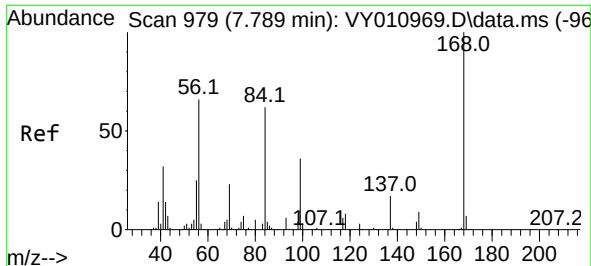

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY011115.D
Acq: 26 Oct 2022 14:50




Instrument :
MSVOA_Y
ClientSampleId :
SB-4


Tgt Ion:168 Resp: 320968
Ion Ratio Lower Upper
168 100
99 55.3 46.9 70.3

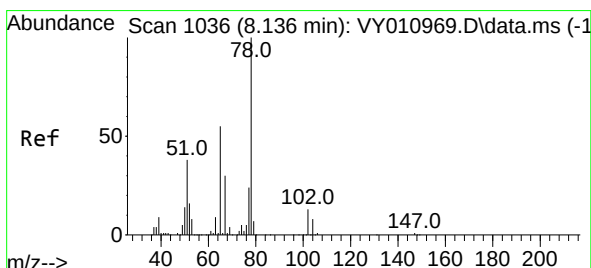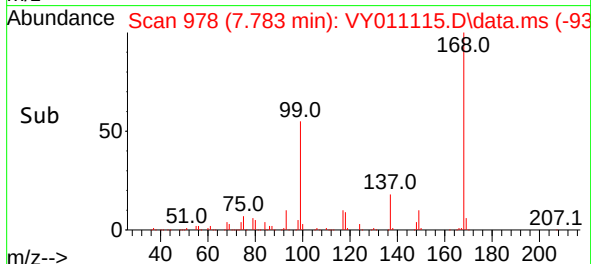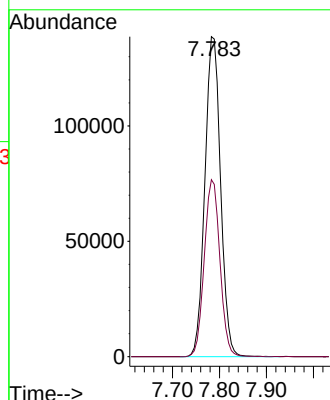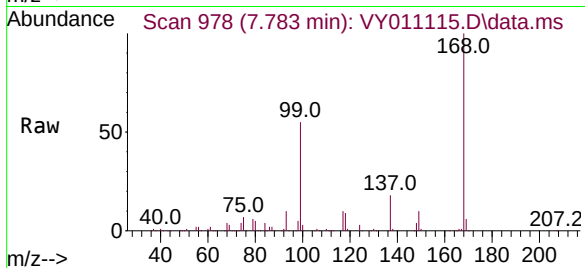

#33
1,2-Dichloroethane-d4
Concen: 42.774 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY011115.D
Acq: 26 Oct 2022 14:50

Tgt Ion: 65 Resp: 126466
Ion Ratio Lower Upper
65 100
67 54.8 0.0 99.4


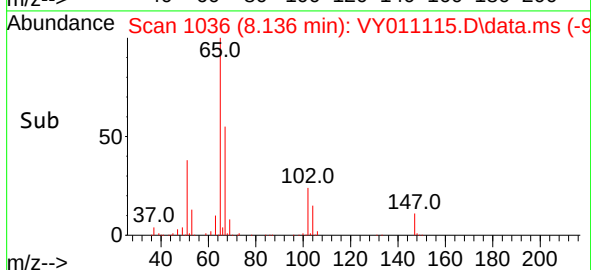
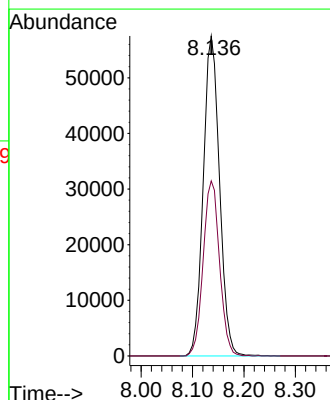
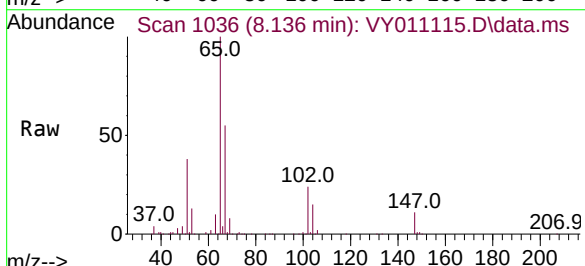


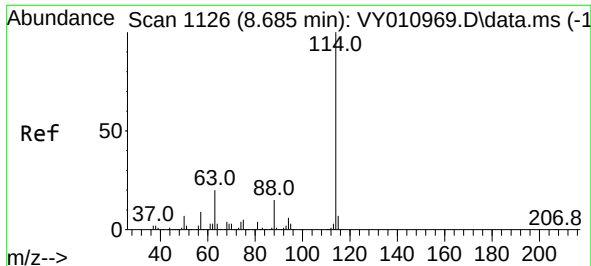

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VY011115.D
Acq: 26 Oct 2022 14:50




Instrument :
MSVOA_Y
ClientSampleId :
SB-4


Tgt Ion:114 Resp: 572592
Ion Ratio Lower Upper
114 100
63 19.0 0.0 43.2
88 15.0 0.0 31.8

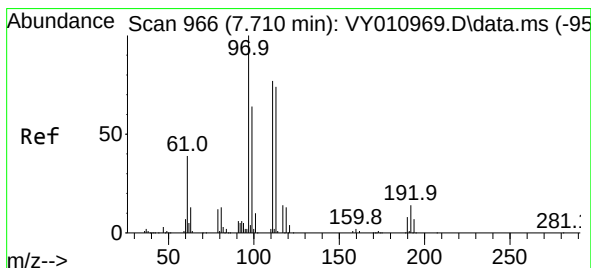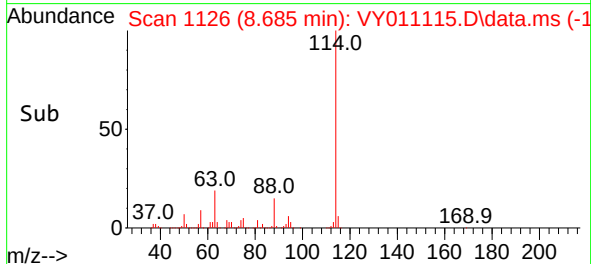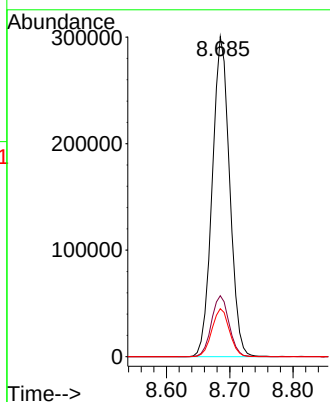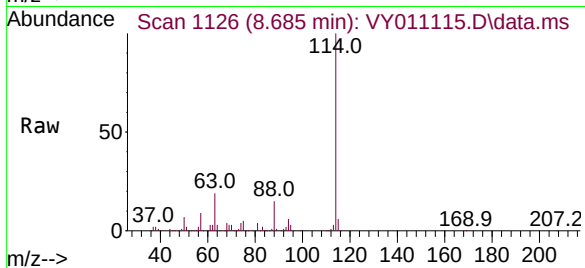

#35
Dibromofluoromethane
Concen: 42.435 ug/l
RT: 7.710 min Scan# 966
Delta R.T. -0.000 min
Lab File: VY011115.D
Acq: 26 Oct 2022 14:50

Tgt Ion:113 Resp: 136483
Ion Ratio Lower Upper
113 100
111 103.0 82.6 124.0
192 19.2 17.6 26.4


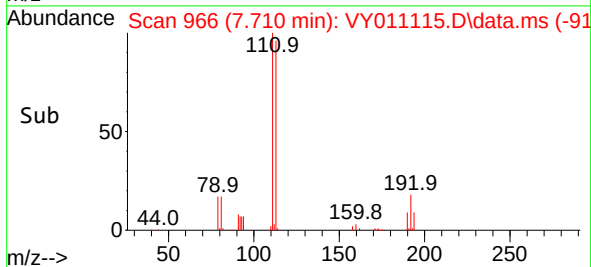
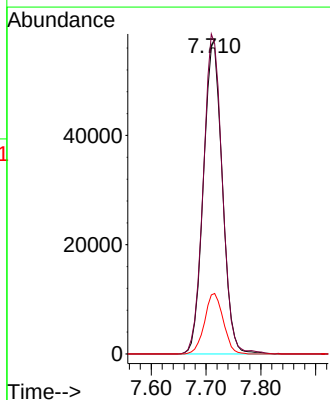
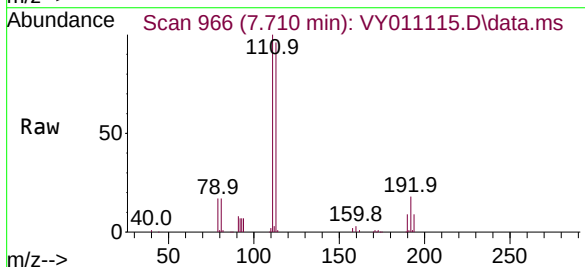


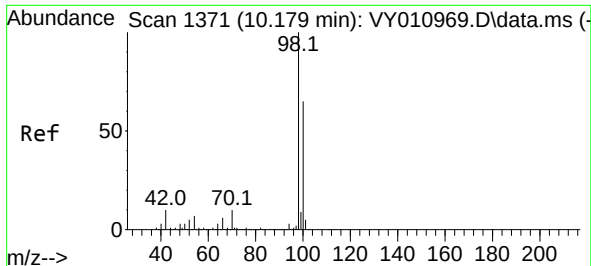

#50
Toluene-d8
Concen: 36.837 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY011115.D
Acq: 26 Oct 2022 14:50




Instrument :
MSVOA_Y
ClientSampleId :
SB-4


Tgt Ion: 98 Resp: 440418
Ion Ratio Lower Upper
98 100
100 64.8 50.2 75.2

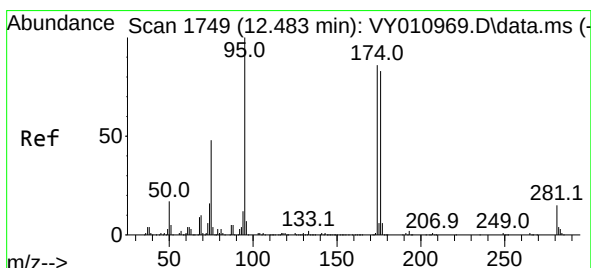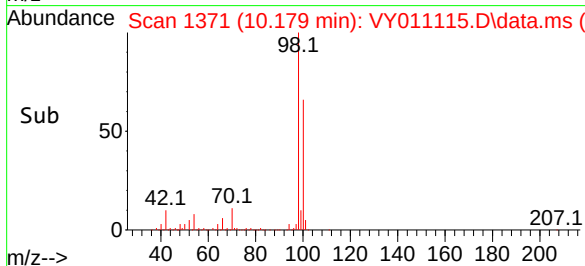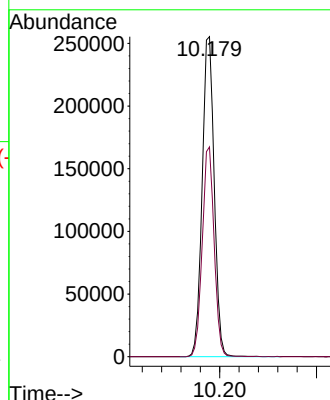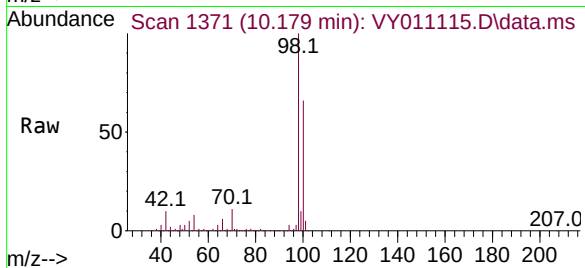

#62
4-Bromofluorobenzene
Concen: 36.859 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY011115.D
Acq: 26 Oct 2022 14:50

Tgt Ion: 95 Resp: 159519
Ion Ratio Lower Upper
95 100
174 82.5 0.0 177.0
176 80.3 0.0 175.8


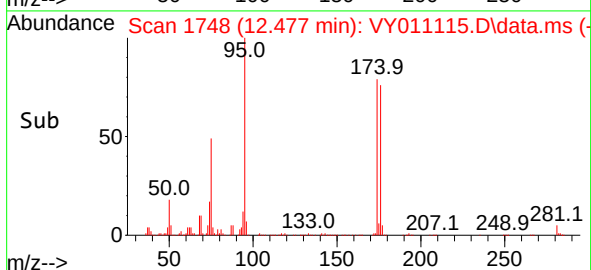
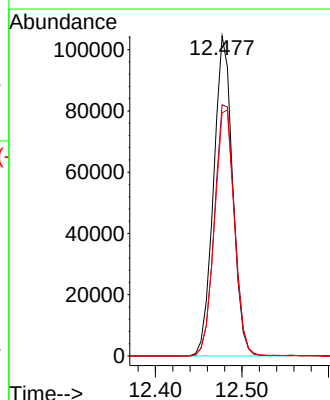
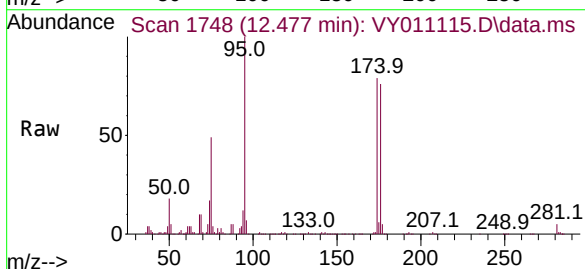


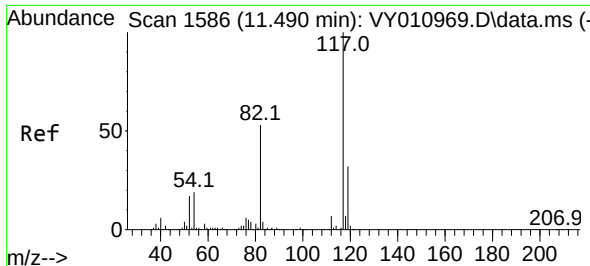

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY011115.D
Acq: 26 Oct 2022 14:50

Instrument :
MSVOA_Y
ClientSampleId :
SB-4

Tgt Ion:117 Resp: 509600
Ion Ratio Lower Upper
117 100
82 54.5 43.0 64.4
119 32.3 25.4 38.0

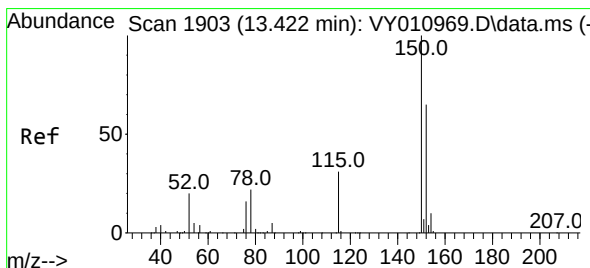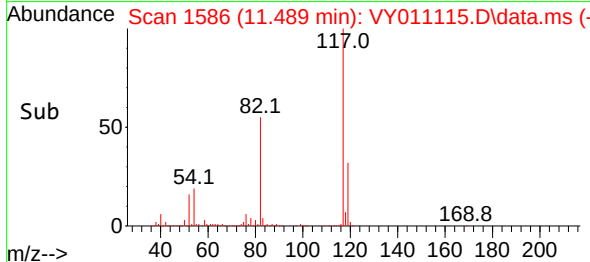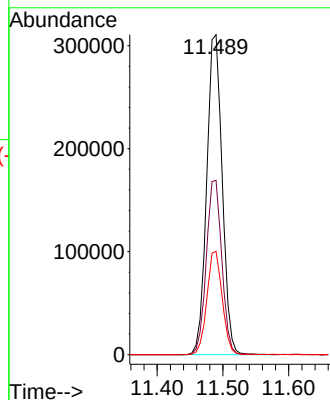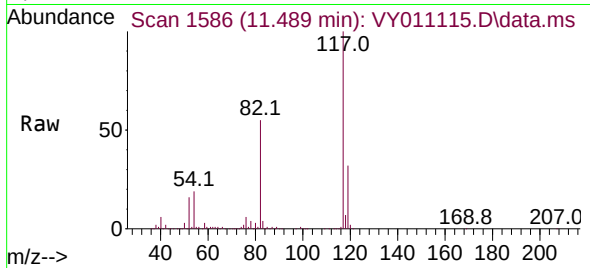

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY011115.D
Acq: 26 Oct 2022 14:50

Tgt Ion:152 Resp: 228537
Ion Ratio Lower Upper
152 100
115 58.2 28.2 84.7
150 156.7 0.0 347.6

