

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102722\
 Data File : VY011137.D
 Acq On : 27 Oct 2022 14:34
 Operator : KP/MD
 Sample : N5281-04RE
 Misc : 6.34g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-4RE

Quant Time: Oct 28 00:46:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101722S.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 18 01:42:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	72173	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	118429	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	106685	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	45290	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	36761	55.295	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	110.580%
35) Dibromofluoromethane	7.716	113	37467	57.059	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	114.120%
50) Toluene-d8	10.179	98	109583	44.315	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	88.640%
62) 4-Bromofluorobenzene	12.477	95	37903	42.831	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	85.660%
Target Compounds						
20) Methylene Chloride	4.704	84	13709	11.419	ug/l	Qvalue # 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102722\
Data File : VY011137.D
Acq On : 27 Oct 2022 14:34
Operator : KP/MD
Sample : N5281-04RE
Misc : 6.34g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-4RE

Quant Time: Oct 28 00:46:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101722S.M
Quant Title : SW846 8260
QLast Update : Tue Oct 18 01:42:42 2022
Response via : Initial Calibration




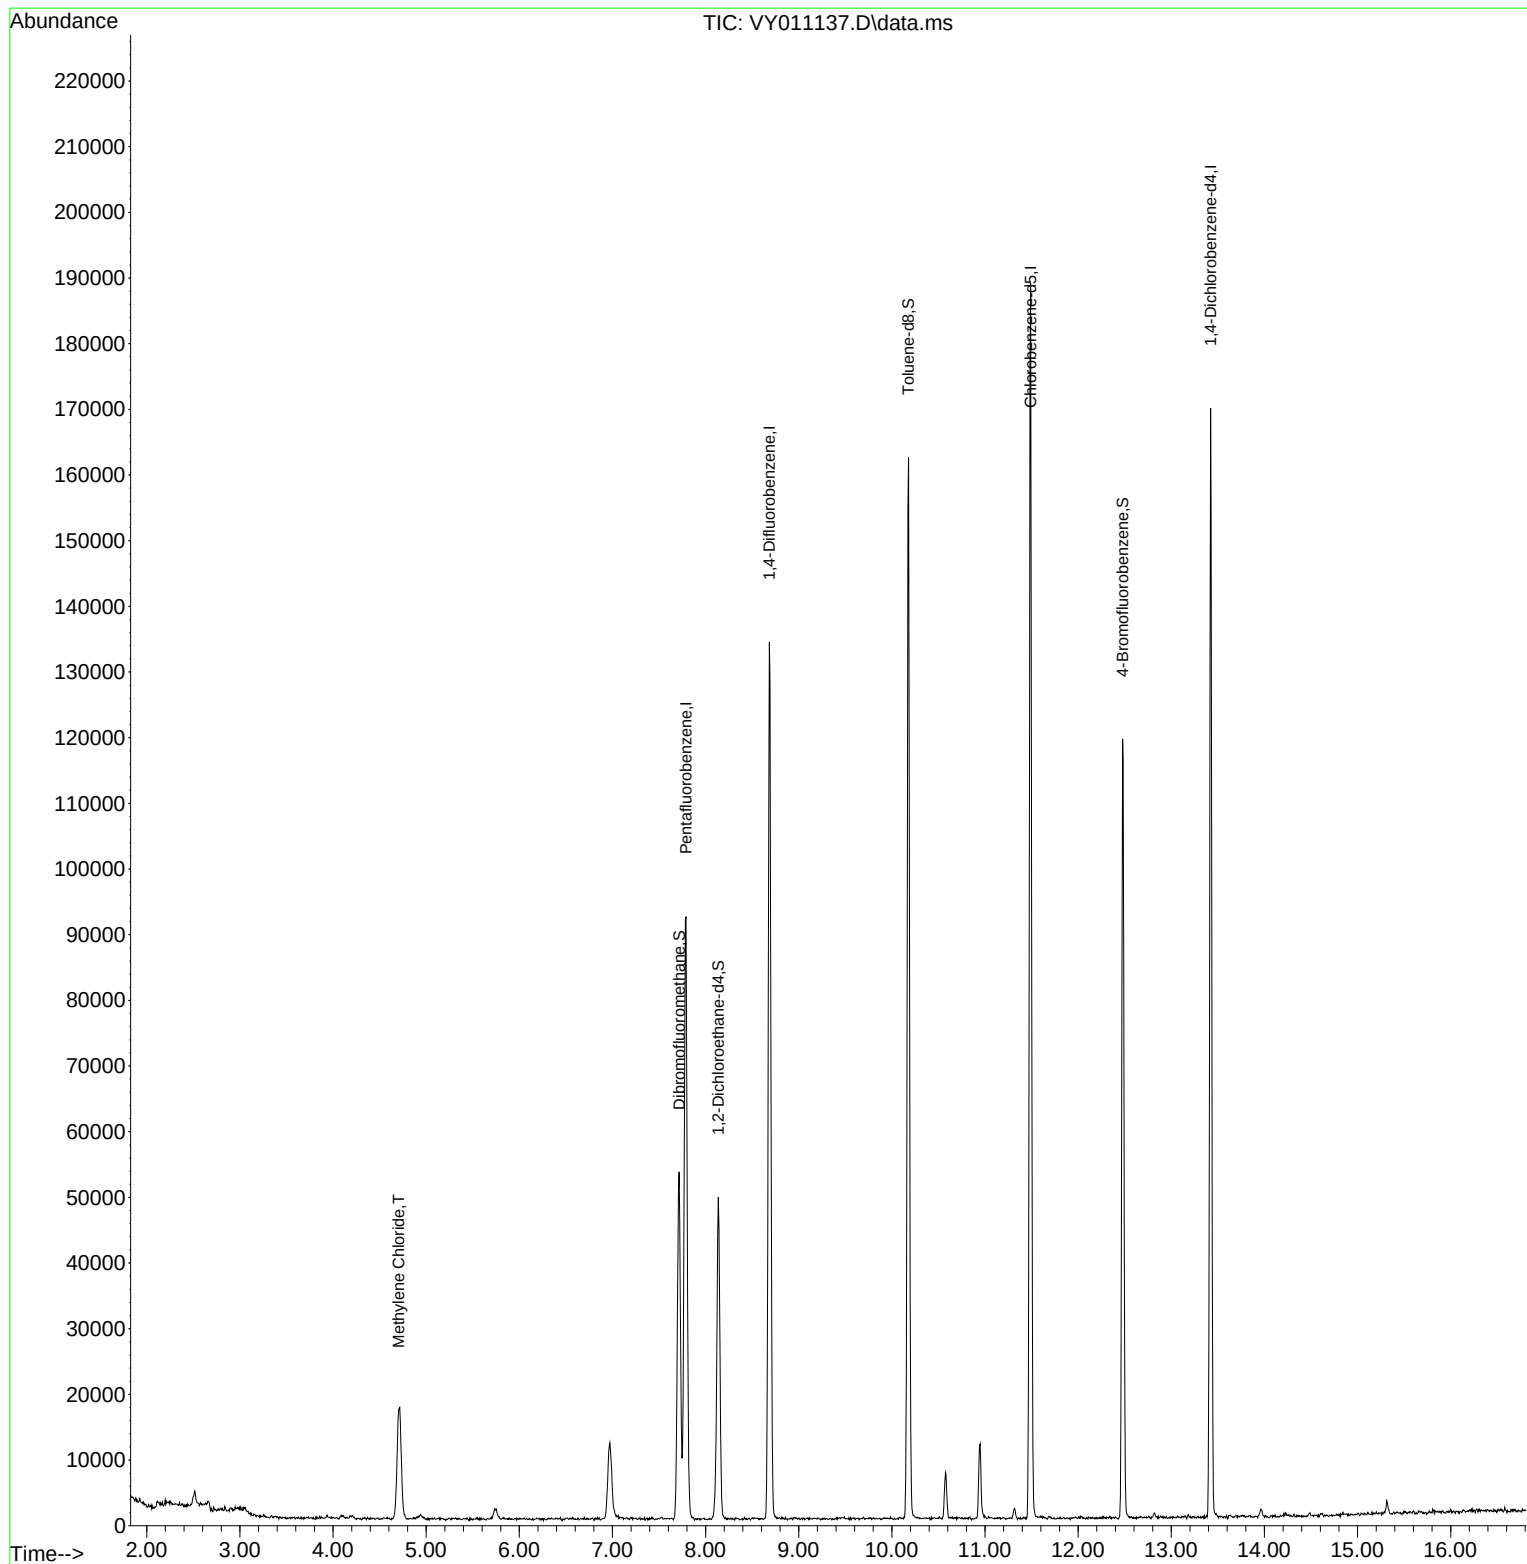


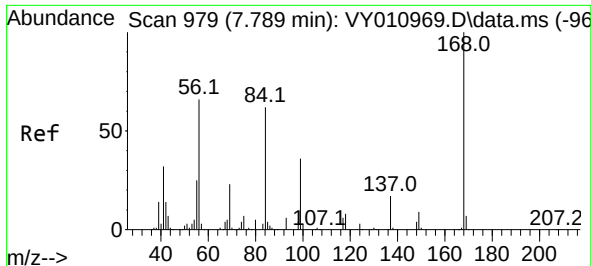

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY011137.D
Acq: 27 Oct 2022 14:34




Instrument :
MSVOA_Y
ClientSampleId :
SB-4RE


Tgt Ion:168 Resp: 72173
Ion Ratio Lower Upper
168 100
99 53.4 46.9 70.3

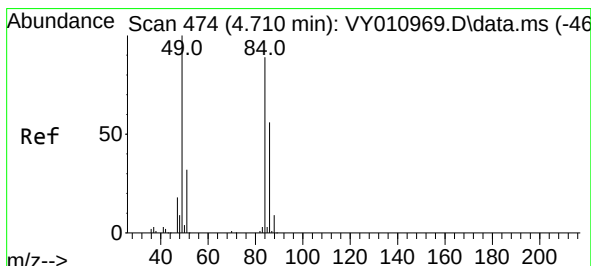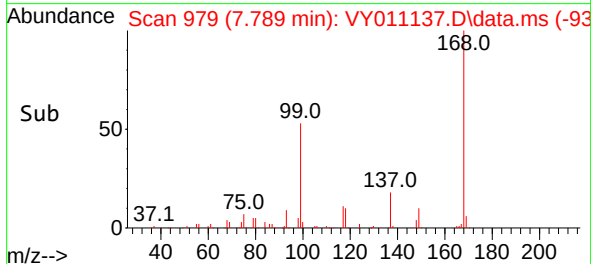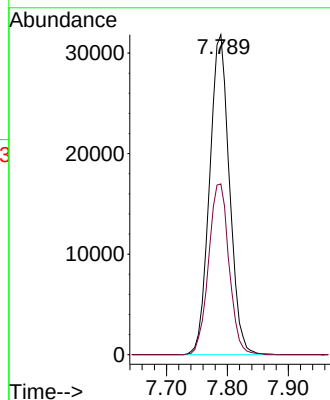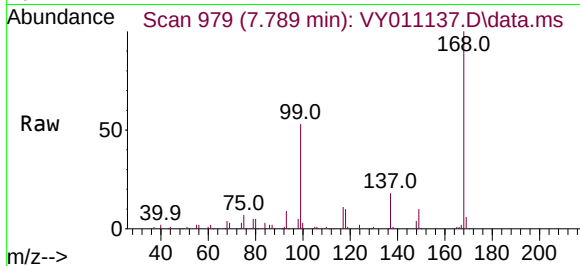

#20
Methylene Chloride
Concen: 11.419 ug/l
RT: 4.704 min Scan# 473
Delta R.T. -0.006 min
Lab File: VY011137.D
Acq: 27 Oct 2022 14:34

Tgt Ion: 84 Resp: 13709
Ion Ratio Lower Upper
84 100
49 114.1 114.4 171.6#
51 38.3 35.3 52.9
86 61.2 53.7 80.5

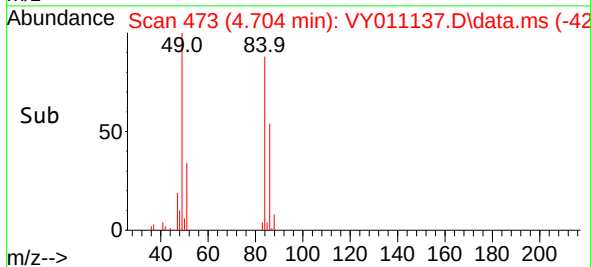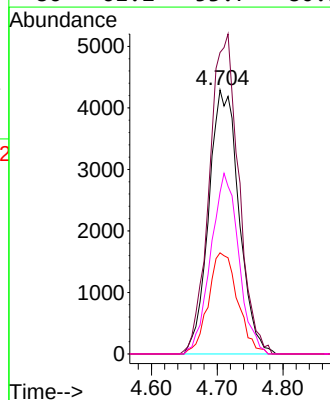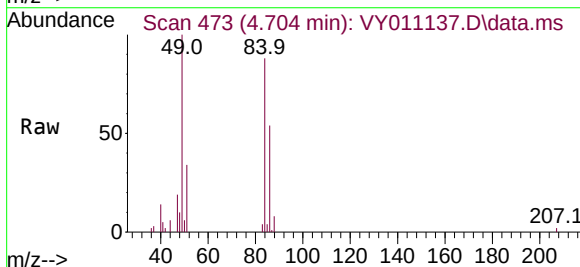

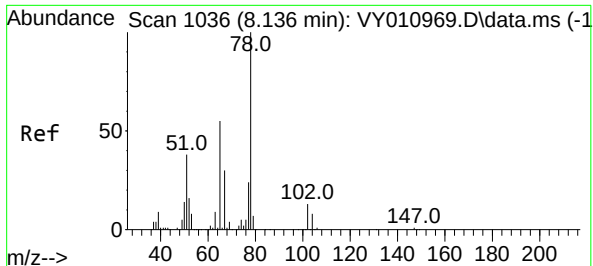

#33

1,2-Dichloroethane-d4

Concen: 55.295 ug/l

RT: 8.137 min Scan# 1036

Delta R.T. 0.001 min

Lab File: VY011137.D

Acq: 27 Oct 2022 14:34

Instrument :

MSVOA_Y

ClientSampleId :





SB-4RE

Tgt Ion: 65 Resp: 36761

Ion Ratio Lower Upper

65 100

67 53.4 0.0 99.4

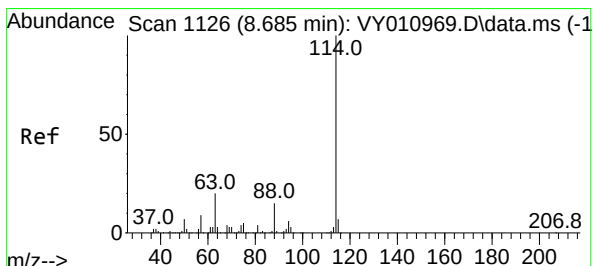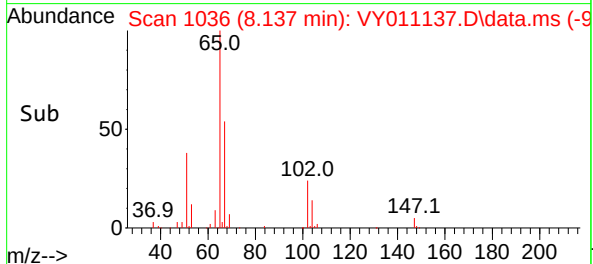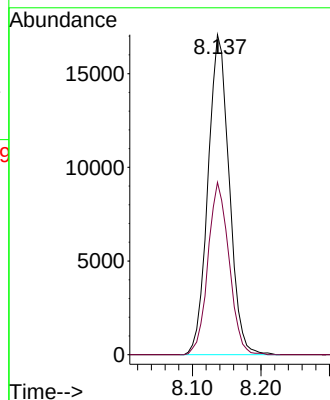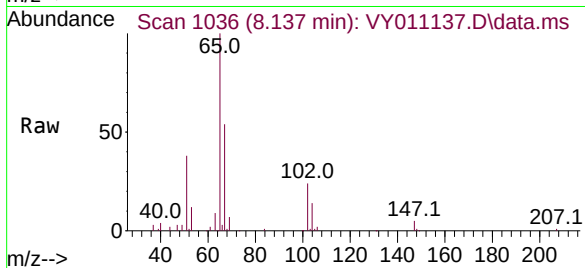

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY011137.D

Acq: 27 Oct 2022 14:34




Tgt Ion:114 Resp: 118429


Ion Ratio Lower Upper

114 100

63 20.1 0.0 43.2

88 15.2 0.0 31.8


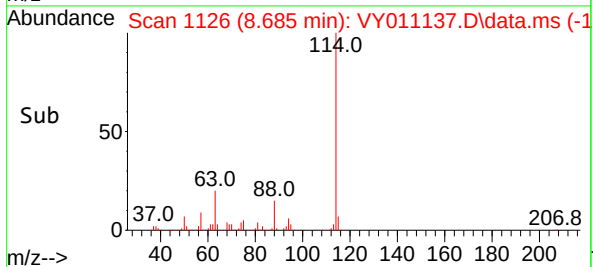
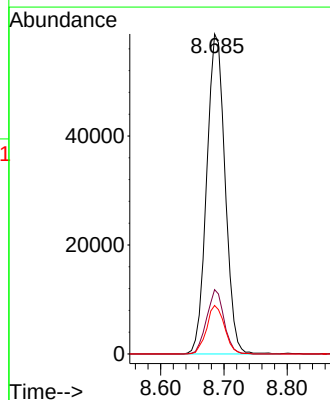
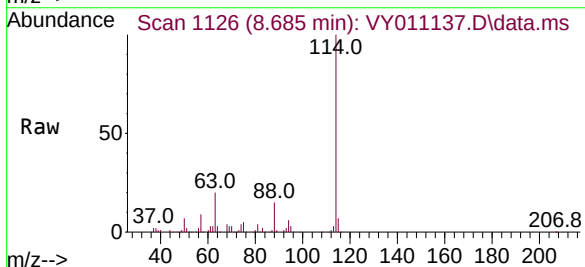


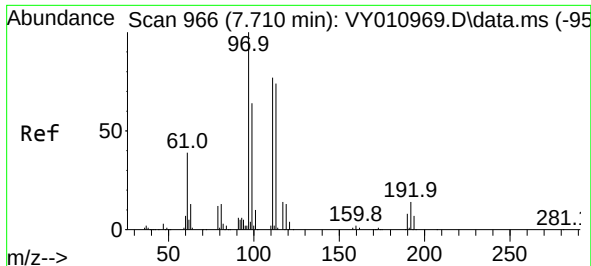

#35
Dibromofluoromethane
Concen: 57.059 ug/l
RT: 7.716 min Scan# 90
Delta R.T. 0.006 min
Lab File: VY011137.D
Acq: 27 Oct 2022 14:34




Instrument :
MSVOA_Y
ClientSampleId :
SB-4RE


Tgt Ion:113 Resp: 37467
Ion Ratio Lower Upper
113 100
111 104.2 82.6 124.0
192 19.3 17.6 26.4

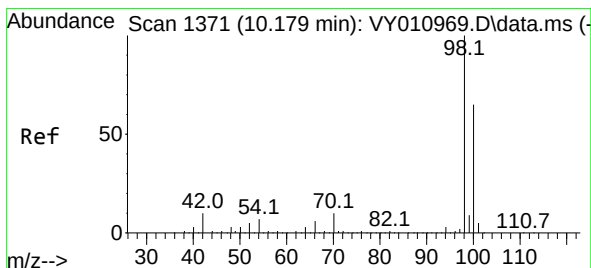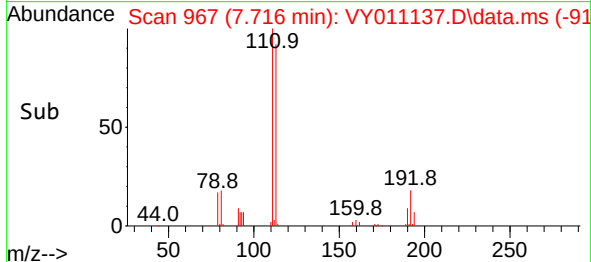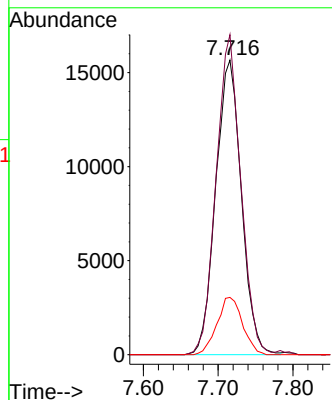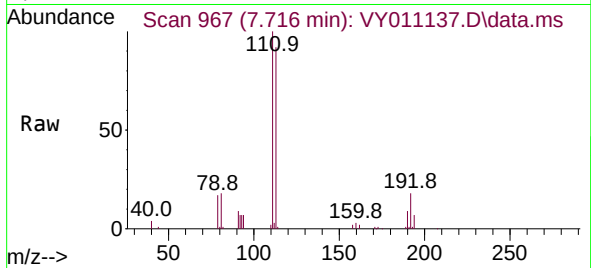

#50
Toluene-d8
Concen: 44.315 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY011137.D
Acq: 27 Oct 2022 14:34

Tgt Ion: 98 Resp: 109583
Ion Ratio Lower Upper
98 100
100 64.5 50.2 75.2


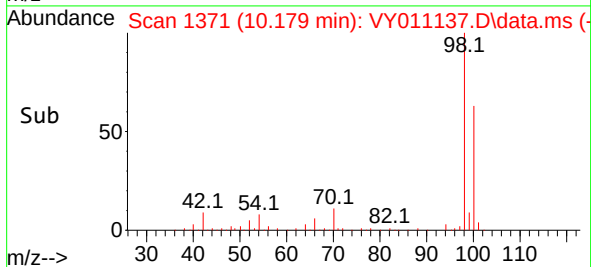
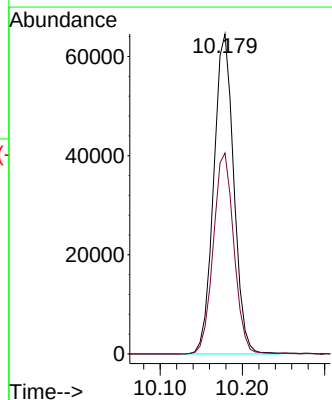
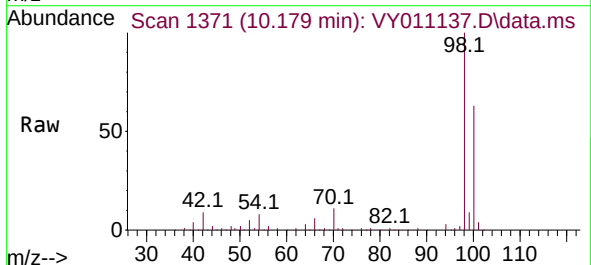


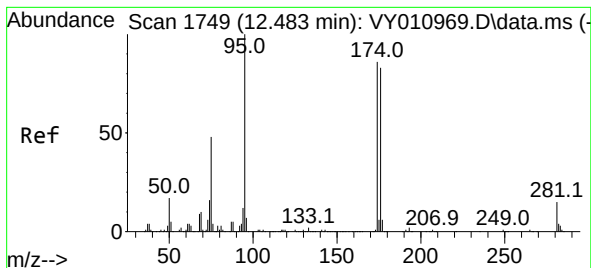

#62
4-Bromofluorobenzene
Concen: 42.831 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY011137.D
Acq: 27 Oct 2022 14:34




Instrument :
MSVOA_Y
ClientSampleId :
SB-4RE


Tgt Ion: 95 Resp: 37903
Ion Ratio Lower Upper
95 100
174 83.3 0.0 177.0
176 81.1 0.0 175.8

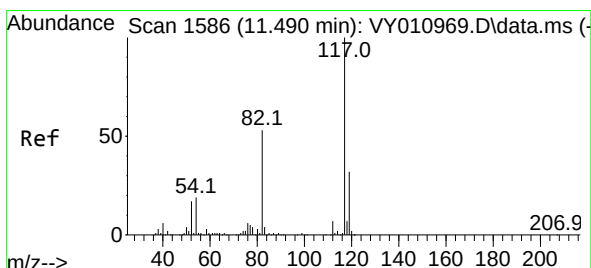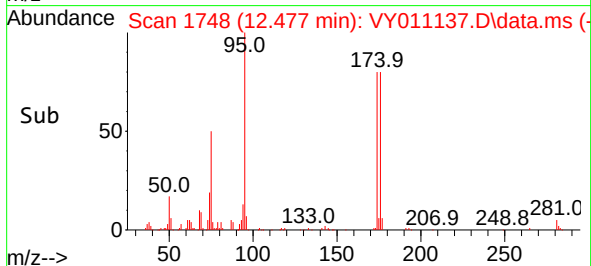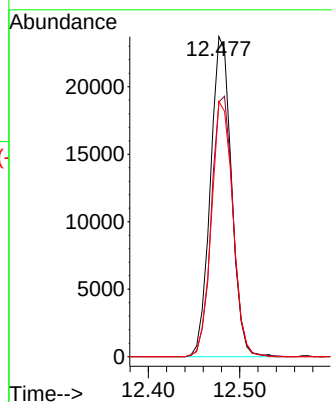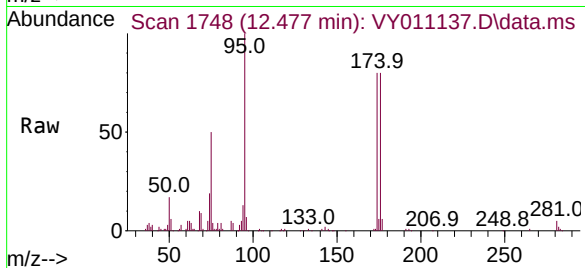

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY011137.D
Acq: 27 Oct 2022 14:34

Tgt Ion: 117 Resp: 106685
Ion Ratio Lower Upper
117 100
82 54.0 43.0 64.4
119 33.2 25.4 38.0

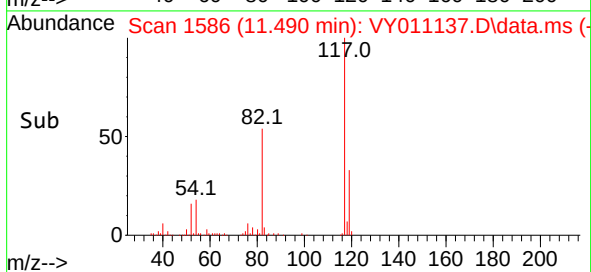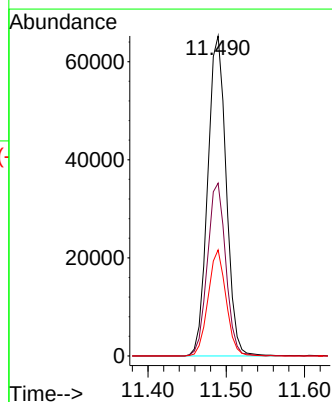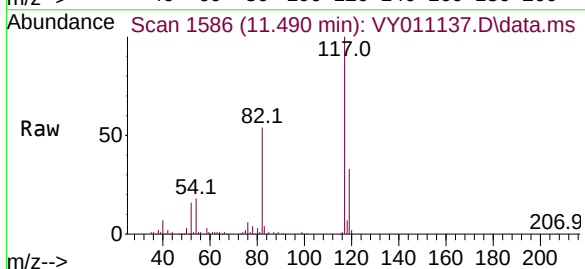

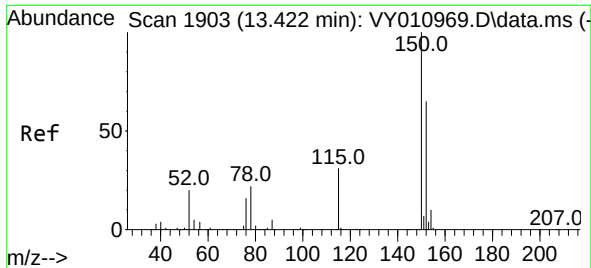

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.422 min Scan# 1903
 Delta R.T. 0.000 min
 Lab File: VY011137.D
 Acq: 27 Oct 2022 14:34

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-4RE

Tgt Ion	Ratio	Lower	Upper
152	100		
115	56.9	28.2	84.7
150	155.6	0.0	347.6

