
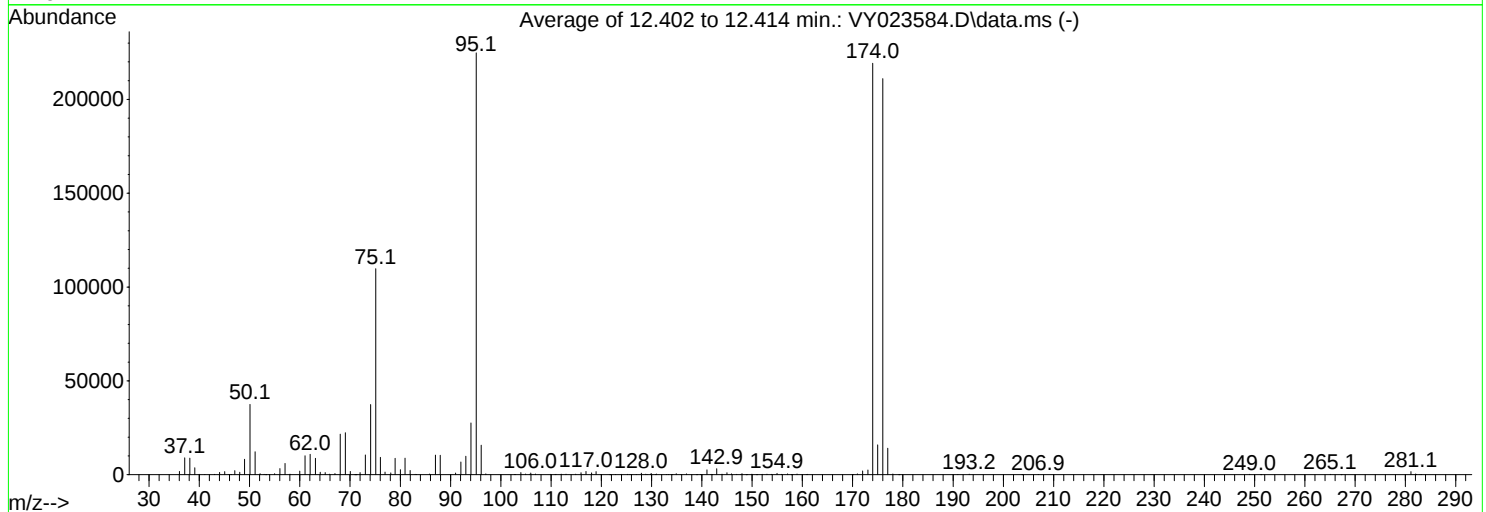


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102725\
Data File : VY023584.D
Acq On : 27 Oct 2025 08:37
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Title : SW846 8260
Last Update : Wed Oct 08 05:12:50 2025

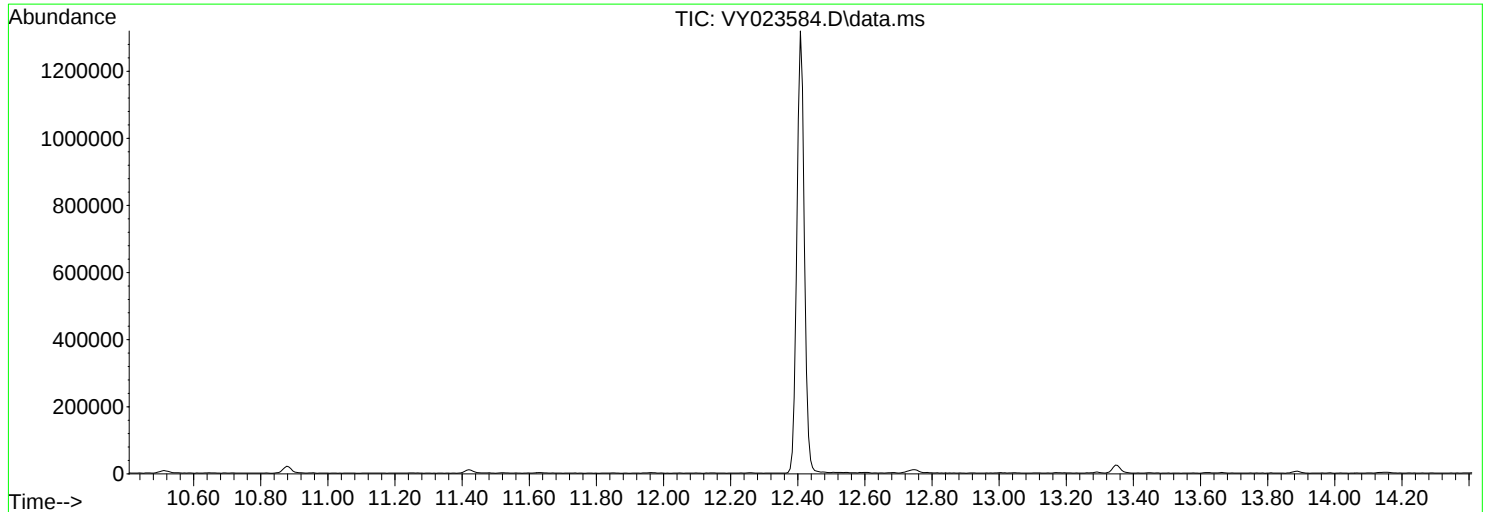

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	37477	PASS
75	95	30	60	48.8	109755	PASS
95	95	100	100	100.0	224832	PASS
96	95	5	9	7.0	15698	PASS
173	174	0.00	2	1.1	2507	PASS
174	95	50	100	97.5	219264	PASS
175	174	5	9	7.3	15911	PASS
176	174	95	101	96.3	211115	PASS
177	176	5	9	6.7	14098	PASS