

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102822\
 Data File : VY011163.D
 Acq On : 28 Oct 2022 17:41
 Operator : KP/MD
 Sample : N5316-13
 Misc : 8.85g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TOTAL-VOC-GRAB-1-PILE-2

Quant Time: Oct 28 23:46:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y102822S.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 28 23:42:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	286308	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	498875	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	435317	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	184533	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	189368	63.965	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	127.940%
35) Dibromofluoromethane	7.716	113	187151	61.003	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	122.000%
50) Toluene-d8	10.179	98	717161	59.006	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	118.020%
62) 4-Bromofluorobenzene	12.477	95	213562	53.701	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	107.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102822\
Data File : VY011163.D
Acq On : 28 Oct 2022 17:41
Operator : KP/MD
Sample : N5316-13
Misc : 8.85g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TOTAL-VOC-GRAB-1-PILE-2

Quant Time: Oct 28 23:46:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y102822S.M
Quant Title : SW846 8260
QLast Update : Fri Oct 28 23:42:14 2022
Response via : Initial Calibration




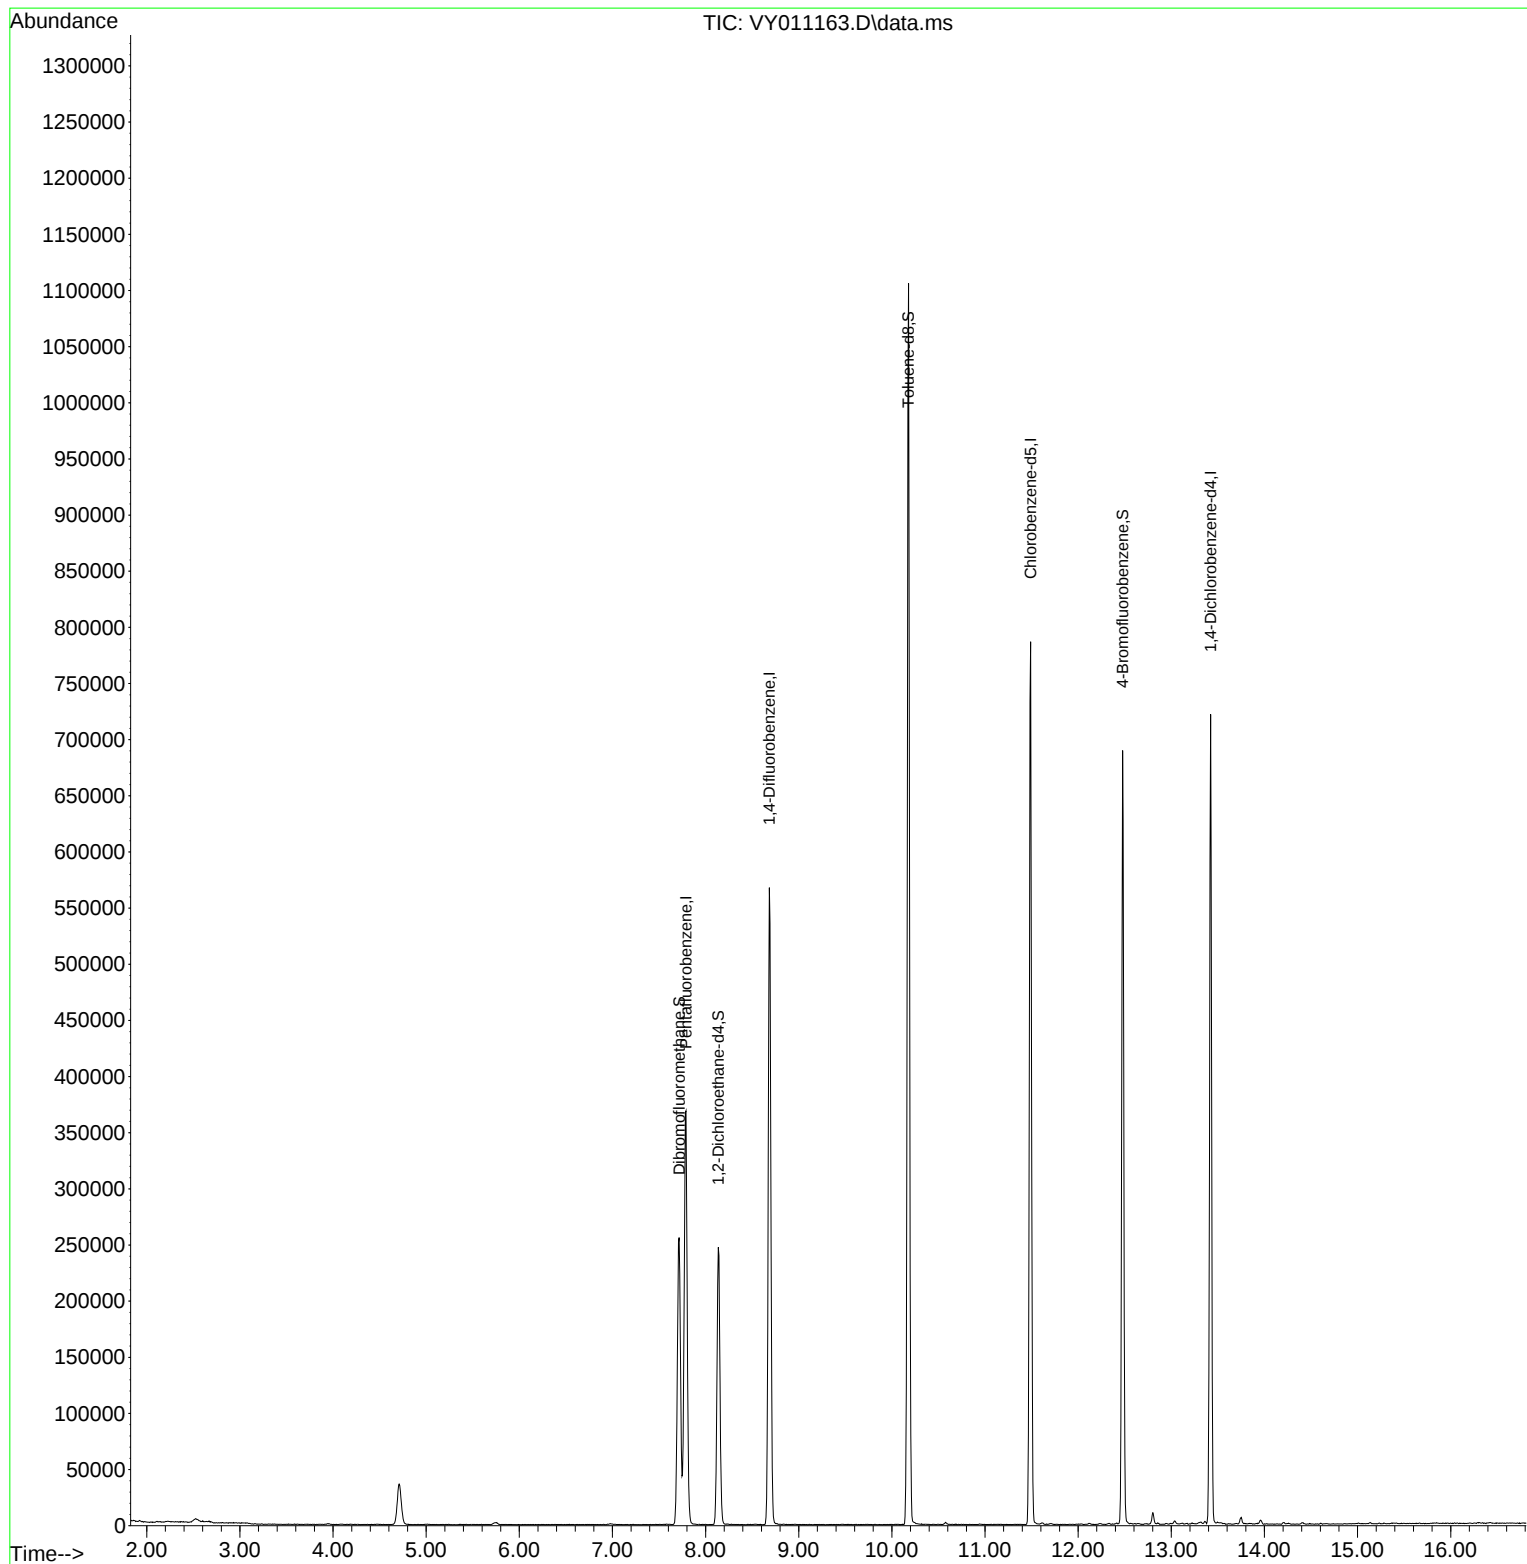


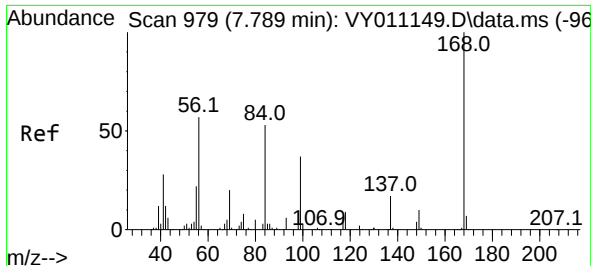

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY011163.D
Acq: 28 Oct 2022 17:41




Instrument :
MSVOA_Y
ClientSampleId :
TOTAL-VOC-GRAB-1-PILE-2


Tgt Ion:168 Resp: 286308
Ion Ratio Lower Upper
168 100
99 53.0 46.9 70.3

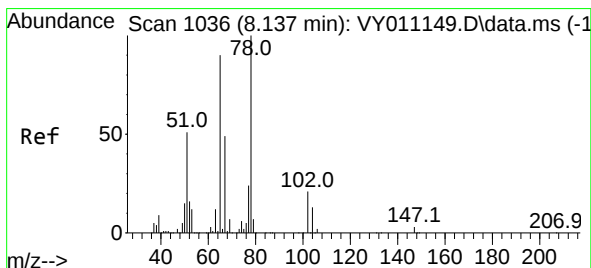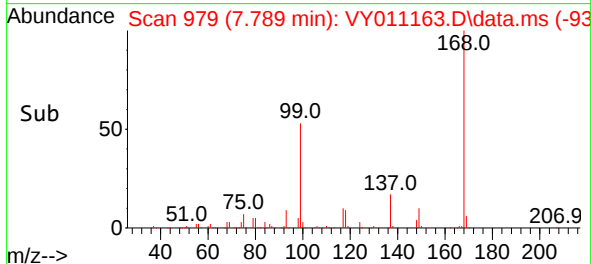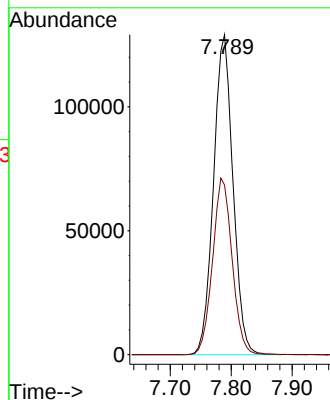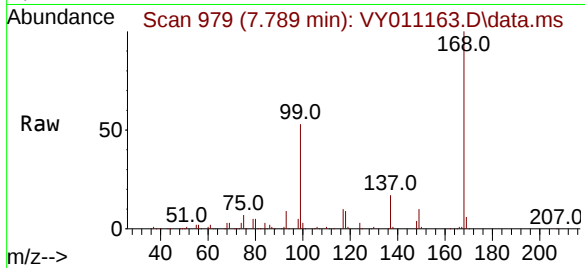

#33
1,2-Dichloroethane-d4
Concen: 63.965 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.001 min
Lab File: VY011163.D
Acq: 28 Oct 2022 17:41

Tgt Ion: 65 Resp: 189368
Ion Ratio Lower Upper
65 100
67 54.6 0.0 99.4


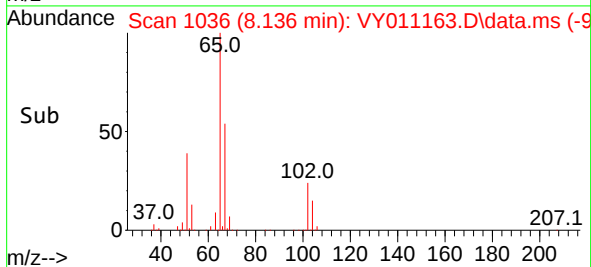
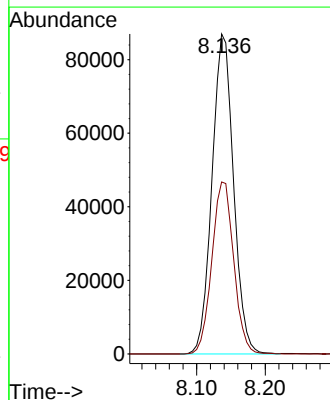
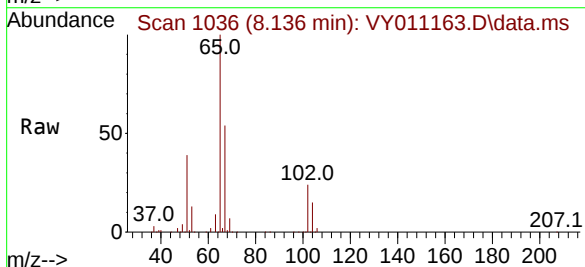


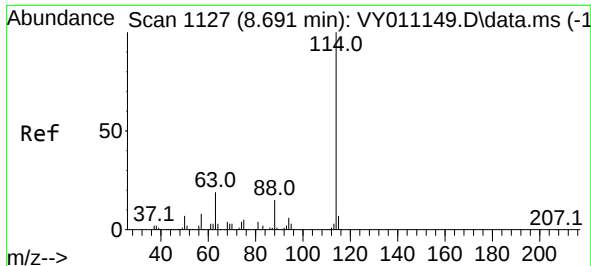

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. -0.006 min
Lab File: VY011163.D
Acq: 28 Oct 2022 17:41




Instrument :
MSVOA_Y
ClientSampleId :
TOTAL-VOC-GRAB-1-PILE-2


Tgt Ion:114 Resp: 498875
Ion Ratio Lower Upper
114 100
63 19.3 0.0 43.2
88 15.5 0.0 31.8

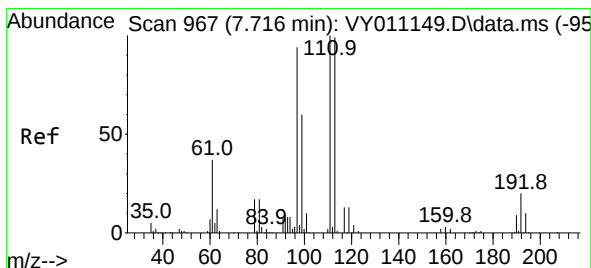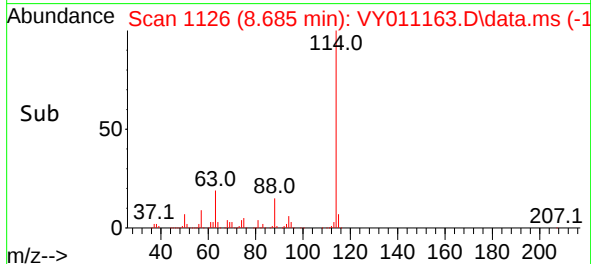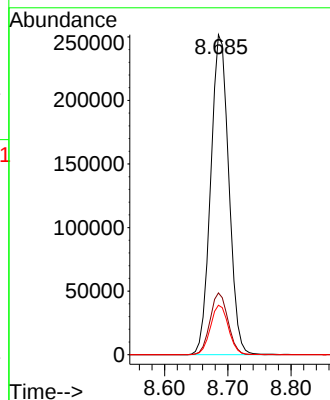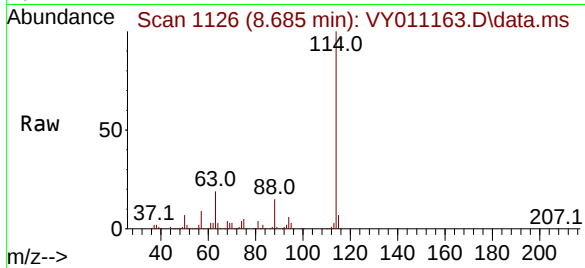

#35
Dibromofluoromethane
Concen: 61.003 ug/l
RT: 7.716 min Scan# 967
Delta R.T. -0.000 min
Lab File: VY011163.D
Acq: 28 Oct 2022 17:41

Tgt Ion:113 Resp: 187151
Ion Ratio Lower Upper
113 100
111 102.8 82.6 124.0
192 19.3 17.6 26.4

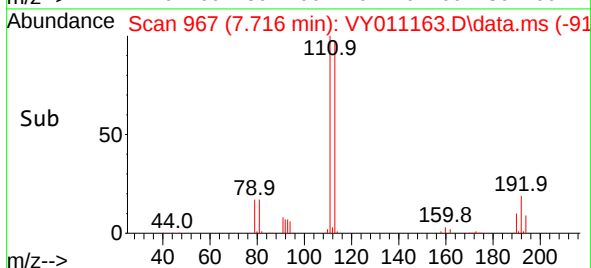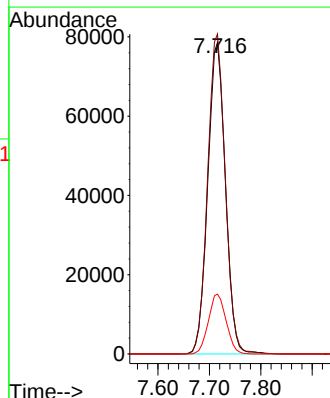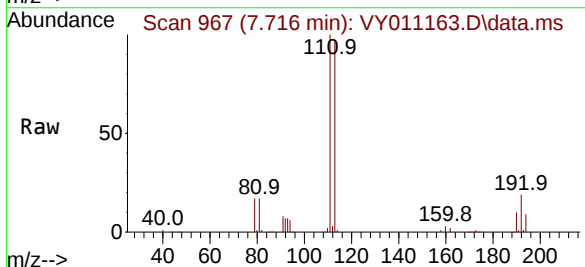

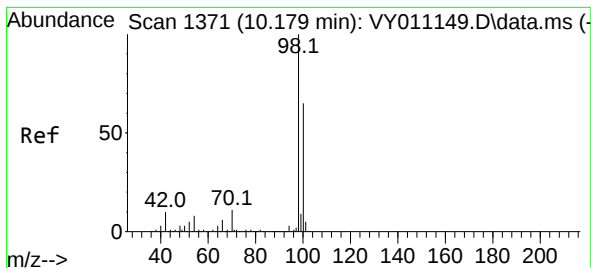

#50

Toluene-d8

Concen: 59.006 ug/l

RT: 10.179 min Scan# 1371

Delta R.T. -0.000 min

Lab File: VY011163.D

Acq: 28 Oct 2022 17:41

Instrument :

MSVOA_Y

ClientSampleId :





TOTAL-VOC-GRAB-1-PILE-2

Tgt Ion: 98 Resp: 717161

Ion Ratio Lower Upper

98 100

100 64.5 50.2 75.2

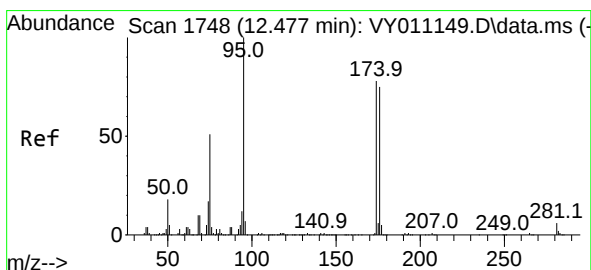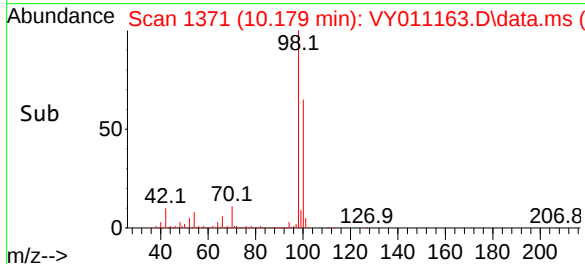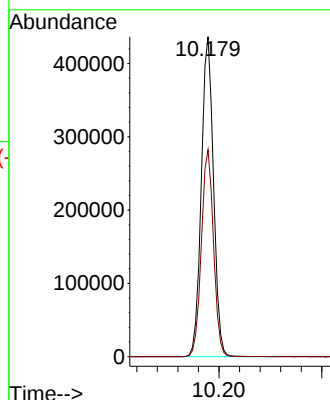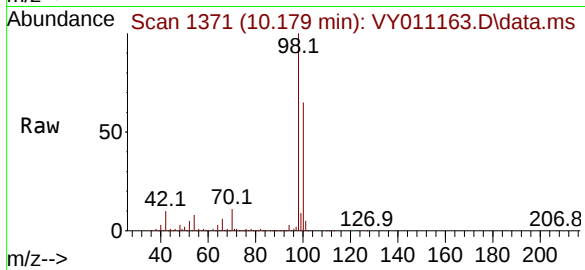

#62

4-Bromofluorobenzene

Concen: 53.701 ug/l

RT: 12.477 min Scan# 1748

Delta R.T. 0.000 min

Lab File: VY011163.D

Acq: 28 Oct 2022 17:41




Tgt Ion: 95 Resp: 213562


Ion Ratio Lower Upper

95 100

174 83.8 0.0 177.0

176 79.8 0.0 175.8


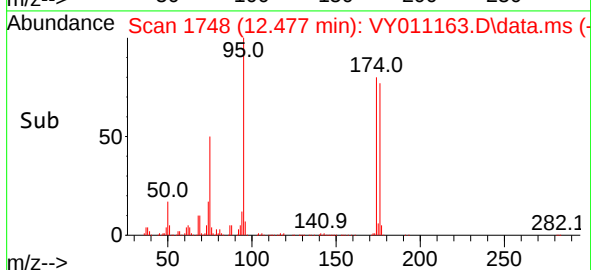
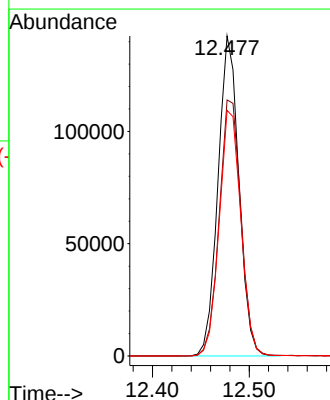
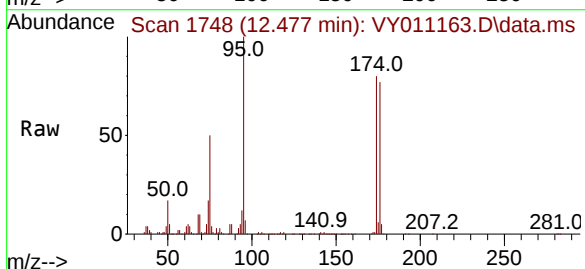


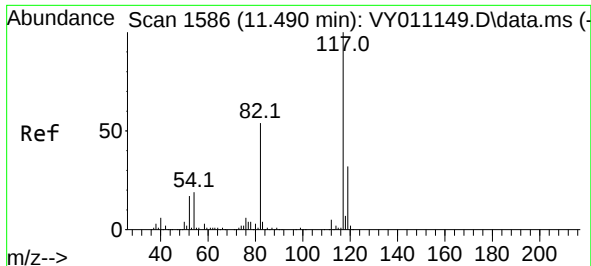

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY011163.D
Acq: 28 Oct 2022 17:41

Instrument :
MSVOA_Y
ClientSampleId :
TOTAL-VOC-GRAB-1-PILE-2

Tgt Ion:117 Resp: 435317
Ion Ratio Lower Upper
117 100
82 54.5 43.0 64.4
119 31.9 25.4 38.0

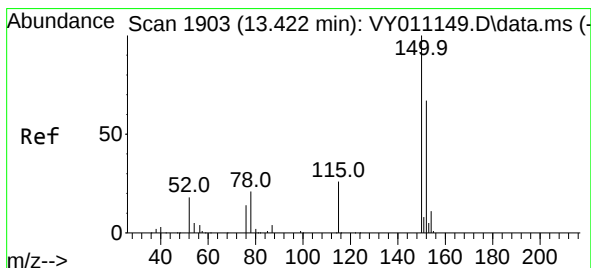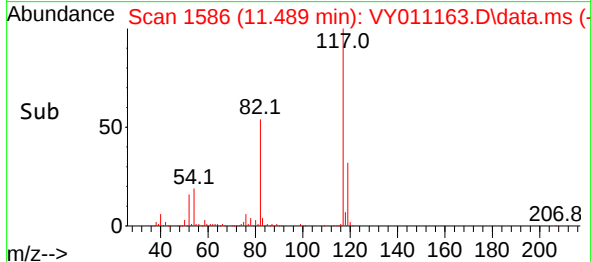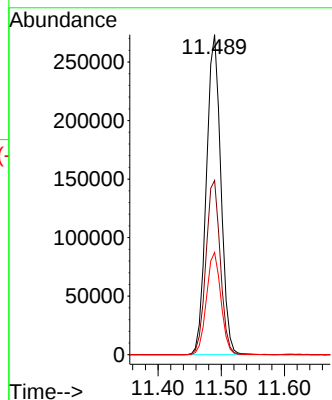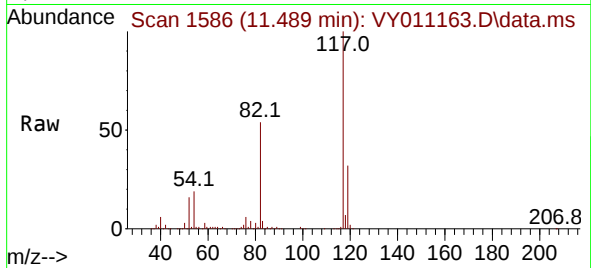

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY011163.D
Acq: 28 Oct 2022 17:41

Tgt Ion:152 Resp: 184533
Ion Ratio Lower Upper
152 100
115 58.2 28.2 84.7
150 156.2 0.0 347.6

