
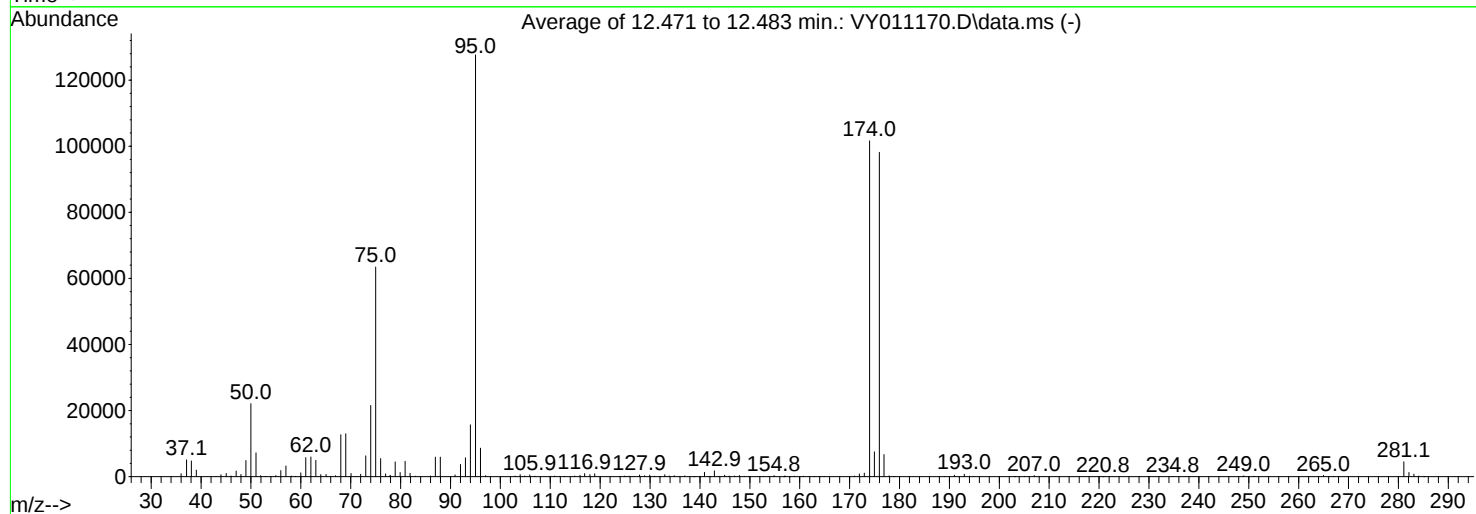


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102822\
Data File : VY011170.D
Acq On : 28 Oct 2022 20:42
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y102822S.M
Title : SW846 8260
Last Update : Fri Oct 28 23:42:14 2022

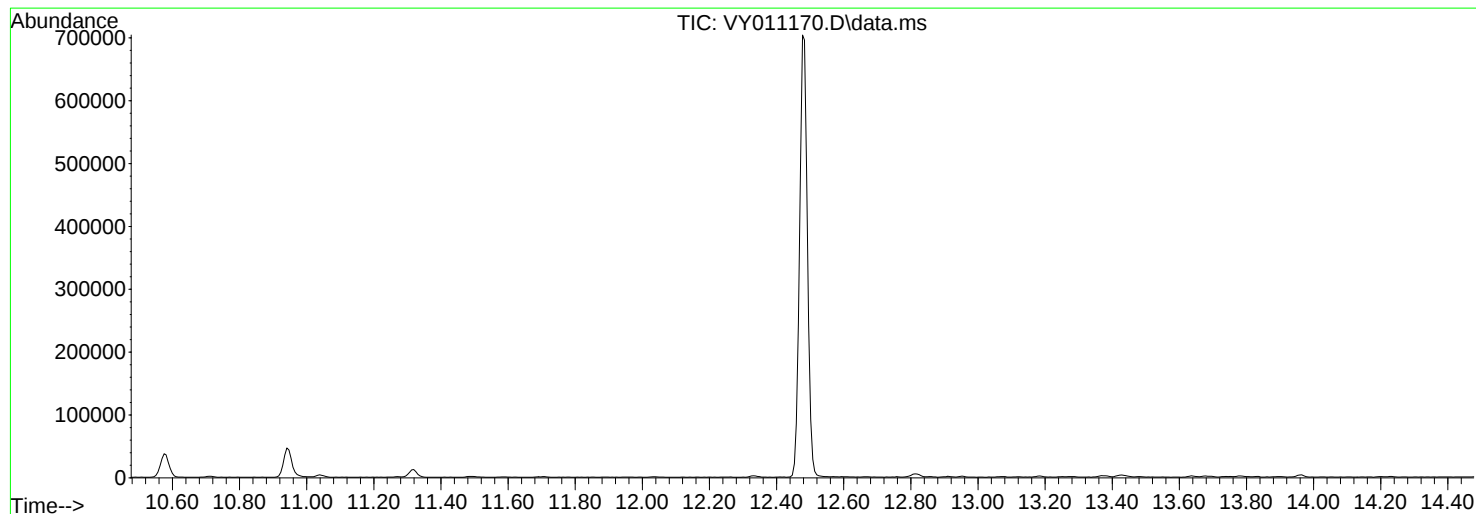

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	22067	PASS
75	95	30	60	49.7	63424	PASS
95	95	100	100	100.0	127653	PASS
96	95	5	9	6.8	8631	PASS
173	174	0.00	2	1.1	1088	PASS
174	95	50	100	79.6	101635	PASS
175	174	5	9	7.4	7531	PASS
176	174	95	101	96.6	98165	PASS
177	176	5	9	6.8	6689	PASS