

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102824\
 Data File : VY020044.D
 Acq On : 28 Oct 2024 17:28
 Operator : SY/MD
 Sample : P4567-07
 Misc : 4.10g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-2-VOC

Quant Time: Oct 29 02:00:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 16 05:44:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	180740	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.616	114	382823	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	350087	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	116145	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	131264	58.983	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	117.960%
35) Dibromofluoromethane	7.634	113	127383	50.425	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.840%
50) Toluene-d8	10.103	98	477706	51.207	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	102.420%
62) 4-Bromofluorobenzene	12.401	95	139811	41.477	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	82.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102824\
Data File : VY020044.D
Acq On : 28 Oct 2024 17:28
Operator : SY/MD
Sample : P4567-07
Misc : 4.10g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-2-VOC

Quant Time: Oct 29 02:00:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100924S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 16 05:44:48 2024
Response via : Initial Calibration




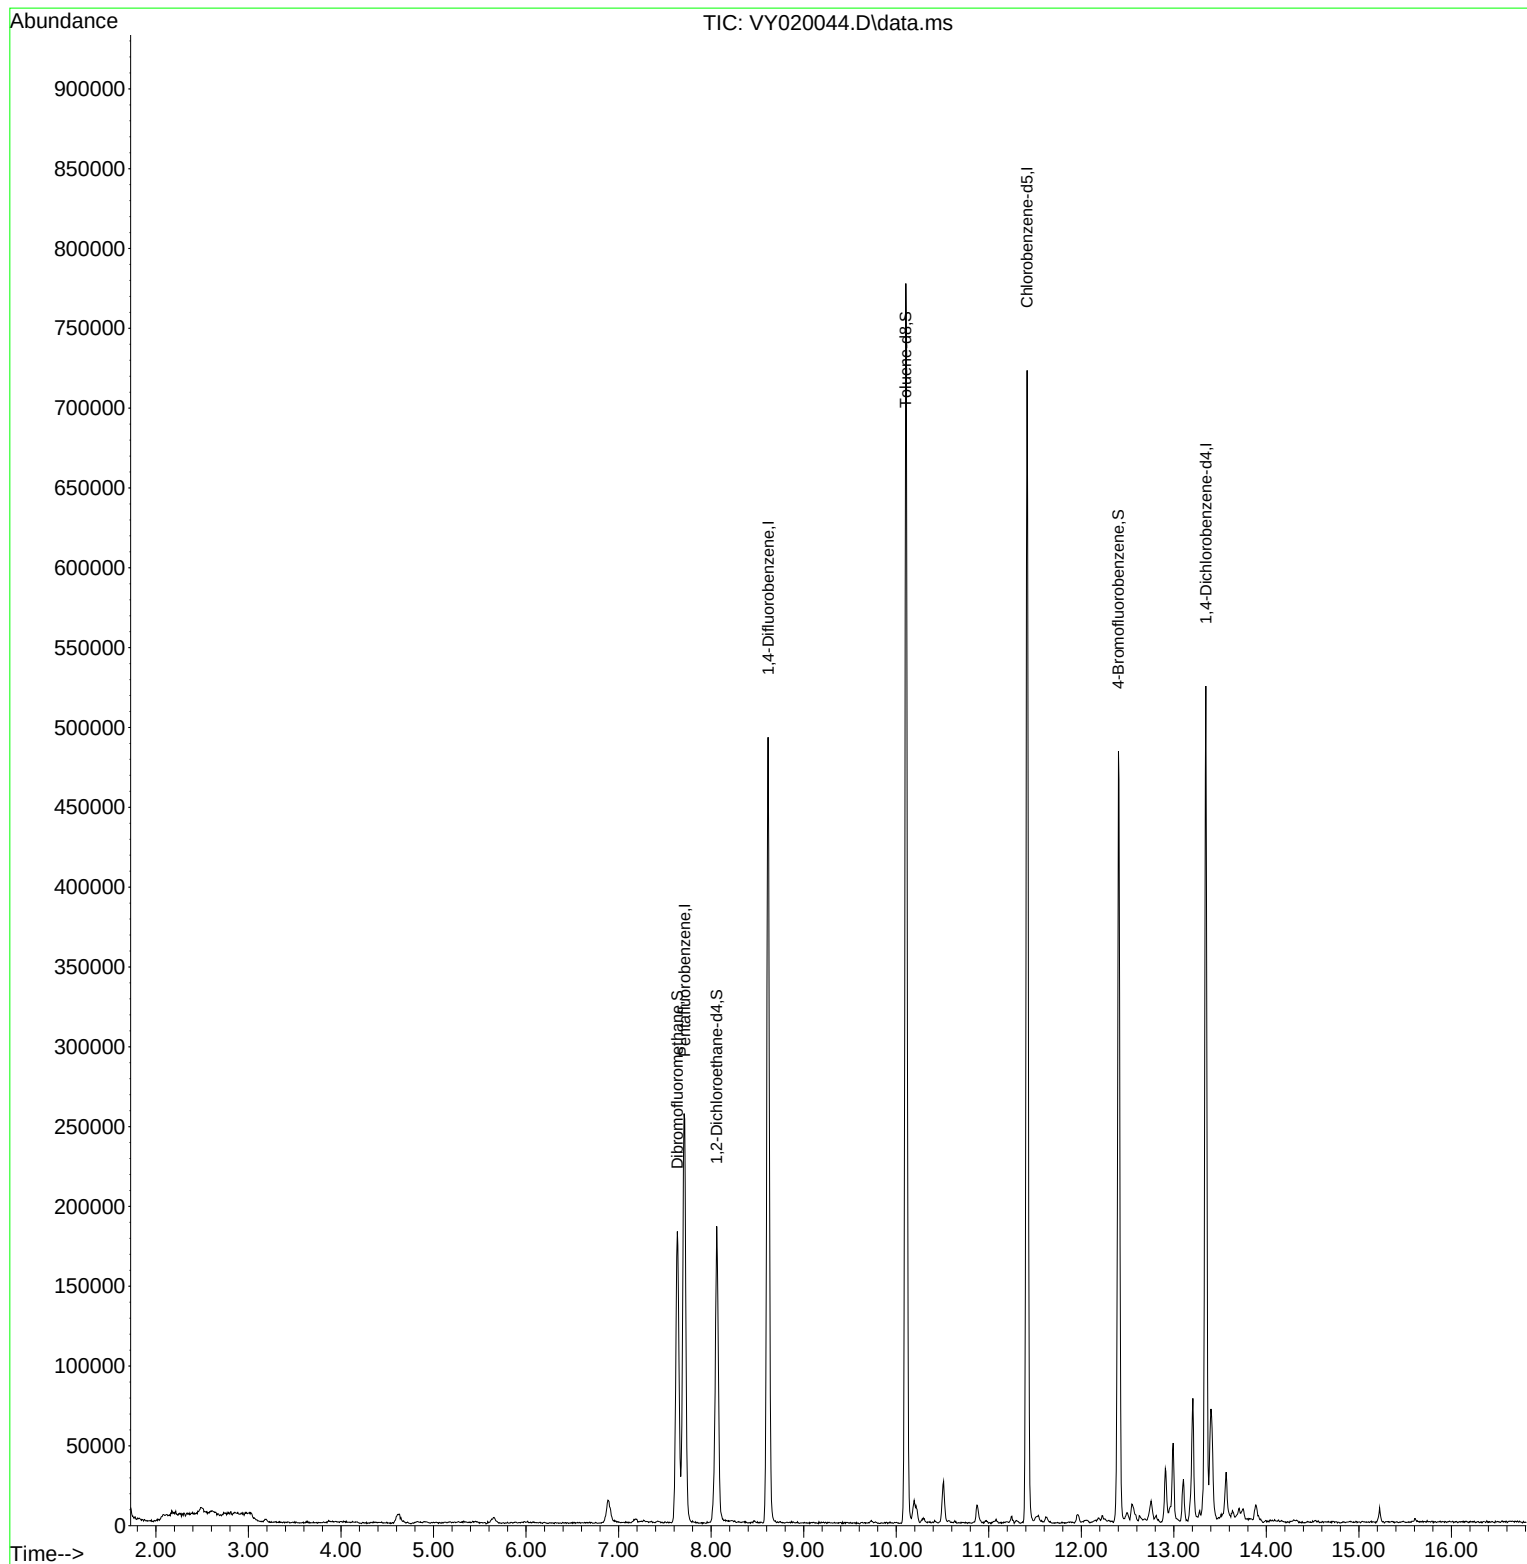


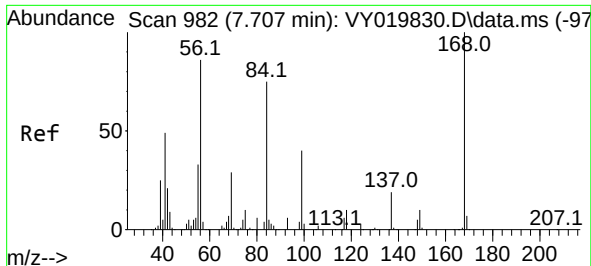

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY020044.D
Acq: 28 Oct 2024 17:28




Instrument :
MSVOA_Y
ClientSampleId :
WC-2-VOC


Tgt Ion:168 Resp: 180740
Ion Ratio Lower Upper
168 100
99 60.1 39.1 58.7#

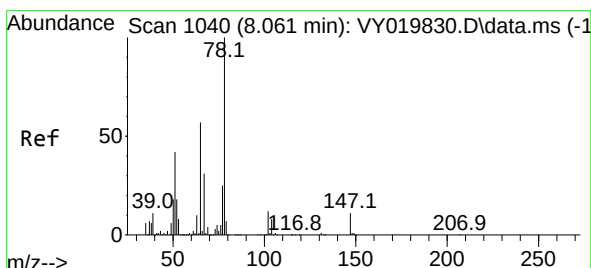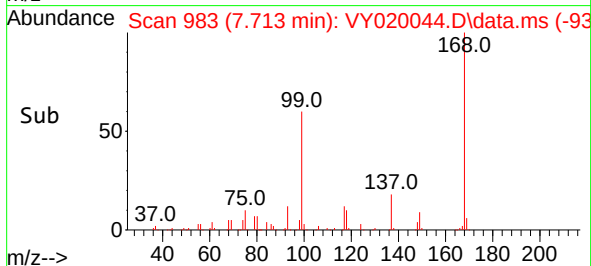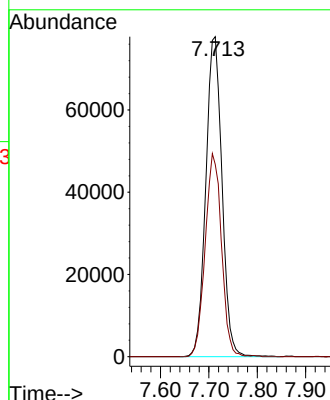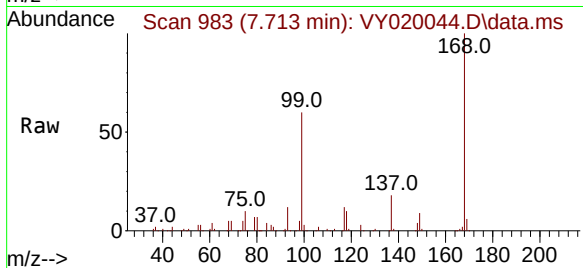

#33
1,2-Dichloroethane-d4
Concen: 58.983 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY020044.D
Acq: 28 Oct 2024 17:28

Tgt Ion: 65 Resp: 131264
Ion Ratio Lower Upper
65 100
67 52.4 0.0 109.6


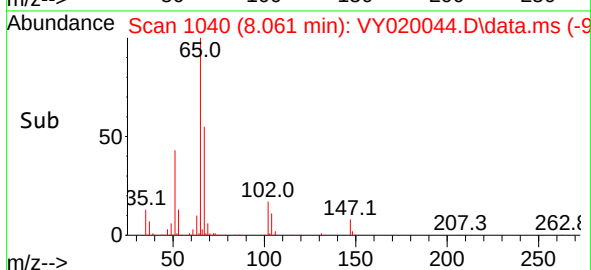
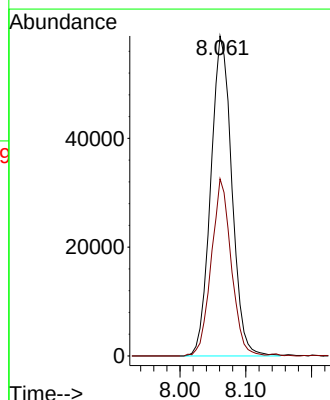
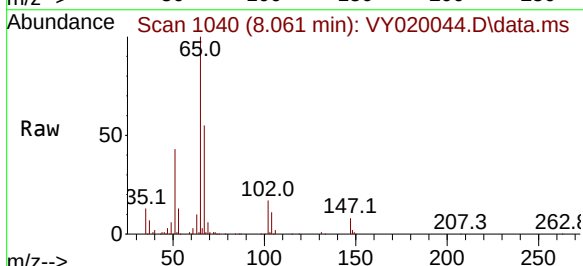


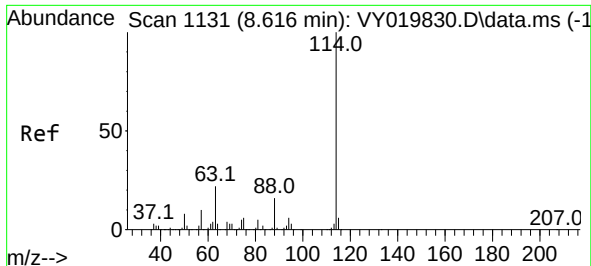

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY020044.D
Acq: 28 Oct 2024 17:28




Instrument :
MSVOA_Y
ClientSampleId :
WC-2-VOC


Tgt Ion:114 Resp: 382823
Ion Ratio Lower Upper
114 100
63 22.9 0.0 35.0
88 16.6 0.0 27.2

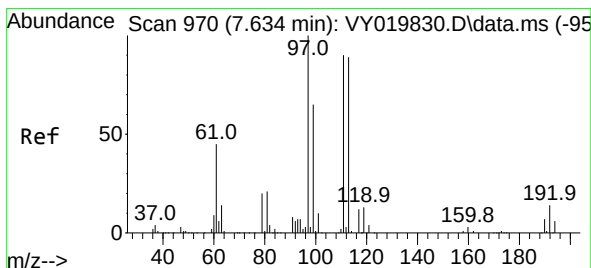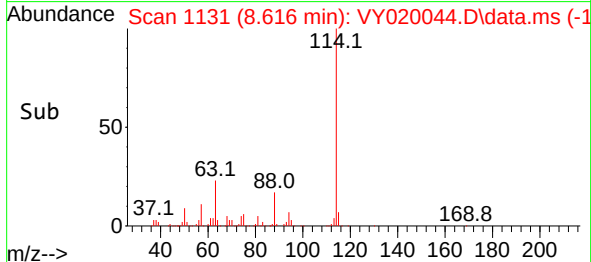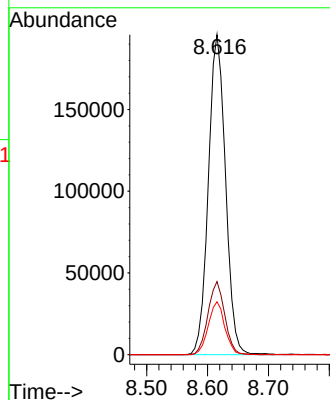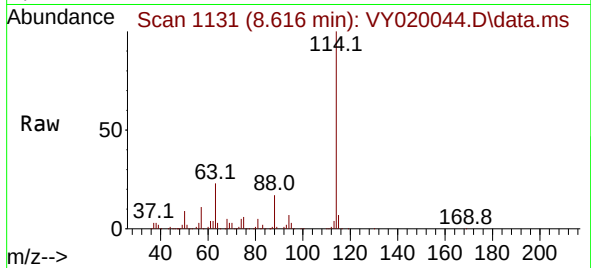

#35
Dibromofluoromethane
Concen: 50.425 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY020044.D
Acq: 28 Oct 2024 17:28

Tgt Ion:113 Resp: 127383
Ion Ratio Lower Upper
113 100
111 103.6 82.2 123.4
192 16.0 15.9 23.9


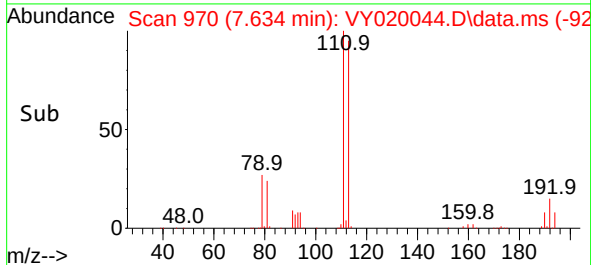
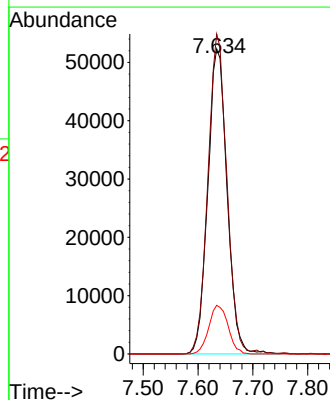
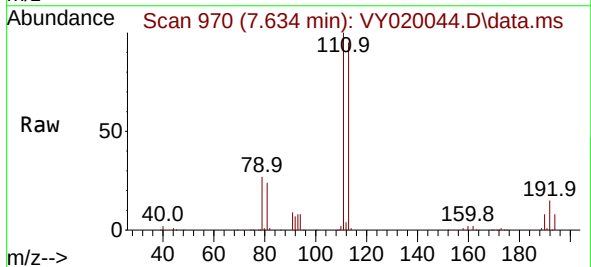


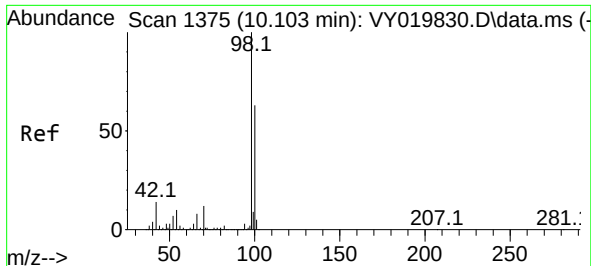

#50
Toluene-d8
Concen: 51.207 ug/l
RT: 10.103 min Scan# 1375
Delta R.T. -0.006 min
Lab File: VY020044.D
Acq: 28 Oct 2024 17:28




Instrument :
MSVOA_Y
ClientSampleId :
WC-2-VOC


Tgt Ion: 98 Resp: 477706
Ion Ratio Lower Upper
98 100
100 64.3 52.0 78.0

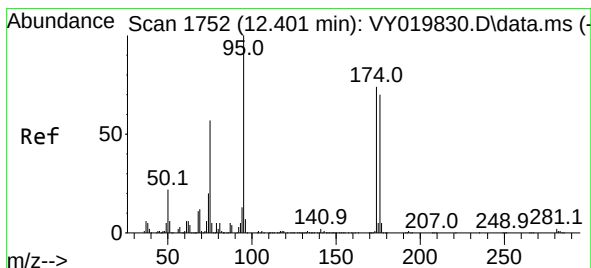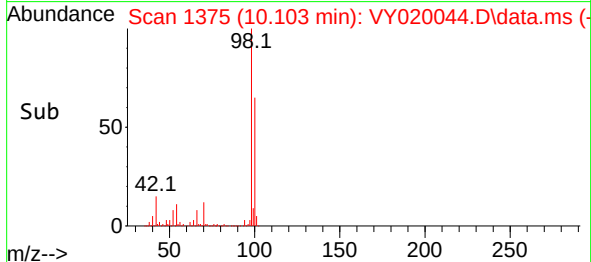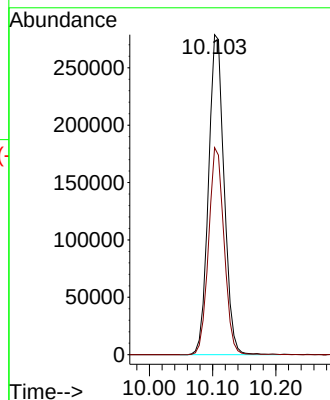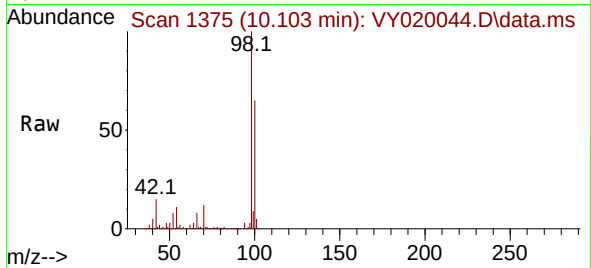

#62
4-Bromofluorobenzene
Concen: 41.477 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. -0.006 min
Lab File: VY020044.D
Acq: 28 Oct 2024 17:28

Tgt Ion: 95 Resp: 139811
Ion Ratio Lower Upper
95 100
174 73.6 0.0 175.6
176 71.1 0.0 171.4

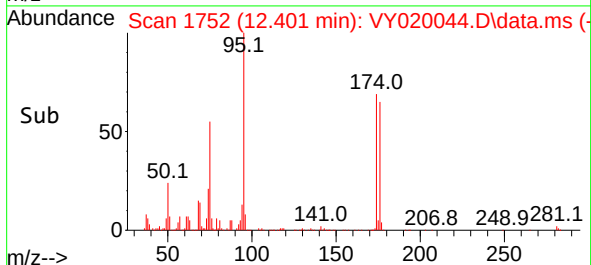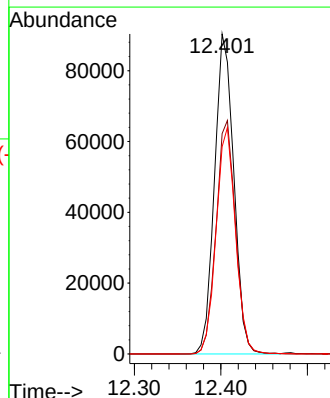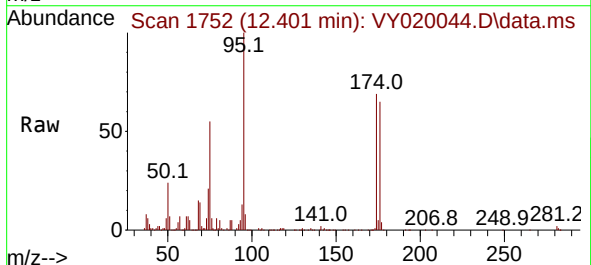

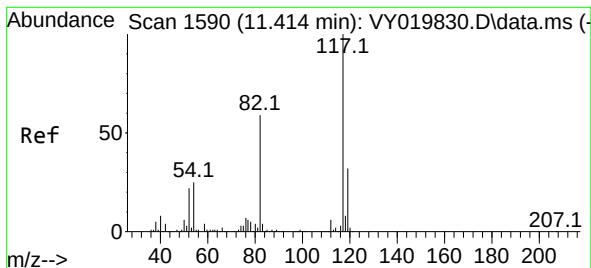

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY020044.D

Acq: 28 Oct 2024 17:28

Instrument :

MSVOA_Y

ClientSampleId :

WC-2-VOC





Tgt Ion:117 Resp: 350087

Ion Ratio Lower Upper

117 100

82 59.5 42.4 63.6

119 32.0 25.9 38.9

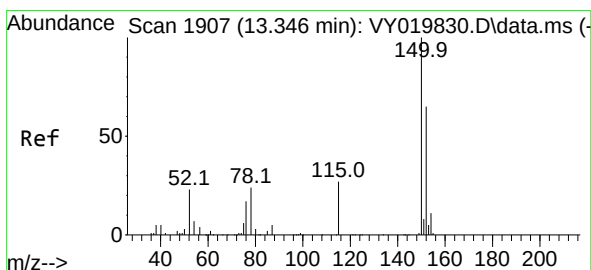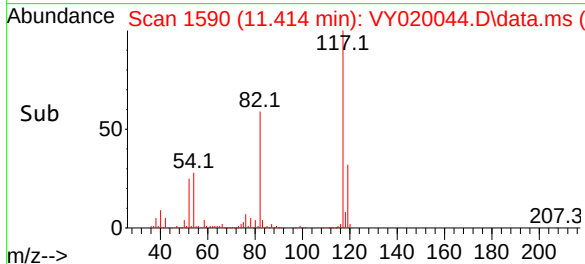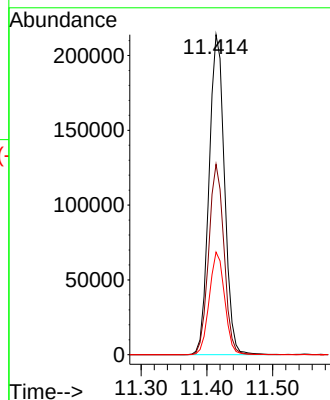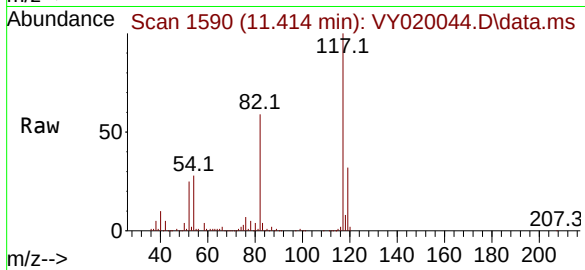

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY020044.D

Acq: 28 Oct 2024 17:28

Tgt Ion:152 Resp: 116145

Ion Ratio Lower Upper

152 100

115 60.7 28.2 84.7

150 158.5 0.0 345.6

