

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102825\
 Data File : VY023602.D
 Acq On : 28 Oct 2025 11:03
 Operator : SY/MD
 Sample : Q3460-19
 Misc : 5.13g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-5-VOC

Quant Time: Oct 29 06:23:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	699508	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	1162114	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	937535	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	332594	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	307782	52.618	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	105.240%
35) Dibromofluoromethane	7.634	113	366598	51.340	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.680%
50) Toluene-d8	10.109	98	1303992	49.036	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	98.080%
62) 4-Bromofluorobenzene	12.408	95	334787	38.133	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	76.260%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102825\
Data File : VY023602.D
Acq On : 28 Oct 2025 11:03
Operator : SY/MD
Sample : Q3460-19
Misc : 5.13g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-5-VOC

Quant Time: Oct 29 06:23:38 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration



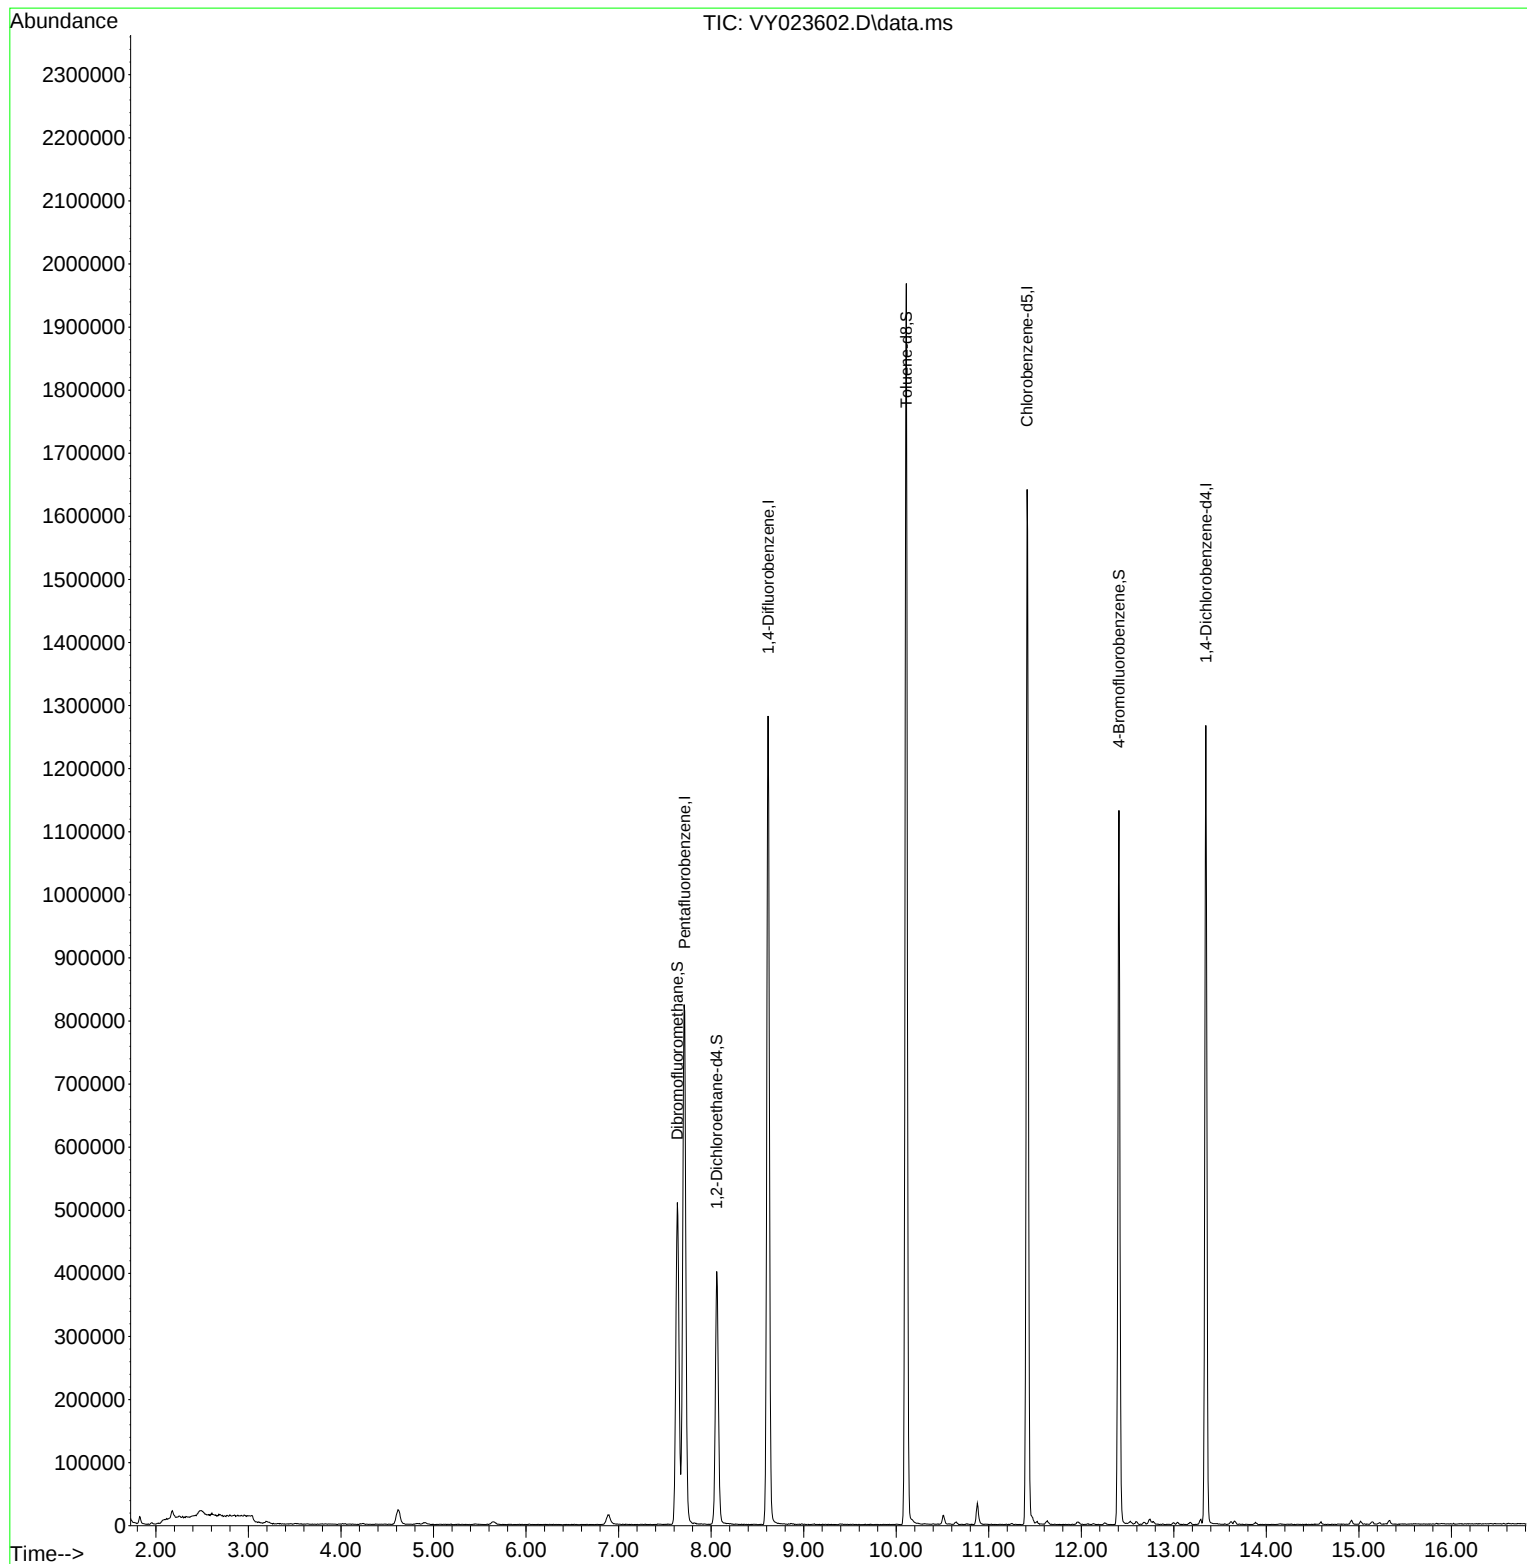




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY023602.D
Acq: 28 Oct 2025 11:03




Instrument :
MSVOA_Y
ClientSampleId :
WC-5-VOC


Tgt Ion:168 Resp: 699508
Ion Ratio Lower Upper
168 100
99 47.6 39.7 59.5

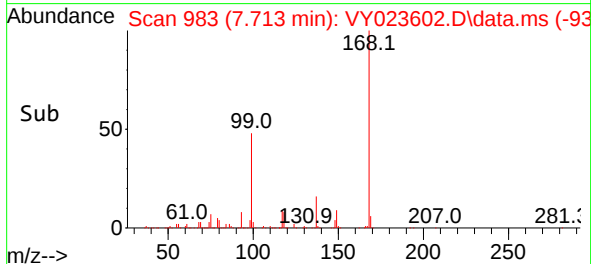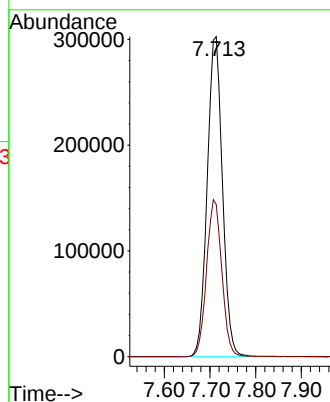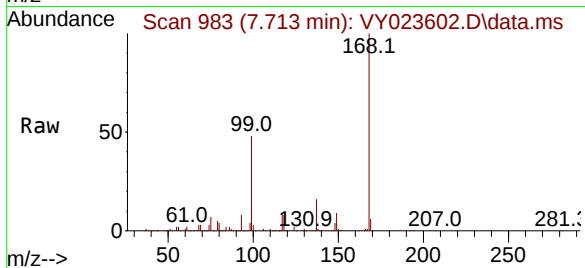

#33
1,2-Dichloroethane-d4
Concen: 52.618 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY023602.D
Acq: 28 Oct 2025 11:03

Tgt Ion: 65 Resp: 307782
Ion Ratio Lower Upper
65 100
67 53.2 0.0 105.8

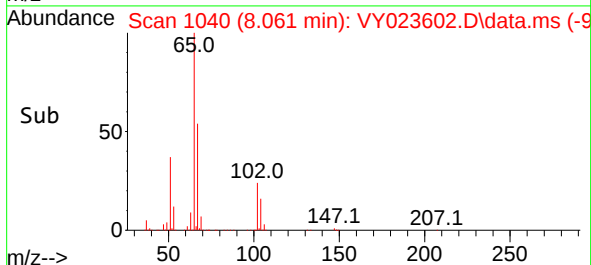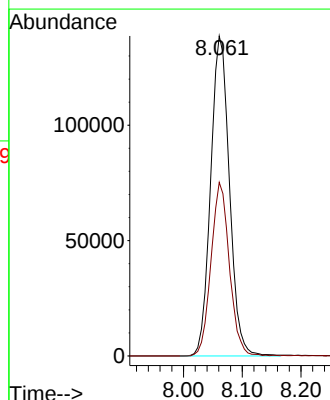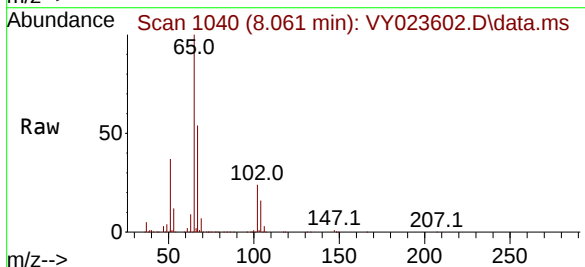

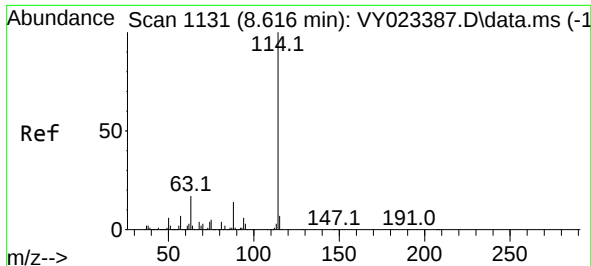

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. 0.000 min

Lab File: VY023602.D

Acq: 28 Oct 2025 11:03

Instrument :

MSVOA_Y

ClientSampleId :

WC-5-VOC





Tgt Ion:114 Resp: 1162114

Ion Ratio Lower Upper

114 100

63 17.2 0.0 34.2

88 14.4 0.0 28.4

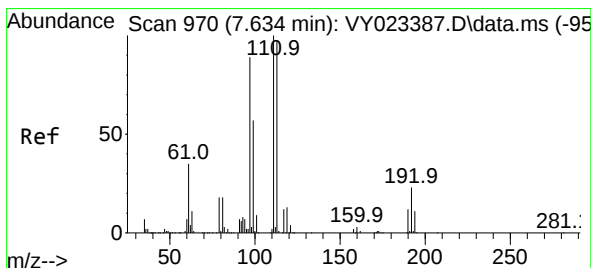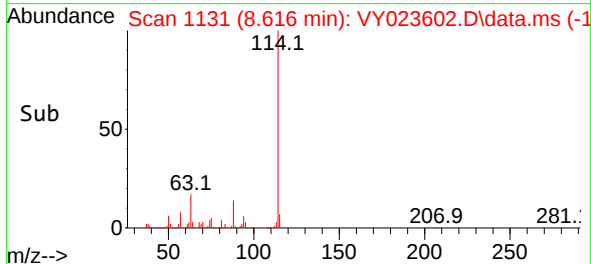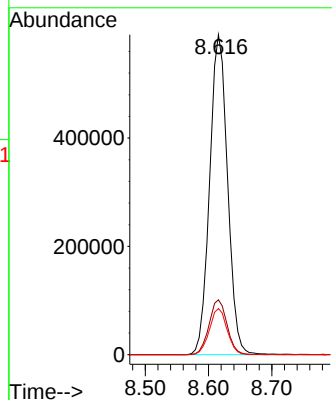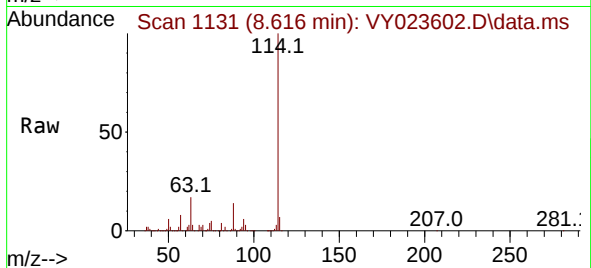

#35

Dibromofluoromethane

Concen: 51.340 ug/l

RT: 7.634 min Scan# 970

Delta R.T. 0.000 min

Lab File: VY023602.D

Acq: 28 Oct 2025 11:03




Tgt Ion:113 Resp: 366598


Ion Ratio Lower Upper

113 100

111 101.6 81.8 122.6

192 22.1 18.0 27.0

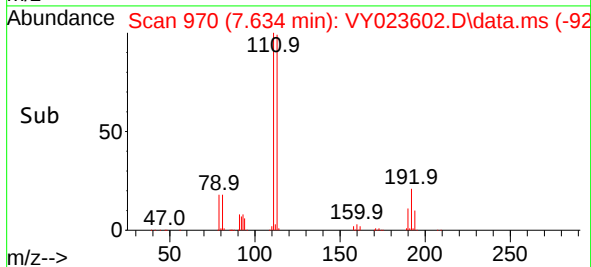
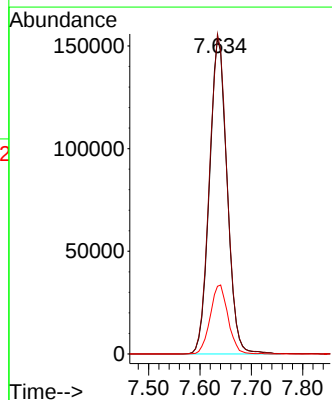
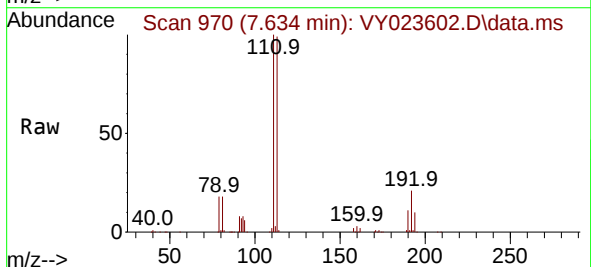


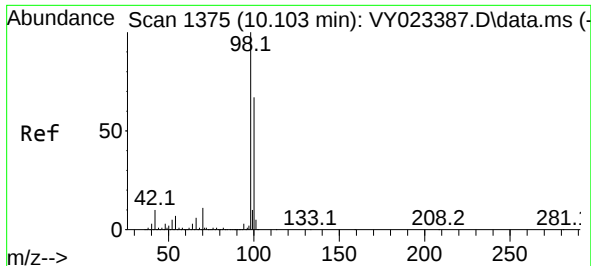

#50
Toluene-d8
Concen: 49.036 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY023602.D
Acq: 28 Oct 2025 11:03




Instrument :
MSVOA_Y
ClientSampleId :
WC-5-VOC

Tgt Ion: 98 Resp: 1303992
Ion Ratio Lower Upper
98 100
100 64.8 53.0 79.4

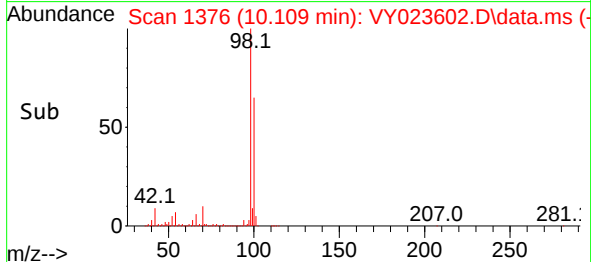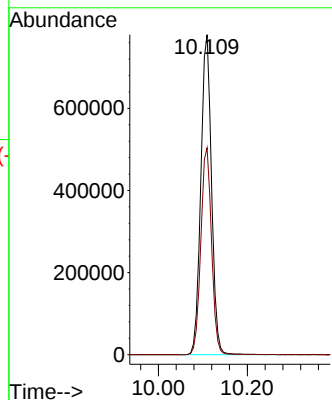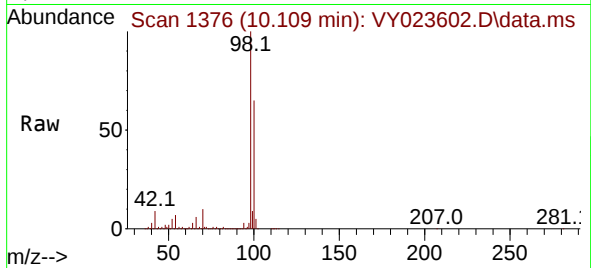

#62
4-Bromofluorobenzene
Concen: 38.133 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY023602.D
Acq: 28 Oct 2025 11:03

Tgt Ion: 95 Resp: 334787
Ion Ratio Lower Upper
95 100
174 95.1 0.0 192.8
176 92.7 0.0 187.6

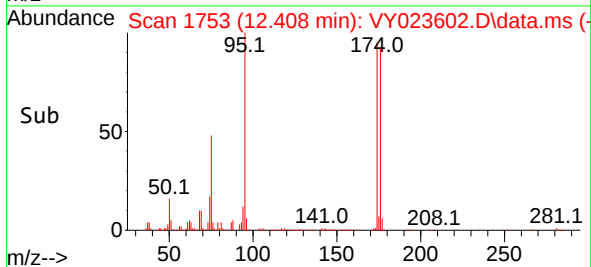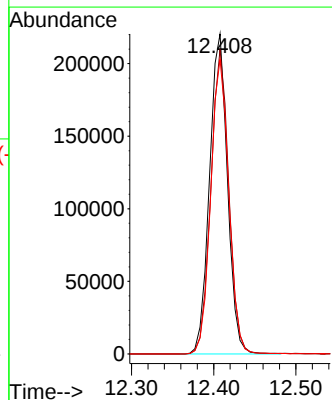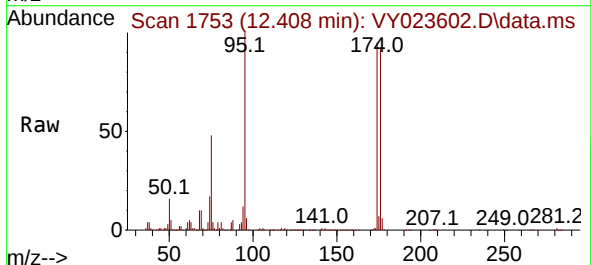



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY023602.D

Acq: 28 Oct 2025 11:03

Instrument :

MSVOA_Y

ClientSampleId :

WC-5-VOC





Tgt Ion:117 Resp: 937535

Ion Ratio Lower Upper

117 100

82 51.3 41.0 61.4

119 32.1 25.6 38.4

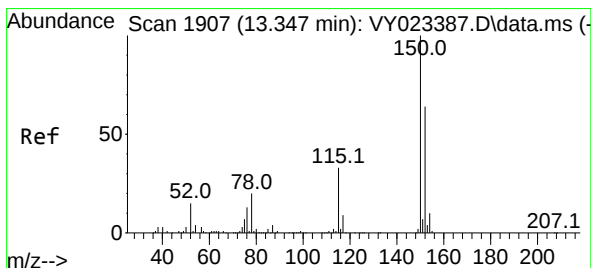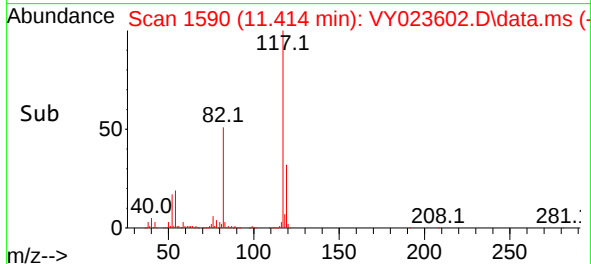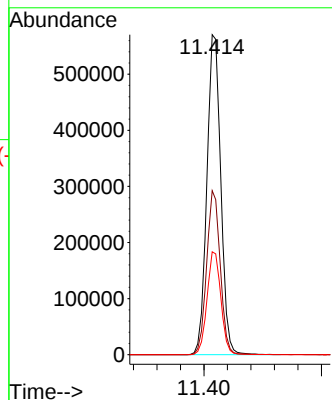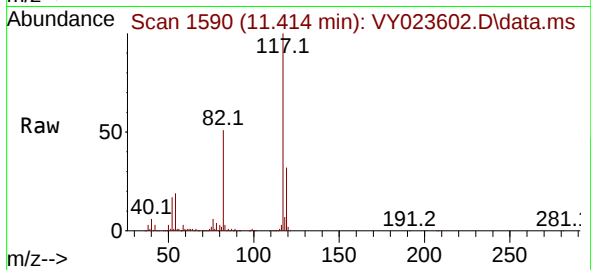

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY023602.D

Acq: 28 Oct 2025 11:03

Tgt Ion:152 Resp: 332594

Ion Ratio Lower Upper

152 100

115 55.4 27.1 81.2

150 157.4 0.0 347.4

