


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY103025\
Data File : VY023619.D
Acq On : 30 Oct 2025 08:39
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Title : SW846 8260
Last Update : Wed Oct 08 05:12:50 2025

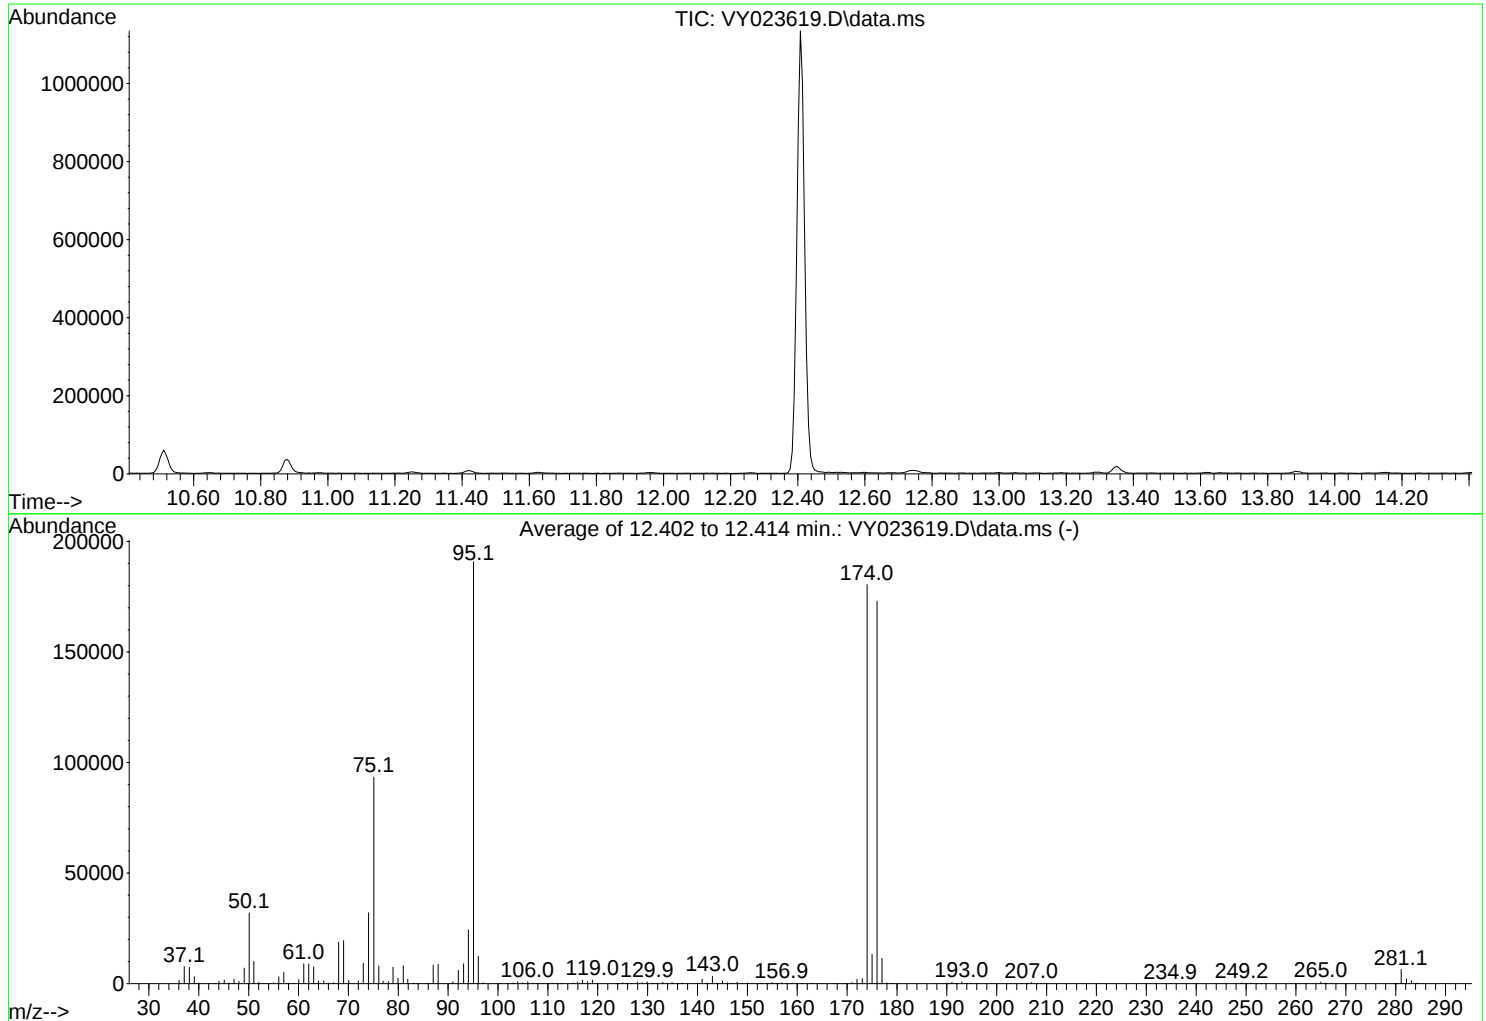

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	31989	PASS
75	95	30	60	49.0	93424	PASS
95	95	100	100	100.0	190763	PASS
96	95	5	9	6.5	12415	PASS
173	174	0.00	2	1.2	2229	PASS
174	95	50	100	94.6	180501	PASS
175	174	5	9	7.3	13251	PASS
176	174	95	101	95.8	172949	PASS
177	176	5	9	6.6	11425	PASS