

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY103124\
 Data File : VY020105.D
 Acq On : 31 Oct 2024 19:19
 Operator : SY/MD
 Sample : P4645-03
 Misc : 3.78g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 Z-02-VOC

Quant Time: Nov 01 03:52:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103024S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 31 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	175543	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.616	114	373000	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	338503	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	122699	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	124928	57.022	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	114.040%
35) Dibromofluoromethane	7.634	113	122235	51.543	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	103.080%
50) Toluene-d8	10.103	98	466618	49.431	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	98.860%
62) 4-Bromofluorobenzene	12.401	95	139931	45.637	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	91.280%
Target Compounds						
16) Acetone	3.866	43	4152	8.149	ug/l	# 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY103124\
Data File : VY020105.D
Acq On : 31 Oct 2024 19:19
Operator : SY/MD
Sample : P4645-03
Misc : 3.78g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
Z-02-VOC

Quant Time: Nov 01 03:52:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103024S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 31 15:23:13 2024
Response via : Initial Calibration




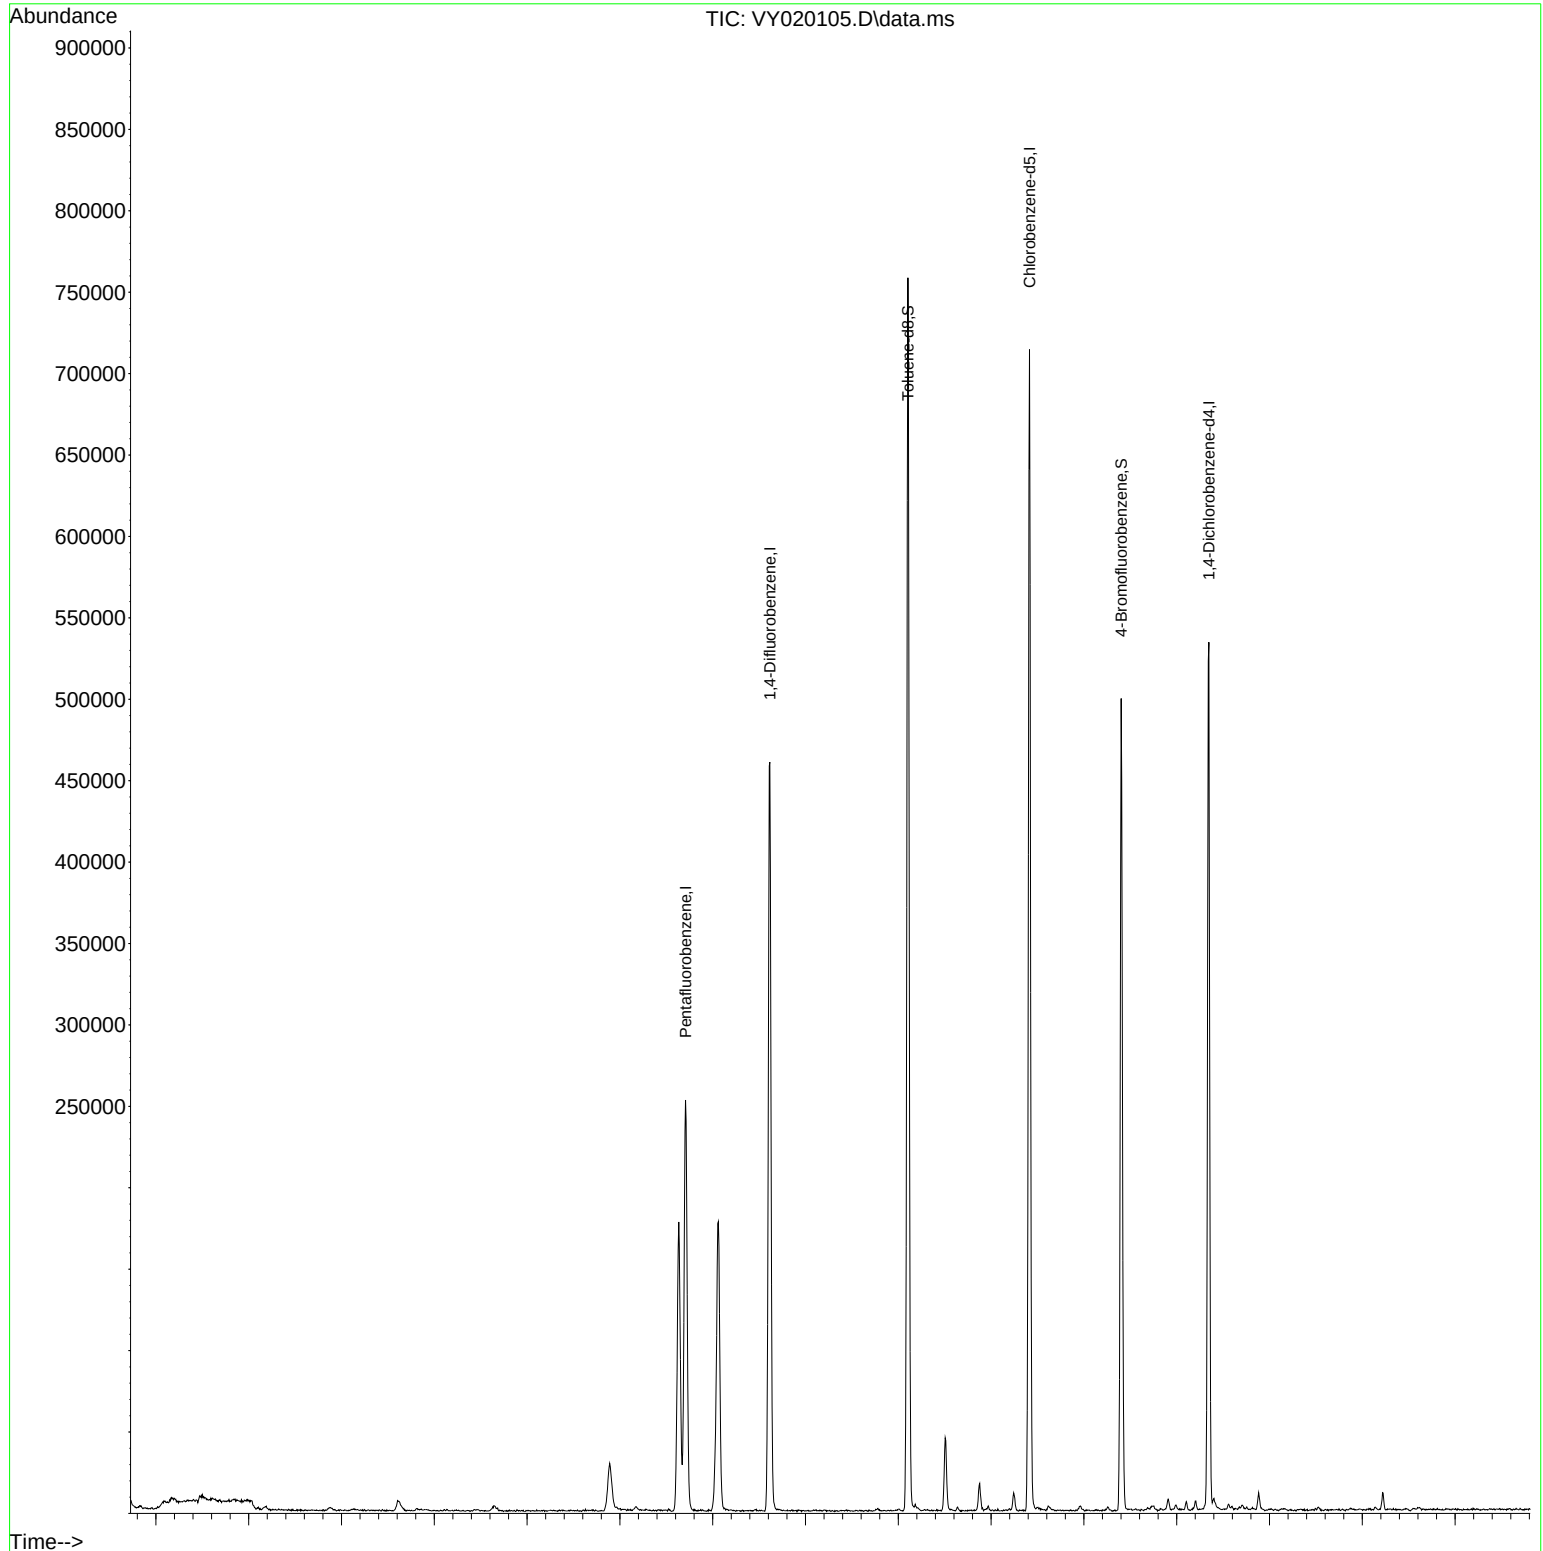


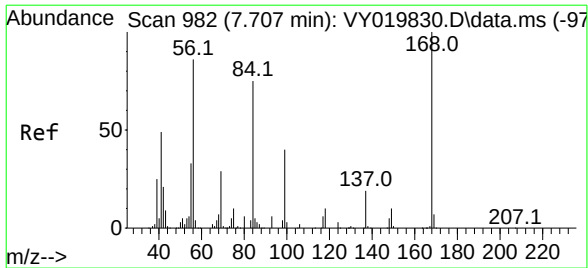

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 98
Delta R.T. 0.000 min
Lab File: VY020105.D
Acq: 31 Oct 2024 19:19




Instrument :
MSVOA_Y
ClientSampleId :
Z-02-VOC


Tgt Ion:168 Resp: 175543
Ion Ratio Lower Upper
168 100
99 64.5 39.1 58.7#

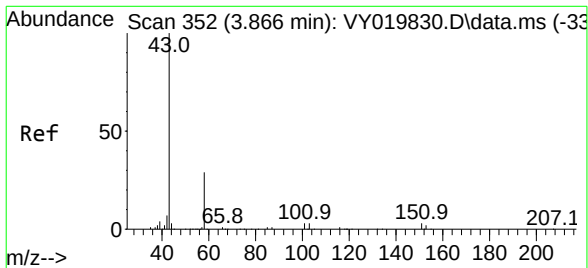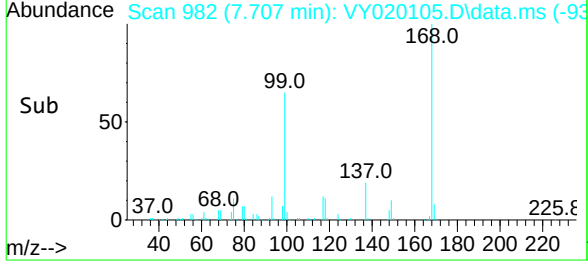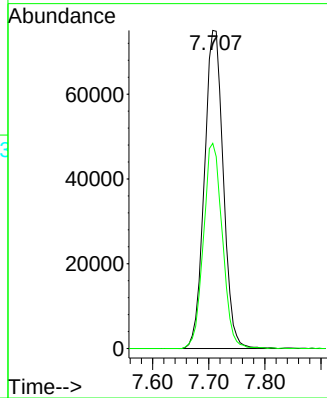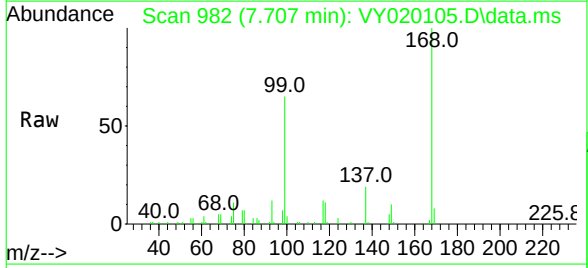

#16
Acetone
Concen: 8.149 ug/l
RT: 3.866 min Scan# 352
Delta R.T. -0.006 min
Lab File: VY020105.D
Acq: 31 Oct 2024 19:19

Tgt Ion: 43 Resp: 4152
Ion Ratio Lower Upper
43 100
58 22.5 31.7 47.5#


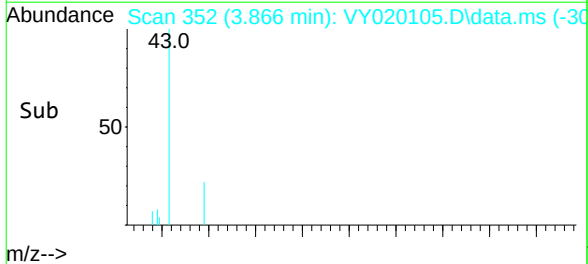
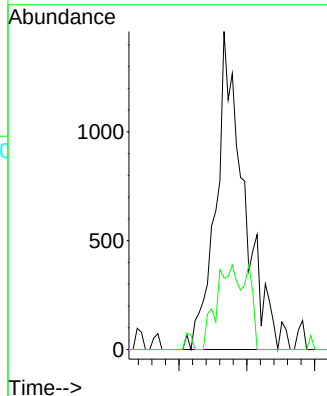
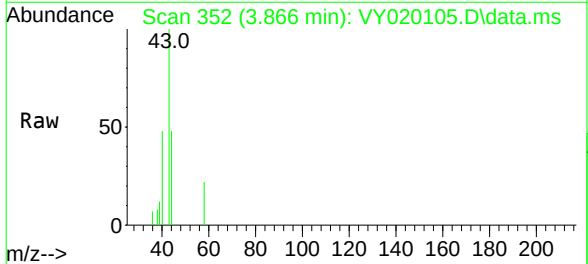


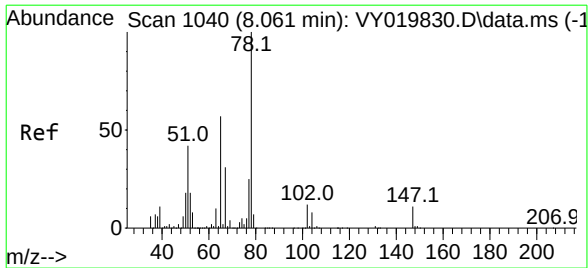

#33
1,2-Dichloroethane-d4
Concen: 57.022 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY020105.D
Acq: 31 Oct 2024 19:19




Instrument :
MSVOA_Y
ClientSampleId :
Z-02-VOC


Tgt Ion: 65 Resp: 124928
Ion Ratio Lower Upper
65 100
67 52.6 0.0 109.6

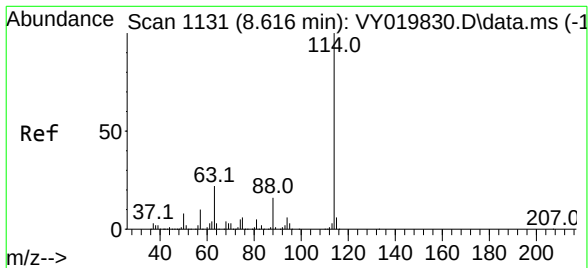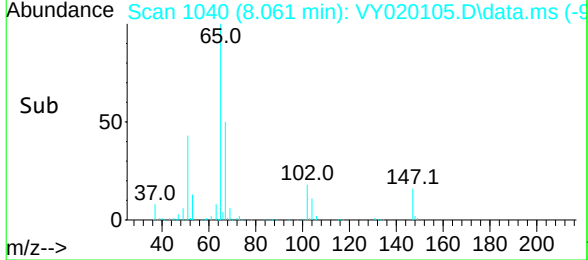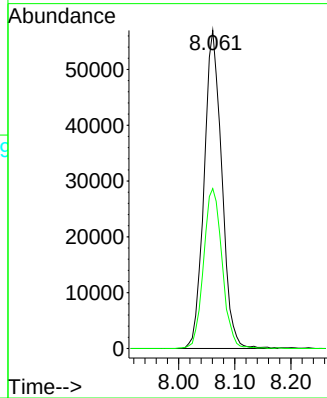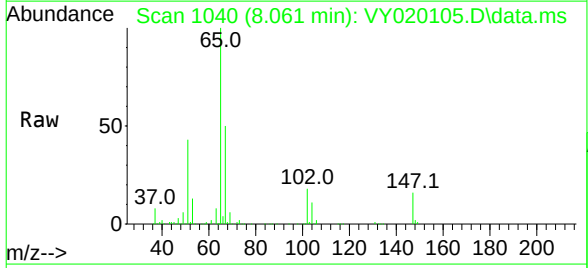

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY020105.D
Acq: 31 Oct 2024 19:19

Tgt Ion: 114 Resp: 373000
Ion Ratio Lower Upper
114 100
63 22.8 0.0 35.0
88 15.8 0.0 27.2

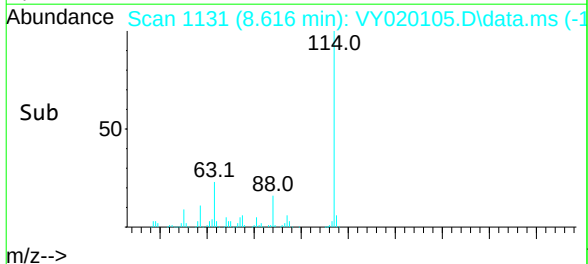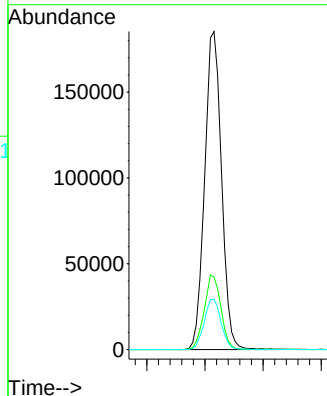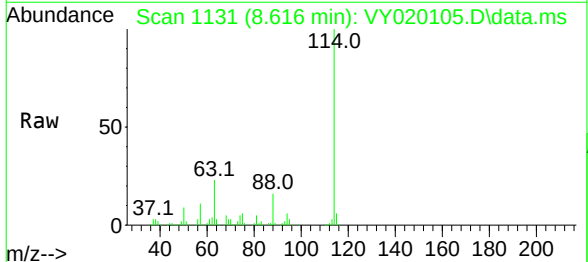

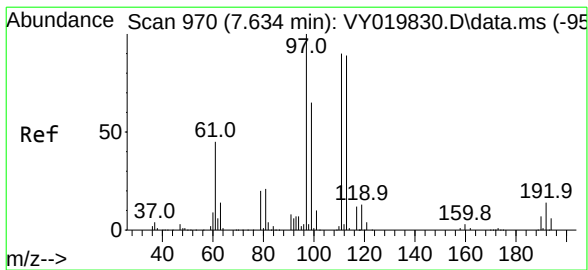

#35

Dibromofluoromethane

Concen: 51.543 ug/l

RT: 7.634 min Scan# 970

Delta R.T. 0.000 min

Lab File: VY020105.D

Acq: 31 Oct 2024 19:19

Instrument :

MSVOA_Y

ClientSampleId :

Z-02-VOC





Tgt Ion:113 Resp: 122235

Ion Ratio Lower Upper

113 100

111 101.8 82.2 123.4

192 16.4 15.9 23.9

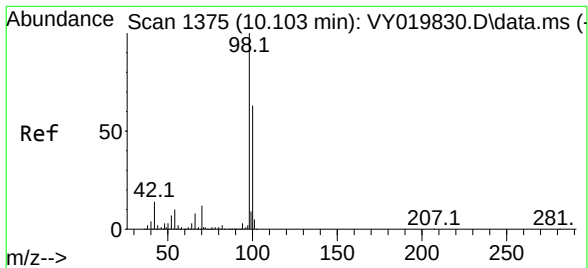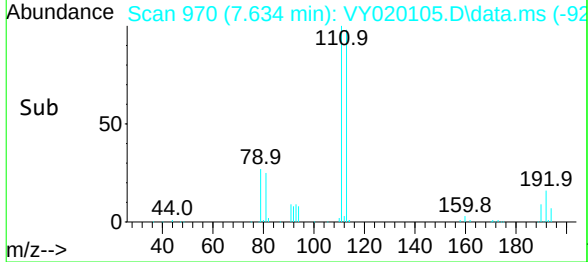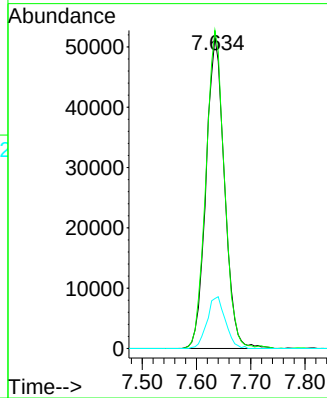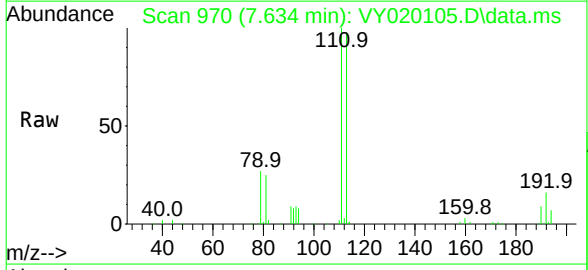

#50

Toluene-d8

Concen: 49.431 ug/l

RT: 10.103 min Scan# 1375

Delta R.T. -0.006 min

Lab File: VY020105.D




Acq: 31 Oct 2024 19:19


Tgt Ion: 98 Resp: 466618

Ion Ratio Lower Upper

98 100

100 63.6 52.0 78.0

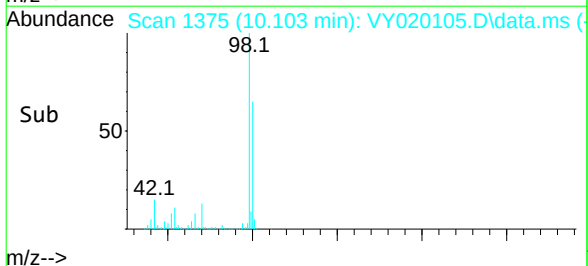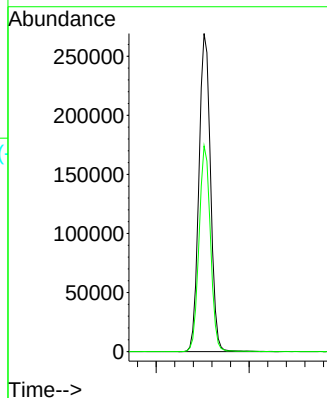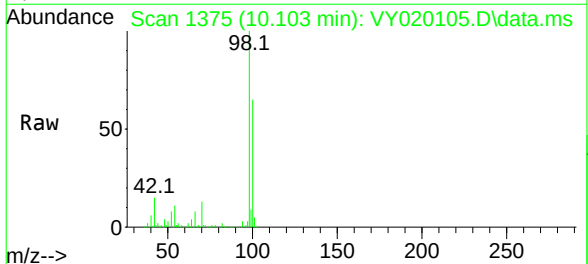

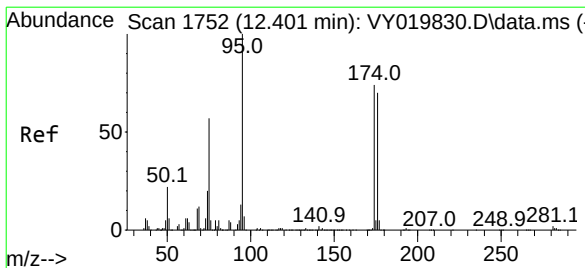

#62

4-Bromofluorobenzene

Concen: 45.637 ug/l

RT: 12.401 min Scan# 1752

Delta R.T. -0.006 min

Lab File: VY020105.D

Acq: 31 Oct 2024 19:19

Instrument :

MSVOA_Y

ClientSampleId :

Z-02-VOC





Tgt Ion: 95 Resp: 139931

Ion Ratio Lower Upper

95 100

174 74.3 0.0 175.6

176 69.9 0.0 171.4

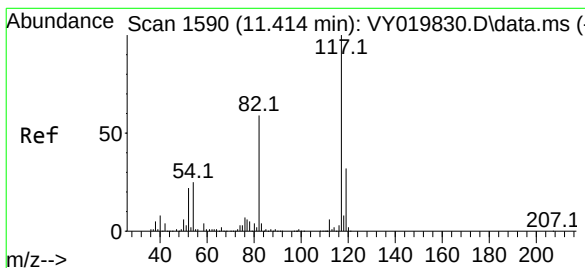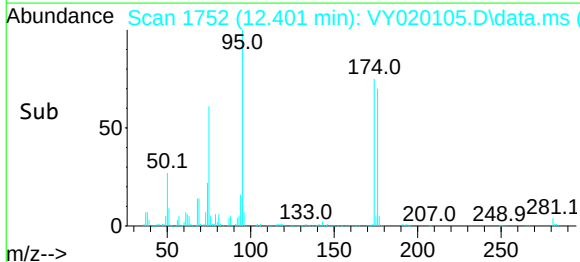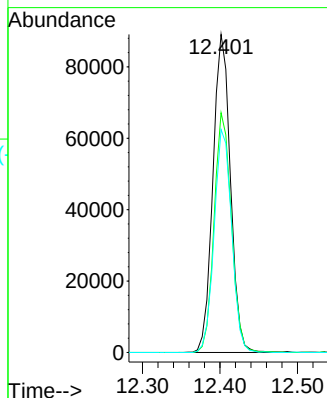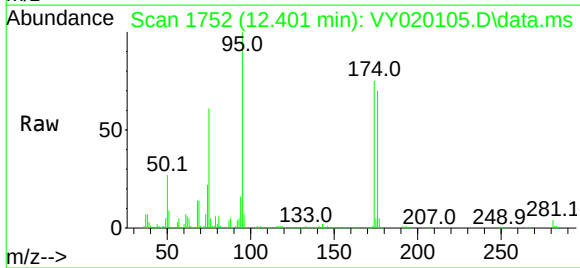

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 1590

Delta R.T. -0.006 min

Lab File: VY020105.D

Acq: 31 Oct 2024 19:19




Tgt Ion: 117 Resp: 338503


Ion Ratio Lower Upper

117 100

82 60.5 42.4 63.6


119 32.5 25.9 38.9

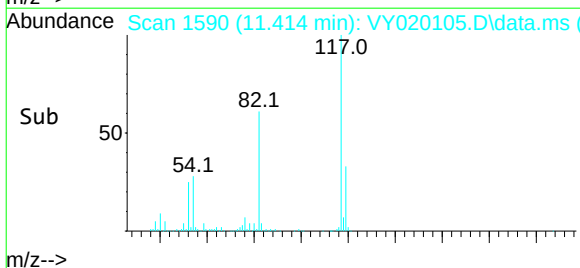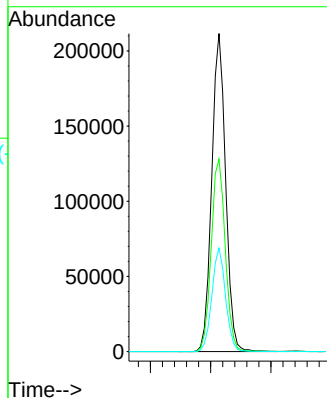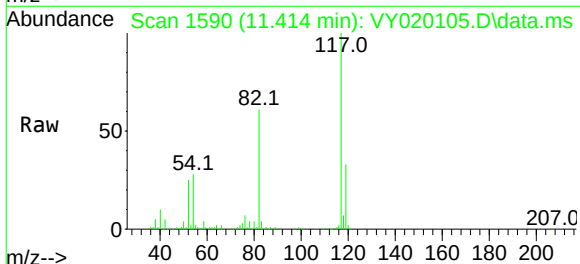

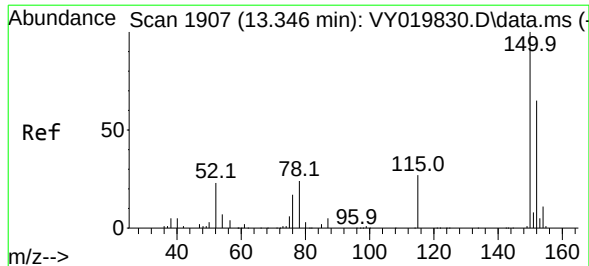

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.346 min Scan# 19
 Delta R.T. 0.000 min
 Lab File: VY020105.D
 Acq: 31 Oct 2024 19:19

Instrument :
 MSVOA_Y
 ClientSampleId :
 Z-02-VOC

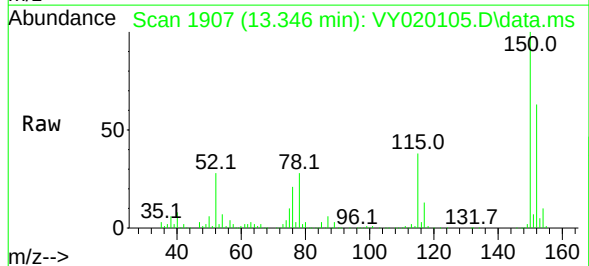

Tgt Ion:	152	Resp:	122699
Ion	Ratio	Lower	Upper
152	100		
115	61.2	28.2	84.7
150	155.1	0.0	345.6

